

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 15:14
 Operator : AR\AJ
 Sample : N2895-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P030-SS001-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/03/2022
 Supervised By :Ankita Jodhani 06/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:06:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	4.188f	9746604	90647729	9.159	10.287m
2) SA Decachlor...	8.195	9.382f	12132477	67351166	11.123	12.454m
Target Compounds						
17) MA 4,4'-DDT	6.354	7.334	9012896	72124095	9.094	9.856

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 15:14
Operator : AR\AJ
Sample : N2895-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P030-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/03/2022
Supervised By : Ankita Jodhani 06/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:06:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

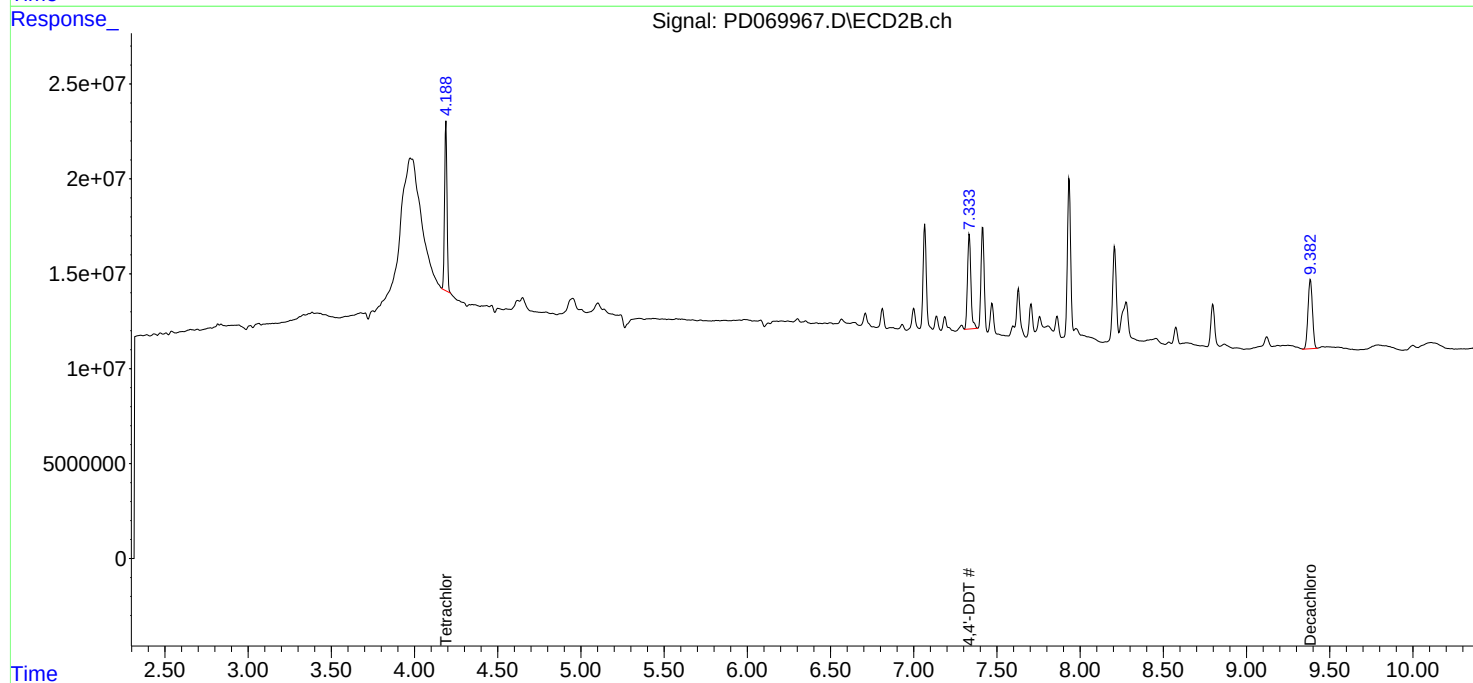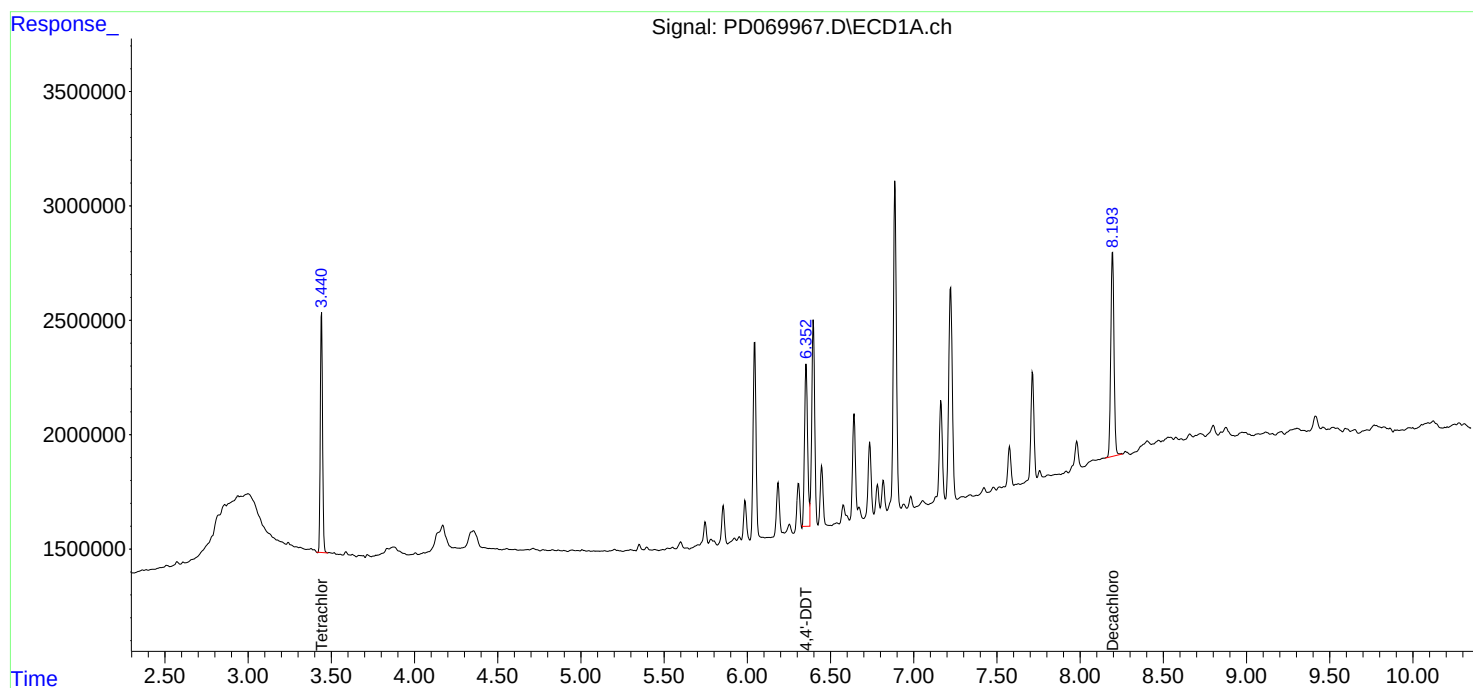

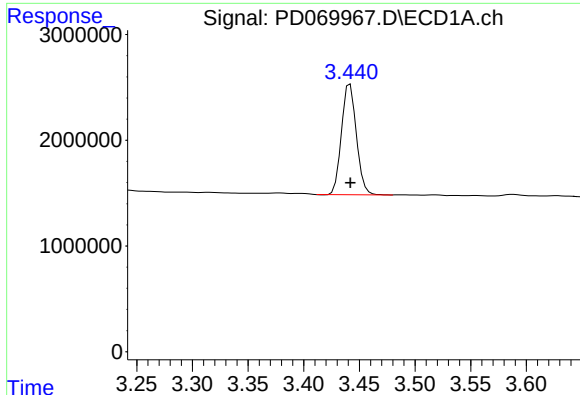


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 9746604
Conc: 9.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

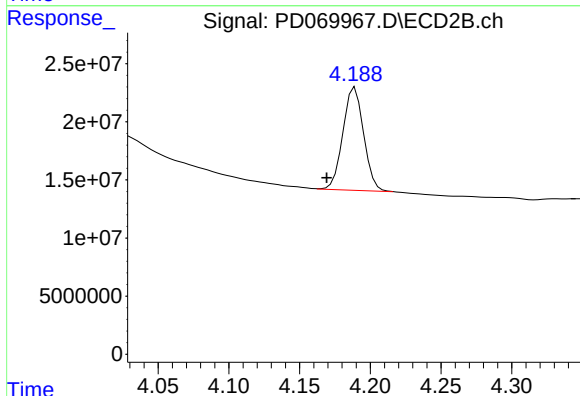


#1 Tetrachloro-m-xylene

R.T.: 4.188 min
Delta R.T.: 0.019 min
Response: 90647729
Conc: 10.29 ng/ml m

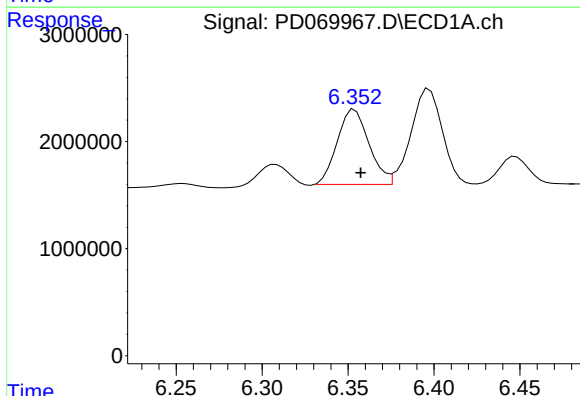


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 9012896
Conc: 9.09 ng/ml

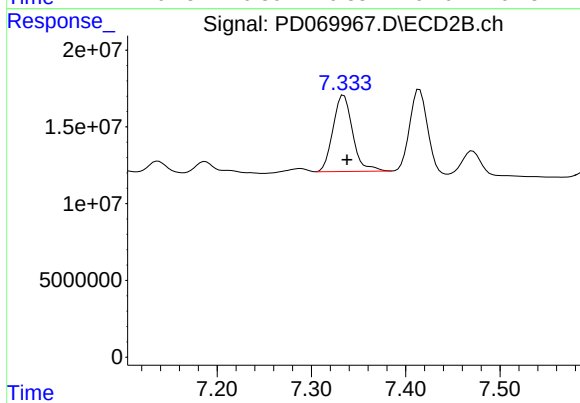

#17 4,4'-DDT

R.T.: 7.334 min
Delta R.T.: -0.003 min
Response: 72124095
Conc: 9.86 ng/ml

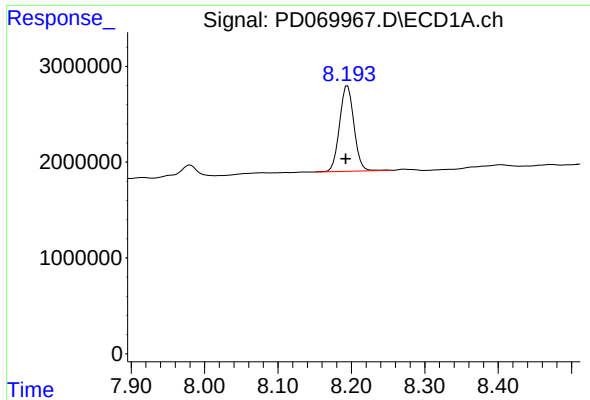


#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.003 min
Response: 12132477
Conc: 11.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

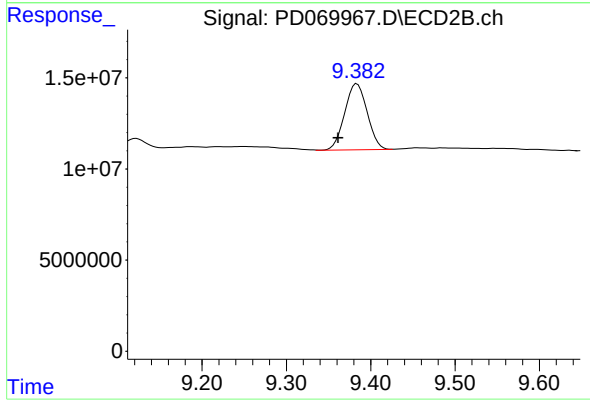

#28 Decachlorobiphenyl

R.T.: 9.382 min
Delta R.T.: 0.021 min
Response: 67351166
Conc: 12.45 ng/ml m