

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 15:28
 Operator : AR\AJ
 Sample : N2895-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P030-SS001-0612-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:07:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.441	4.169	10342102	96779444	9.718	10.983
28) SA Decachlor...	8.194	9.364	10261147	56492128	9.408	10.446
Target Compounds						
12) B 4,4'-DDE	5.601	6.546	770044	8430495	0.608	0.932 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 15:28
Operator : AR\AJ
Sample : N2895-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0612-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:07:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

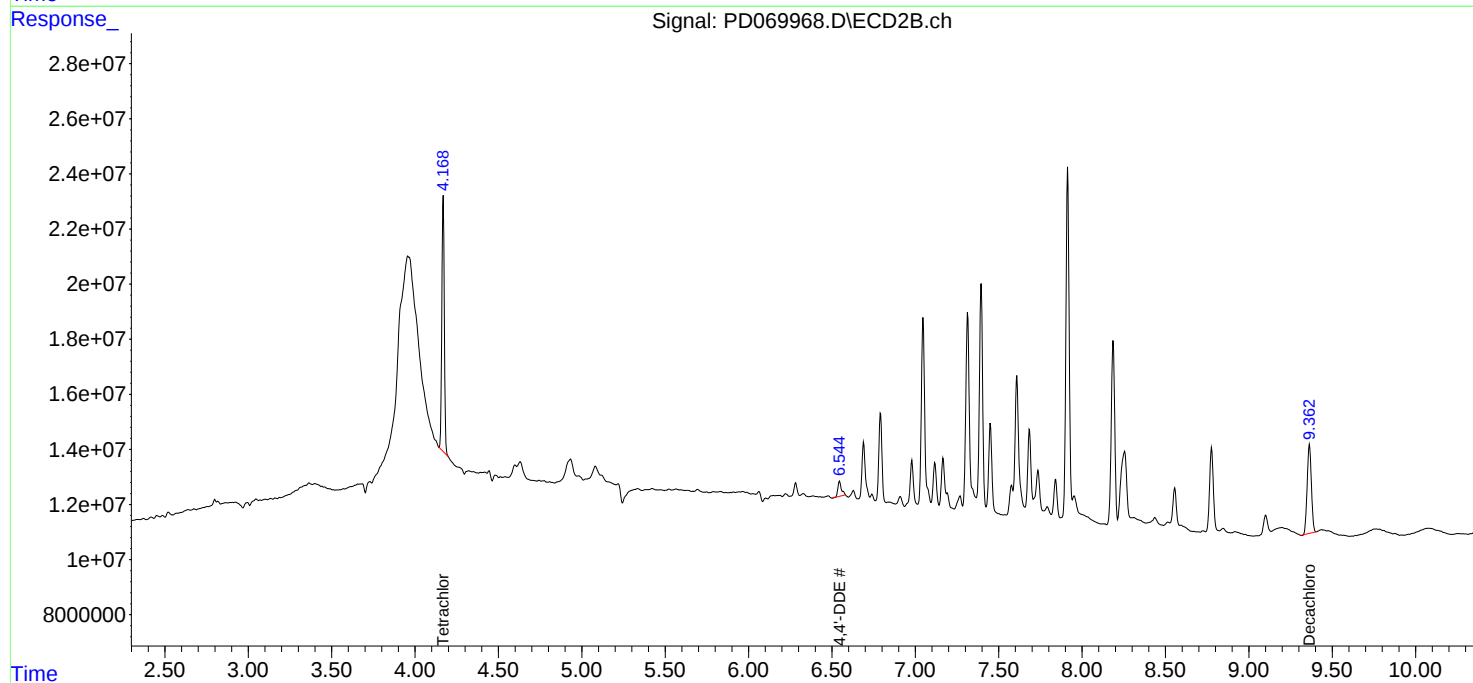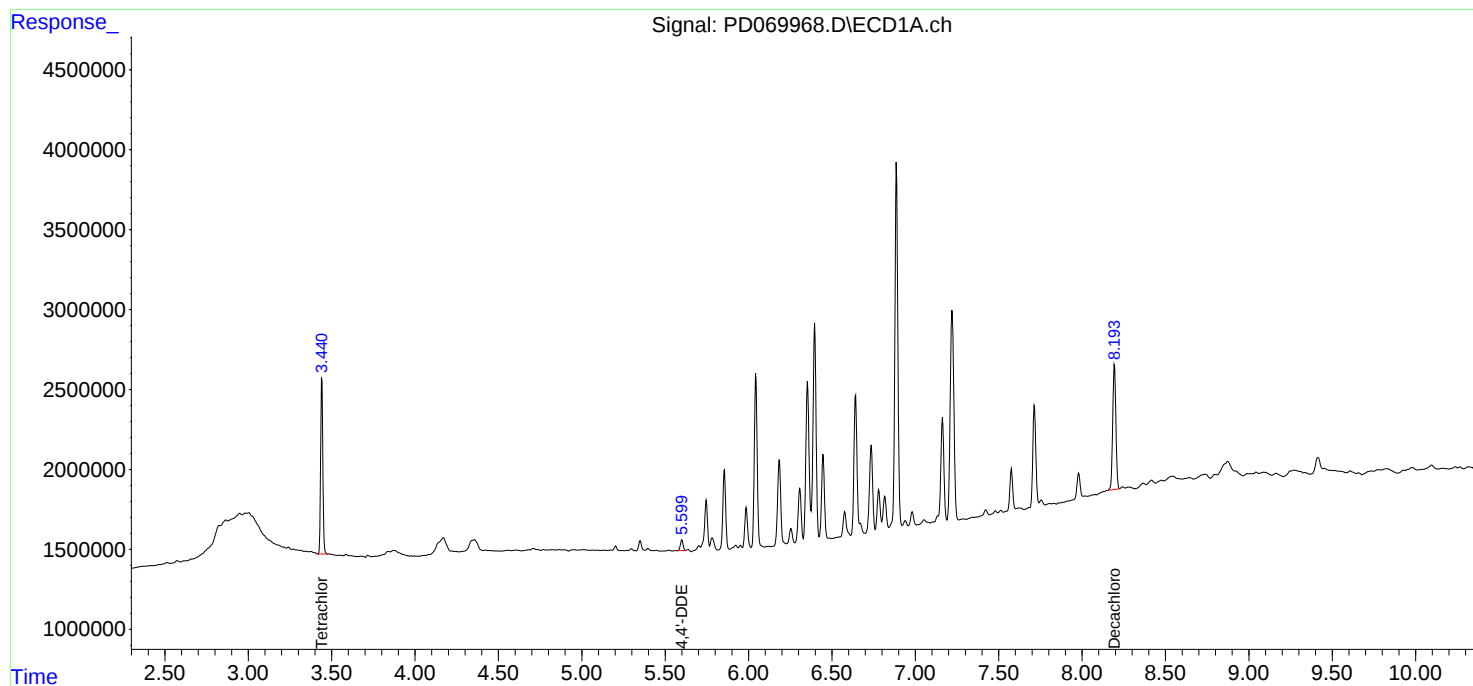


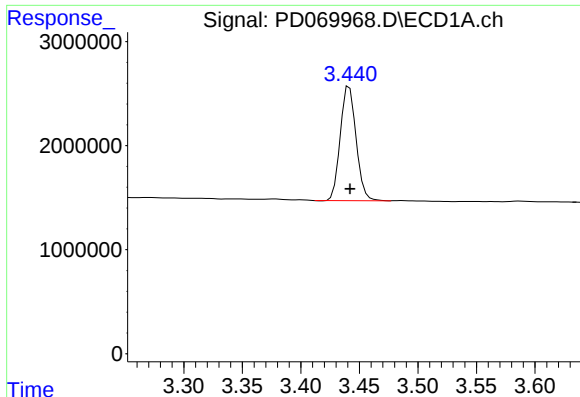

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 10342102
Conc: 9.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0612-01

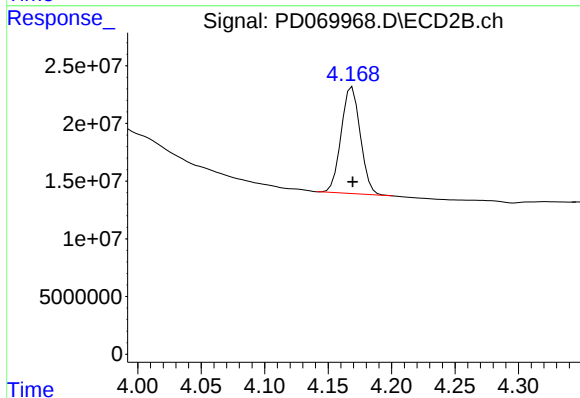


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 96779444
Conc: 10.98 ng/ml

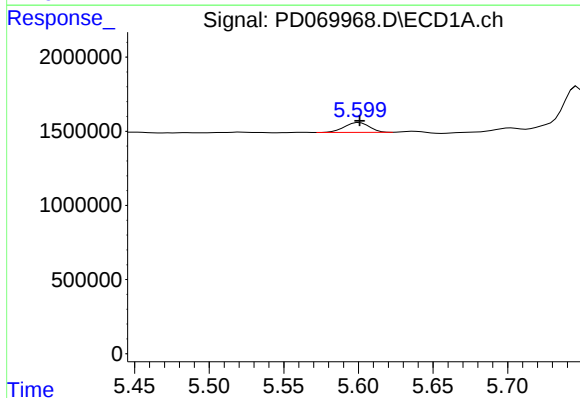


#12 4,4'-DDE

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 770044
Conc: 0.61 ng/ml

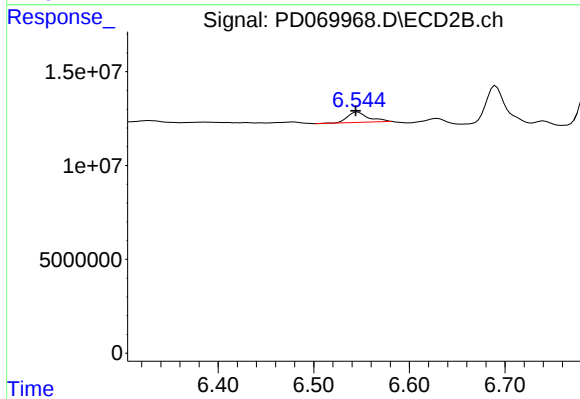

#12 4,4'-DDE


R.T.: 6.546 min
Delta R.T.: 0.002 min
Response: 8430495
Conc: 0.93 ng/ml

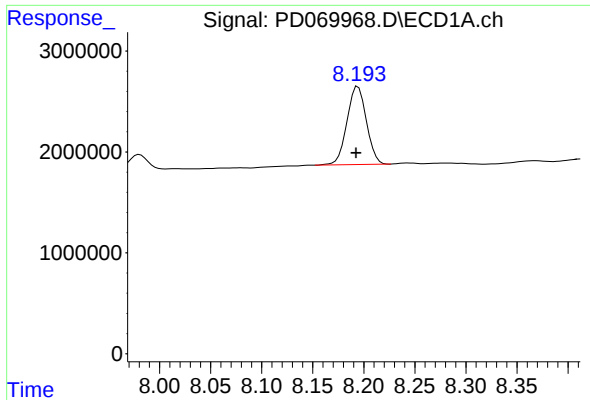

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 10261147
Conc: 9.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0612-01

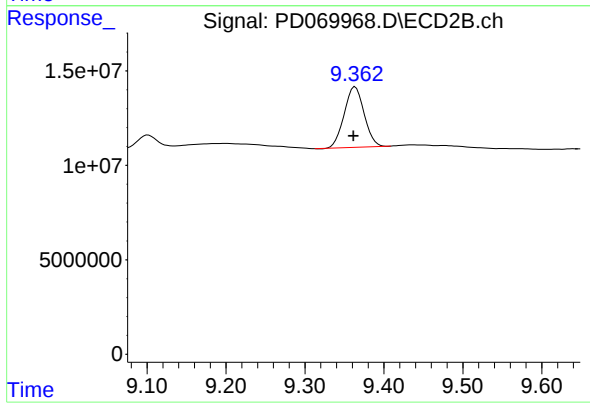

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.002 min
Response: 56492128
Conc: 10.45 ng/ml