

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 15:42
 Operator : AR\AJ
 Sample : N2894-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P008-SS002-0006-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:07:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	18091215	169.8E6	17.000	19.270
28)	SA Decachlor...	8.195	9.363	14698943	85128417	13.476	15.741
Target Compounds							
12)	B 4,4'-DDE	5.602	6.545	3303464	30384261	2.607	3.358 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 15:42
Operator : AR\AJ
Sample : N2894-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
P008-SS002-0006-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:07:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

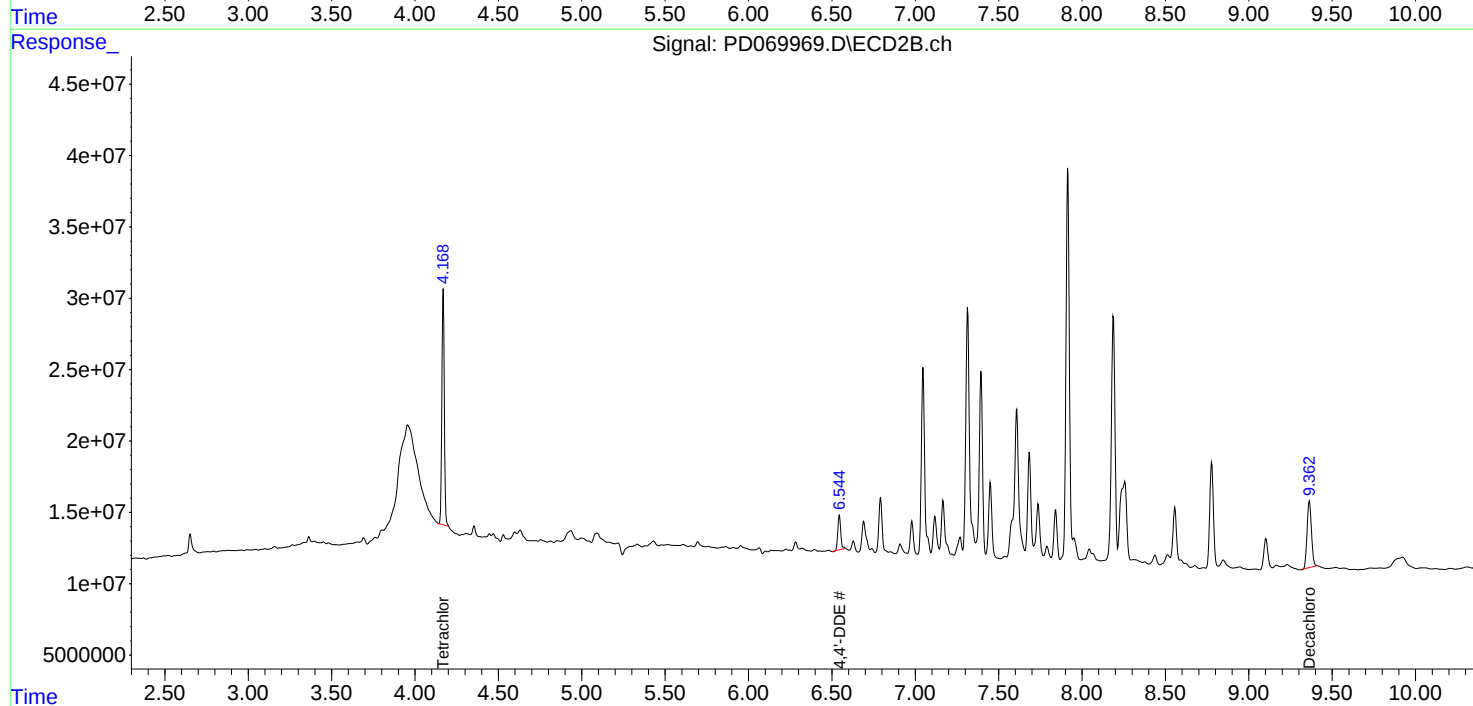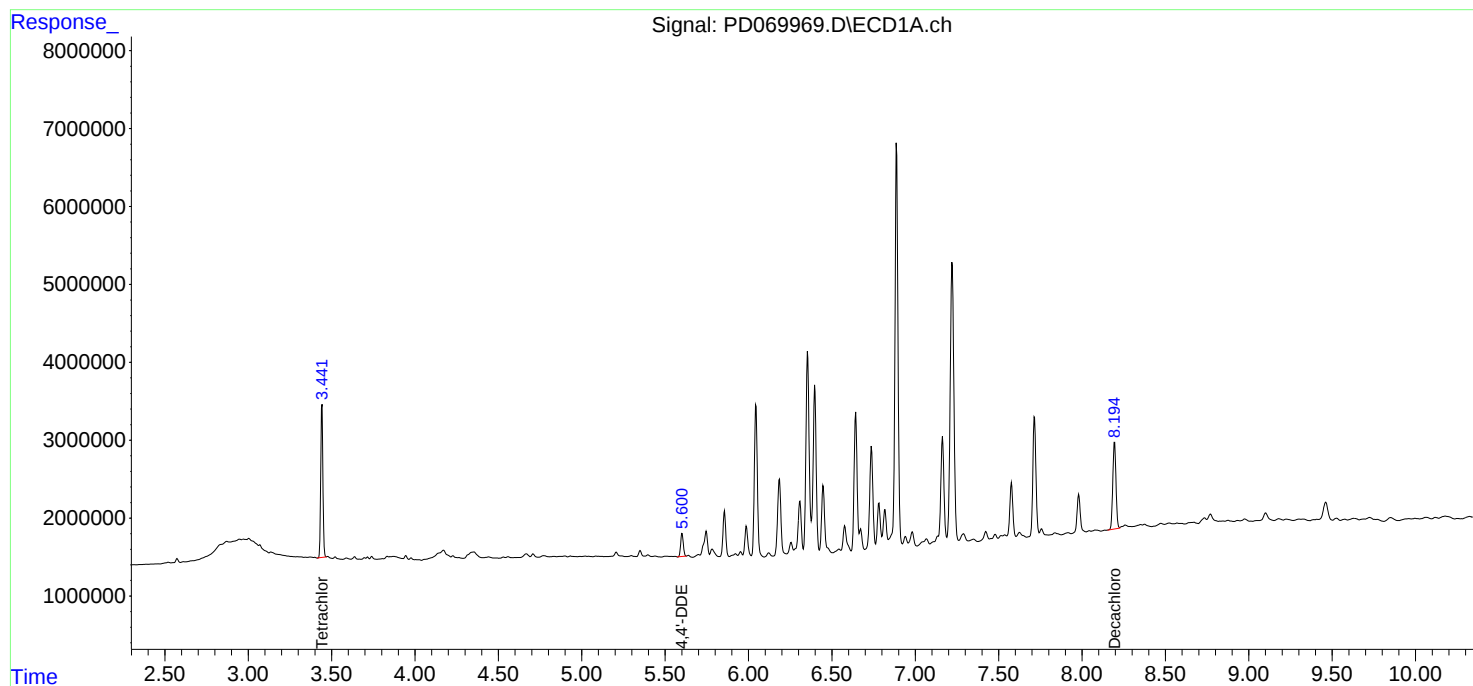


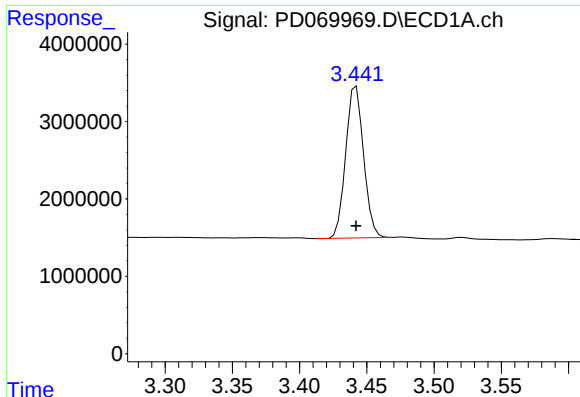

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 18091215
Conc: 17.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS002-0006-01

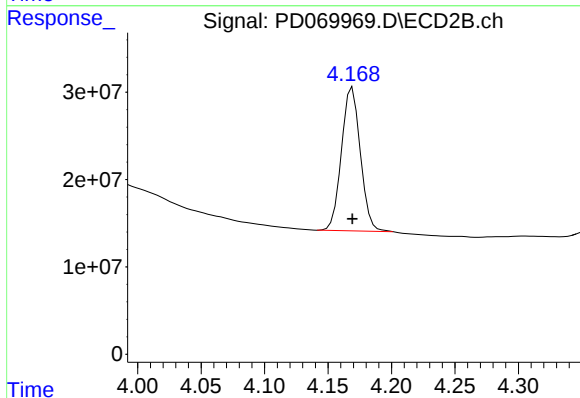


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 169799224
Conc: 19.27 ng/ml

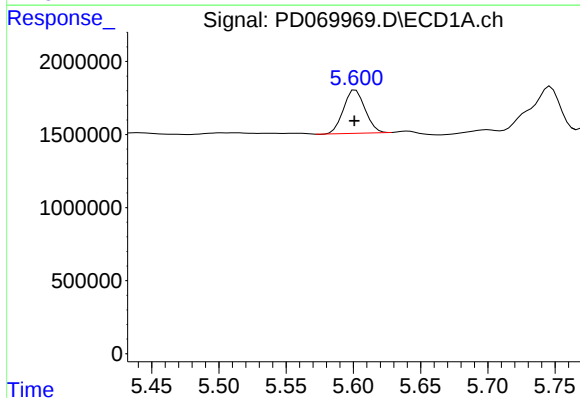


#12 4,4'-DDE

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 3303464
Conc: 2.61 ng/ml

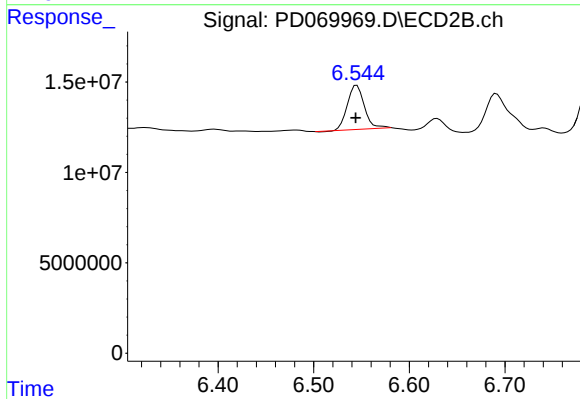

#12 4,4'-DDE


R.T.: 6.545 min
Delta R.T.: 0.001 min
Response: 30384261
Conc: 3.36 ng/ml

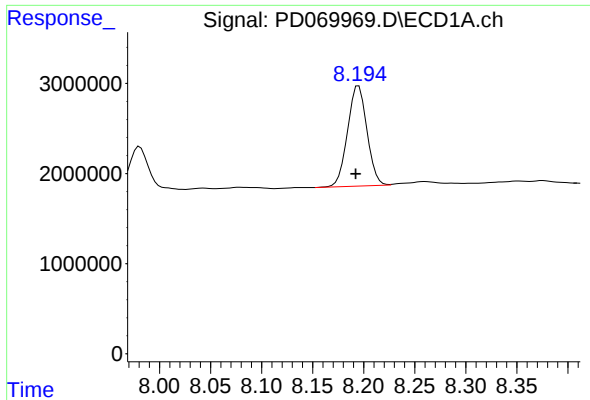

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.003 min
Response: 14698943
Conc: 13.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS002-0006-01

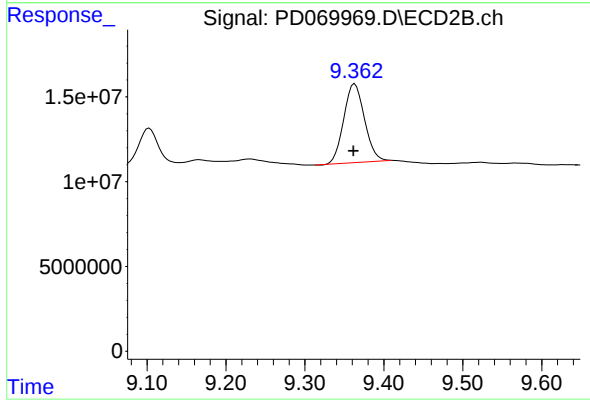

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.002 min
Response: 85128417
Conc: 15.74 ng/ml