

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 00:27
 Operator : AR\AJ
 Sample : N2984-17
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P021-SS001-0612-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/03/2022
 Supervised By : Ankita Jodhani 06/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:14:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	11454876	112.4E6	10.764	12.757
28)	SA Decachlor...	8.194	9.363	15558444	85124284	14.264	15.740
Target Compounds							
12)	B 4,4'-DDE	5.601	6.544	41909509	497.3E6	33.079	54.966m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 00:27
Operator : AR\AJ
Sample : N2984-17
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P021-SS001-0612-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/03/2022
Supervised By : Ankita Jodhani 06/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:14:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

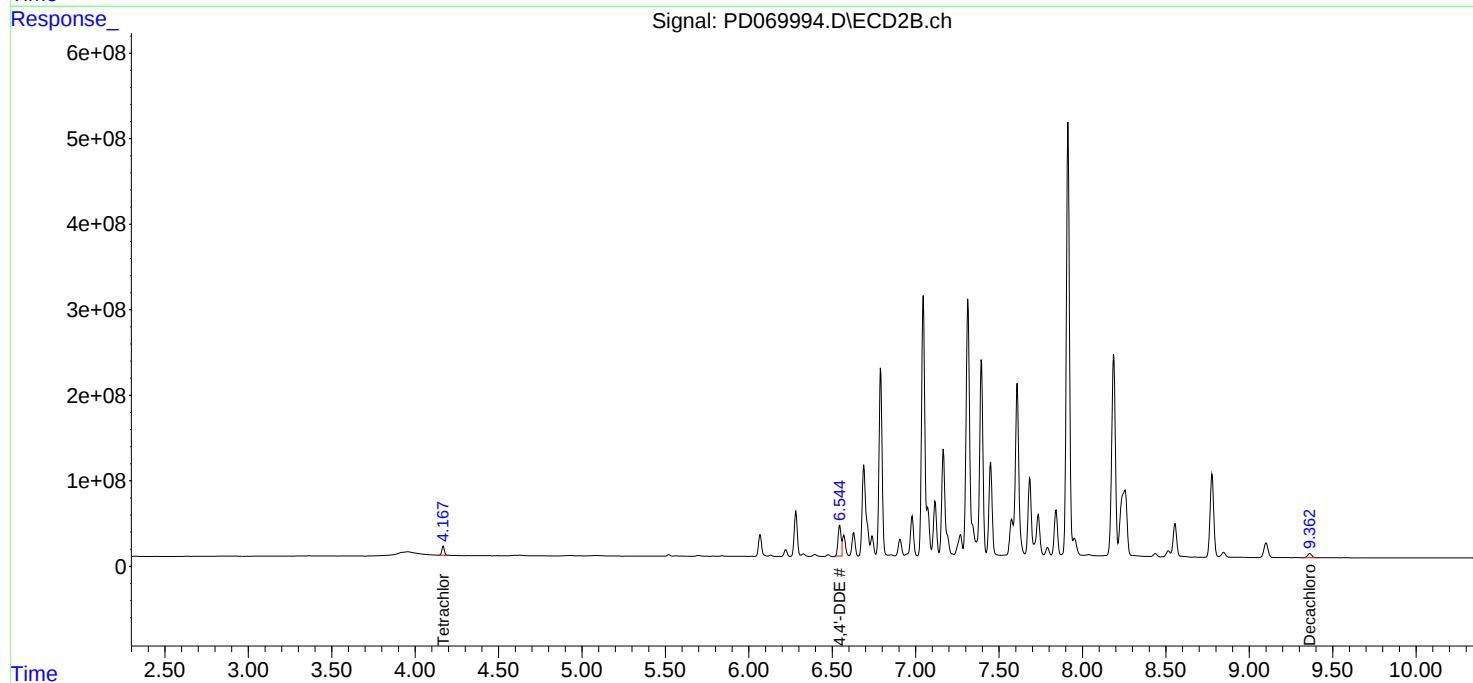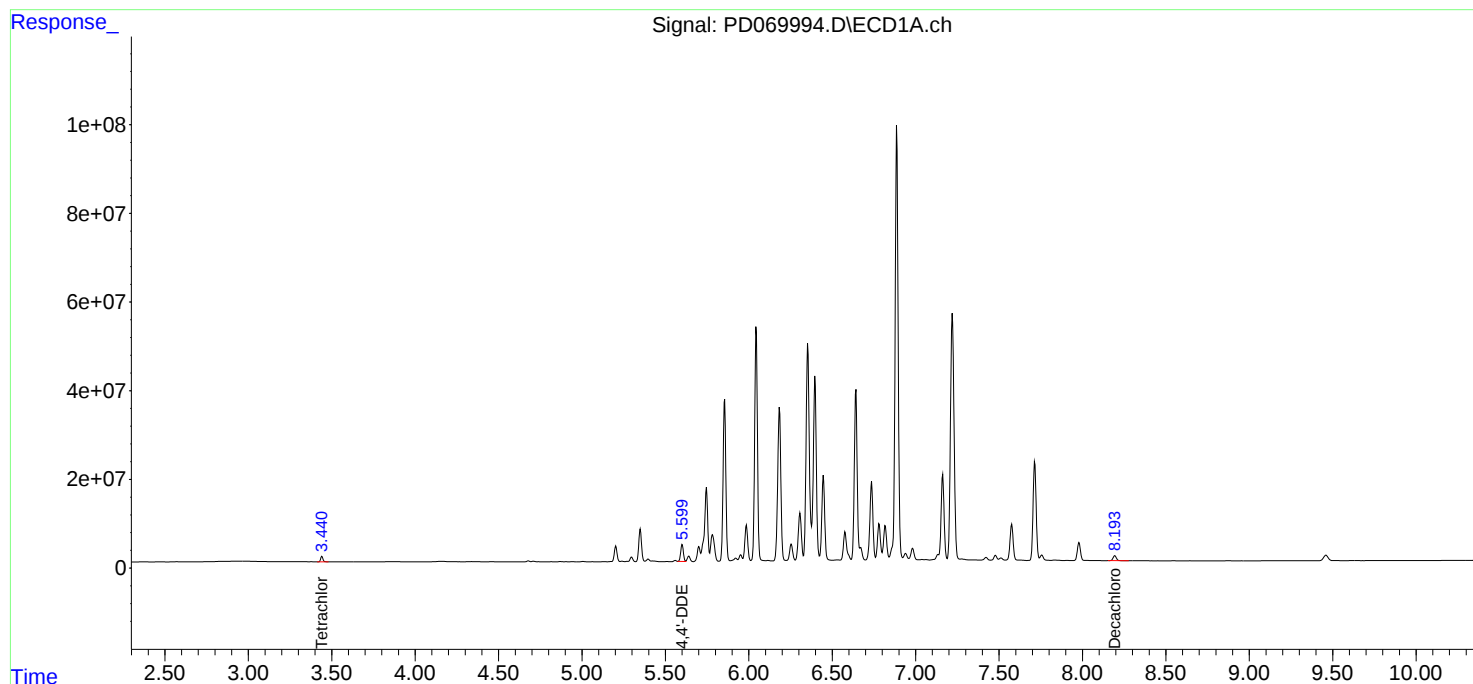

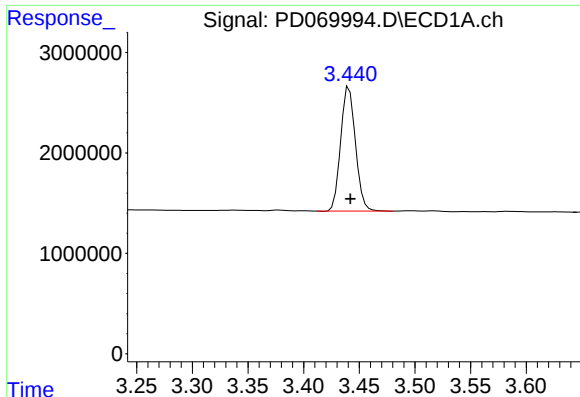


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: -0.001 min
Response: 11454876
Conc: 10.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
P021-SS001-0612-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

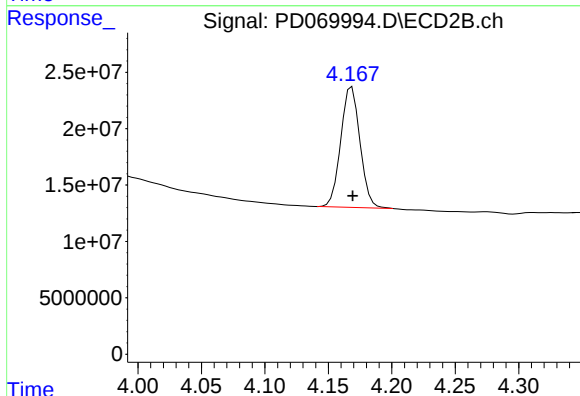


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 112407980
Conc: 12.76 ng/ml

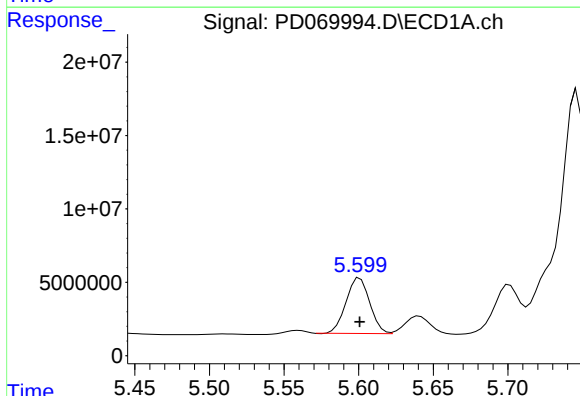


#12 4,4'-DDE

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 41909509
Conc: 33.08 ng/ml

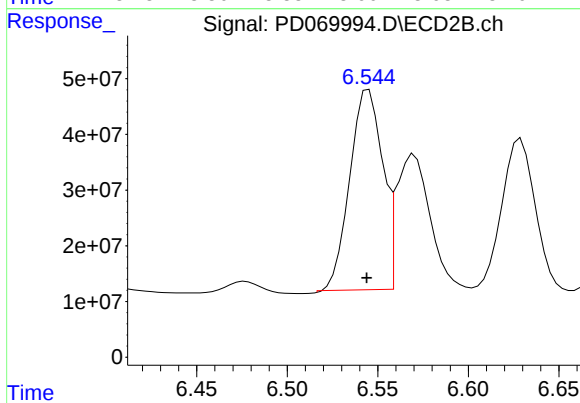

#12 4,4'-DDE

R.T.: 6.544 min
Delta R.T.: 0.000 min
Response: 497321356
Conc: 54.97 ng/ml m

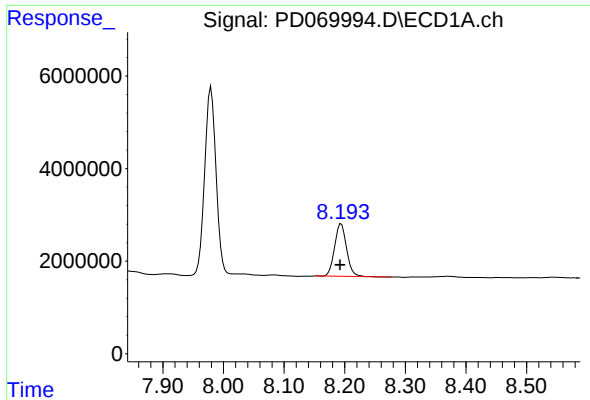


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 15558444
Conc: 14.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
P021-SS001-0612-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

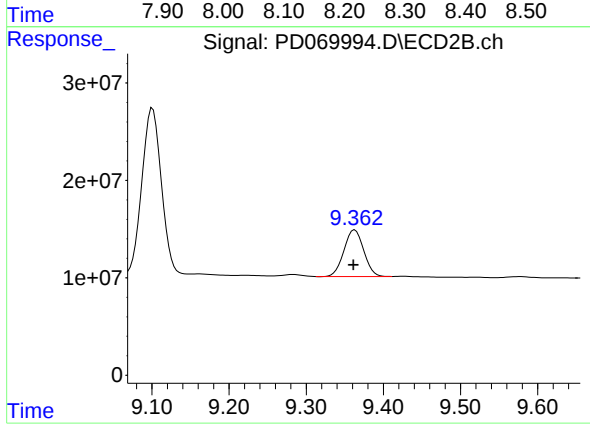

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.002 min
Response: 85124284
Conc: 15.74 ng/ml