

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
 Data File : PD075672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 08:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:56:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
4) MA	Heptachlor	0.000	3.934	0	9657	<MDL
5) MB	Aldrin	0.000	4.270f	0	813828	0.576
6) B	beta-BHC	0.000	3.913	0	90288	0.131
7) B	delta-BHC	0.000	4.146	0	552747	0.381
8) B	Heptachlo...	5.703	4.812f	19409753	3975368	3.021 #
13) MA	Dieldrin	0.000	5.338	0	696281	0.534
14) MA	Endrin	0.000	5.656	0	431082	0.375
15) B	Endosulfa...	0.000	5.920	0	102855	<MDL
20) A	Methoxychlor	7.446f	6.668f	4406658	92771	0.192 #
22)	Toxaphene-1	6.277	0.000	1370556	0	67.032 #
23)	Toxaphene-2	0.000	5.656	0	431082	60.928
24)	Toxaphene-3	0.000	5.920f	0	102855	12.178
25)	Toxaphene-4	0.000	6.668f	0	92771	4.489
26)	Toxaphene-5	0.000	6.668f	0	92771	2.865


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
Data File : PD075672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 08:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:56:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

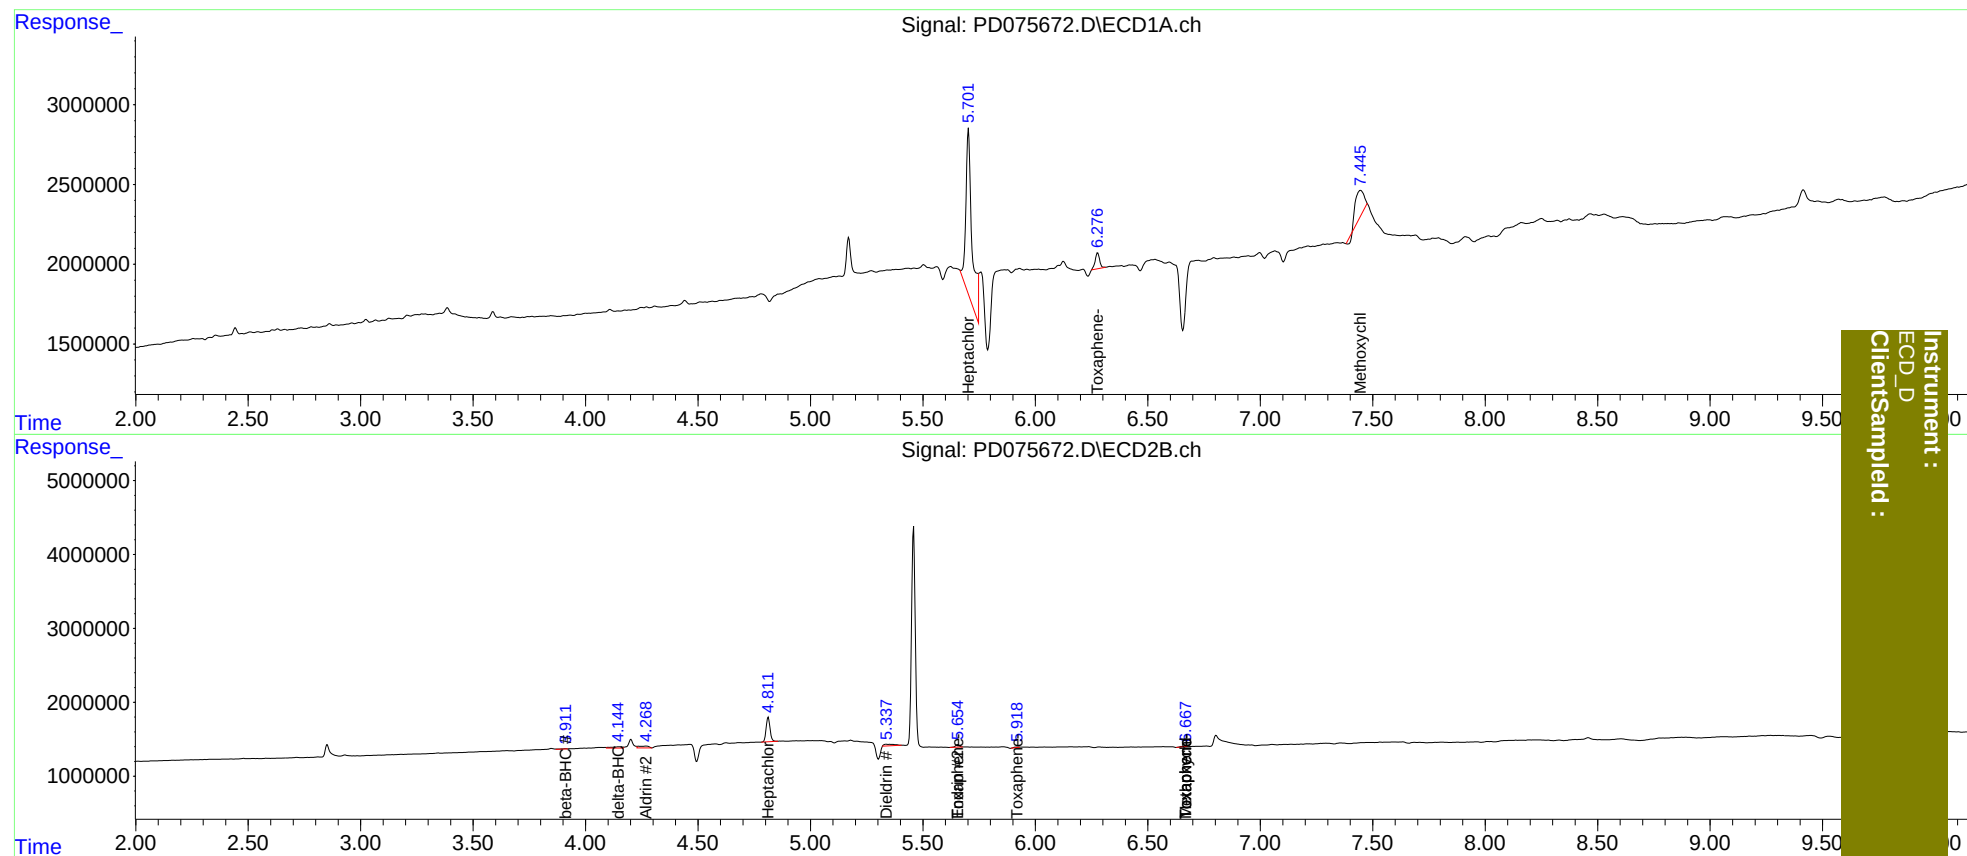


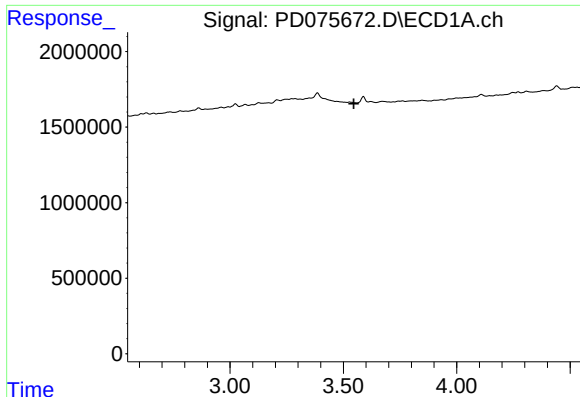

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.546 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

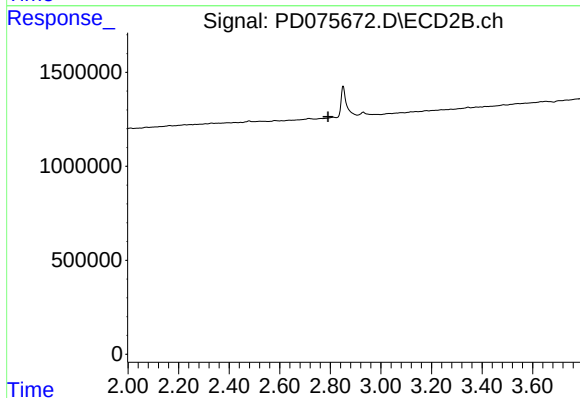


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.791 min
Response: 0
Conc: N.D.

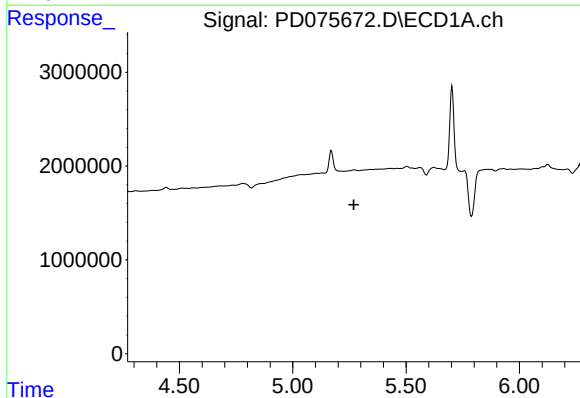


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.269 min
Response: 0
Conc: N.D.

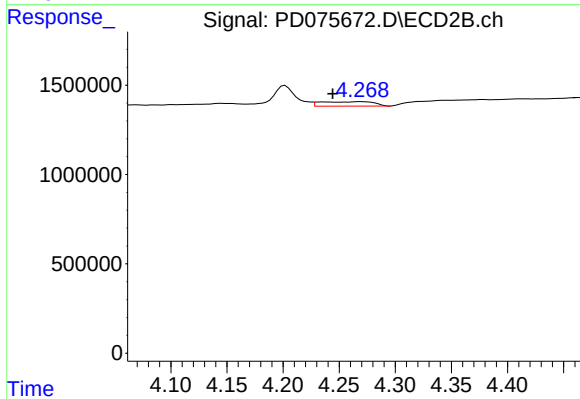

#5 Aldrin


R.T.: 4.270 min
Delta R.T.: 0.026 min
Response: 813828
Conc: 0.58 ng/ml

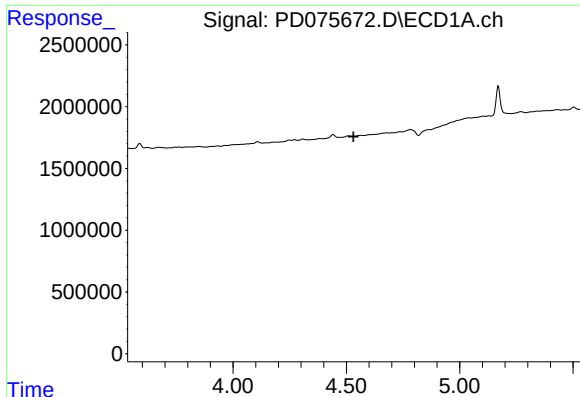

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.531 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

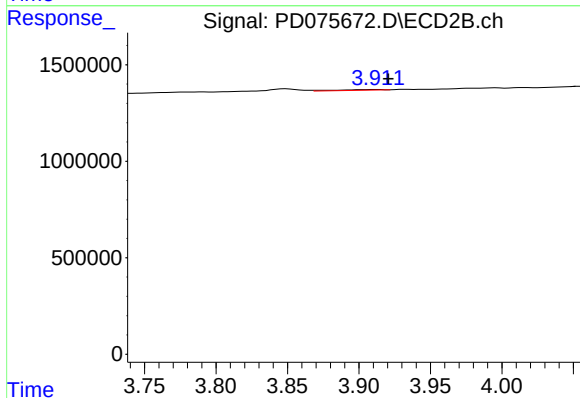


#6 beta-BHC

R.T.: 3.913 min
Delta R.T.: -0.007 min
Response: 90288
Conc: 0.13 ng/ml

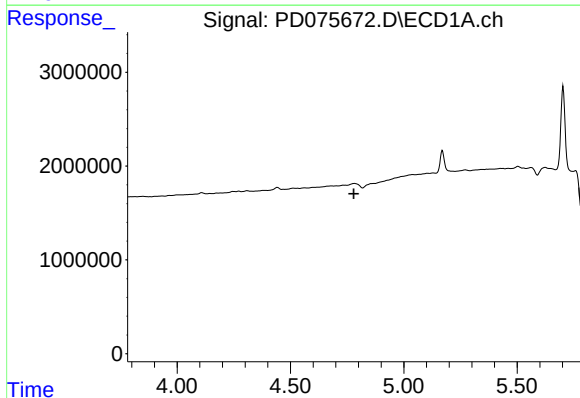


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.779 min
Response: 0
Conc: N.D.

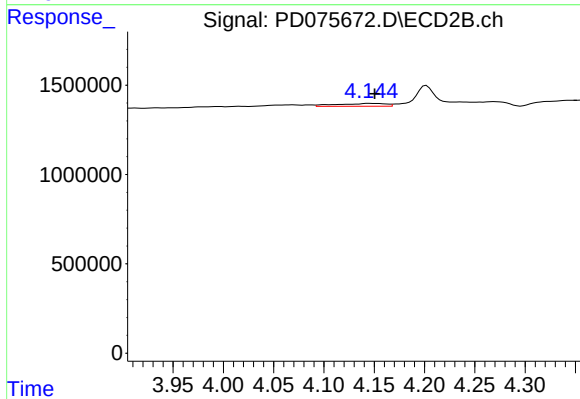

#7 delta-BHC


R.T.: 4.146 min
Delta R.T.: -0.005 min
Response: 552747
Conc: 0.38 ng/ml

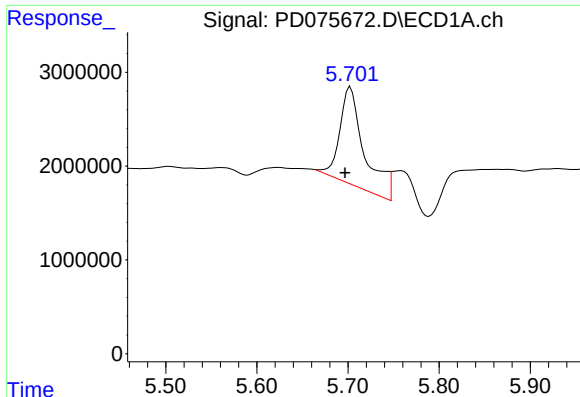

#8 Heptachlor epoxide


R.T.: 5.703 min
Delta R.T.: 0.006 min
Response: 19409753
Conc: 6.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

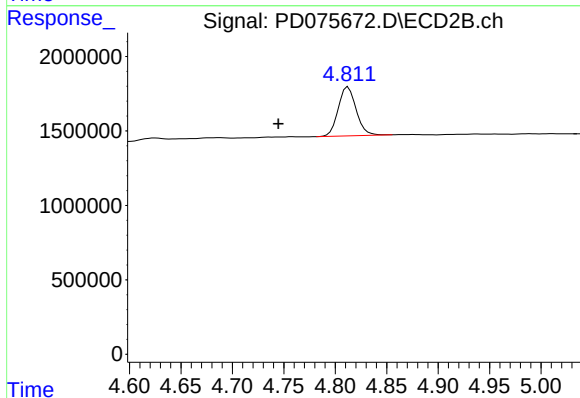


#8 Heptachlor epoxide

R.T.: 4.812 min
Delta R.T.: 0.068 min
Response: 3975368
Conc: 3.02 ng/ml

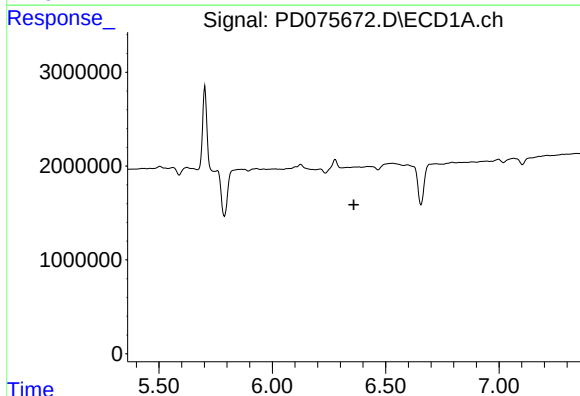


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.359 min
Response: 0
Conc: N.D.

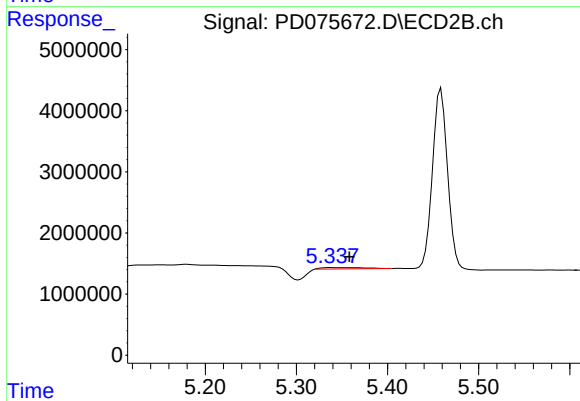

#13 Dieldrin


R.T.: 5.338 min
Delta R.T.: -0.021 min
Response: 696281
Conc: 0.53 ng/ml

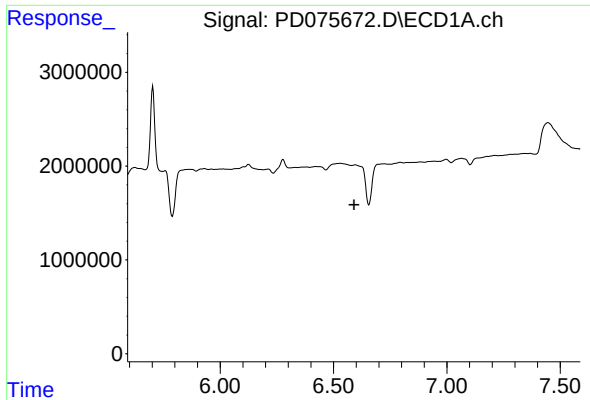

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

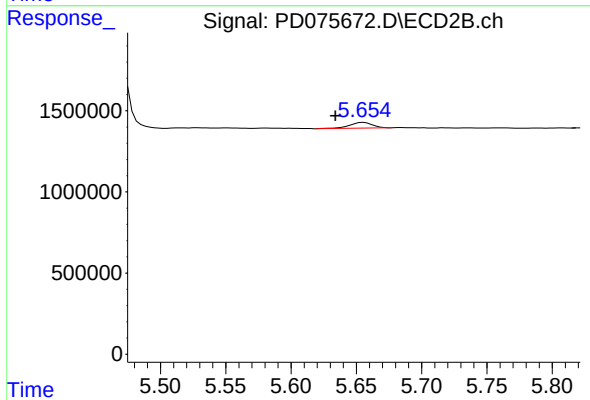


#14 Endrin

R.T.: 5.656 min
Delta R.T.: 0.022 min
Response: 431082
Conc: 0.38 ng/ml

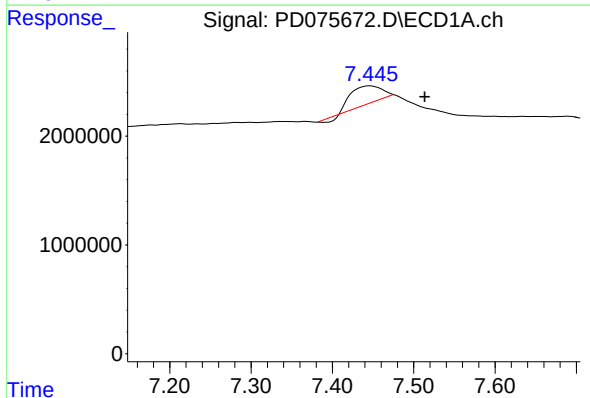


#20 Methoxychlor

R.T.: 7.446 min
Delta R.T.: -0.068 min
Response: 4406658
Conc: 3.53 ng/ml

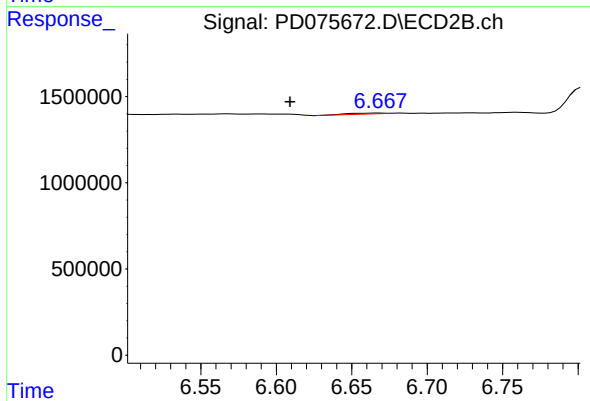

#20 Methoxychlor


R.T.: 6.668 min
Delta R.T.: 0.059 min
Response: 92771
Conc: 0.19 ng/ml

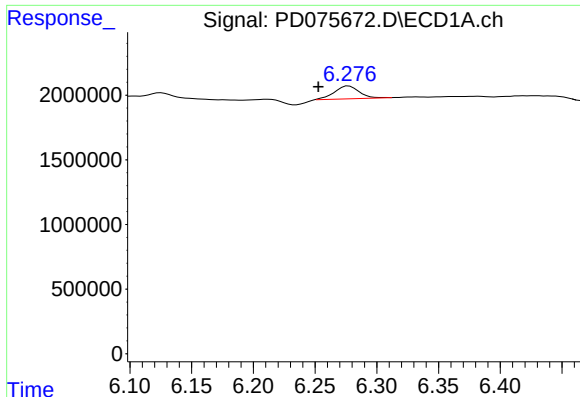

#22 Toxaphene-1


R.T.: 6.277 min
Delta R.T.: 0.024 min
Response: 1370556
Conc: 67.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

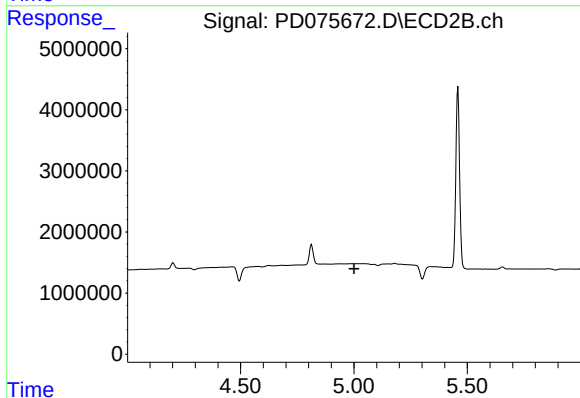


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

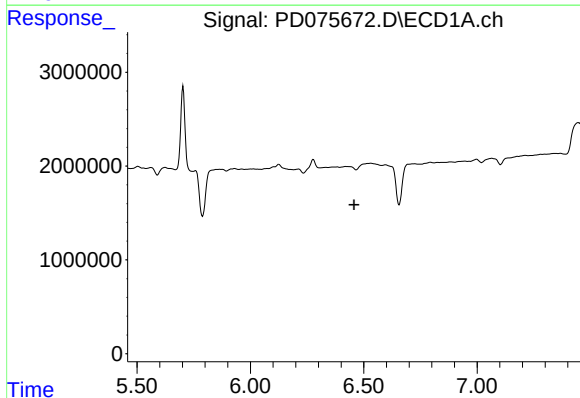


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.457 min
Response: 0
Conc: N.D.

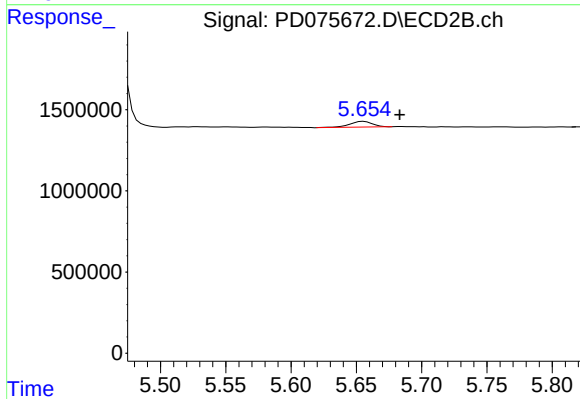

#23 Toxaphene-2


R.T.: 5.656 min
Delta R.T.: -0.028 min
Response: 431082
Conc: 60.93 ng/ml

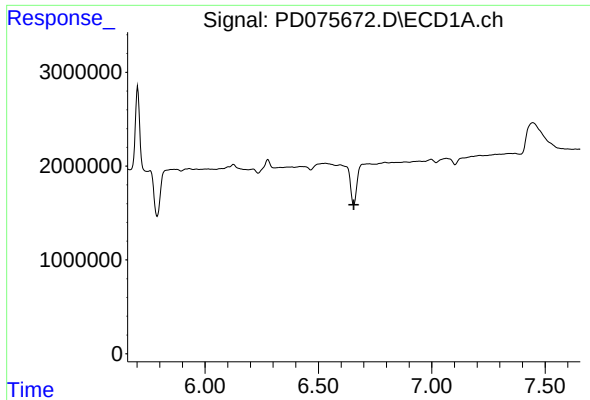

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

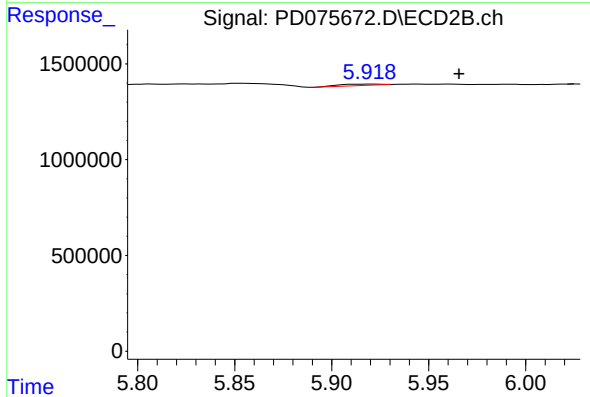


#24 Toxaphene-3

R.T.: 5.920 min
Delta R.T.: -0.045 min
Response: 102855
Conc: 12.18 ng/ml

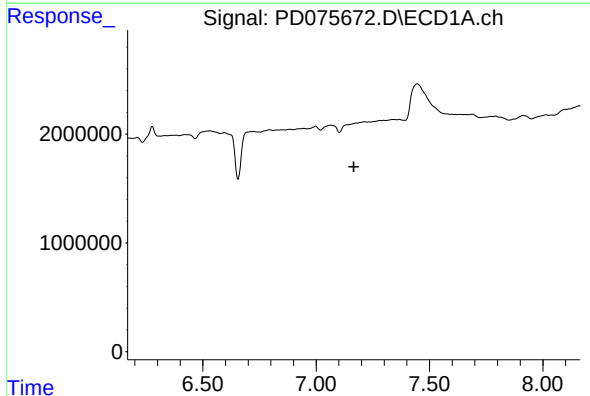


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.166 min
Response: 0
Conc: N.D.

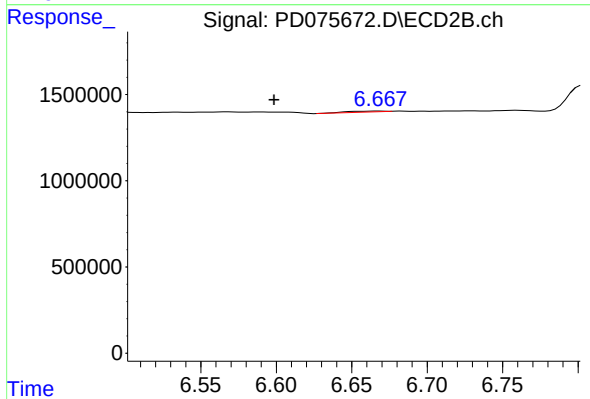

#25 Toxaphene-4


R.T.: 6.668 min
Delta R.T.: 0.070 min
Response: 92771
Conc: 4.49 ng/ml

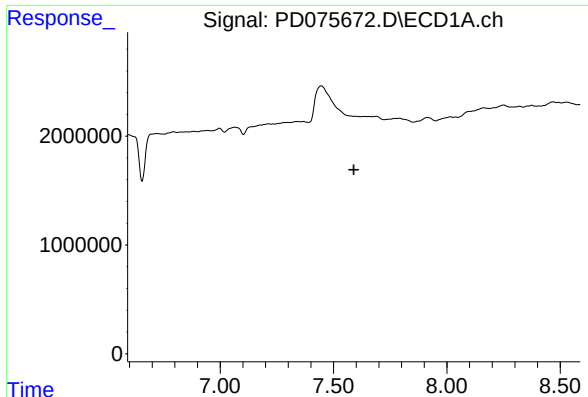

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.589 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

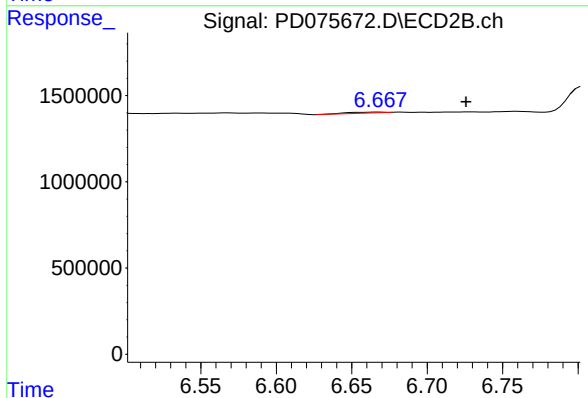


#26 Toxaphene-5

R.T.: 6.668 min
Delta R.T.: -0.058 min
Response: 92771
Conc: 2.87 ng/ml

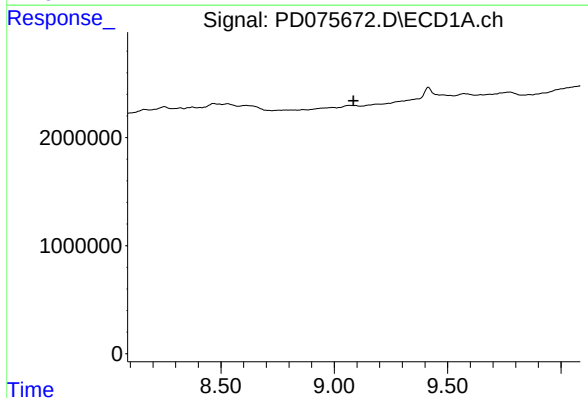

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.085 min
Response: 0
Conc: N.D.

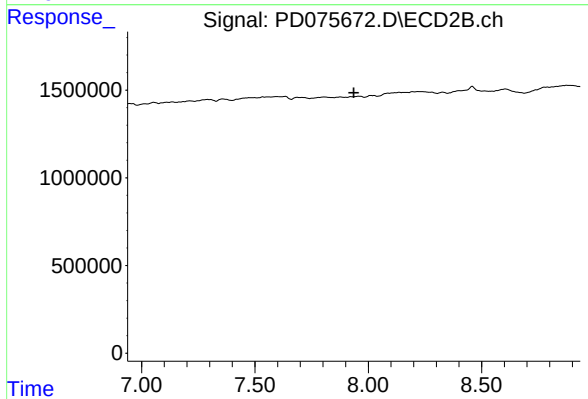

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.936 min
Response: 0
Conc: N.D.