

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
 Data File : PD075689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 12:59
 Operator : AR\AJ
 Sample : 02950-13MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW990MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2023
 Supervised By : Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:41:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.770	26412000	14048760	13.212	13.857
27)	SA Decachlor...	9.091	7.916	56513902	21847984	24.640	23.265
Target Compounds							
2)	A alpha-BHC	4.004	3.272	139.8E6	62774463	41.981	41.968
3)	MA gamma-BHC...	4.338	3.601	127.5E6	57529626	40.766	41.444
4)	MA Heptachlor	4.929	3.942	131.8E6	55906981	40.637	40.837
5)	MB Aldrin	5.272	4.222	135.1E6	58953714	41.710	41.717
6)	B beta-BHC	4.534	3.897	53557135	24408556	37.899	35.543m
7)	B delta-BHC	4.781	4.129	125.7E6	55846009	39.631m	38.524
8)	B Heptachlo...	5.699	4.724	117.7E6	52399622	38.506	39.826
9)	A Endosulfan I	6.087	5.095	110.0E6	47399381	41.529	41.044
10)	B trans-Chl...	5.957	4.975	117.3E6	51408437	40.132	40.427
11)	B cis-Chlor...	6.036	5.040	122.1E6	50509202	40.541	38.752
12)	B 4,4'-DDE	6.208	5.229	236.7E6	97332843	84.536	85.574
13)	MA Dieldrin	6.362	5.360	260.5E6	107.4E6	87.537	82.350
14)	MA Endrin	6.593	5.636	223.1E6	97233233	88.809	84.695
15)	B Endosulfa...	6.812	5.930	216.7E6	90006004	84.689	80.118
16)	A 4,4'-DDD	6.726	5.784	192.1E6	79039563	90.506	89.950
17)	MA 4,4'-DDT	7.042	6.036	200.2E6	79428756	97.528	97.622
18)	B Endrin al...	6.943	6.110	149.8E6	64323115	72.439	71.172
19)	B Endosulfa...	7.178	6.333	196.8E6	82814327	82.364	78.984
20)	A Methoxychlor	7.517	6.611	564.0E6	219.1E6	452.309	453.977
21)	B Endrin ke...	7.665	6.839	225.7E6	96013833	85.278	82.104

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
Data File : PD075689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 12:59
Operator : AR\AJ
Sample : 02950-13MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:41:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

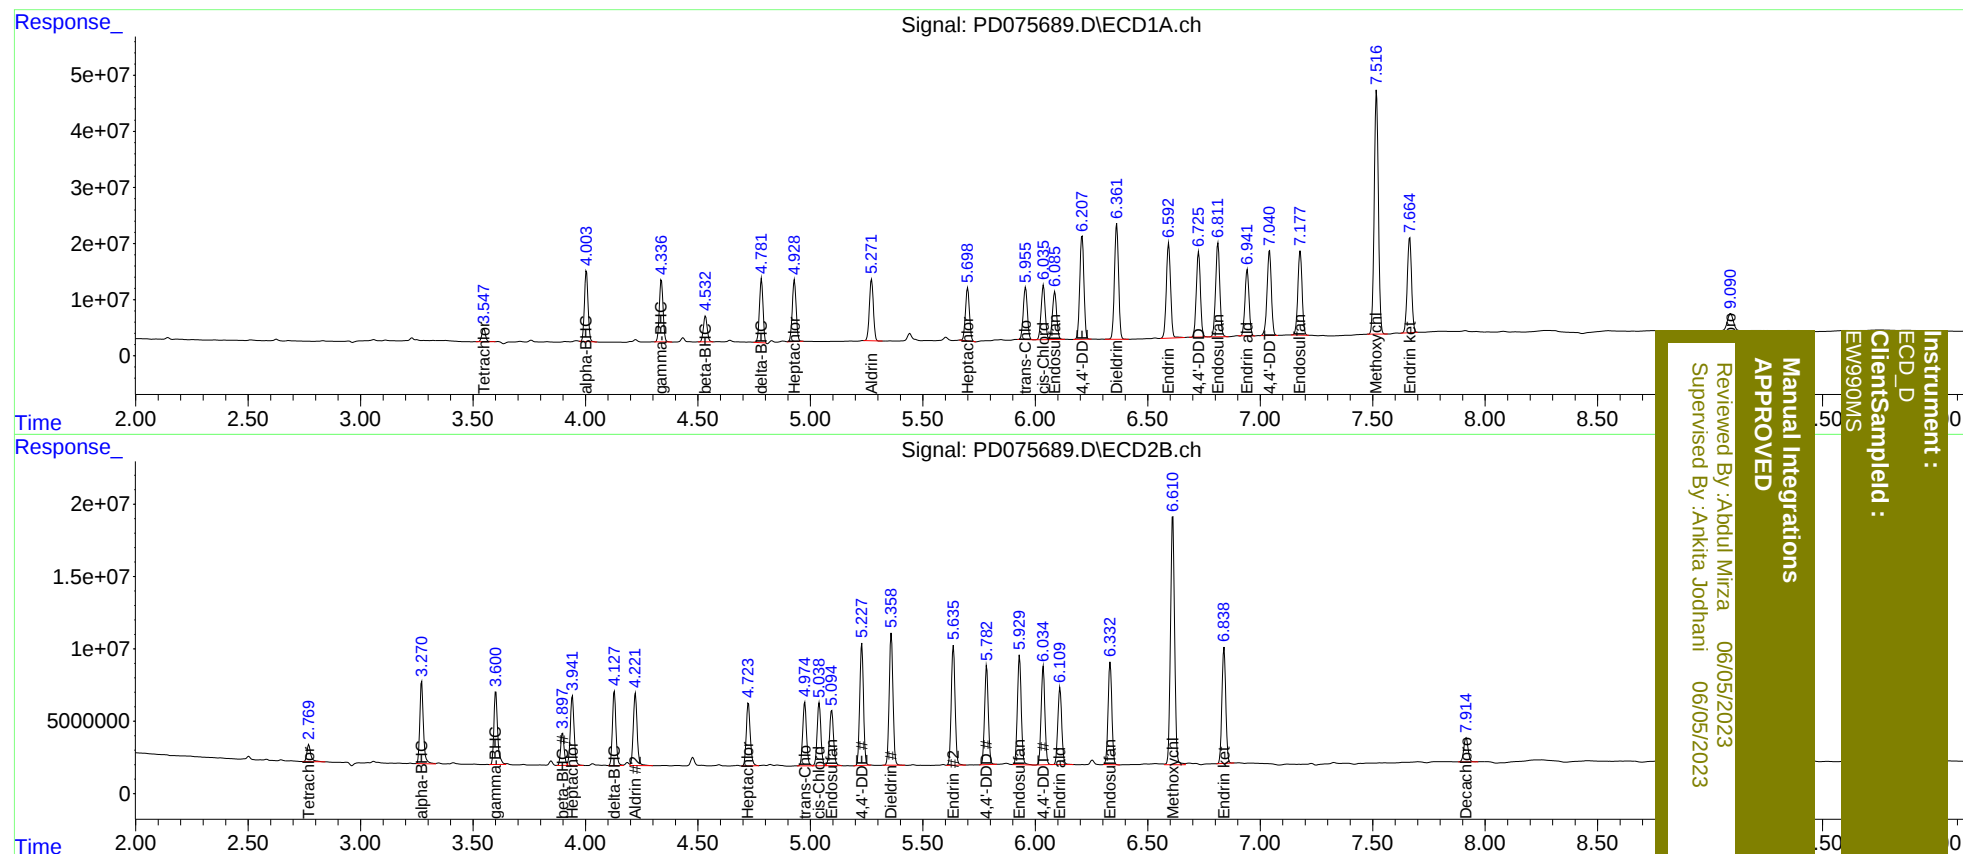

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/05/2023
Supervised By: Ankita Jodhani 06/05/2023

Instrument :
ECD_D
Client Sampled :
EW/990MS