

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
 Data File : PD075678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 10:31
 Operator : AR\AJ
 Sample : 02950-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW979

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2023
 Supervised By : Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:57:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

06/05/2023
 Supervised By : Ankita
 Jodhani

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	06/05/2023


System Monitoring Compounds							
1) SA Tetrachlo...	3.548	2.793	22069919	12366244	11.040	12.197	
27) SA Decachlor...	9.085	7.936	43869595	16555510	19.127m	17.629m	
Target Compounds							
20) A Methoxychlor	7.516	6.632	167.0E6	81538968	133.903	168.912m#	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
Data File : PD075678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 10:31
Operator : AR\AJ
Sample : 02950-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:57:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

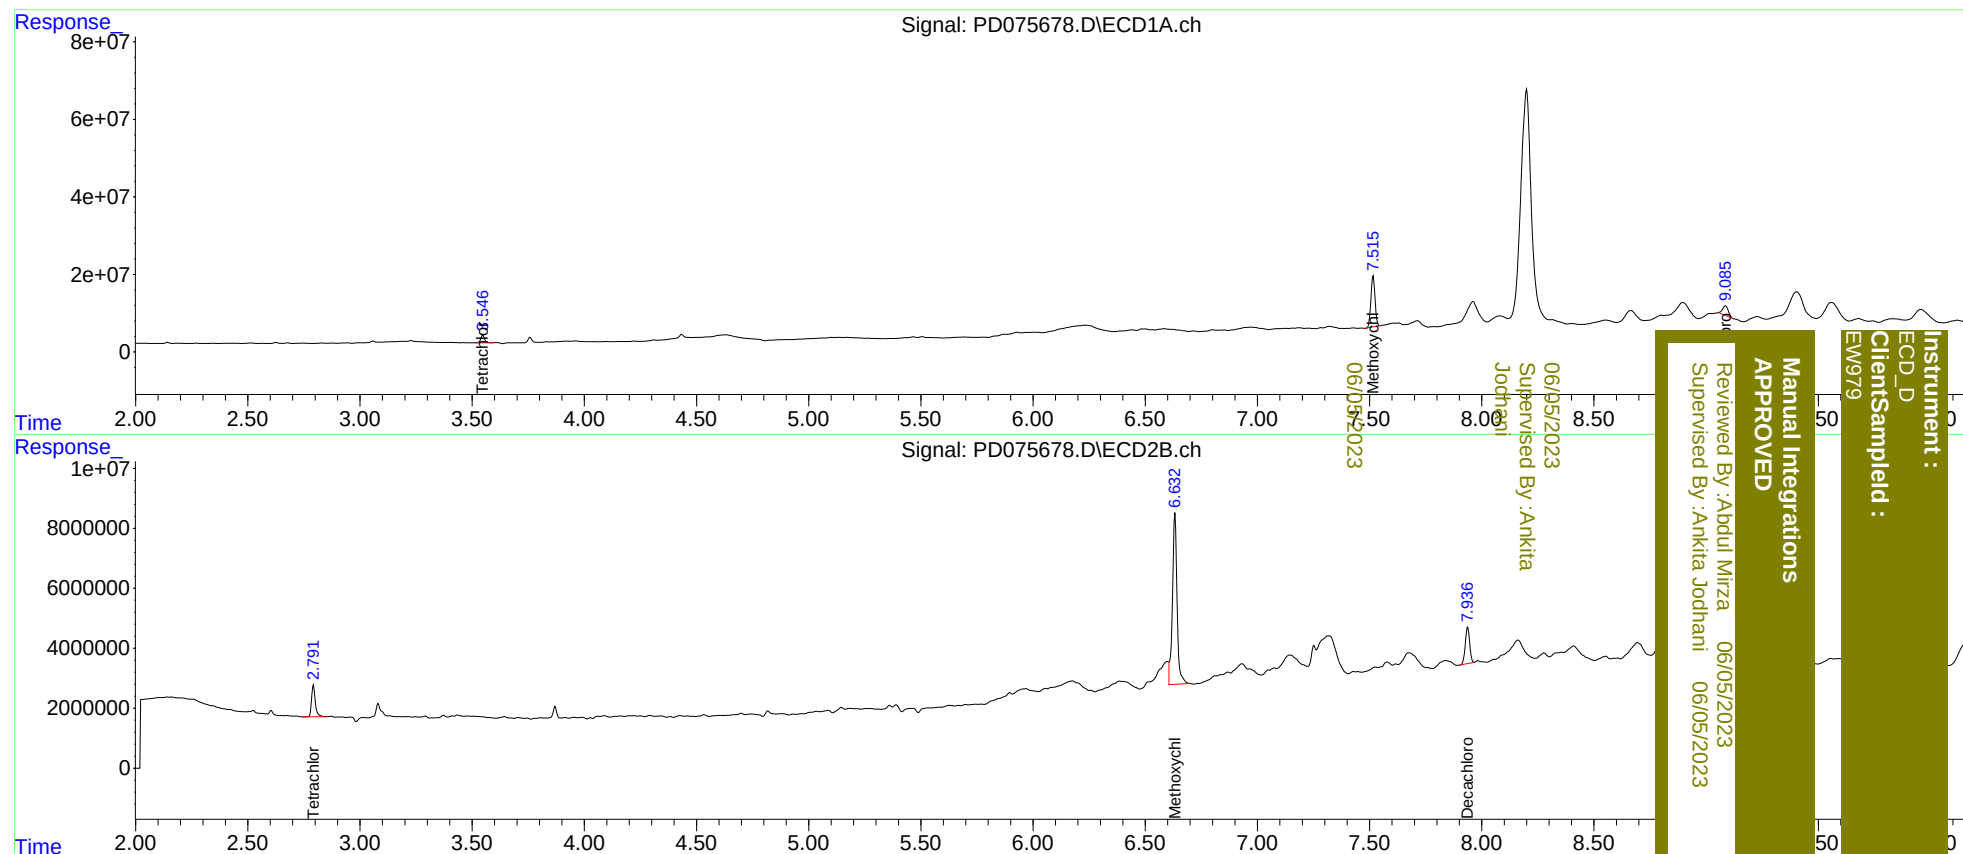

Reviewed By: Abdul Mirza 06/05/2023
Supervised By: Ankita Jodhani 06/05/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW/979