

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
 Data File : PD075690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 13:12
 Operator : AR\AJ
 Sample : 02950-14MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW990MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2023
 Supervised By : Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:44:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	27660900	14052951	13.837	13.861
27)	SA Decachlor...	9.091	7.915	52719314	22502134	22.986	23.961
Target Compounds							
2)	A alpha-BHC	4.004	3.271	141.0E6	63027951	42.327	42.138
3)	MA gamma-BHC...	4.338	3.601	129.5E6	57657277	41.408	41.536
4)	MA Heptachlor	4.929	3.942	133.4E6	56020091	41.129	40.920
5)	MB Aldrin	5.272	4.222	136.7E6	59109654	42.193	41.827
6)	B beta-BHC	4.534	3.897	54084878	24457142	38.272	35.614m
7)	B delta-BHC	4.781	4.128	125.6E6	55832286	39.596m	38.514
8)	B Heptachlo...	5.699	4.724	116.9E6	52652970	38.250	40.018
9)	A Endosulfan I	6.086	5.095	109.9E6	47824075	41.485	41.411
10)	B trans-Chl...	5.956	4.975	118.7E6	51923215	40.636	40.832
11)	B cis-Chlor...	6.035	5.039	122.3E6	50920990	40.610	39.068
12)	B 4,4'-DDE	6.208	5.228	237.0E6	97441401	84.617	85.669
13)	MA Dieldrin	6.362	5.360	260.2E6	107.5E6	87.434	82.500
14)	MA Endrin	6.593	5.636	218.8E6	97131941	87.103	84.607
15)	B Endosulfa...	6.812	5.930	214.2E6	89442606	83.699	79.617
16)	A 4,4'-DDD	6.726	5.783	190.1E6	79198897	89.543	90.131
17)	MA 4,4'-DDT	7.040	6.035	196.2E6	78612615	95.599	96.619
18)	B Endrin al...	6.942	6.109	147.4E6	64675154	71.299	71.561
19)	B Endosulfa...	7.177	6.332	192.5E6	82437947	80.603	78.625
20)	A Methoxychlor	7.517	6.610	537.2E6	214.1E6	430.756	443.571
21)	B Endrin ke...	7.664	6.839	219.6E6	96293504	82.965	82.344

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060323\
Data File : PD075690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 13:12
Operator : AR\AJ
Sample : 02950-14MSD
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:44:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

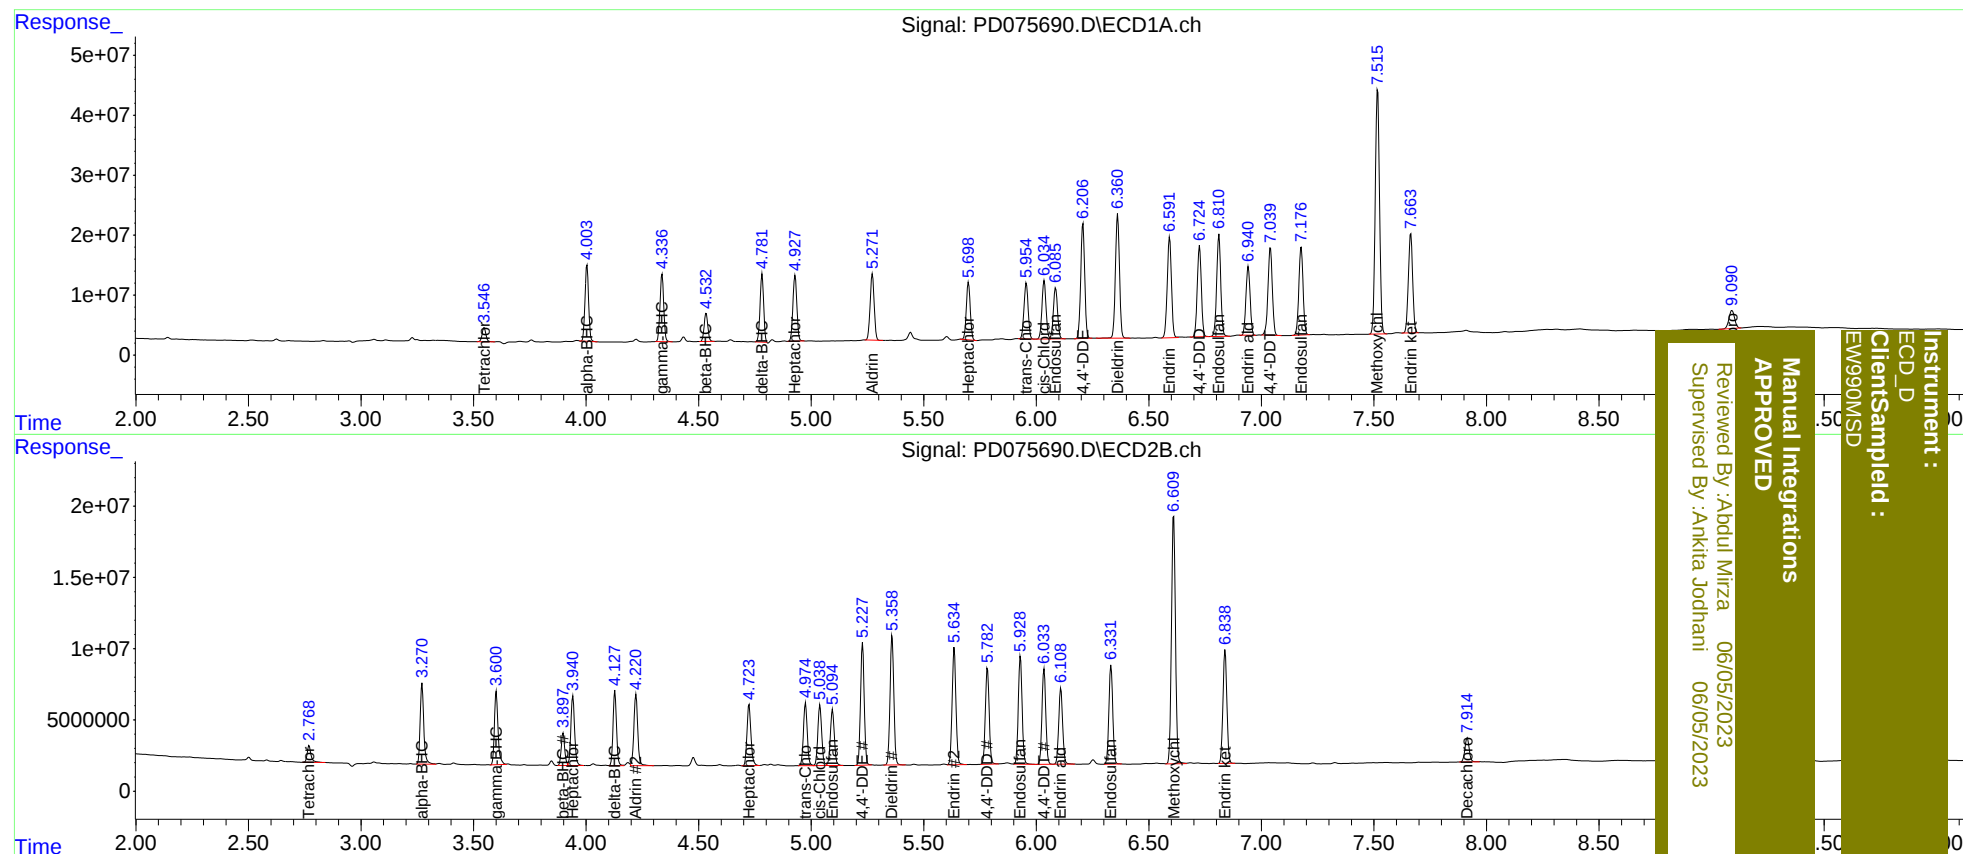

Instrument :
ECD_D
ClientSampled :
EW/990MSD
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 06/05/2023
Supervised By :Ankita Jodhani 06/05/2023