

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 09:17
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 17:18:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.028	0	2300411	N.D.	0.166 #
Target Compounds							
8)	B Heptachlo...	0.000	5.849	0	38564005	N.D.	2.110 #
9)	A Endosulfan I	0.000	6.207	0	123048	N.D.	0.007 #
10)	B gamma-Chl...	0.000	6.056f	0	2809887	N.D.	0.151 #
11)	B alpha-Chl...	0.000	6.131f	0	249875	N.D.	0.014 #
13)	MA Dieldrin	0.000	6.449	0	1161435	N.D.	0.064 #
15)	B Endosulfa...	0.000	6.897f	0	673104	N.D.	0.046 #
17)	MA 4,4'-DDT	0.000	7.104	0	4097121	N.D.	0.272 #
18)	B Endrin al...	0.000	7.005	0	2183145	N.D.	0.180 #
20)	A Methoxychlor	0.000	7.572f	0	2129868	N.D.	0.288 #
22)	Mirex	0.000	8.139	0	12645086	N.D.	1.265 #
25)	Chlordane-3	0.000	6.056f	0	2809887	N.D.	1.137 #
26)	Chlordane-4	0.000	6.131f	0	249875	N.D.	0.087 #
27)	Chlordane-5	0.000	6.930f	0	400559	N.D.	0.767 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 09:17
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 17:18:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

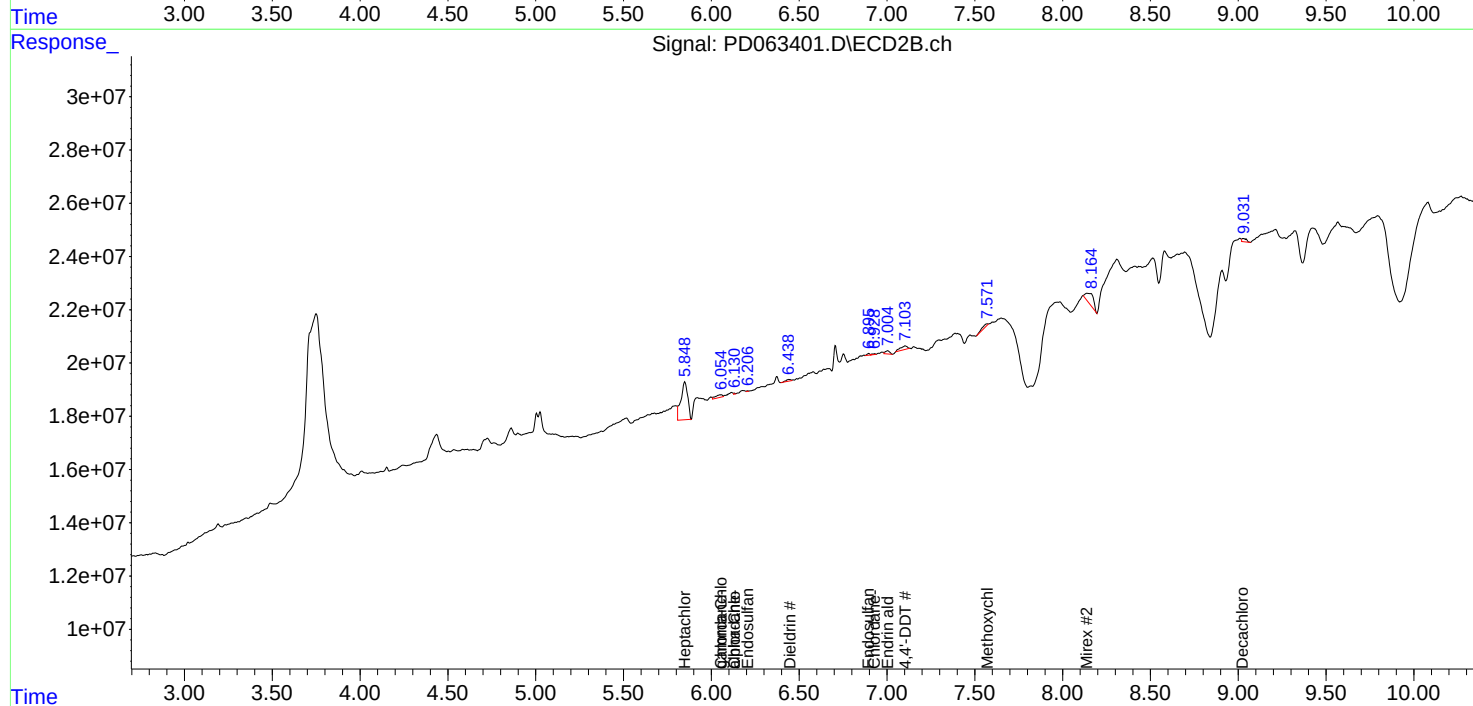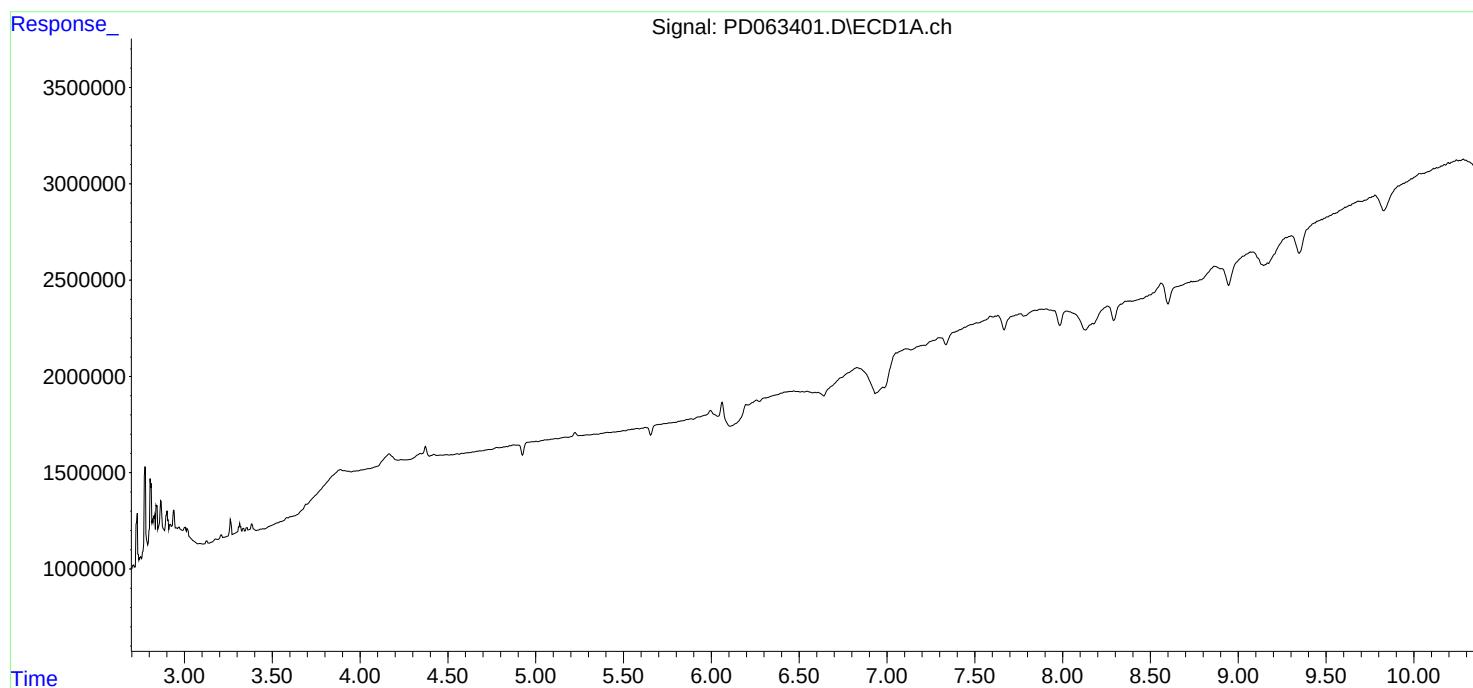


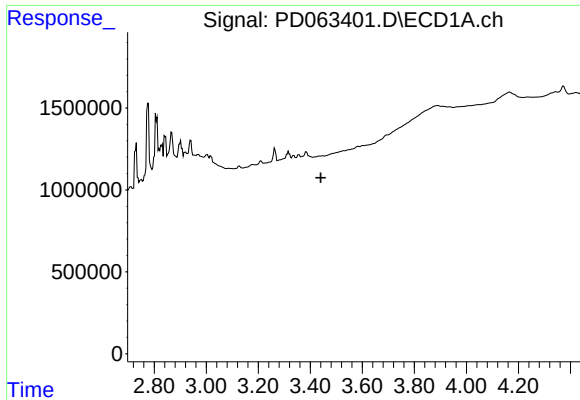

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

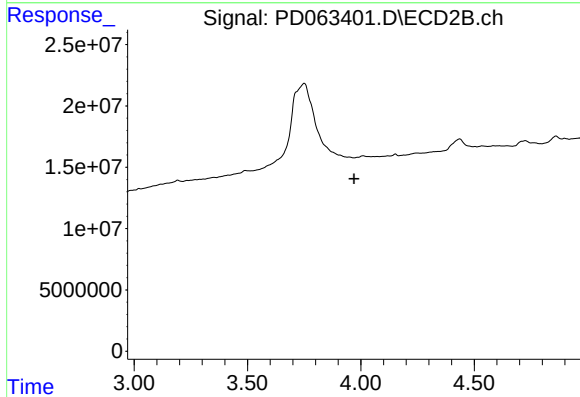


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

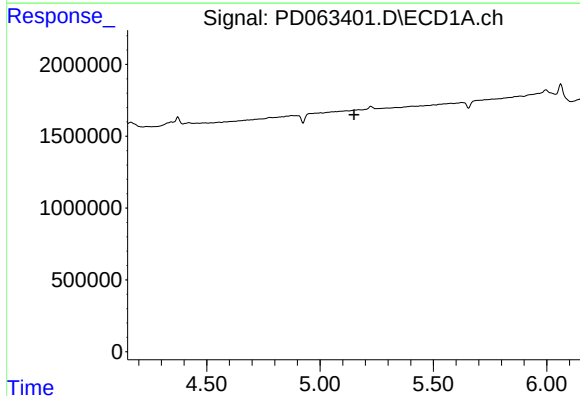


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.150 min
Response: 0
Conc: N.D.

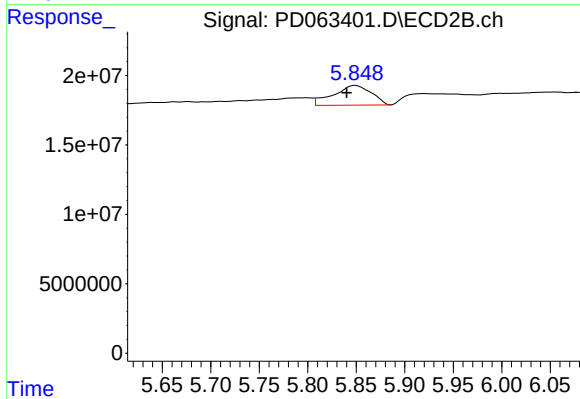

#8 Heptachlor epoxide


R.T.: 5.849 min
Delta R.T.: 0.009 min
Response: 38564005
Conc: 2.11 ng/ml

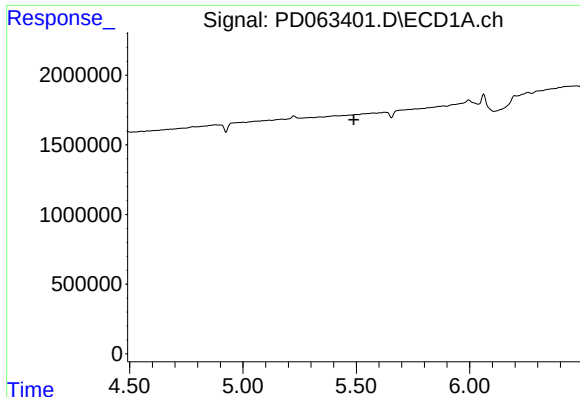

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

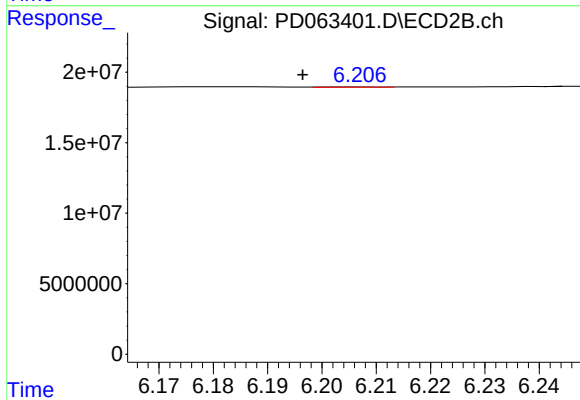


#9 Endosulfan I

R.T.: 6.207 min
Delta R.T.: 0.011 min
Response: 123048
Conc: 0.01 ng/ml

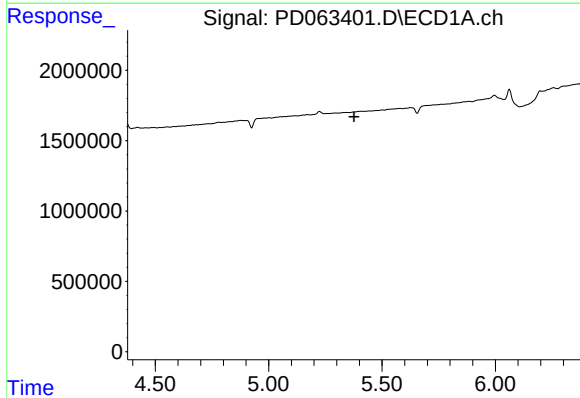


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.377 min
Response: 0
Conc: N.D.

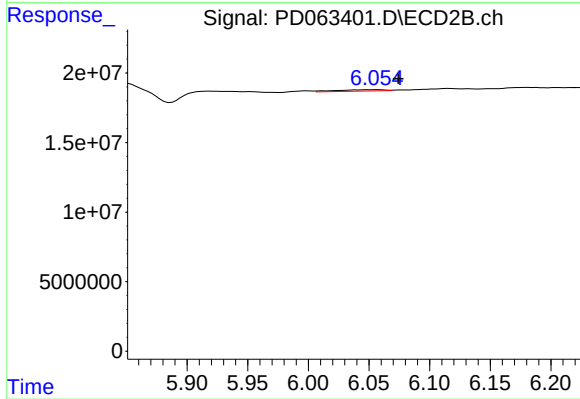

#10 gamma-Chlordane


R.T.: 6.056 min
Delta R.T.: -0.018 min
Response: 2809887
Conc: 0.15 ng/ml

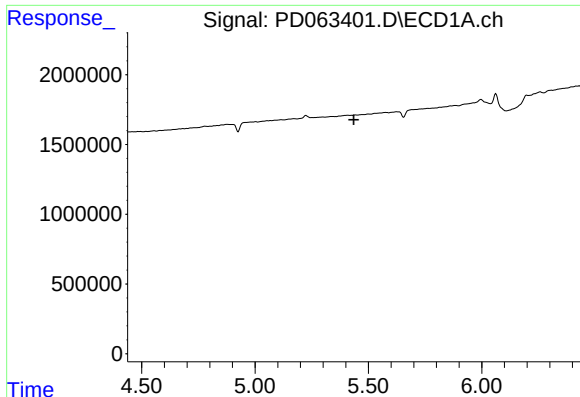

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

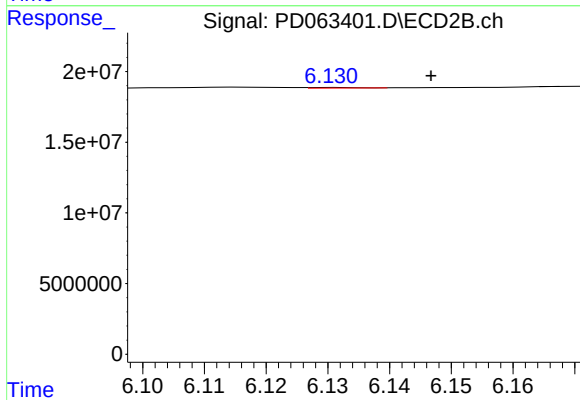


#11 alpha-Chlordane

R.T.: 6.131 min
Delta R.T.: -0.015 min
Response: 249875
Conc: 0.01 ng/ml

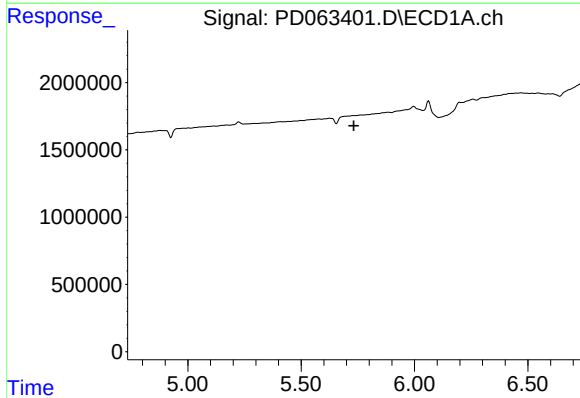


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.732 min
Response: 0
Conc: N.D.

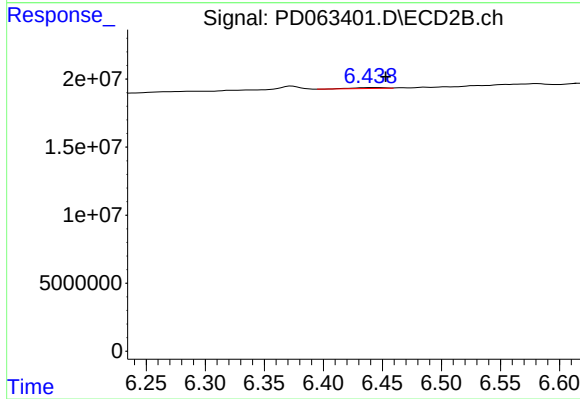

#13 Dieldrin


R.T.: 6.449 min
Delta R.T.: -0.004 min
Response: 1161435
Conc: 0.06 ng/ml

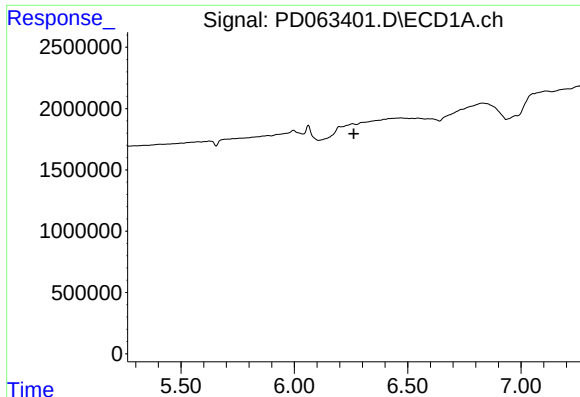

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

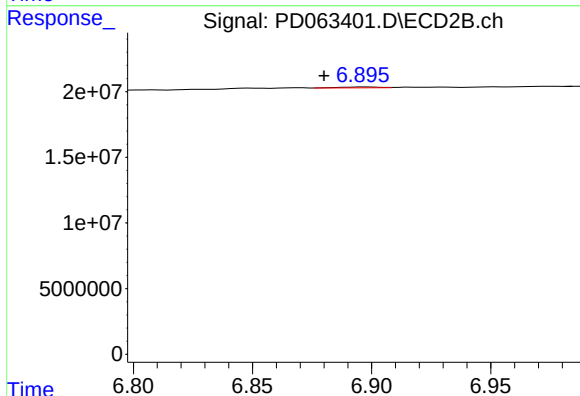


#15 Endosulfan II

R.T.: 6.897 min
Delta R.T.: 0.017 min
Response: 673104
Conc: 0.05 ng/ml

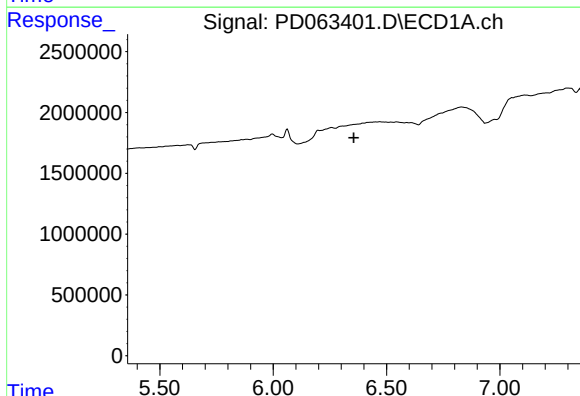


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.356 min
Response: 0
Conc: N.D.

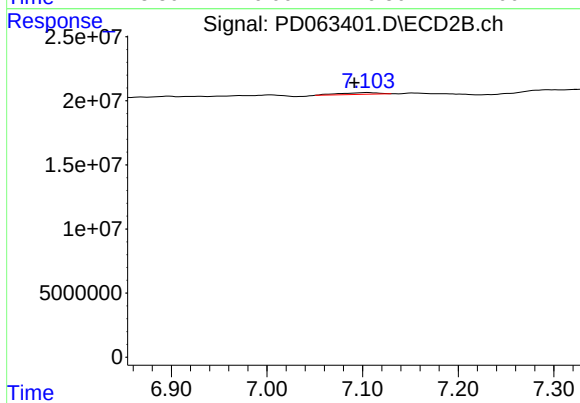

#17 4,4'-DDT


R.T.: 7.104 min
Delta R.T.: 0.013 min
Response: 4097121
Conc: 0.27 ng/ml

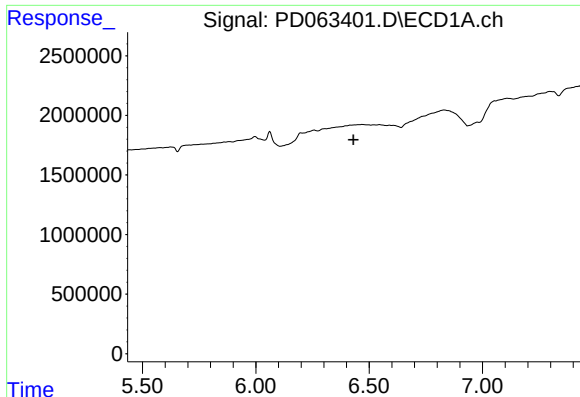

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

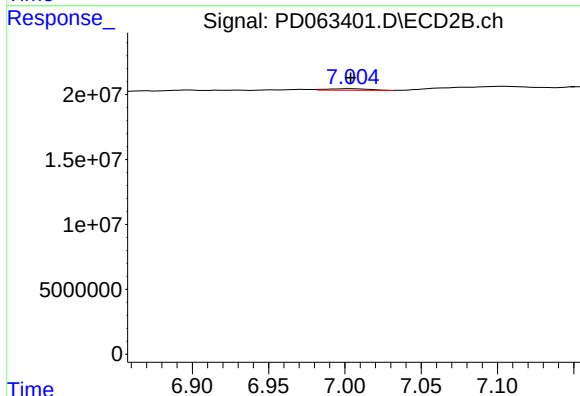


#18 Endrin aldehyde

R.T.: 7.005 min
Delta R.T.: 0.001 min
Response: 2183145
Conc: 0.18 ng/ml

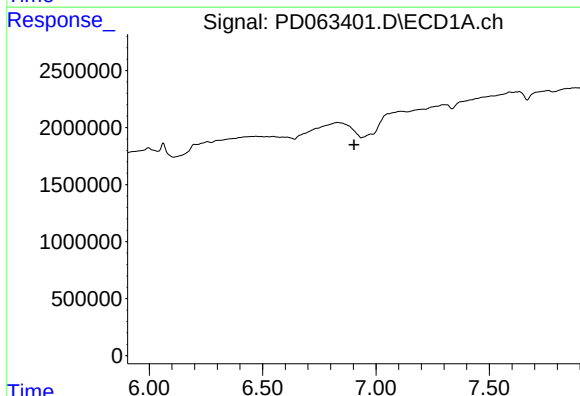


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.903 min
Response: 0
Conc: N.D.

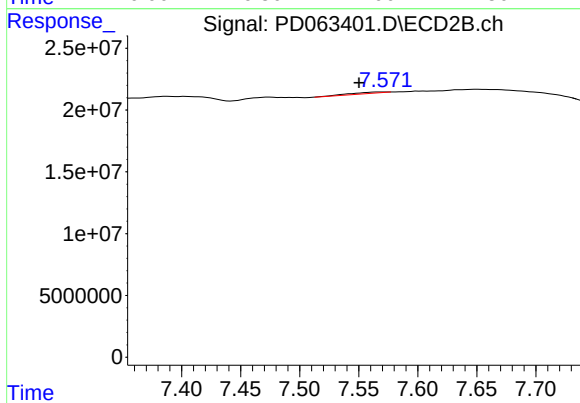

#20 Methoxychlor


R.T.: 7.572 min
Delta R.T.: 0.021 min
Response: 2129868
Conc: 0.29 ng/ml

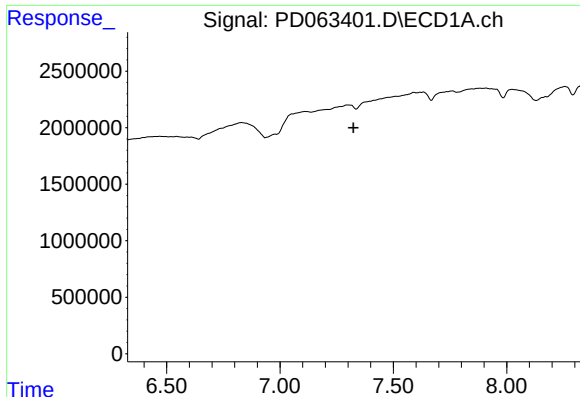

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.325 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

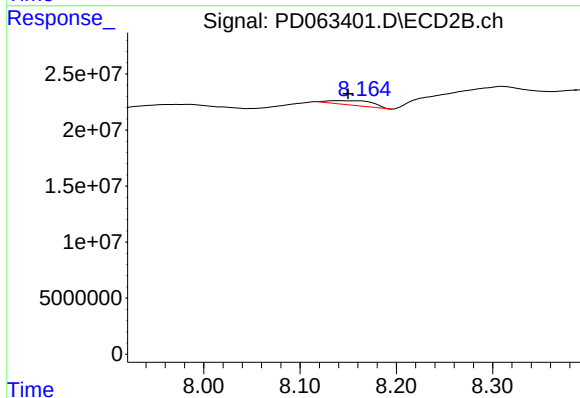


#22 Mirex

R.T.: 8.139 min
Delta R.T.: -0.011 min
Response: 12645086
Conc: 1.26 ng/ml

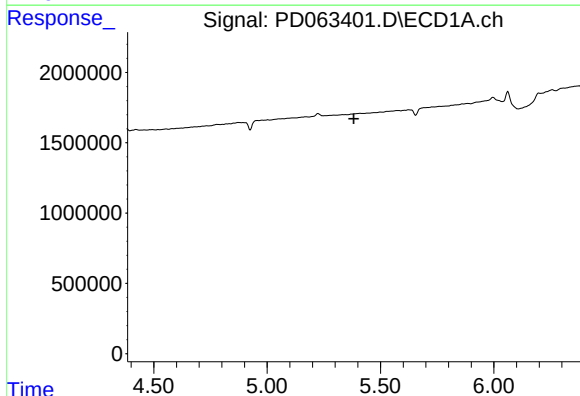


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

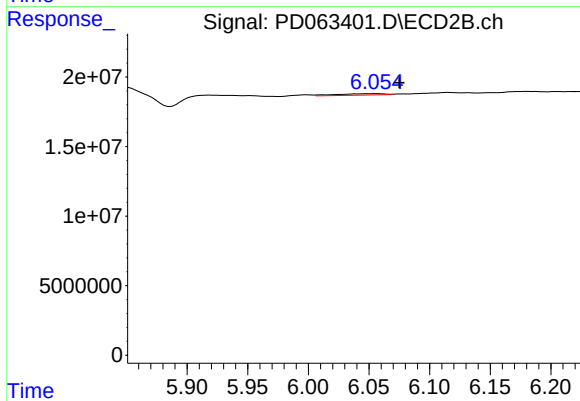

#25 Chlordane-3


R.T.: 6.056 min
Delta R.T.: -0.019 min
Response: 2809887
Conc: 1.14 ng/ml

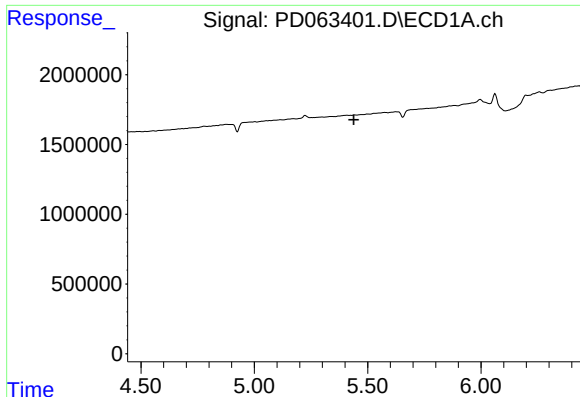

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

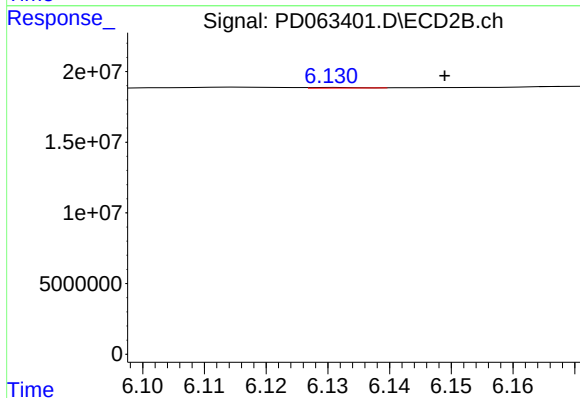


#26 Chlordane-4

R.T.: 6.131 min
Delta R.T.: -0.018 min
Response: 249875
Conc: 0.09 ng/ml

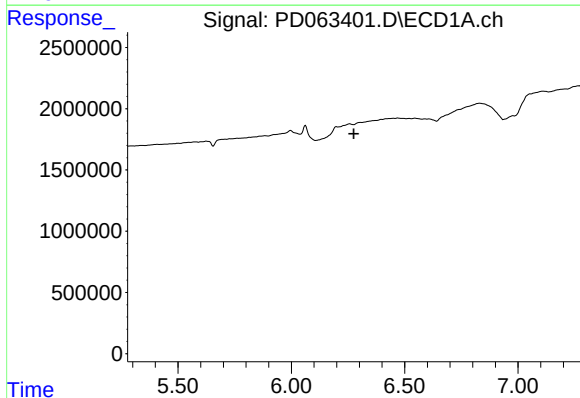


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.276 min
Response: 0
Conc: N.D.

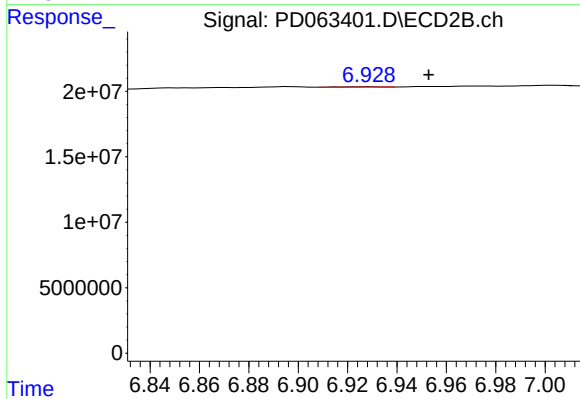

#27 Chlordane-5

R.T.: 6.930 min
Delta R.T.: -0.023 min
Response: 400559
Conc: 0.77 ng/ml

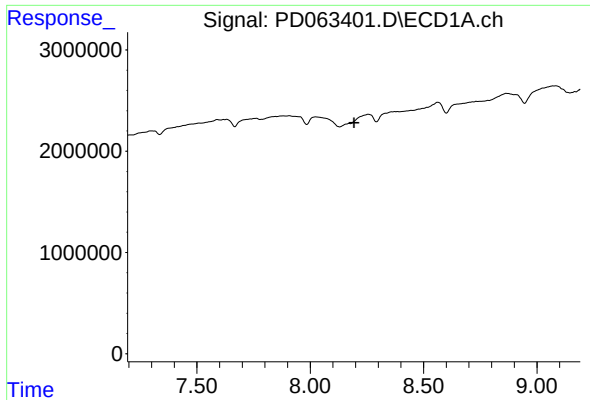

#28 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T.: 8.194 min

Response: 0

Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

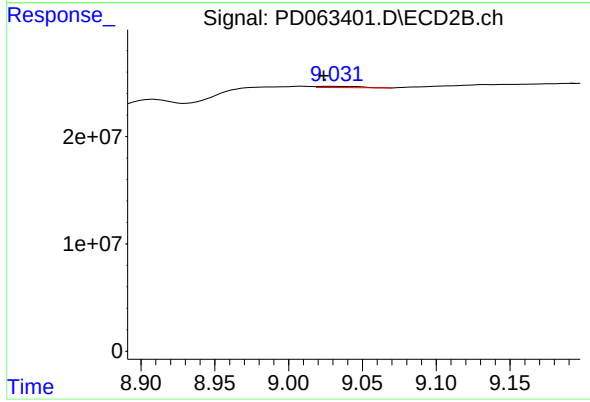

#28 Decachlorobiphenyl

R.T.: 9.028 min

Delta R.T.: 0.004 min

Response: 2300411

Conc: 0.17 ng/ml