

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 18:02
 Operator : AR\AJ
 Sample : PB136813TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB136813TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:29:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	25249267	263.0E6	18.247	19.628
28)	SA Decachlor...	8.196	9.025	27565979	263.8E6	17.528	19.087
Target Compounds							
5)	MB Aldrin	0.000	5.472f	0	234362	N.D.	0.012 #
8)	B Heptachlo...	0.000	5.851	0	17729214	N.D.	0.970 #
9)	A Endosulfan I	0.000	6.188	0	832506	N.D.	0.049 #
10)	B gamma-Chl...	0.000	6.101f	0	2411029	N.D.	0.130 #
11)	B alpha-Chl...	0.000	6.150	0	960462	N.D.	0.054 #
14)	MA Endrin	0.000	6.679	0	1396668	N.D.	0.091 #
15)	B Endosulfa...	0.000	6.896f	0	5418204	N.D.	0.367 #
22)	Mirex	0.000	8.144	0	1939431	N.D.	0.194 #
25)	Chlordane-3	0.000	6.101f	0	2411029	N.D.	0.976 #
26)	Chlordane-4	0.000	6.150	0	960462	N.D.	0.336 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 18:02
Operator : AR\AJ
Sample : PB136813TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB136813TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:29:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

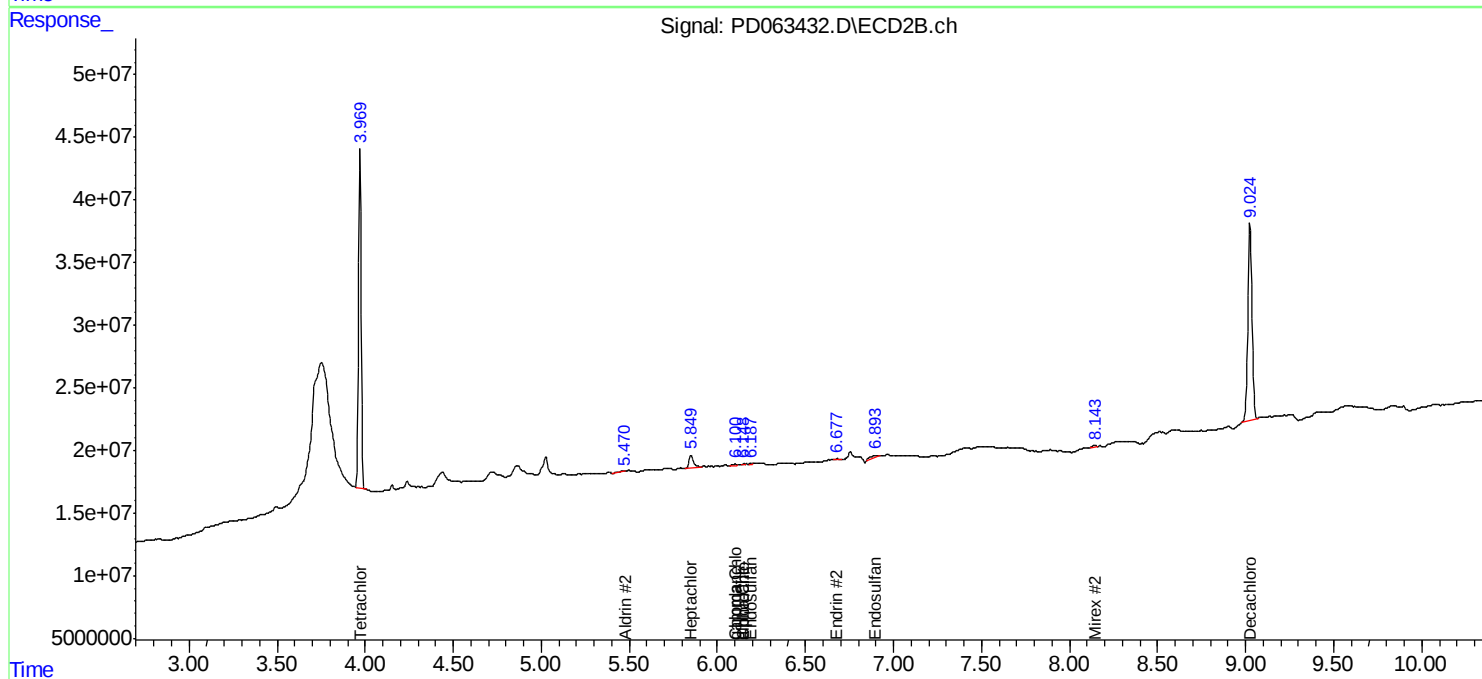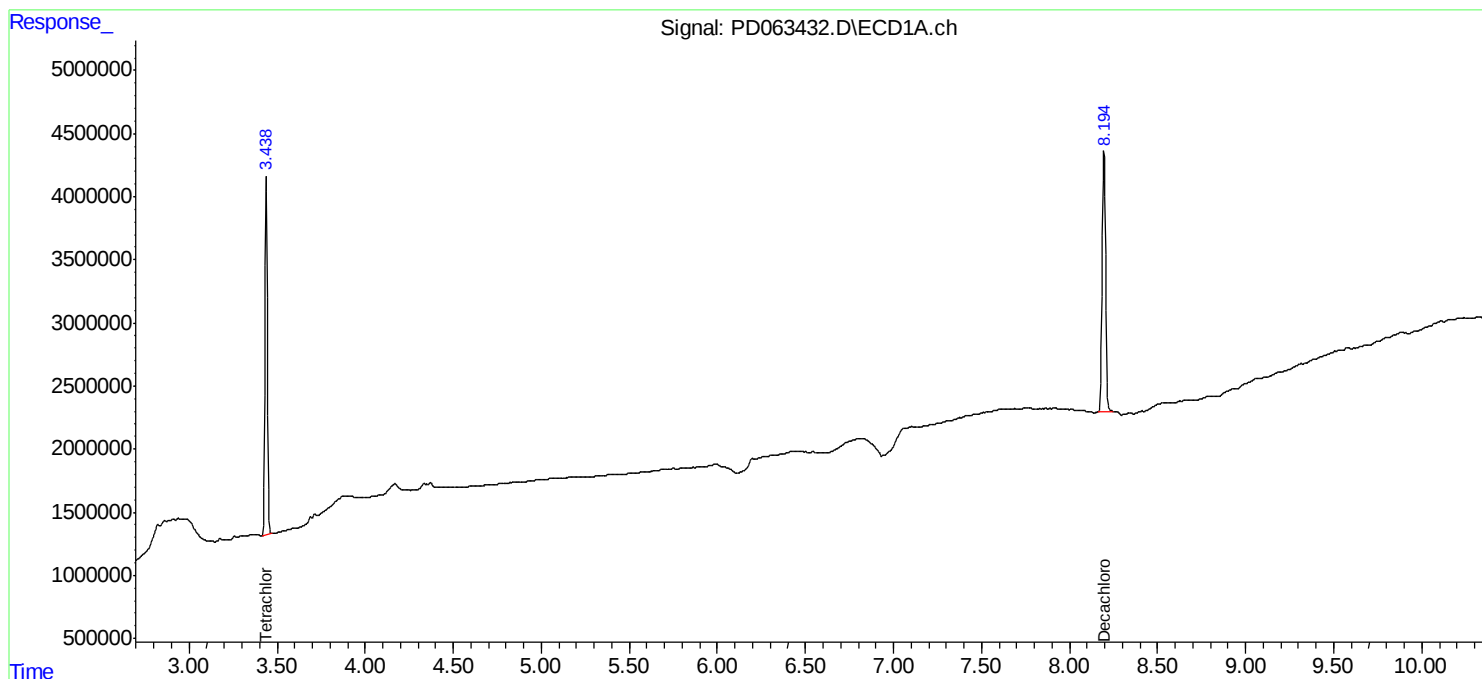


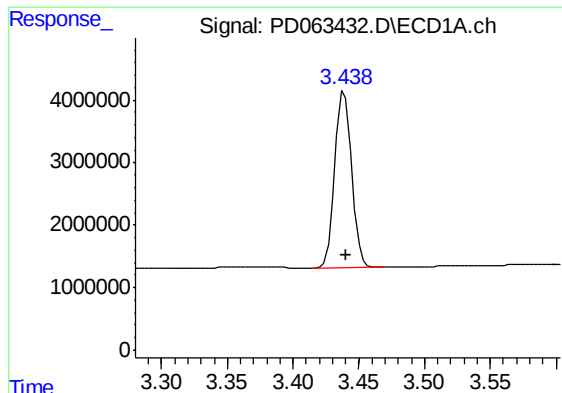

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 25249267
Conc: 18.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136813TB

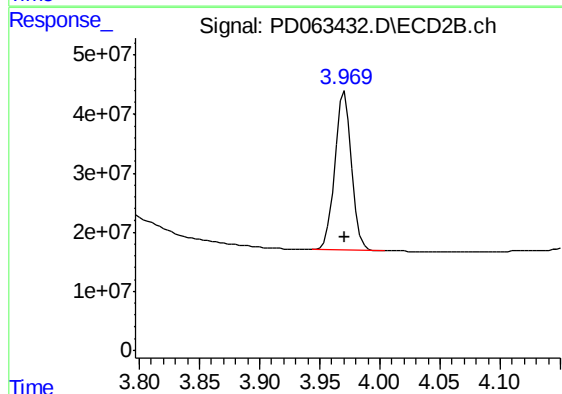


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 262982364
Conc: 19.63 ng/ml

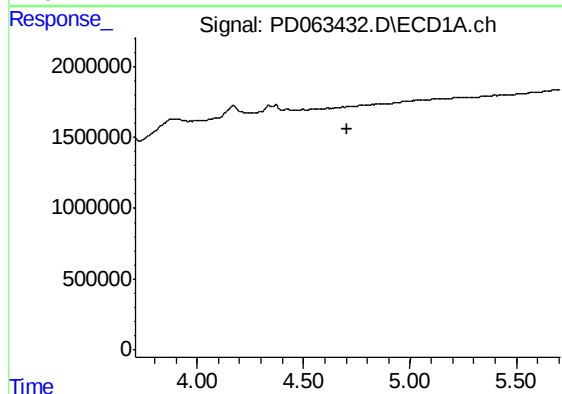


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.707 min
Response: 0
Conc: N.D.

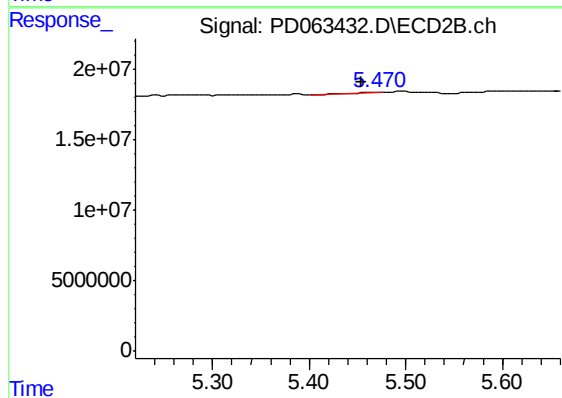

#5 Aldrin


R.T.: 5.472 min
Delta R.T.: 0.018 min
Response: 234362
Conc: 0.01 ng/ml

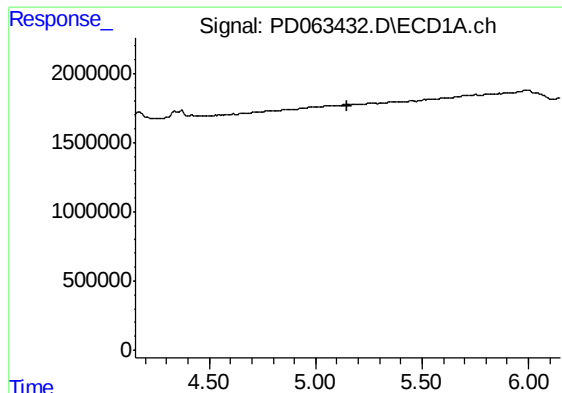

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.150 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136813TB

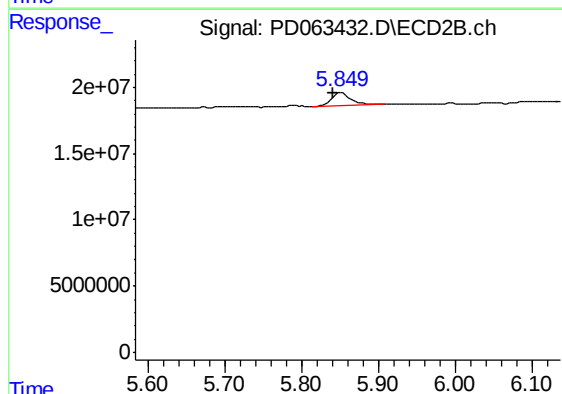


#8 Heptachlor epoxide

R.T.: 5.851 min
Delta R.T.: 0.011 min
Response: 17729214
Conc: 0.97 ng/ml

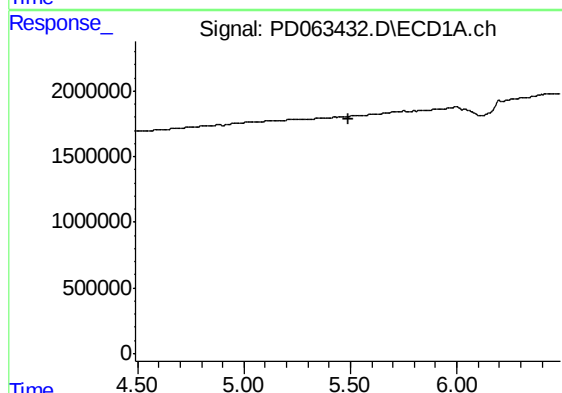


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.489 min
Response: 0
Conc: N.D.

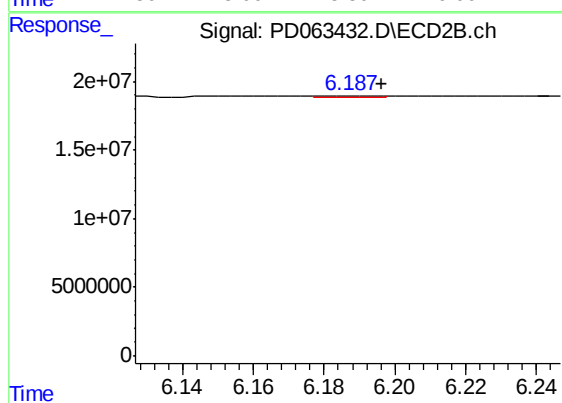

#9 Endosulfan I


R.T.: 6.188 min
Delta R.T.: -0.008 min
Response: 832506
Conc: 0.05 ng/ml

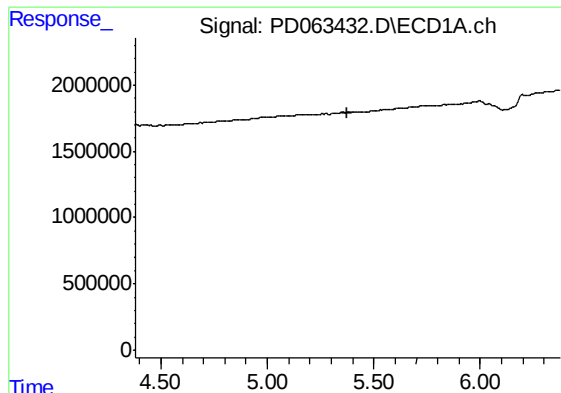

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136813TB

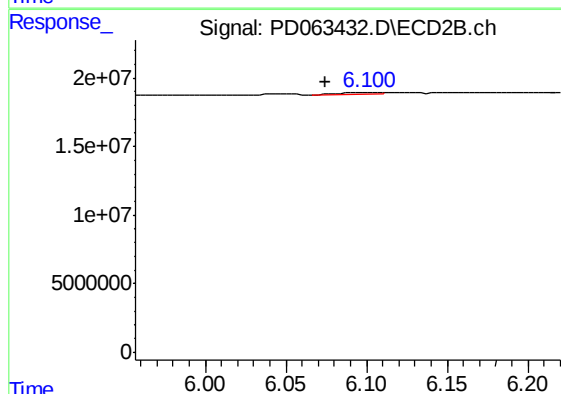


#10 gamma-Chlordane

R.T.: 6.101 min
Delta R.T.: 0.027 min
Response: 2411029
Conc: 0.13 ng/ml

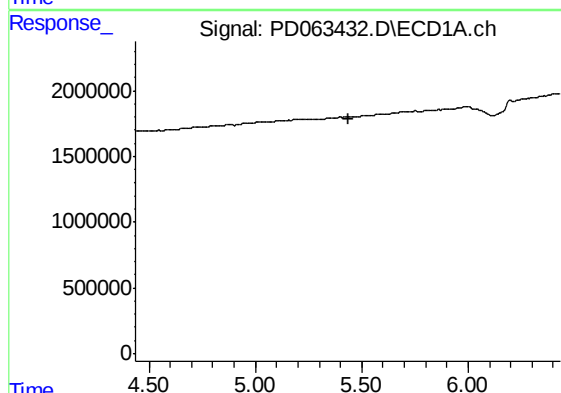


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.436 min
Response: 0
Conc: N.D.

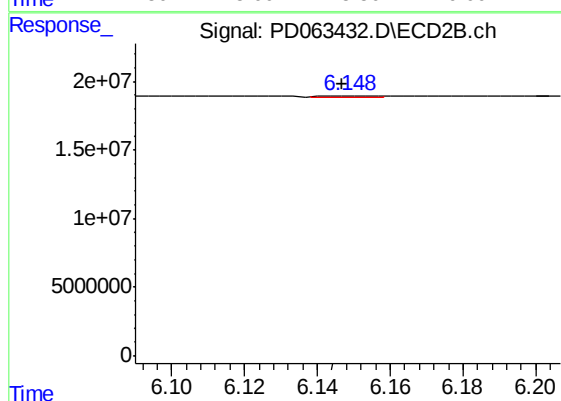

#11 alpha-Chlordane


R.T.: 6.150 min
Delta R.T.: 0.003 min
Response: 960462
Conc: 0.05 ng/ml

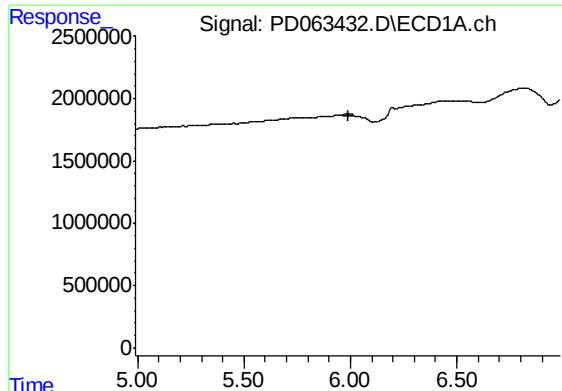

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.990 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136813TB

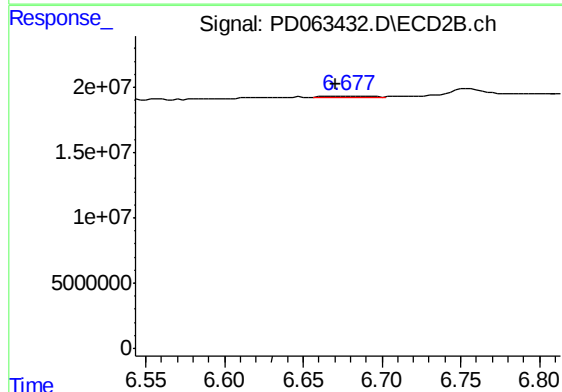


#14 Endrin

R.T.: 6.679 min
Delta R.T.: 0.008 min
Response: 1396668
Conc: 0.09 ng/ml

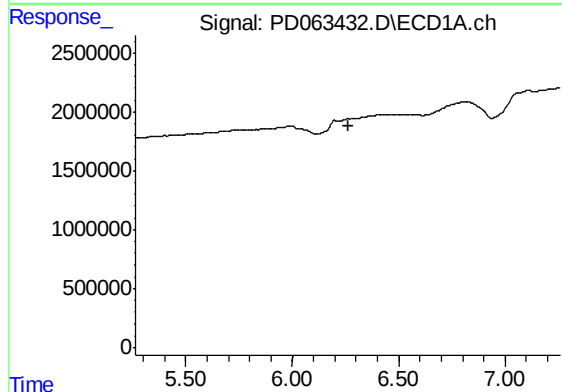


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.263 min
Response: 0
Conc: N.D.

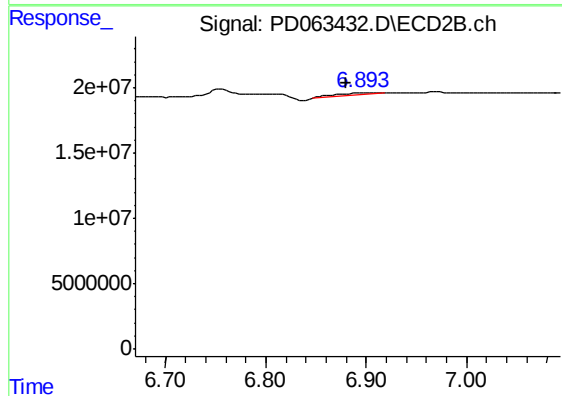

#15 Endosulfan II


R.T.: 6.896 min
Delta R.T.: 0.016 min
Response: 5418204
Conc: 0.37 ng/ml

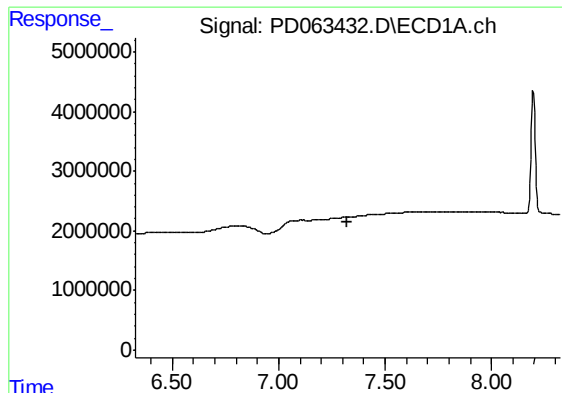

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.325 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136813TB

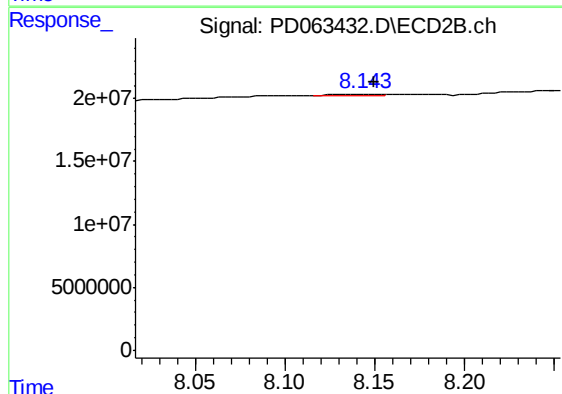


#22 Mirex

R.T.: 8.144 min
Delta R.T.: -0.006 min
Response: 1939431
Conc: 0.19 ng/ml

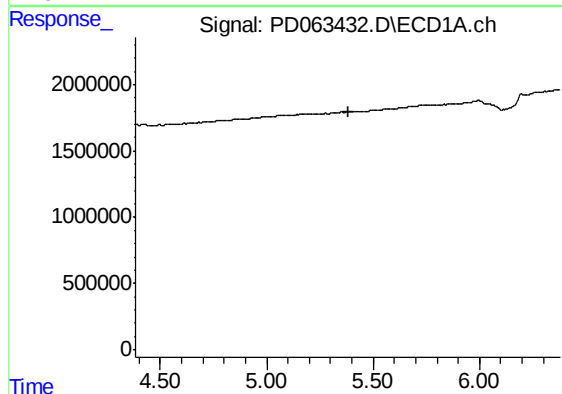


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

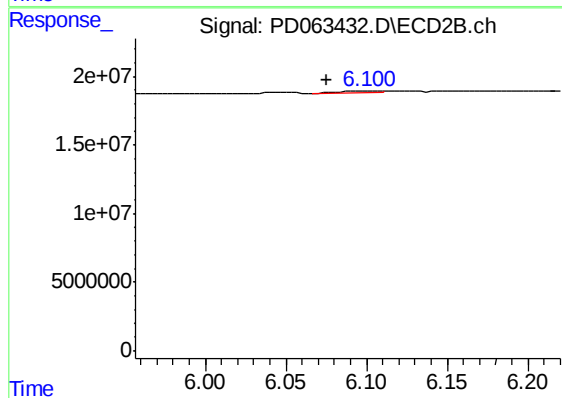

#25 Chlordane-3


R.T.: 6.101 min
Delta R.T.: 0.026 min
Response: 2411029
Conc: 0.98 ng/ml

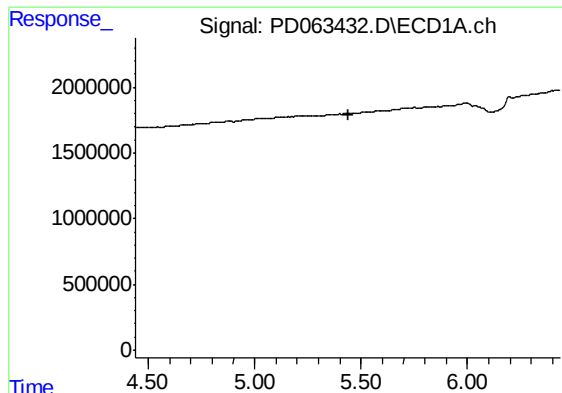

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136813TB

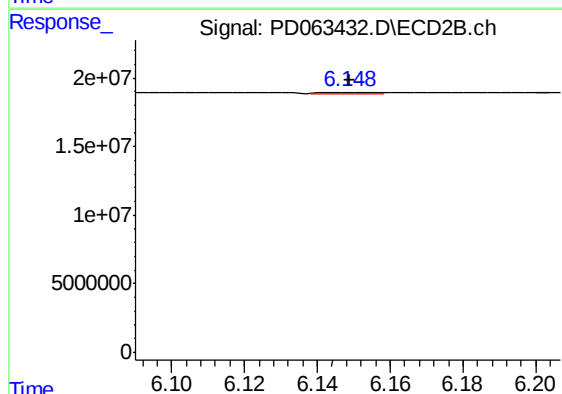


#26 Chlordane-4

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 960462
Conc: 0.34 ng/ml

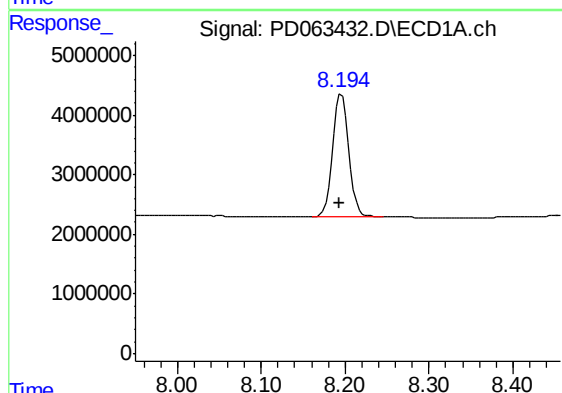

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: 0.002 min
Response: 27565979
Conc: 17.53 ng/ml

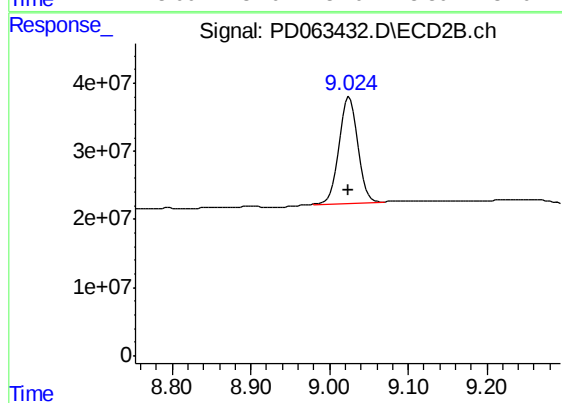

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.002 min
Response: 263760986
Conc: 19.09 ng/ml