

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 15:08
 Operator : AR\AJ
 Sample : M2584-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EO-03-060221

Manual Integrations
 APPROVED

Ankita
 6/4/2021 12:10:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 17:21:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.969	16108110	102.2E6	11.641	7.627m#
28)	SA Decachlor...	8.194	9.025	14912521	140.9E6	9.482	10.199
Target Compounds							
10)	B gamma-Chl...	5.378	6.072	1179558	13280601	0.661m	0.715m
11)	B alpha-Chl...	5.434	6.146	1566187	38237188	0.886m	2.151m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 15:08
Operator : AR\AJ
Sample : M2584-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
EO-03-060221


Manual Integrations
APPROVED

Ankita
6/4/2021 12:10:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 17:21:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

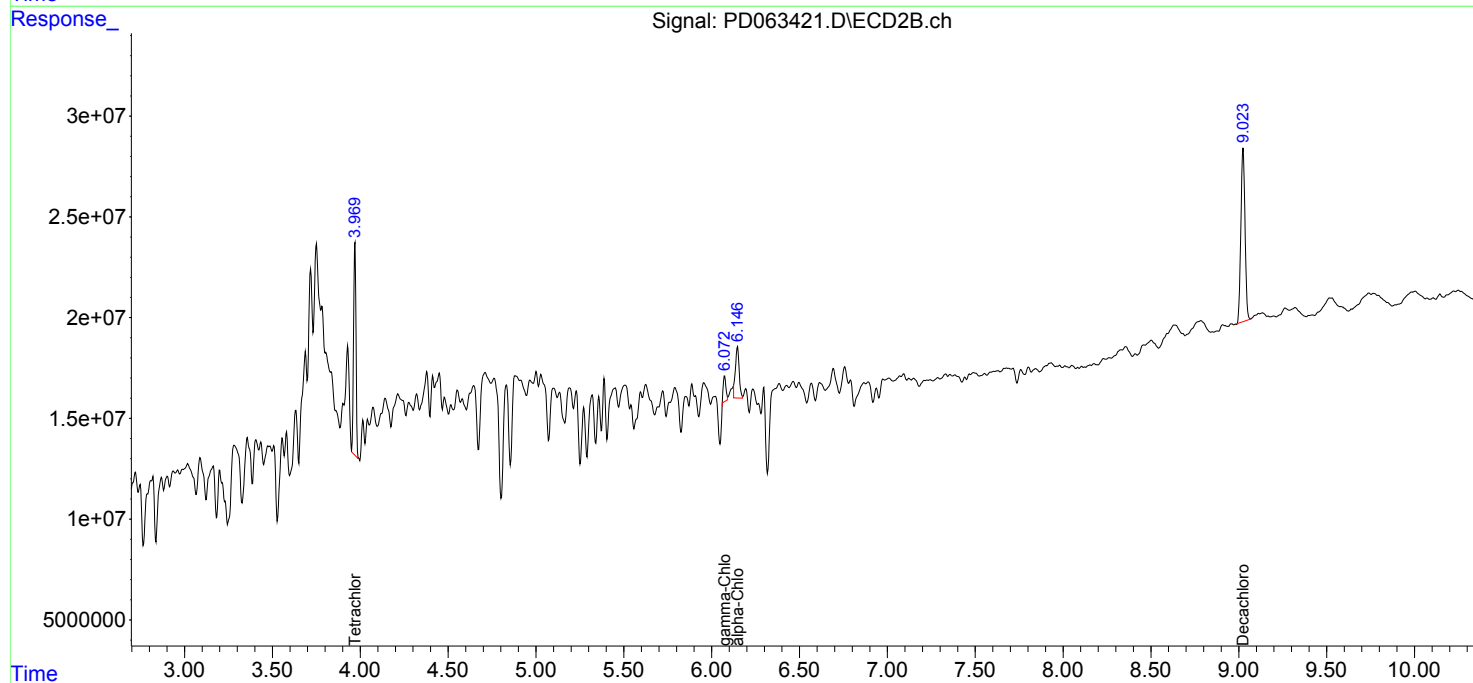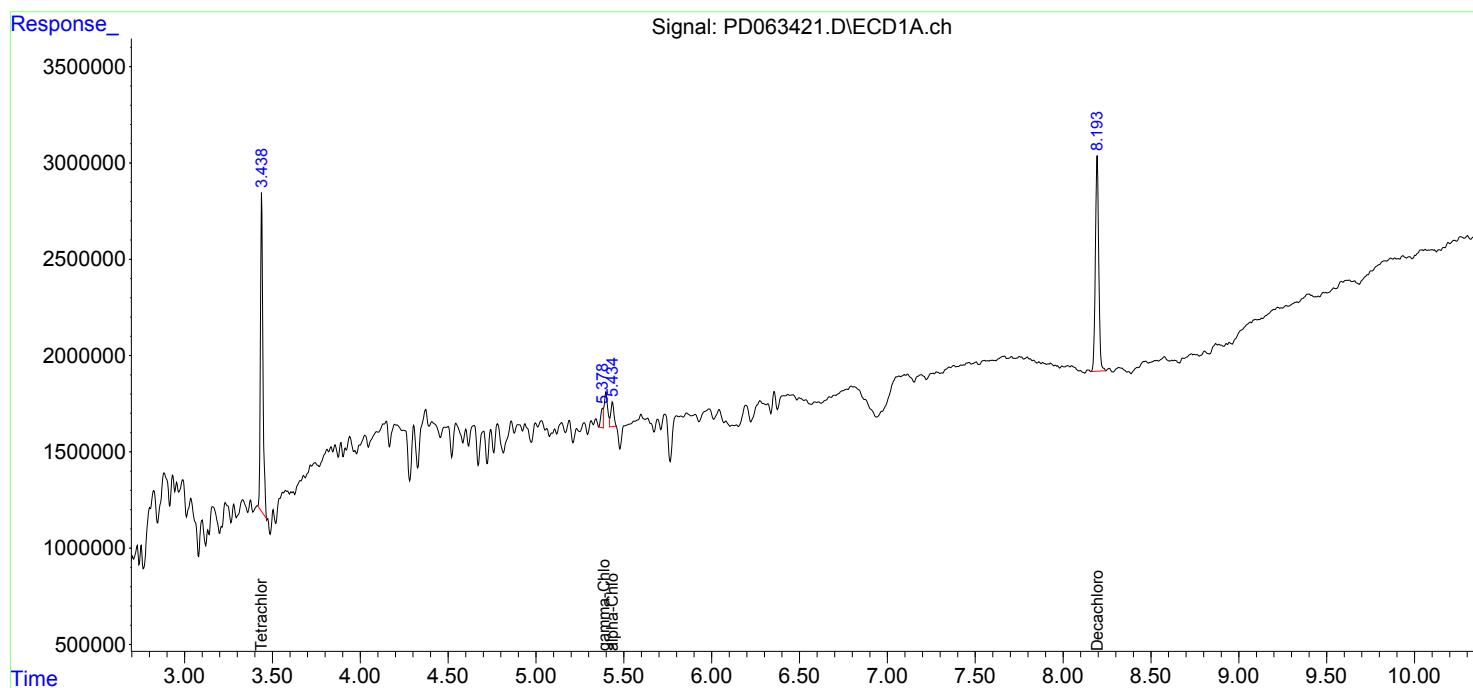

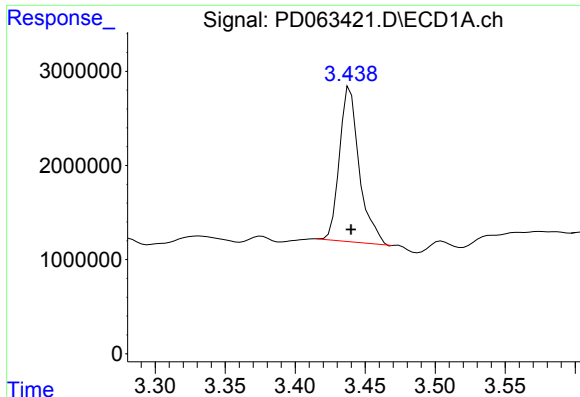


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 16108110
Conc: 11.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-03-060221


Manual Integrations
APPROVED

Ankita
6/4/2021 12:10:32 PM

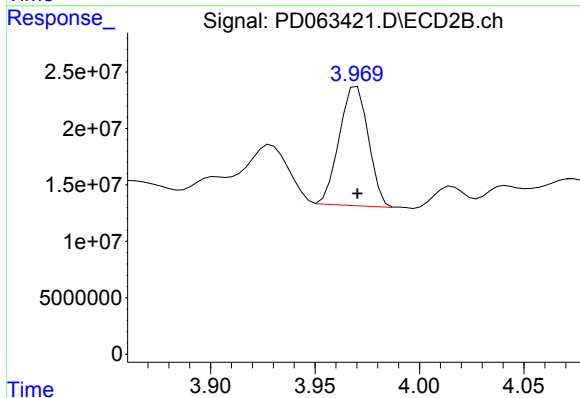


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.002 min
Response: 102197854
Conc: 7.63 ng/ml m

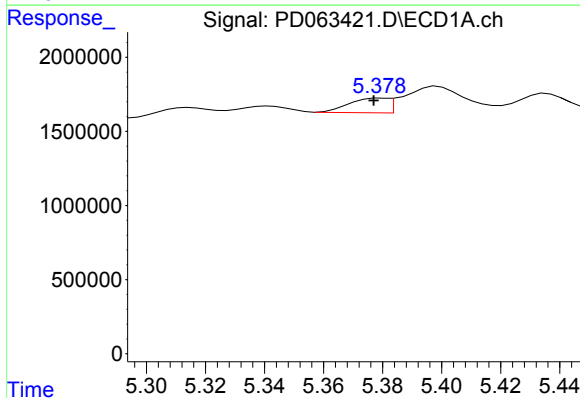


#10 gamma-Chlordane

R.T.: 5.378 min
Delta R.T.: 0.000 min
Response: 1179558
Conc: 0.66 ng/ml m

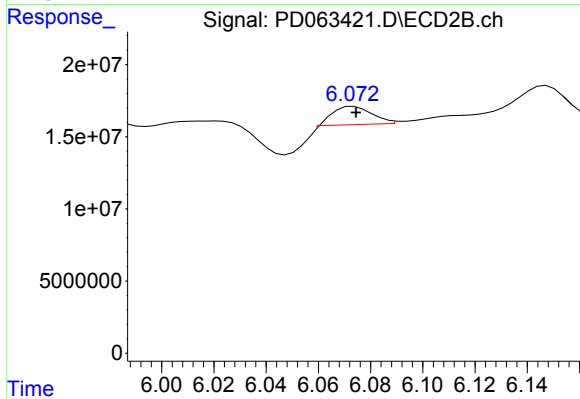

#10 gamma-Chlordane

R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 13280601
Conc: 0.71 ng/ml m

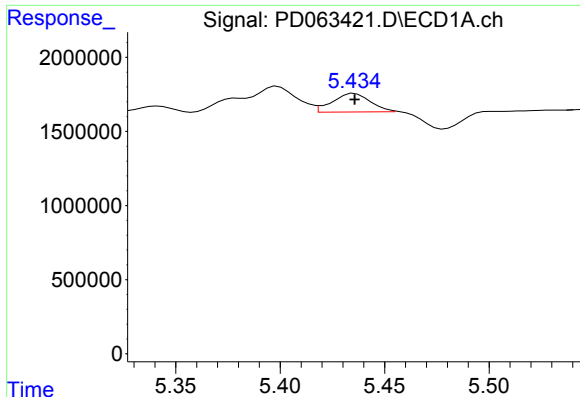


#11 alpha-Chlordane

R.T.: 5.434 min
Delta R.T.: -0.001 min
Response: 1566187
Conc: 0.89 ng/ml m

Instrument :
ECD_D
ClientSampleId :
EO-03-060221


Manual Integrations
APPROVED

Ankita
6/4/2021 12:10:32 PM

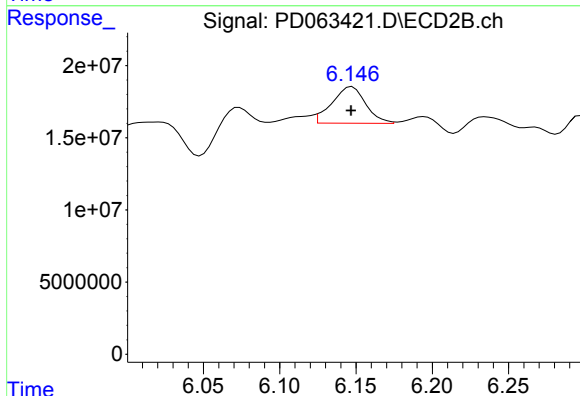


#11 alpha-Chlordane

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 38237188
Conc: 2.15 ng/ml m

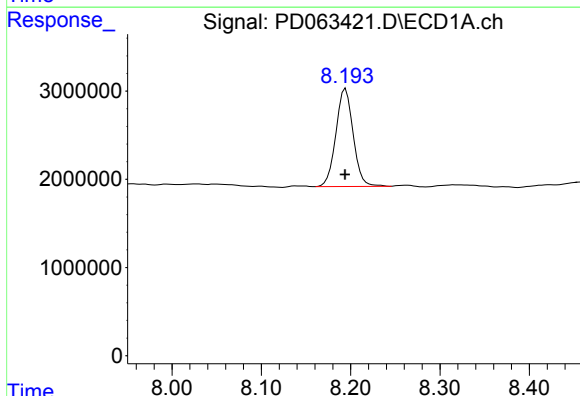

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 14912521
Conc: 9.48 ng/ml

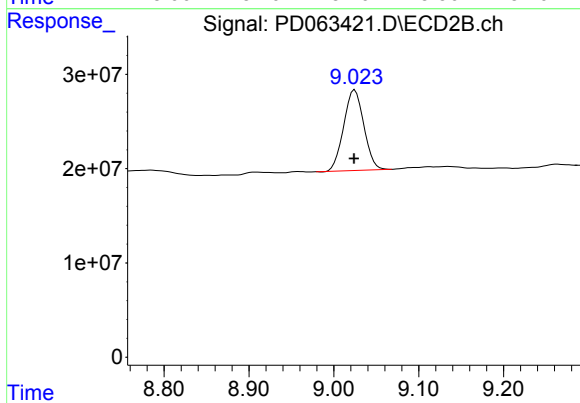

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.001 min
Response: 140930142
Conc: 10.20 ng/ml