

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 18:58
 Operator : AR\AJ
 Sample : M2580-19
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 18-B1(2-4)

Manual Integrations
 APPROVED

Ankita
 6/4/2021 11:26:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:31:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	32162161	313.8E6	23.243	23.420
28)	SA Decachlor...	8.195	9.025	31137353	297.3E6	19.799	21.512
Target Compounds							
3)	MA gamma-BHC...	4.163	4.636	1557759	22272649	0.793m	1.174m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 18:58
Operator : AR\AJ
Sample : M2580-19
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
18-B1(2-4)


Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:31:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

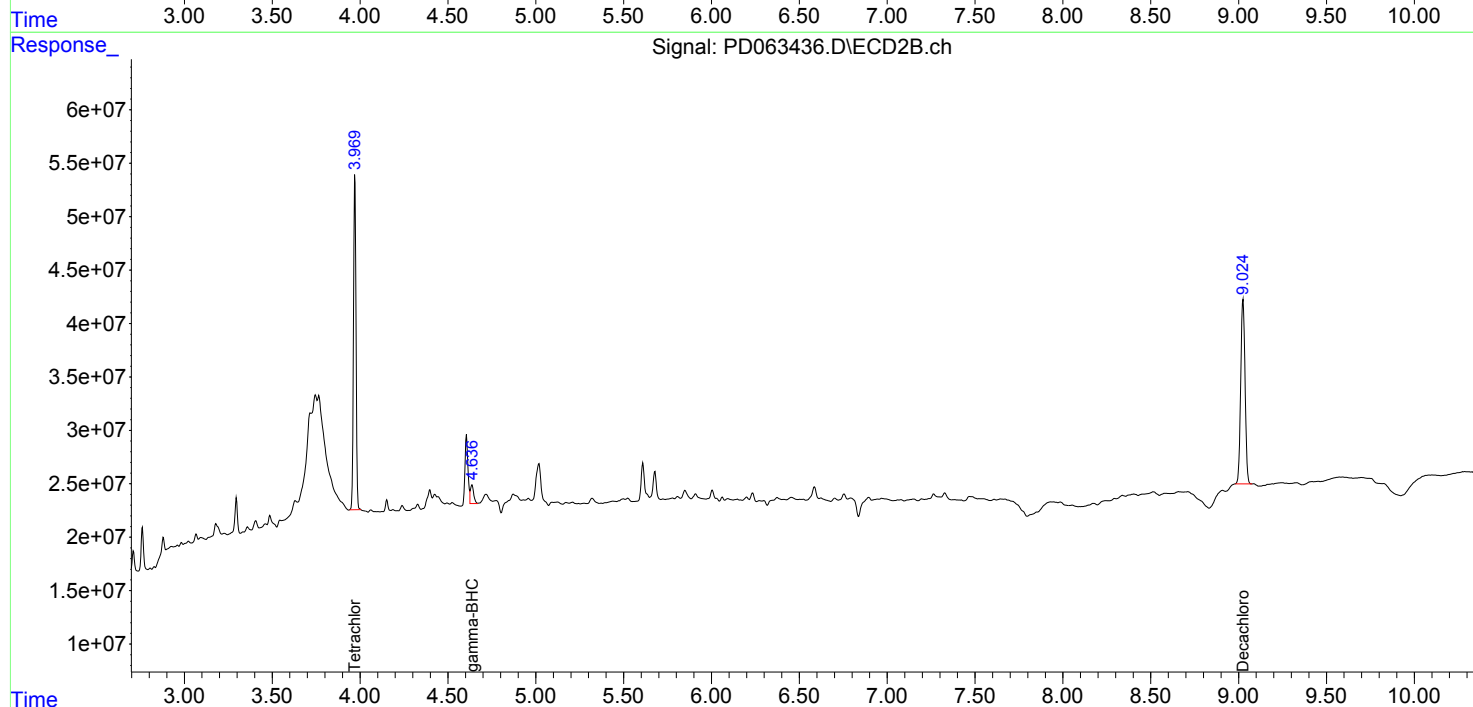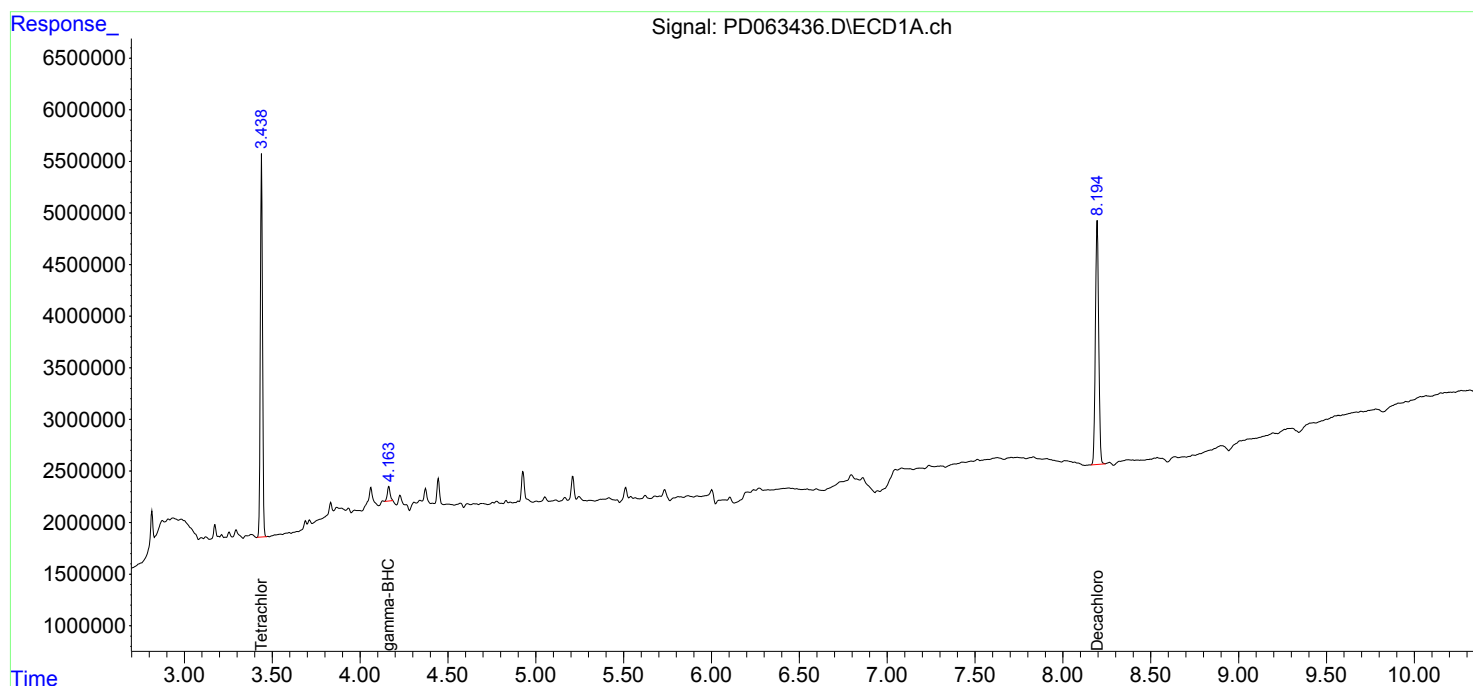

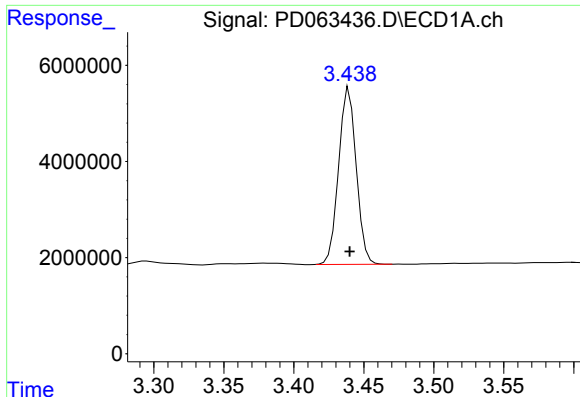


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 32162161
Conc: 23.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B1(2-4)


Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:08 AM

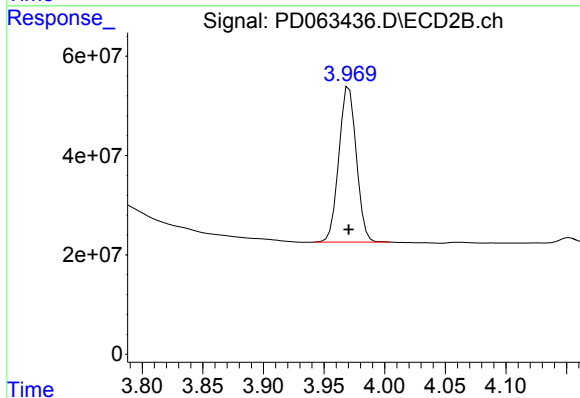


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 313798879
Conc: 23.42 ng/ml

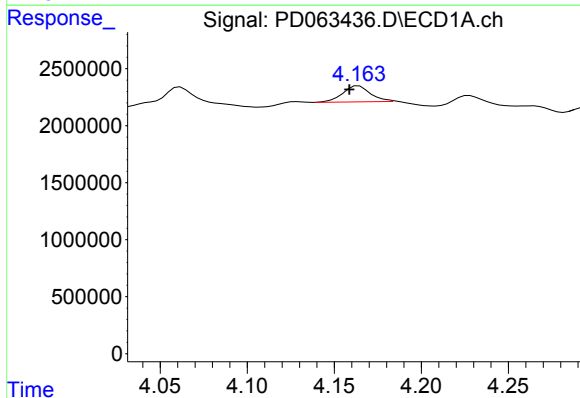


#3 gamma-BHC (Lindane)

R.T.: 4.163 min
Delta R.T.: 0.004 min
Response: 1557759
Conc: 0.79 ng/ml m

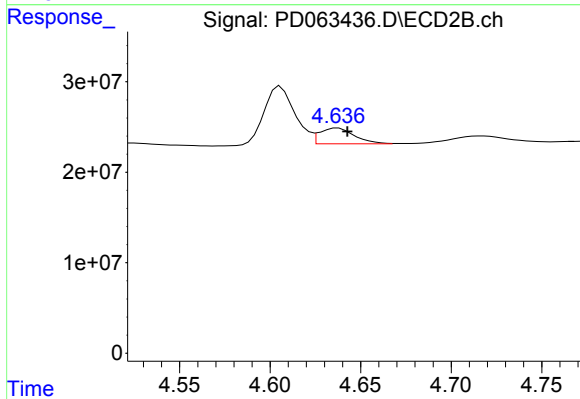

#3 gamma-BHC (Lindane)

R.T.: 4.636 min
Delta R.T.: -0.006 min
Response: 22272649
Conc: 1.17 ng/ml m

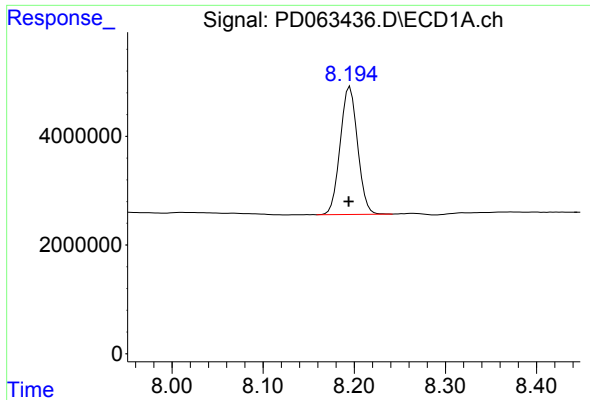


#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.002 min
Response: 31137353
Conc: 19.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B1(2-4)

Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:08 AM

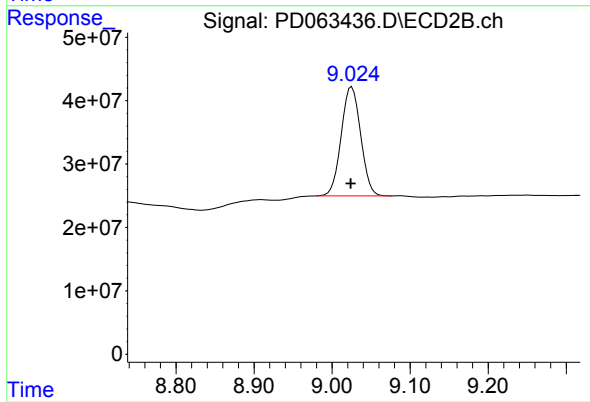

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.002 min
Response: 297266428
Conc: 21.51 ng/ml