

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 19:11
 Operator : AR\AJ
 Sample : M2580-20
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 18-B1(4-6)

Manual Integrations
 APPROVED

Ankita
 6/4/2021 11:26:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:31:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.969	35430652	302.8E6	25.605m	22.598m
28)	SA Decachlor...	8.195	9.026	21435080	196.4E6	13.629	14.214

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 19:11
Operator : AR\AJ
Sample : M2580-20
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
18-B1(4-6)


Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:31:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

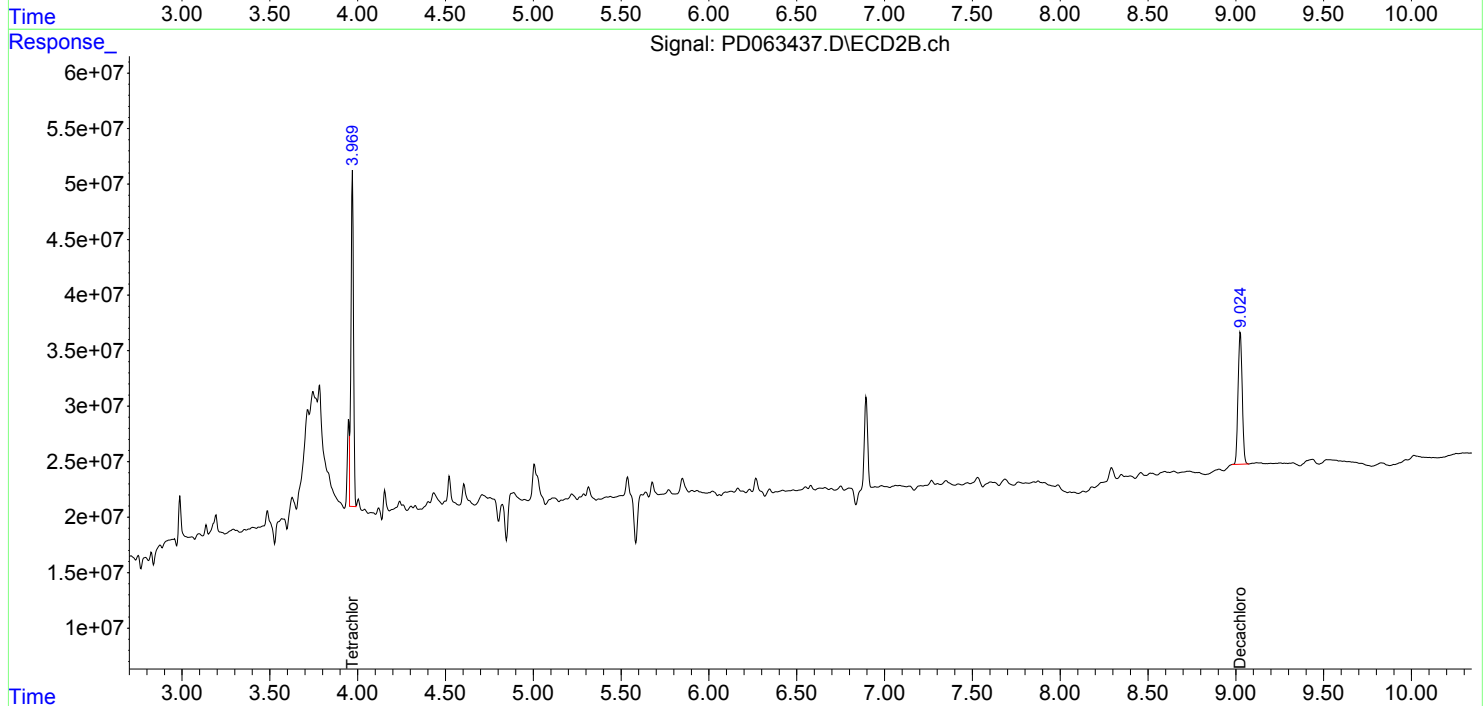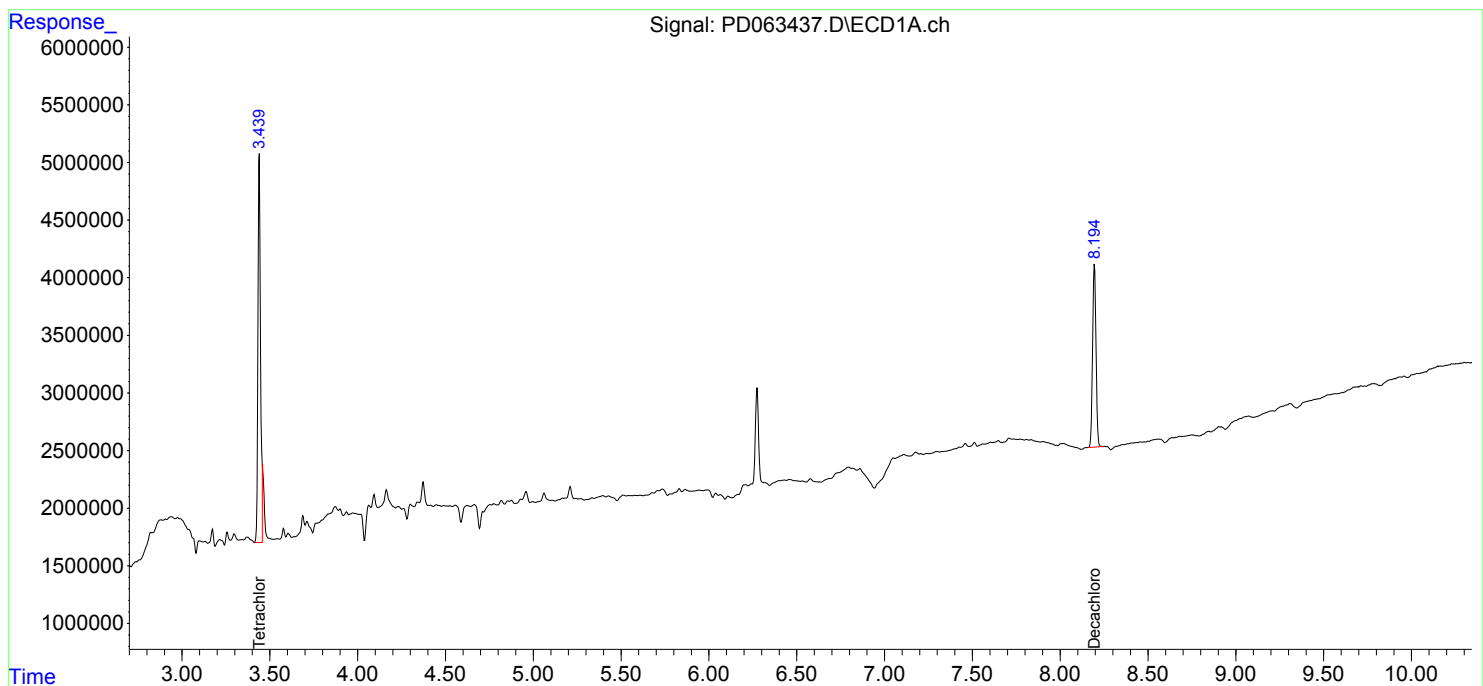

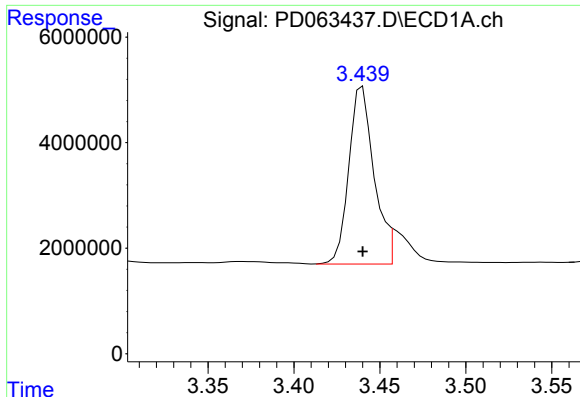


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 35430652
Conc: 25.60 ng/ml m

Instrument :
ECD_D
ClientSampleId :
18-B1(4-6)


Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:10 AM

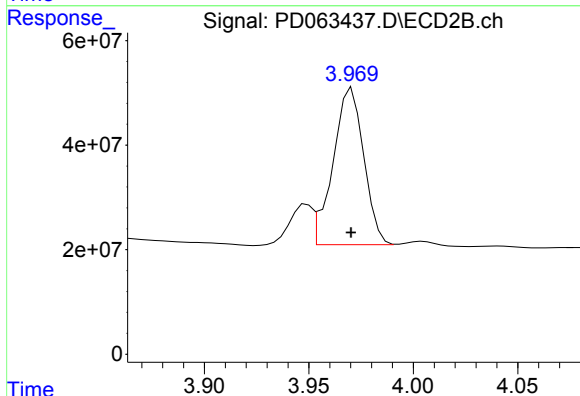


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 302779381
Conc: 22.60 ng/ml m

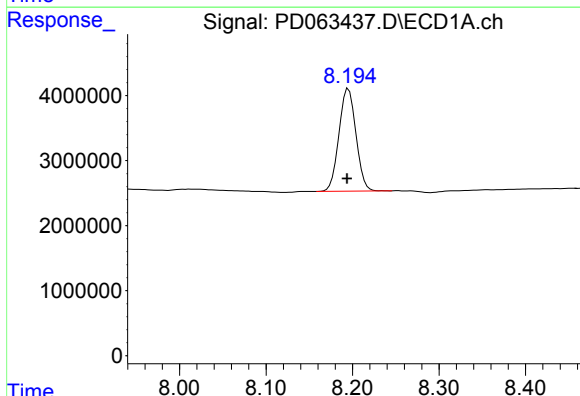

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.002 min
Response: 21435080
Conc: 13.63 ng/ml

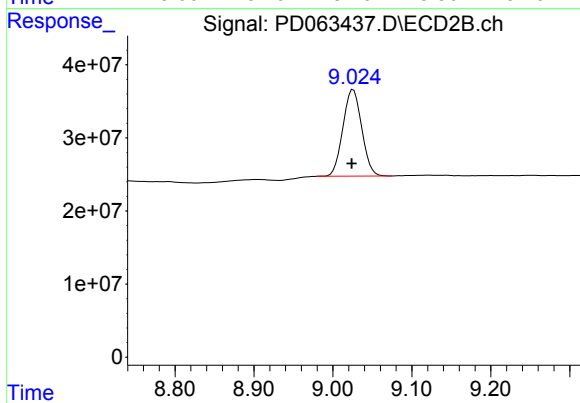

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.002 min
Response: 196419886
Conc: 14.21 ng/ml