

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 21:58
 Operator : AR\AJ
 Sample : M2580-26
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 18-B3(4-6)

Manual Integrations
 APPROVED

Ankita
 6/4/2021 11:26:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:35:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	32516737	320.3E6	23.499	23.908m
28)	SA Decachlor...	8.196	9.026	27007675	254.6E6	17.173	18.428
Target Compounds							
13)	MA Dieldrin	5.741	6.449	3985373	8216928	2.269m	0.454 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 21:58
Operator : AR\AJ
Sample : M2580-26
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
18-B3(4-6)


Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:35:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

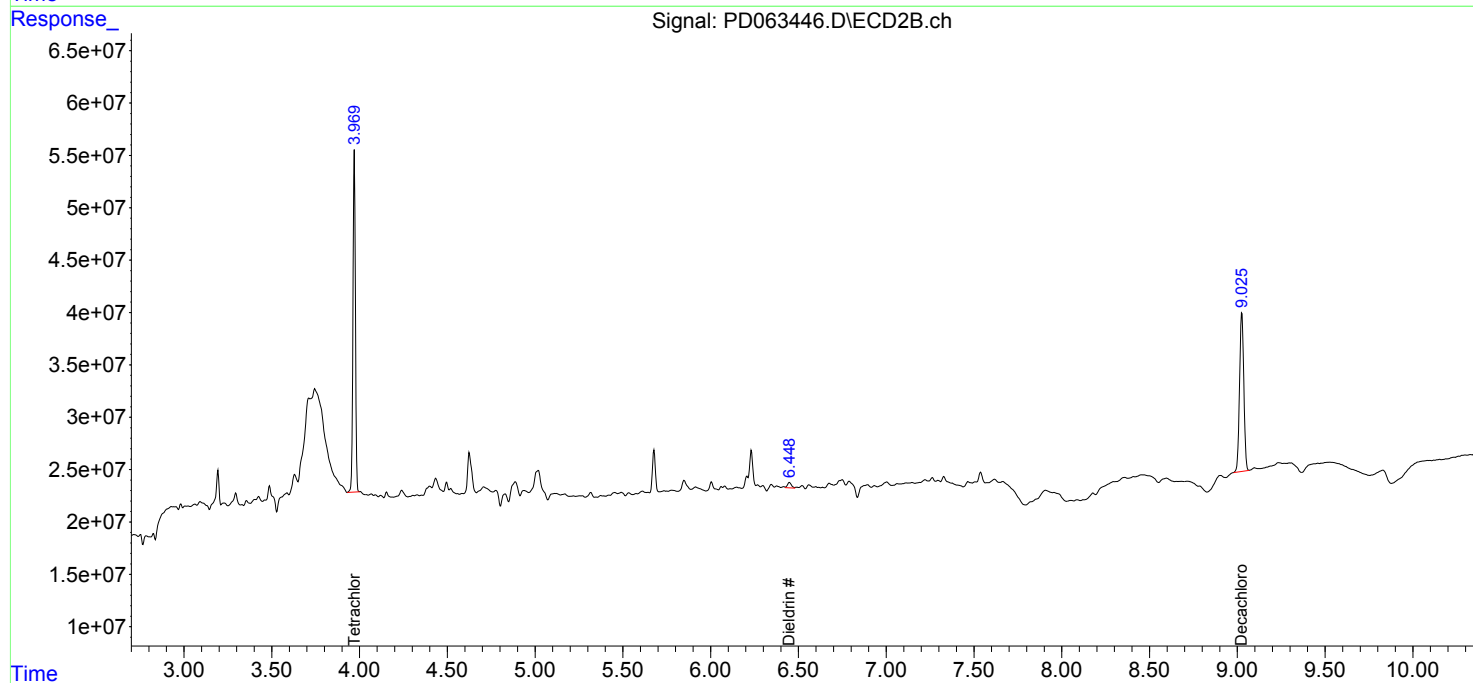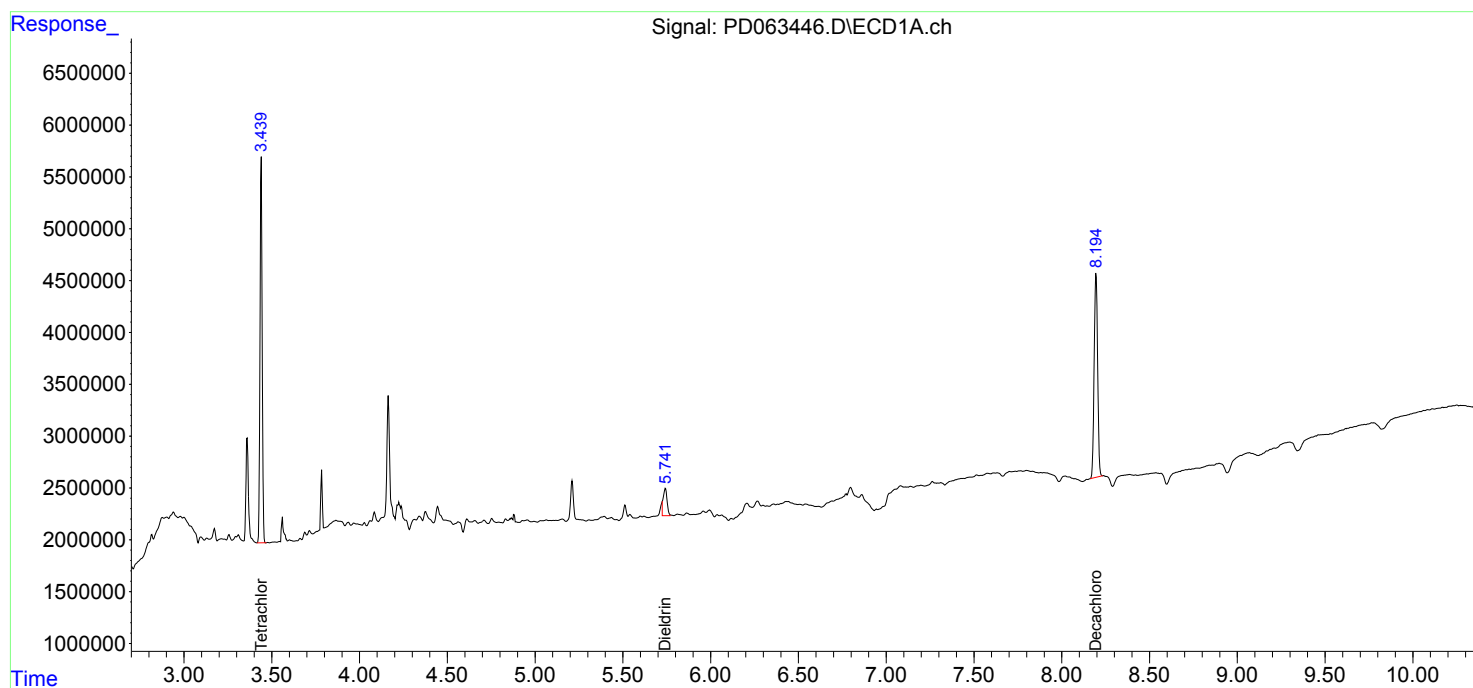

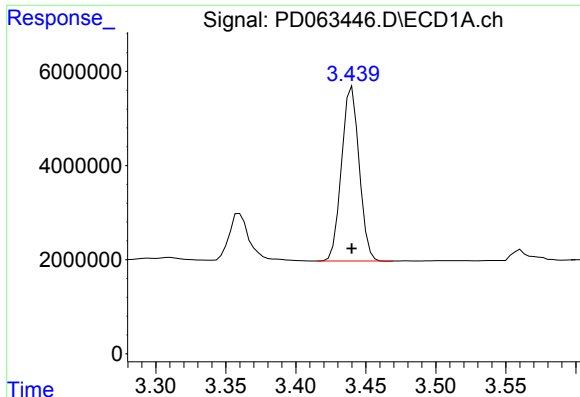


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 32516737
Conc: 23.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B3(4-6)


Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:17 AM

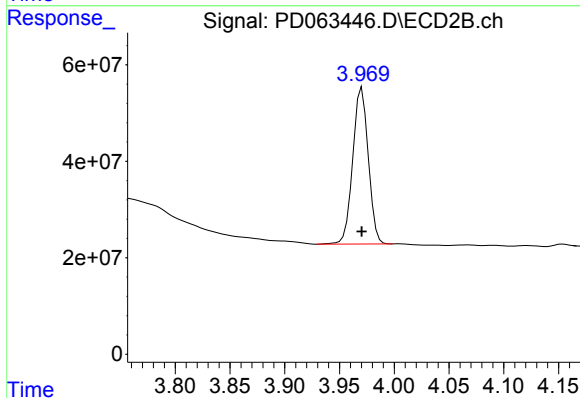


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 320332276
Conc: 23.91 ng/ml m

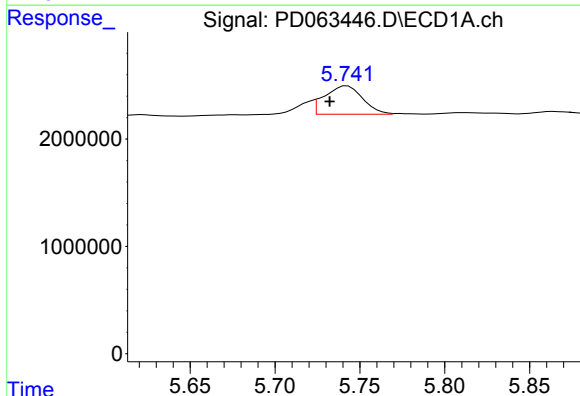


#13 Dieldrin

R.T.: 5.741 min
Delta R.T.: 0.009 min
Response: 3985373
Conc: 2.27 ng/ml m

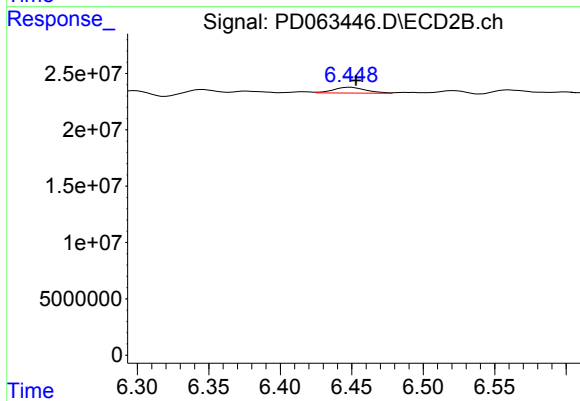

#13 Dieldrin

R.T.: 6.449 min
Delta R.T.: -0.004 min
Response: 8216928
Conc: 0.45 ng/ml

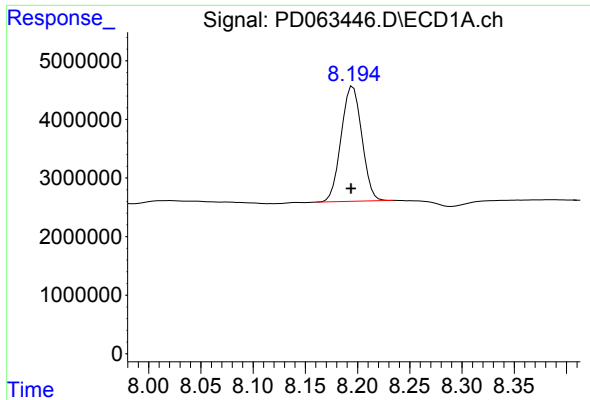


#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: 0.002 min
Response: 27007675
Conc: 17.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B3(4-6)

Manual Integrations
APPROVED

Ankita
6/4/2021 11:26:17 AM

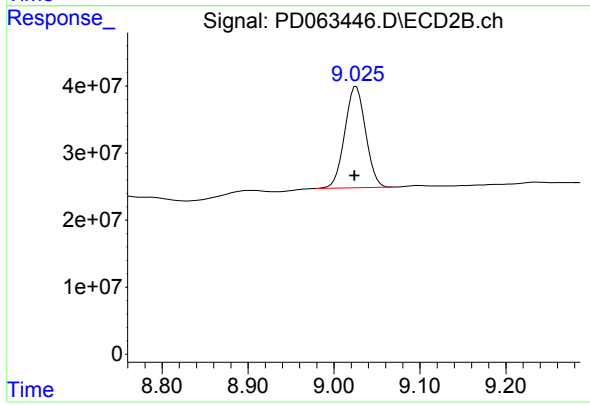

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.002 min
Response: 254647567
Conc: 18.43 ng/ml