

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
 Data File : PD063449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 22:40
 Operator : AR\AJ
 Sample : M2580-29
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 18-B4(4-6)

Manual Integrations
 APPROVED

Ankita
 6/4/2021 12:11:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 02:37:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	31837320	305.7E6	23.008	22.814
28)	SA Decachlor...	8.196	9.026	38065834	363.2E6	24.204	26.286
Target Compounds							
13)	MA Dieldrin	5.741	6.448	1295240	21761947	0.737m	1.202m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060421\
Data File : PD063449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 22:40
Operator : AR\AJ
Sample : M2580-29
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
18-B4(4-6)


Manual Integrations
APPROVED

Ankita
6/4/2021 12:11:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 02:37:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

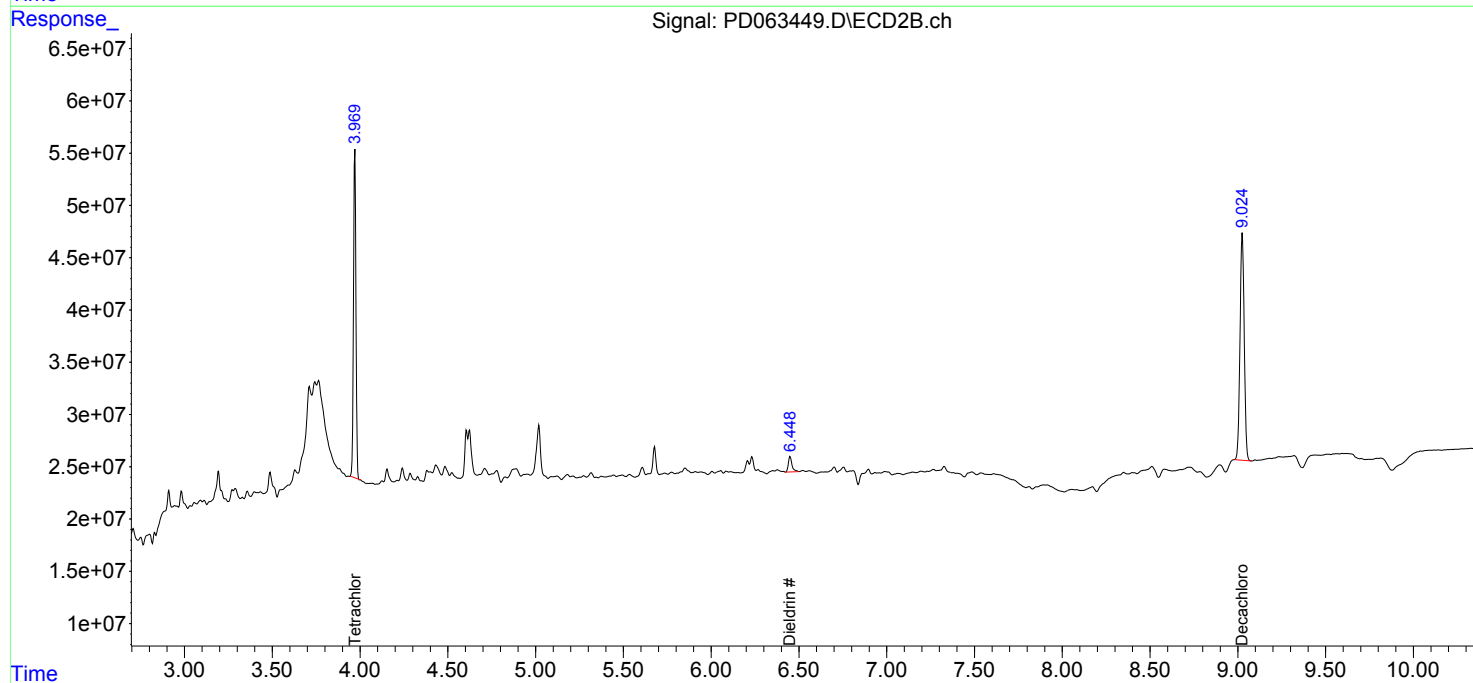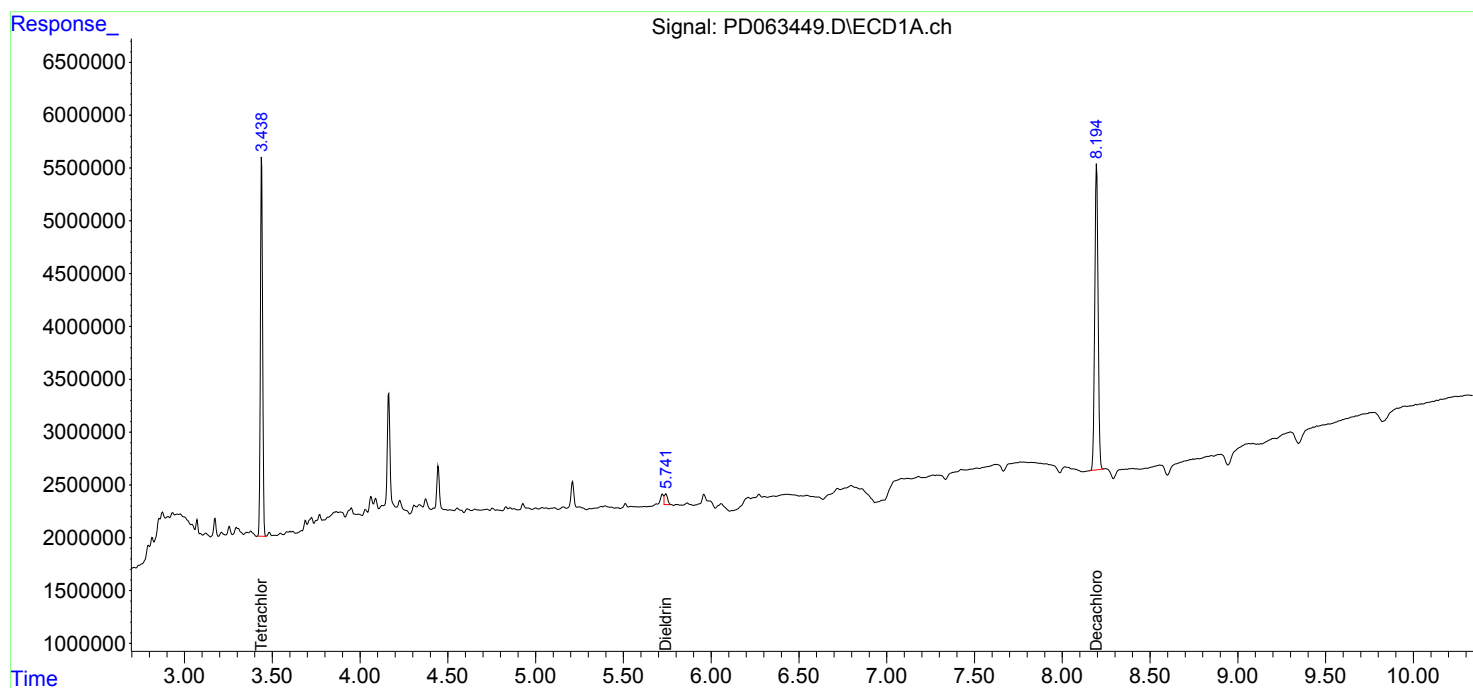

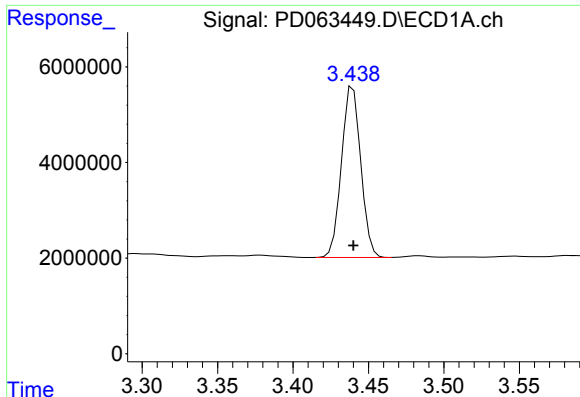


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 31837320
Conc: 23.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B4(4-6)


Manual Integrations
APPROVED

Ankita
6/4/2021 12:11:58 PM

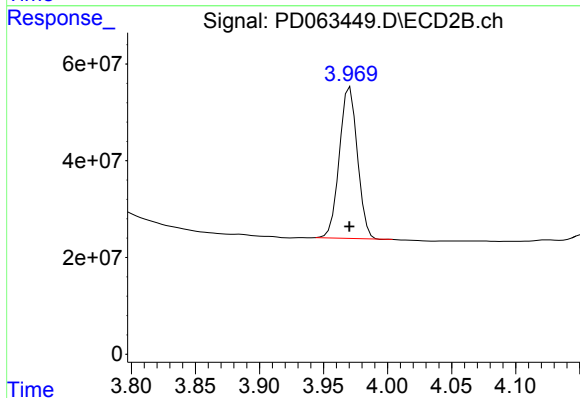


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 305676261
Conc: 22.81 ng/ml

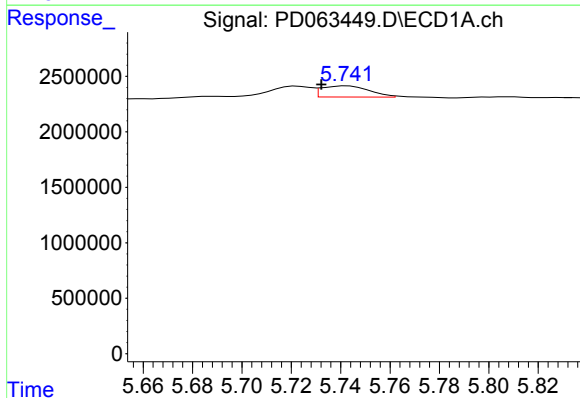


#13 Dieldrin

R.T.: 5.741 min
Delta R.T.: 0.009 min
Response: 1295240
Conc: 0.74 ng/ml m

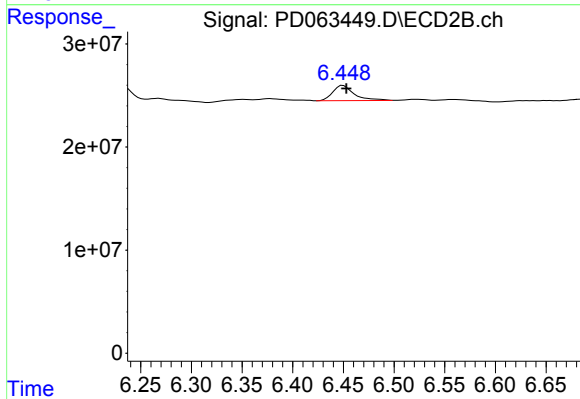

#13 Dieldrin

R.T.: 6.448 min
Delta R.T.: -0.005 min
Response: 21761947
Conc: 1.20 ng/ml m

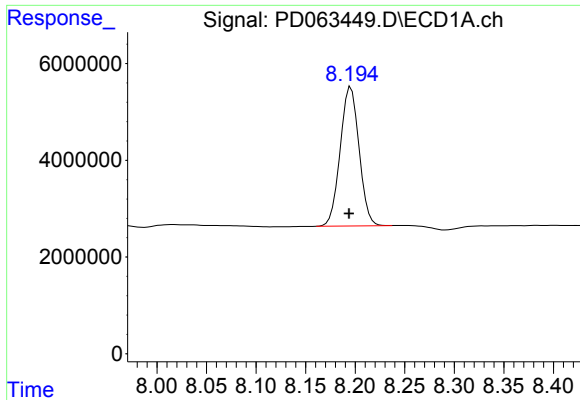


#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: 0.002 min
Response: 38065834
Conc: 24.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B4(4-6)

Manual Integrations
APPROVED

Ankita
6/4/2021 12:11:58 PM

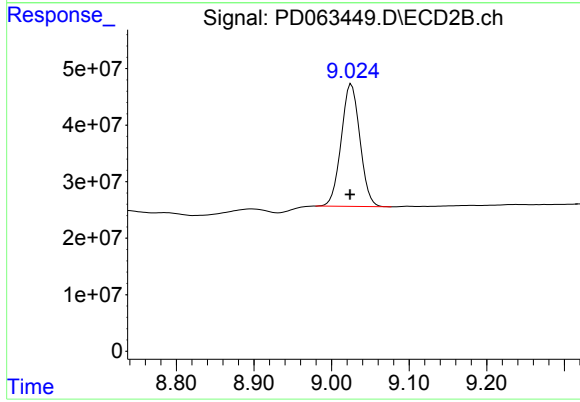

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.002 min
Response: 363239966
Conc: 26.29 ng/ml