

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
 Data File : PD070013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 12:47
 Operator : AR\AJ
 Sample : N2895-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:33:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	9226550	95641943	8.670	10.854 #
28)	SA Decachlor...	8.195	9.363	11330240	69361760	10.388	12.826
Target Compounds							
3)	MA gamma-BHC...	4.165	0.000	3462776	0	2.006	N.D. #
13)	MA Dieldrin	5.748	6.690	967238	7793050	0.735	0.826
14)	MA Endrin	5.988	0.000	1879536	0	1.628	N.D. #
15)	B Endosulfa...	0.000	7.119	0	9346181	N.D.	1.258 #
16)	A 4,4'-DDD	0.000	7.046	0	62705185	N.D.	8.468 #
17)	MA 4,4'-DDT	6.354	7.313f	8737621	75391659	8.816	10.302
18)	B Endrin al...	6.448	0.000	3075993	0	3.580	N.D. #
19)	B Endosulfa...	6.643	7.450f	5434304	-1598350	4.714	N.D. #
20)	A Methoxychlor	6.888f	0.000	15020394	0	26.477	N.D. #
21)	B Endrin ke...	7.164f	7.954	5357026	8793136	4.020	1.104 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
Data File : PD070013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 12:47
Operator : AR\AJ
Sample : N2895-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:33:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

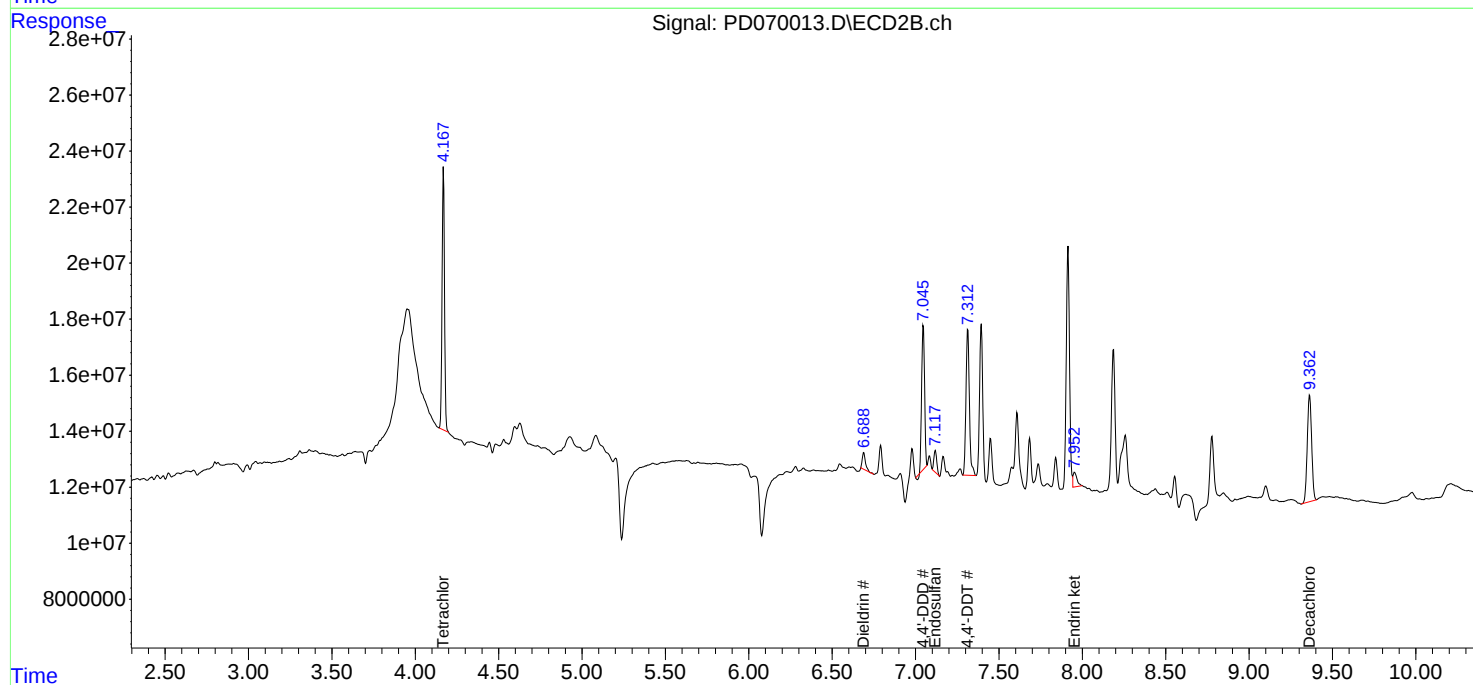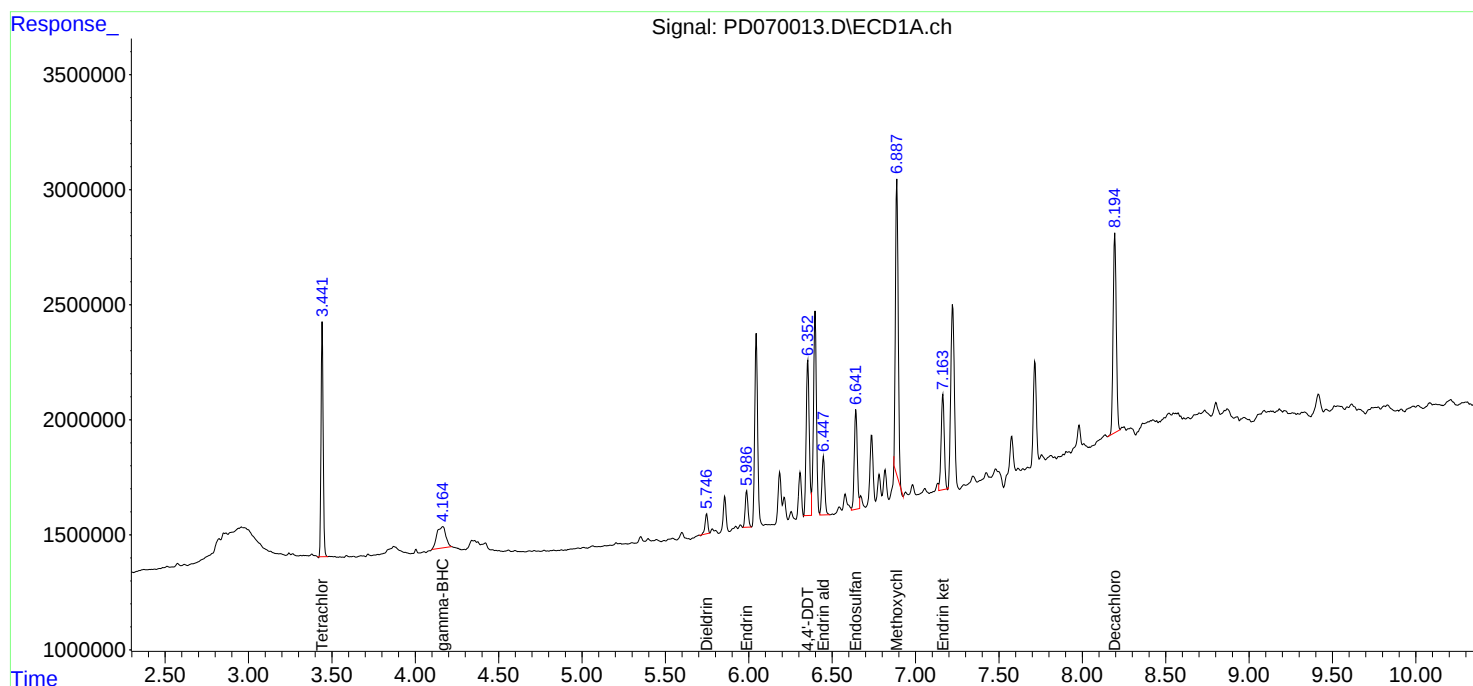


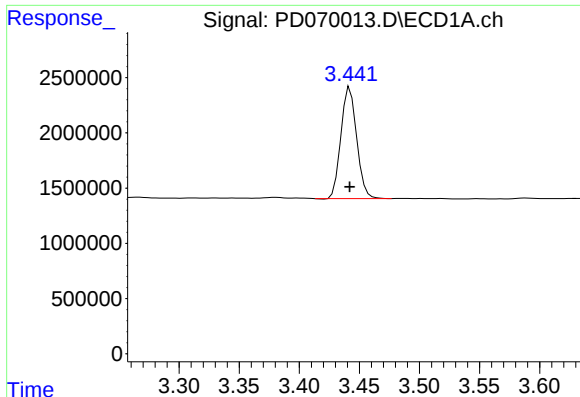

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 9226550
Conc: 8.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

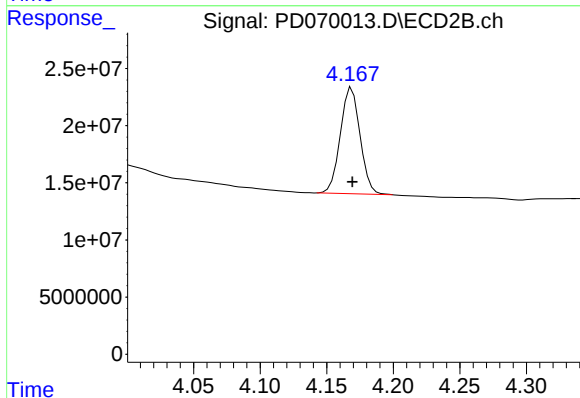


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 95641943
Conc: 10.85 ng/ml

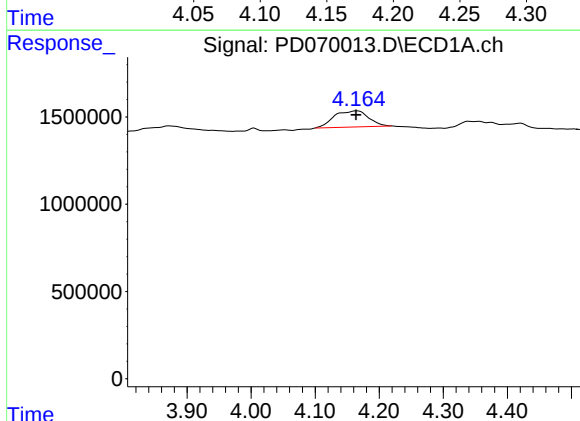


#3 gamma-BHC (Lindane)

R.T.: 4.165 min
Delta R.T.: 0.002 min
Response: 3462776
Conc: 2.01 ng/ml

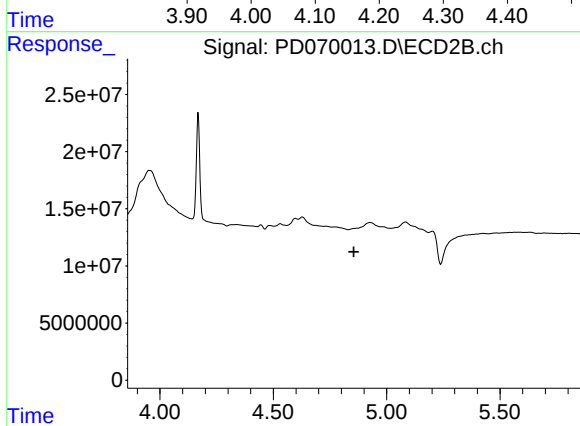

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

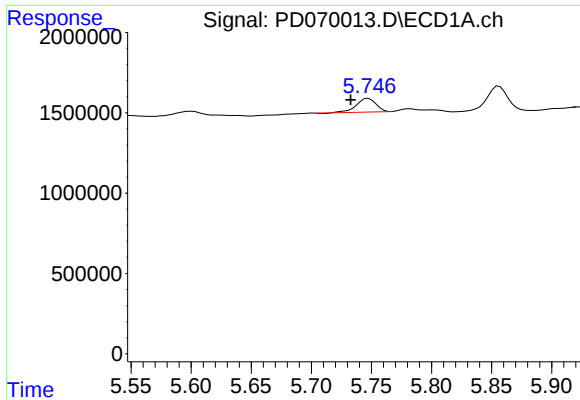

#13 Dieldrin


R.T.: 5.748 min
Delta R.T.: 0.015 min
Response: 967238
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

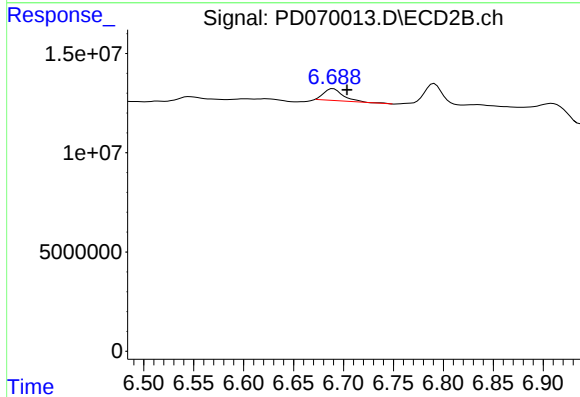


#13 Dieldrin

R.T.: 6.690 min
Delta R.T.: -0.014 min
Response: 7793050
Conc: 0.83 ng/ml

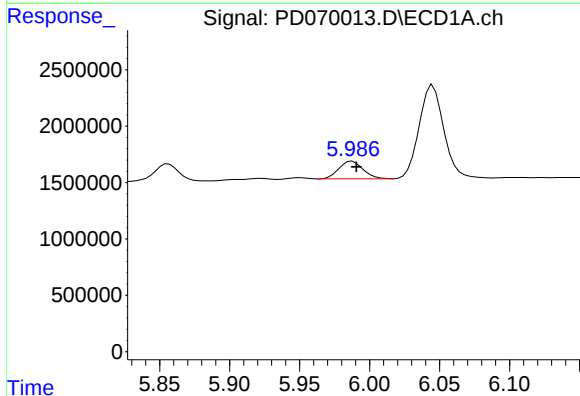


#14 Endrin

R.T.: 5.988 min
Delta R.T.: -0.003 min
Response: 1879536
Conc: 1.63 ng/ml

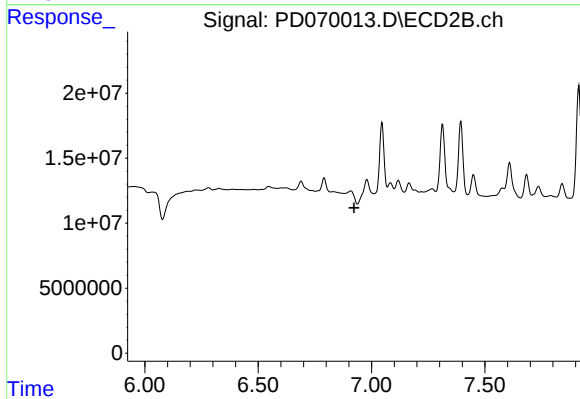

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

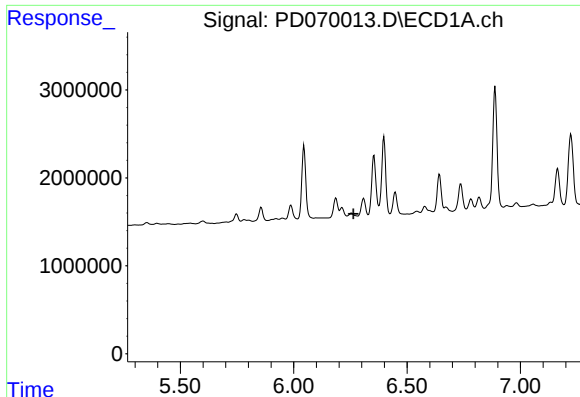

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

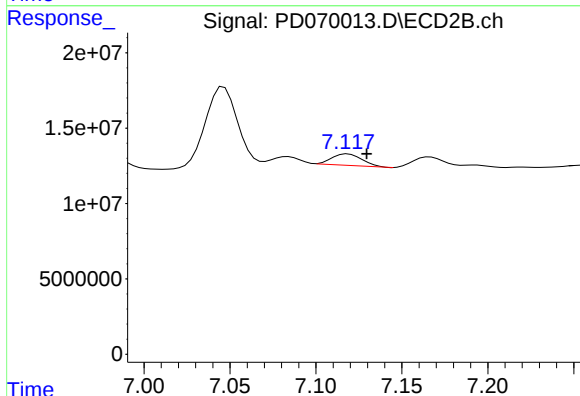


#15 Endosulfan II

R.T.: 7.119 min
Delta R.T.: -0.011 min
Response: 9346181
Conc: 1.26 ng/ml

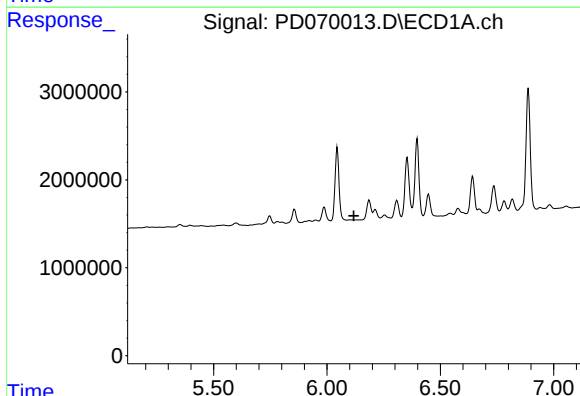


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.118 min
Response: 0
Conc: N.D.

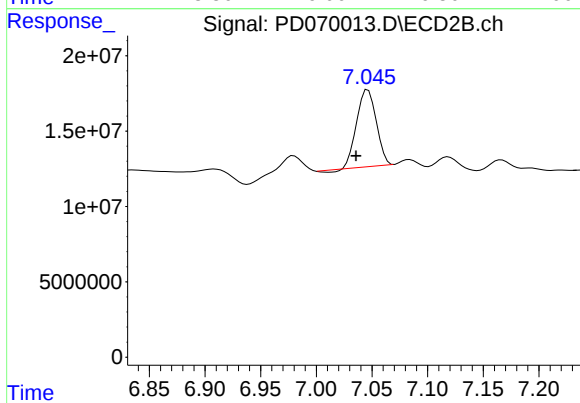

#16 4,4'-DDD


R.T.: 7.046 min
Delta R.T.: 0.011 min
Response: 62705185
Conc: 8.47 ng/ml

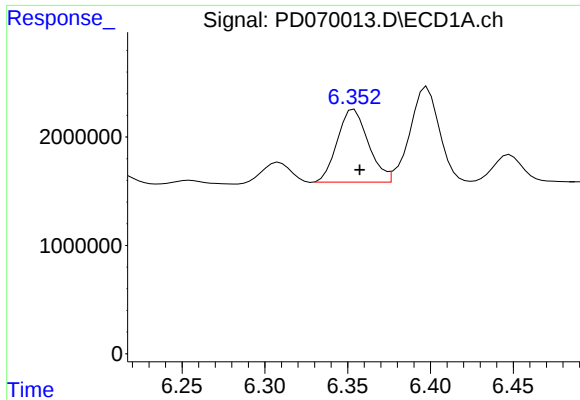

#17 4,4'-DDT


R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 8737621
Conc: 8.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

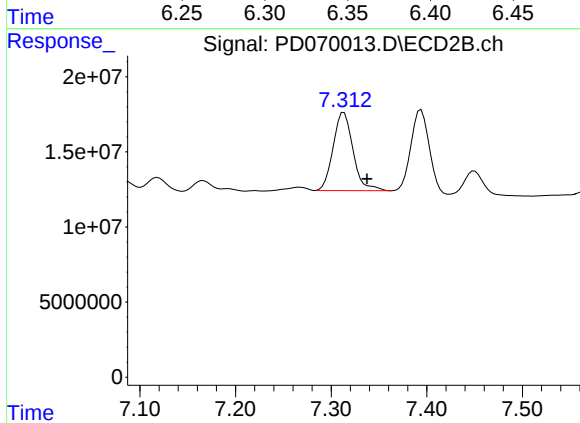


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: -0.024 min
Response: 75391659
Conc: 10.30 ng/ml

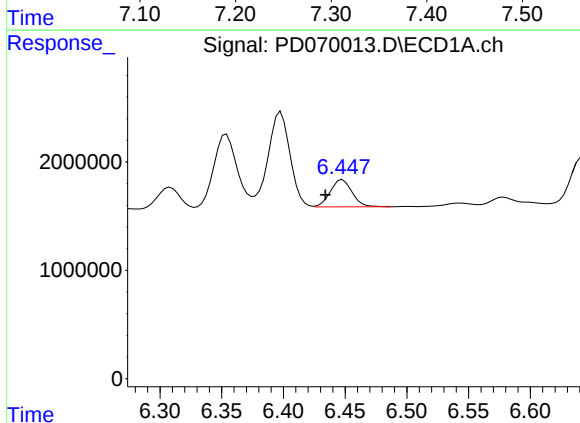


#18 Endrin aldehyde

R.T.: 6.448 min
Delta R.T.: 0.014 min
Response: 3075993
Conc: 3.58 ng/ml

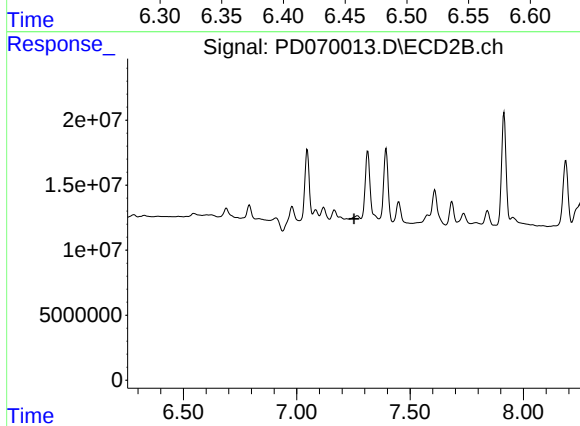

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

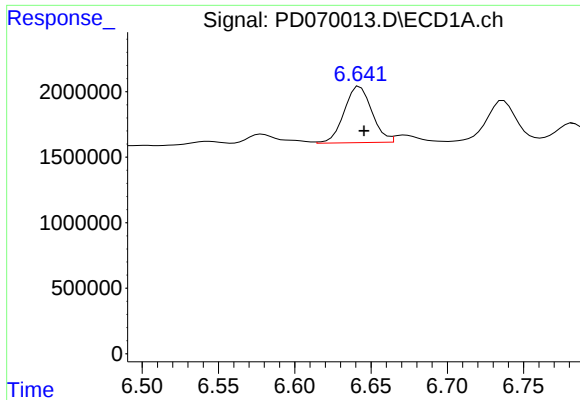

#19 Endosulfan Sulfate


R.T.: 6.643 min
Delta R.T.: -0.003 min
Response: 5434304
Conc: 4.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

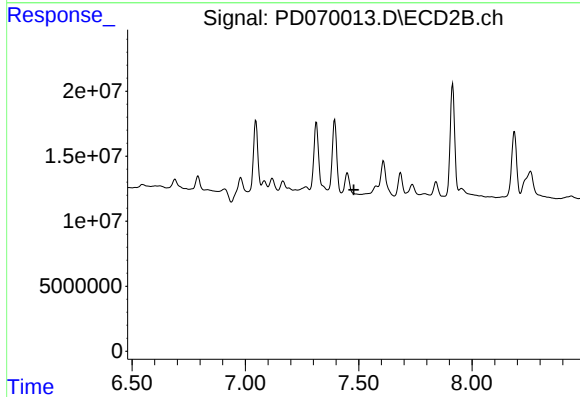


#19 Endosulfan Sulfate

R.T.: 7.450 min
Delta R.T.: -0.028 min
Response: -1598350
Conc: N.D.

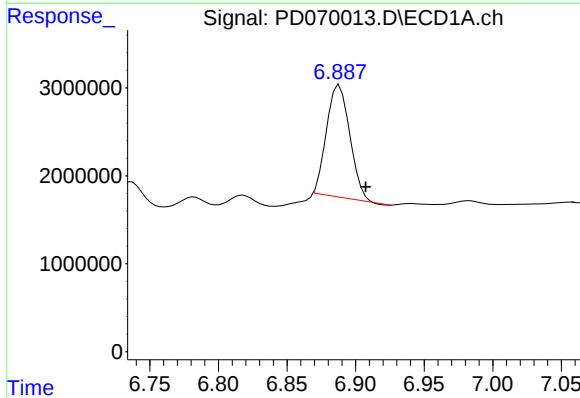


#20 Methoxychlor

R.T.: 6.888 min
Delta R.T.: -0.019 min
Response: 15020394
Conc: 26.48 ng/ml

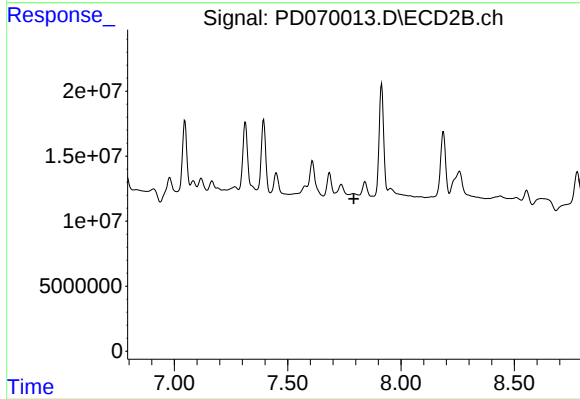

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

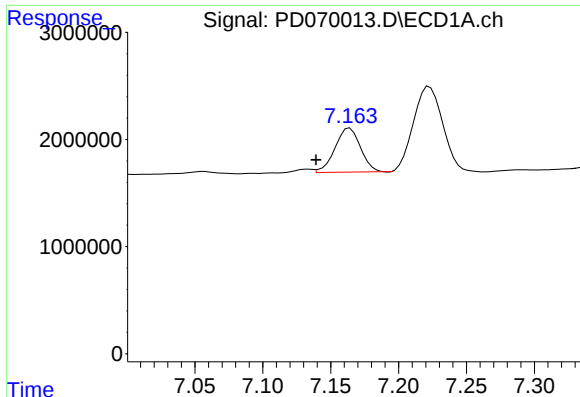

#21 Endrin ketone


R.T.: 7.164 min
Delta R.T.: 0.025 min
Response: 5357026
Conc: 4.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

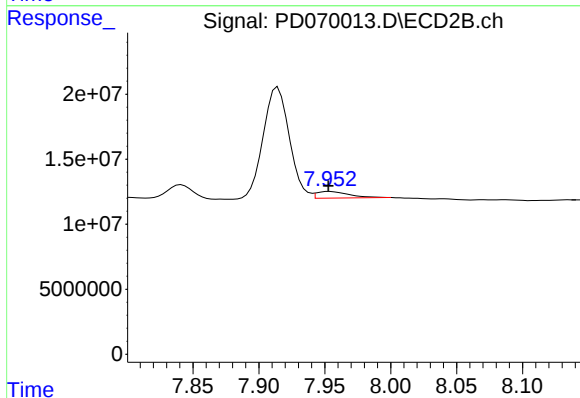


#21 Endrin ketone

R.T.: 7.954 min
Delta R.T.: 0.000 min
Response: 8793136
Conc: 1.10 ng/ml

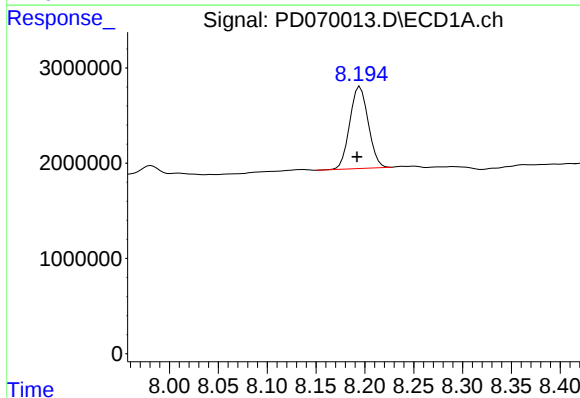

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.003 min
Response: 11330240
Conc: 10.39 ng/ml

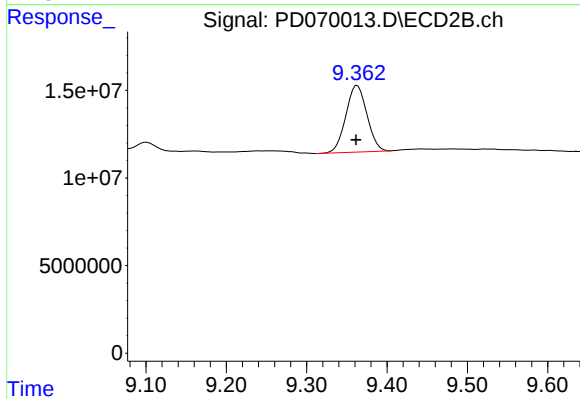

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.002 min
Response: 69361760
Conc: 12.83 ng/ml