

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
 Data File : PD070020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 14:27
 Operator : AR\AJ
 Sample : PB145264BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:34:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	19829693	188.7E6	18.633	21.419
28)	SA Decachlor...	8.194	9.364	19851512	119.1E6	18.200	22.015
Target Compounds							
3)	MA gamma-BHC...	4.165	0.000	2097279	0	1.215	N.D. #
20)	A Methoxychlor	0.000	7.773f	0	30518967	N.D.	8.559 #
23)	Chlordane-1	4.339f	0.000	198137	0	5.059	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
Data File : PD070020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 14:27
Operator : AR\AJ
Sample : PB145264BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:34:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

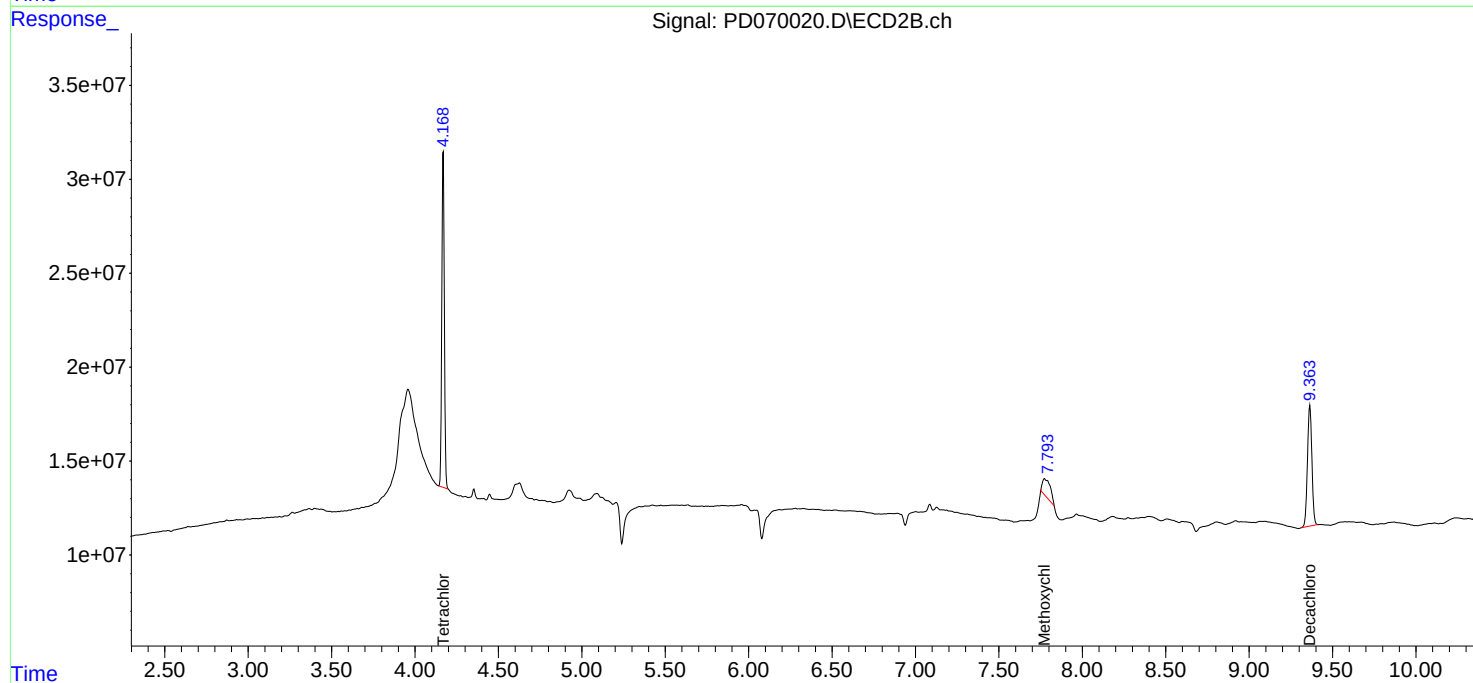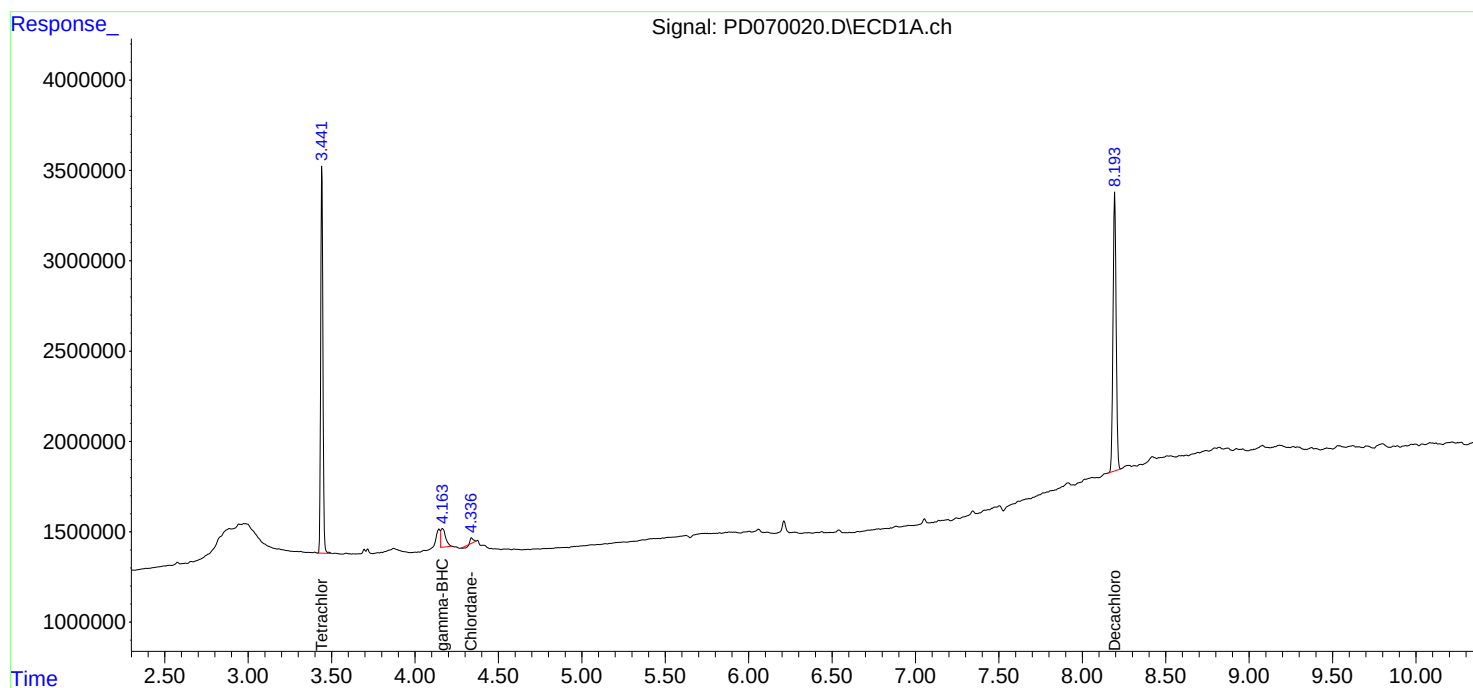


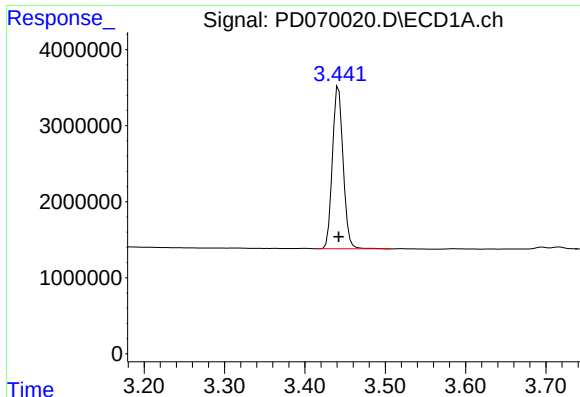

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 19829693
Conc: 18.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

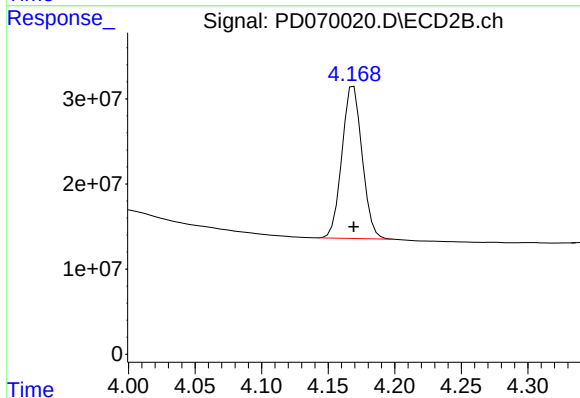


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 188737214
Conc: 21.42 ng/ml

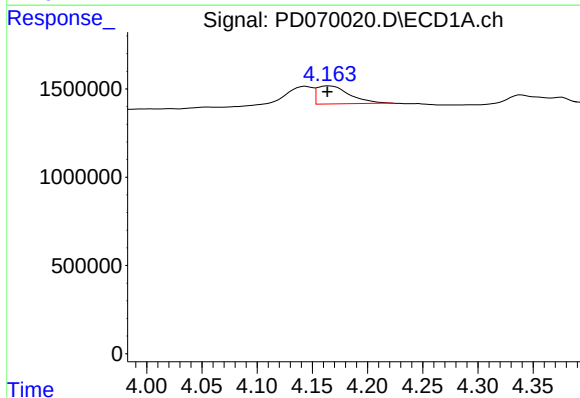


#3 gamma-BHC (Lindane)

R.T.: 4.165 min
Delta R.T.: 0.001 min
Response: 2097279
Conc: 1.22 ng/ml

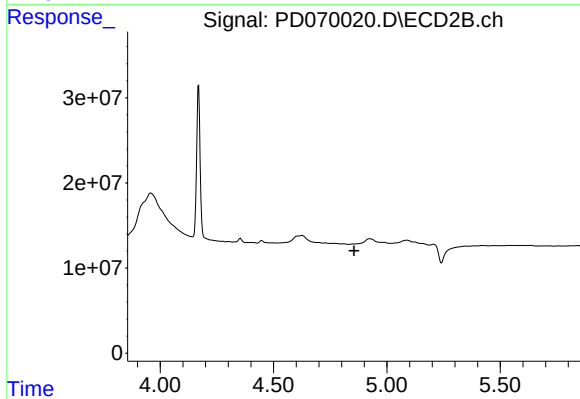

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

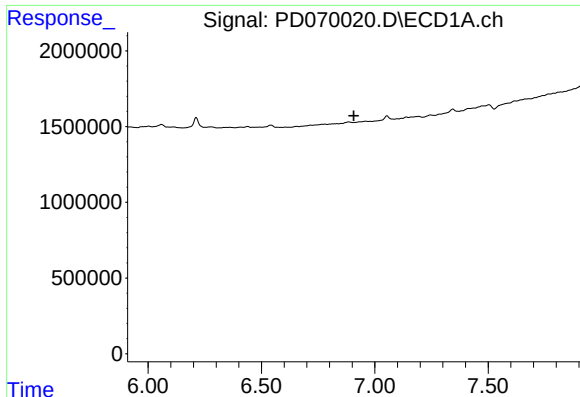

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

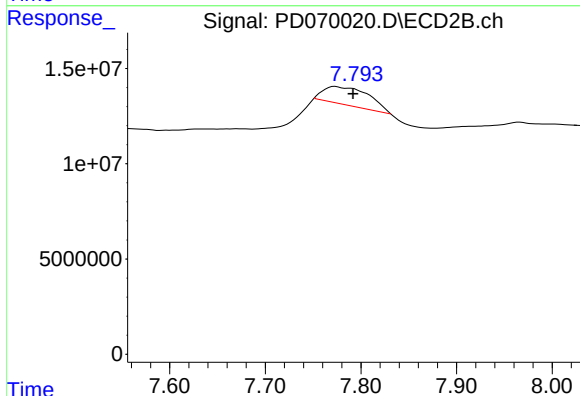


#20 Methoxychlor

R.T.: 7.773 min
Delta R.T.: -0.018 min
Response: 30518967
Conc: 8.56 ng/ml

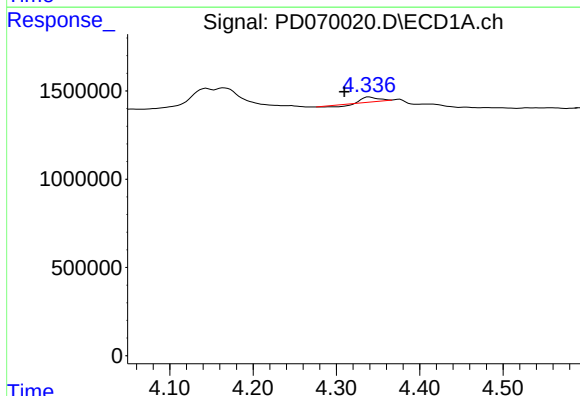


#23 Chlordane-1

R.T.: 4.339 min
Delta R.T.: 0.030 min
Response: 198137
Conc: 5.06 ng/ml

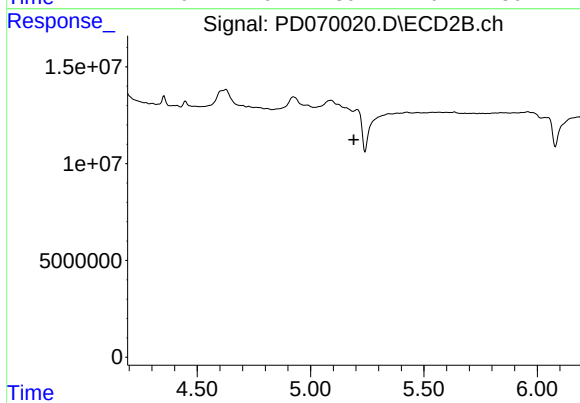

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.190 min
Response: 0
Conc: N.D.

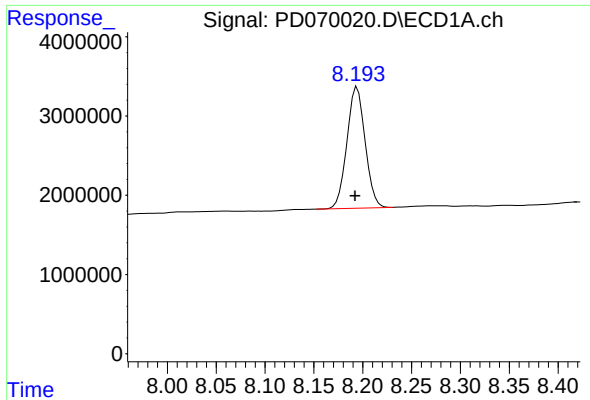

#28 Decachlorobiphenyl


R.T.: 8.194 min

Delta R.T.: 0.002 min

Response: 19851512

Conc: 18.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

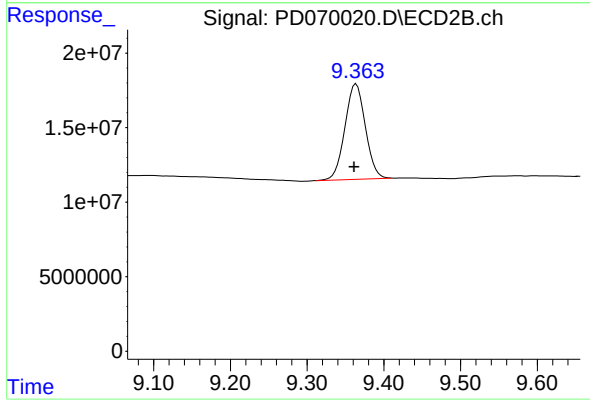

#28 Decachlorobiphenyl

R.T.: 9.364 min

Delta R.T.: 0.003 min

Response: 119056676

Conc: 22.01 ng/ml