

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
 Data File : PD070029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 17:20
 Operator : AR\AJ
 Sample : N2988-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:38:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	11024415	109.6E6	10.359	12.433
28)	SA Decachlor...	8.195	9.364	13100207	67494900	12.010	12.480
Target Compounds							
3)	MA gamma-BHC...	4.162	0.000	4091574	0	2.371	N.D. #
14)	MA Endrin	5.988	0.000	1029846	0	0.892	N.D. #
16)	A 4,4'-DDD	0.000	7.047	0	37574294	N.D.	5.074 #
17)	MA 4,4'-DDT	6.355	7.314f	6302545	55079996	6.359	7.527
18)	B Endrin al...	6.448	0.000	1552116	0	1.806	N.D. #
19)	B Endosulfa...	6.643	0.000	2329671	0	2.021	N.D. #
20)	A Methoxychlor	6.888f	7.775f	10001605	259.7E6	17.630	72.835 #
21)	B Endrin ke...	7.164f	0.000	4639210	0	3.481	N.D. #
23)	Chlordane-1	4.339f	0.000	1553649	0	39.668	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
Data File : PD070029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 17:20
Operator : AR\AJ
Sample : N2988-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:38:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

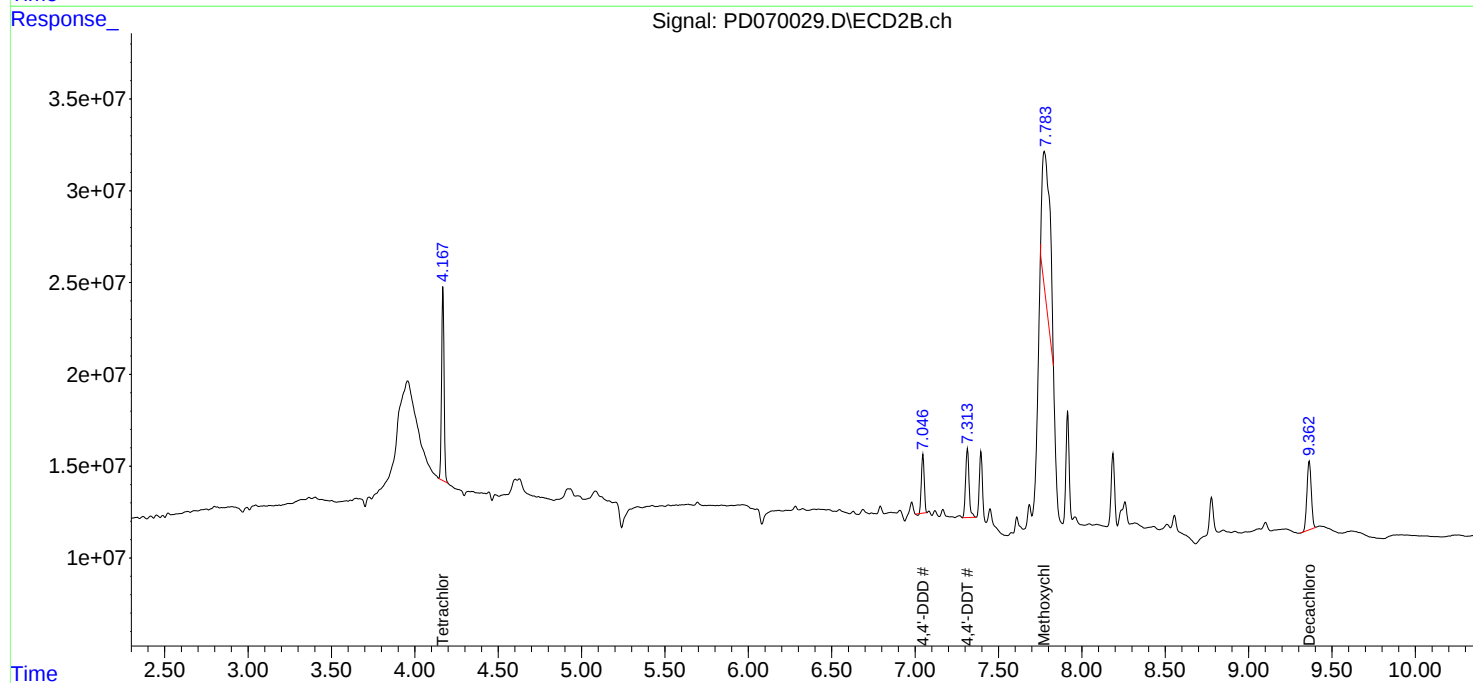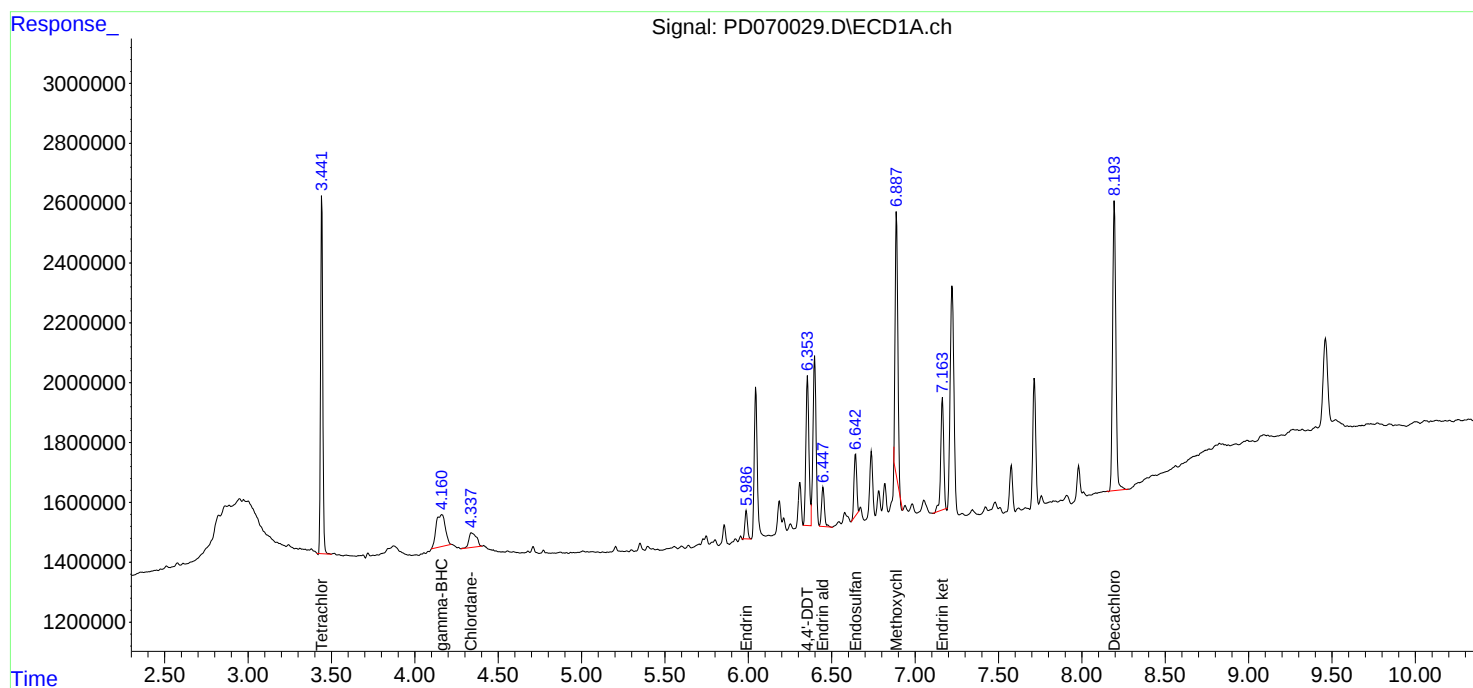


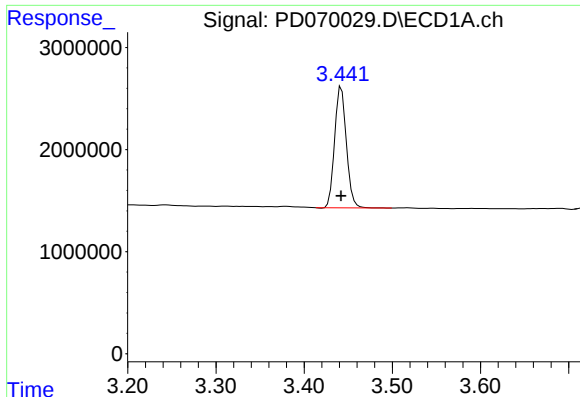

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 11024415
Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

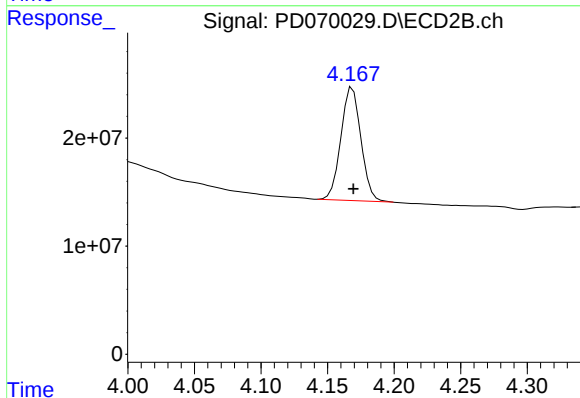


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 109553209
Conc: 12.43 ng/ml

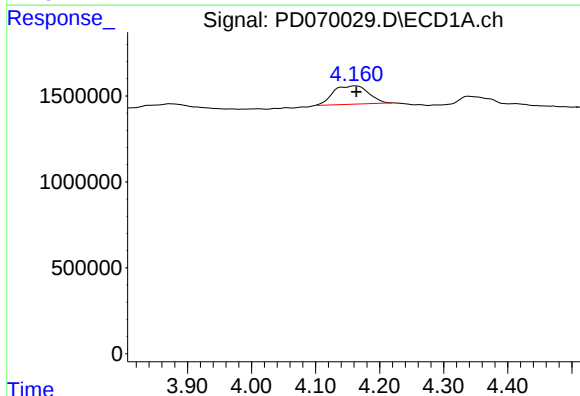


#3 gamma-BHC (Lindane)

R.T.: 4.162 min
Delta R.T.: -0.002 min
Response: 4091574
Conc: 2.37 ng/ml

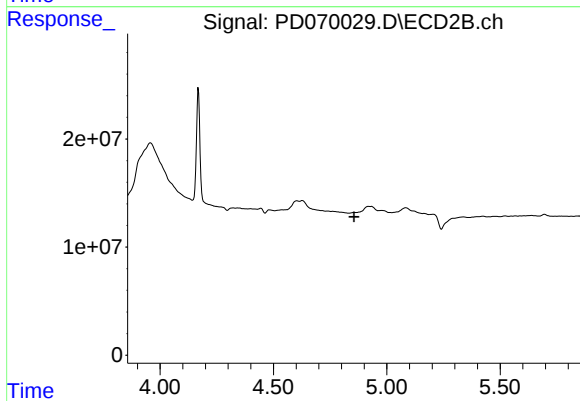

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

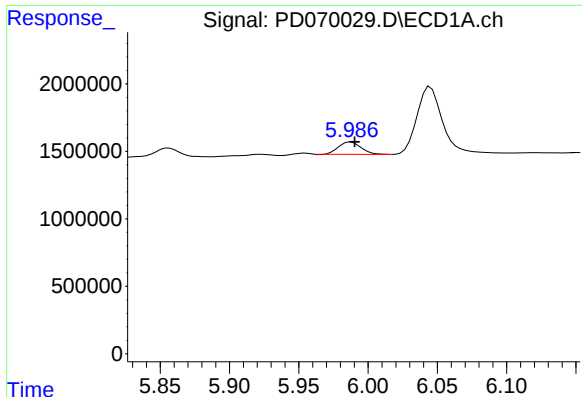

#14 Endrin


R.T.: 5.988 min
Delta R.T.: -0.003 min
Response: 1029846
Conc: 0.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

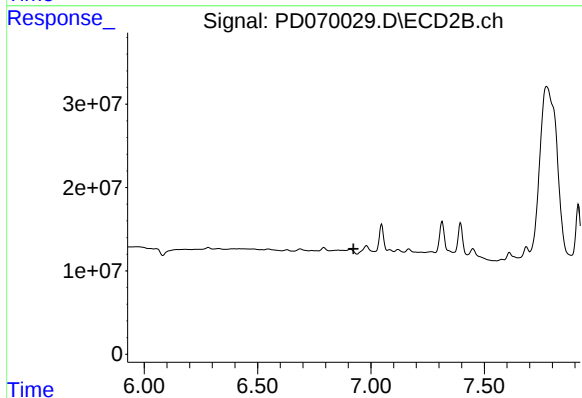


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

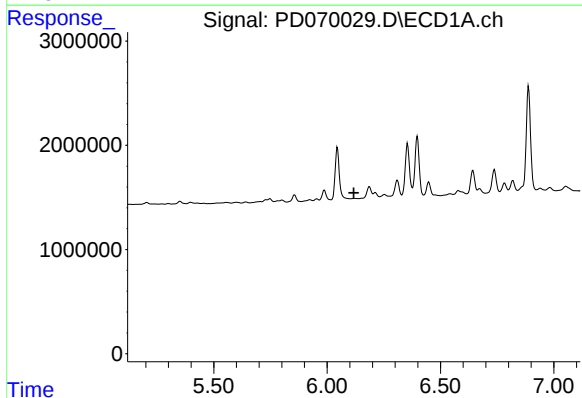


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

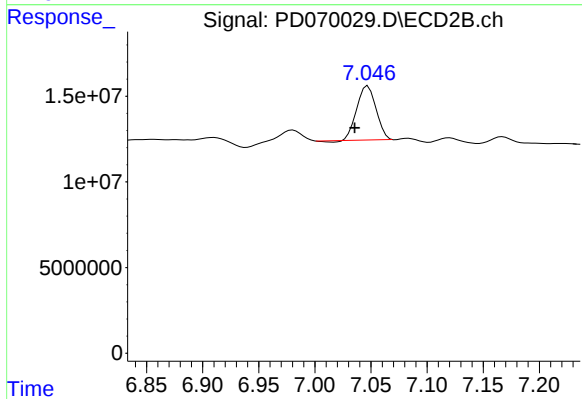

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: 0.012 min
Response: 37574294
Conc: 5.07 ng/ml

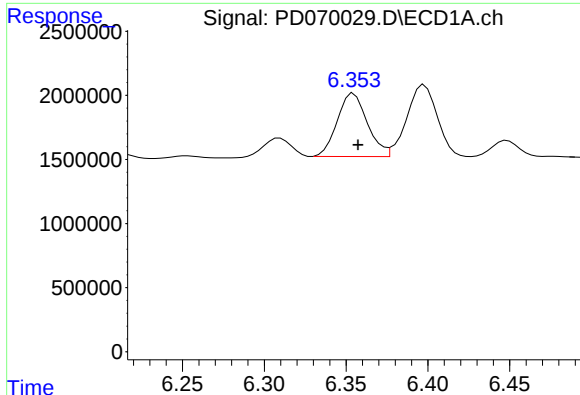

#17 4,4'-DDT


R.T.: 6.355 min
Delta R.T.: -0.003 min
Response: 6302545
Conc: 6.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

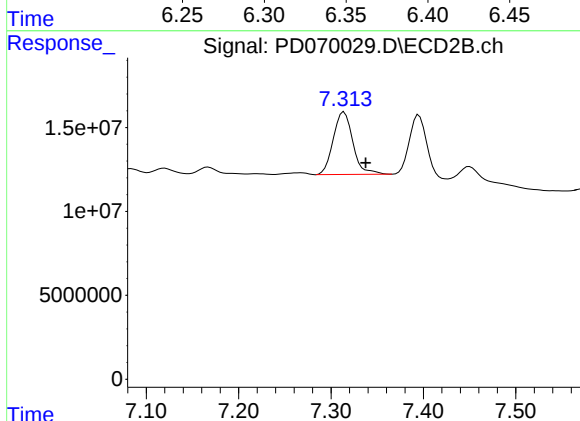


#17 4,4'-DDT

R.T.: 7.314 min
Delta R.T.: -0.023 min
Response: 55079996
Conc: 7.53 ng/ml

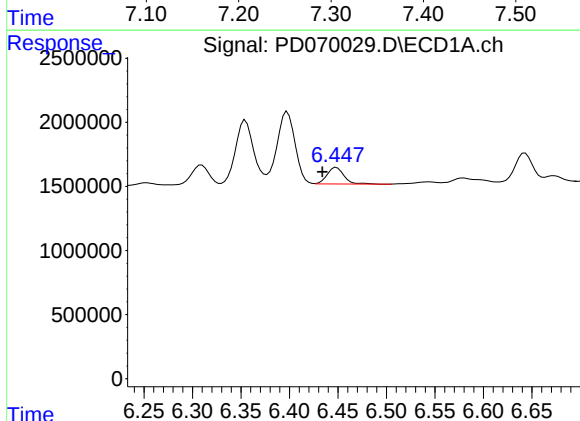


#18 Endrin aldehyde

R.T.: 6.448 min
Delta R.T.: 0.014 min
Response: 1552116
Conc: 1.81 ng/ml

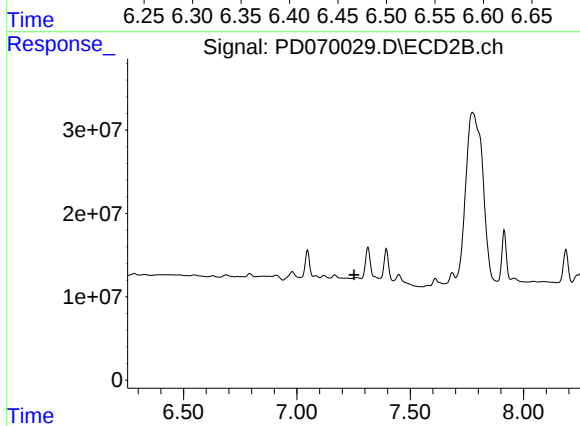

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

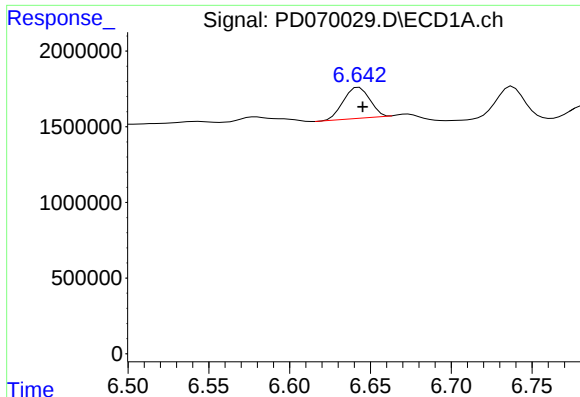

#19 Endosulfan Sulfate


R.T.: 6.643 min
Delta R.T.: -0.002 min
Response: 2329671
Conc: 2.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

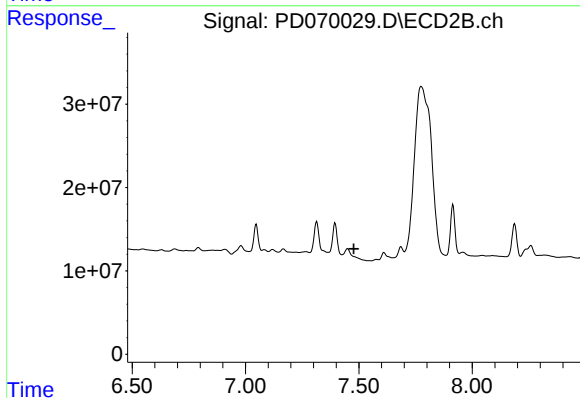


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

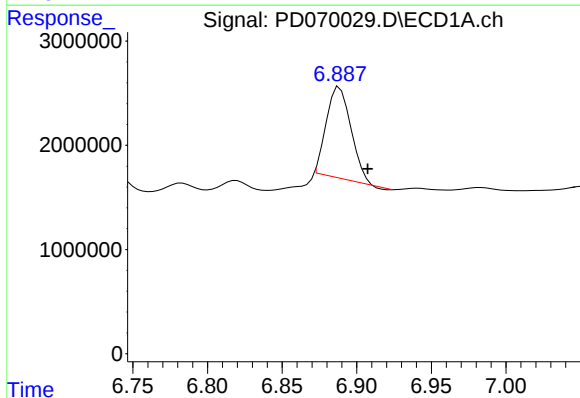


#20 Methoxychlor

R.T.: 6.888 min
Delta R.T.: -0.019 min
Response: 10001605
Conc: 17.63 ng/ml

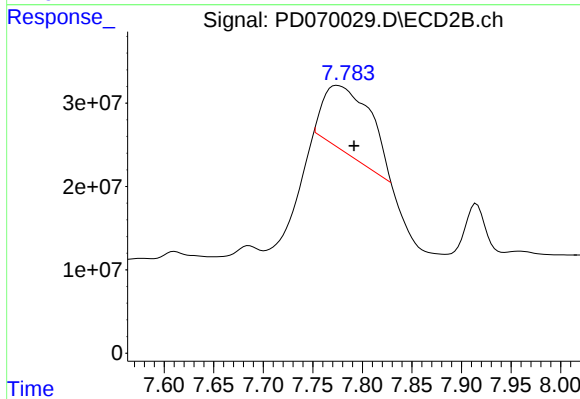

#20 Methoxychlor


R.T.: 7.775 min
Delta R.T.: -0.017 min
Response: 259700818
Conc: 72.83 ng/ml

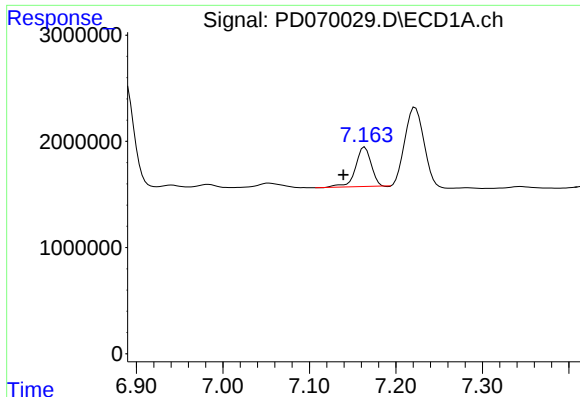

#21 Endrin ketone


R.T.: 7.164 min
Delta R.T.: 0.025 min
Response: 4639210
Conc: 3.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

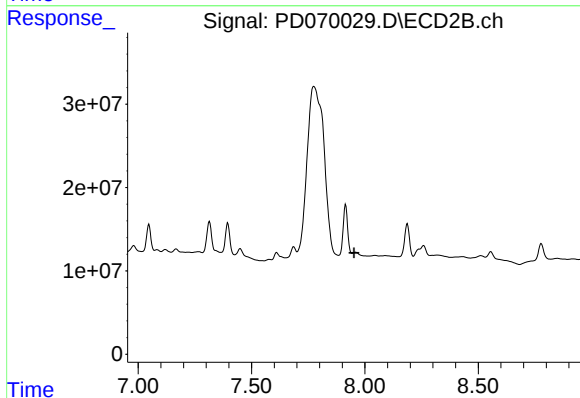


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

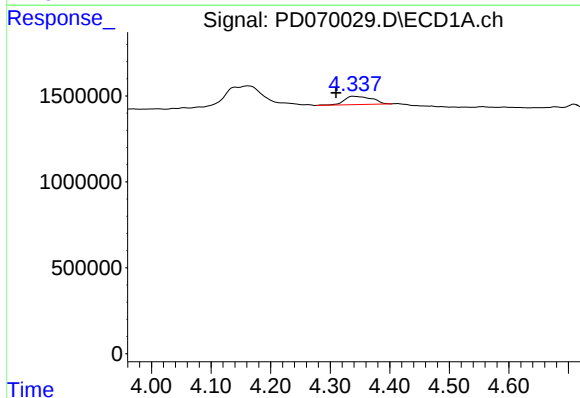


#23 Chlordane-1

R.T.: 4.339 min
Delta R.T.: 0.029 min
Response: 1553649
Conc: 39.67 ng/ml

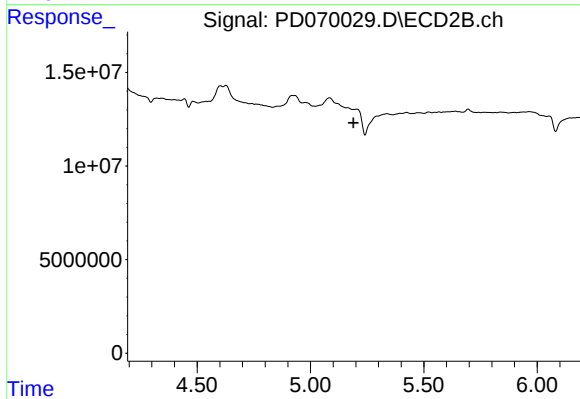

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

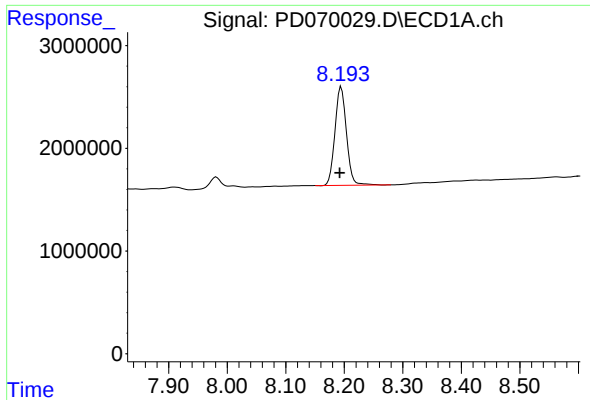

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.003 min
Response: 13100207
Conc: 12.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

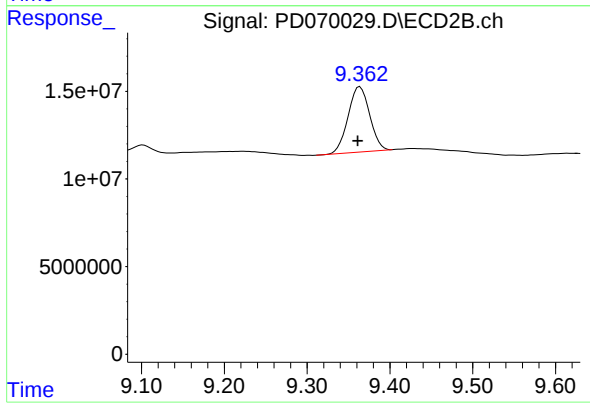

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.002 min
Response: 67494900
Conc: 12.48 ng/ml