

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
 Data File : PD070037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 19:28
 Operator : AR\AJ
 Sample : N2990-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:41:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	19790945	192.5E6	18.597	21.846
28)	SA Decachlor...	8.194	9.364	18288658	101.5E6	16.767	18.762
Target Compounds							
3)	MA gamma-BHC...	4.169	0.000	1563687	0	0.906	N.D. #
17)	MA 4,4'-DDT	6.353	7.313f	1687146	13925866	1.702	1.903
19)	B Endosulfa...	6.643	0.000	532135	0	0.462	N.D. #
20)	A Methoxychlor	6.887f	0.000	2456500	0	4.330	N.D. #
21)	B Endrin ke...	7.163f	0.000	741732	0	0.557	N.D. #
23)	Chlordane-1	4.338f	0.000	1725280	0	44.050	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
Data File : PD070037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 19:28
Operator : AR\AJ
Sample : N2990-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:41:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

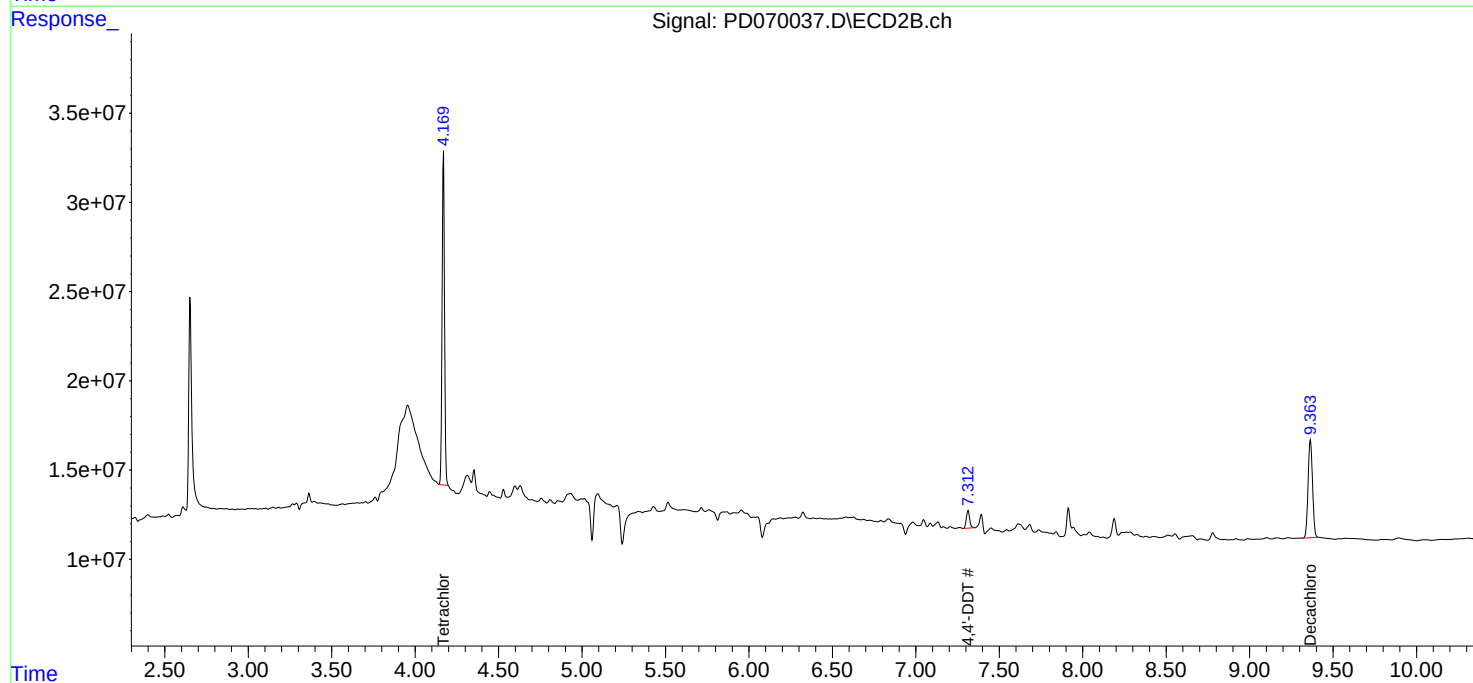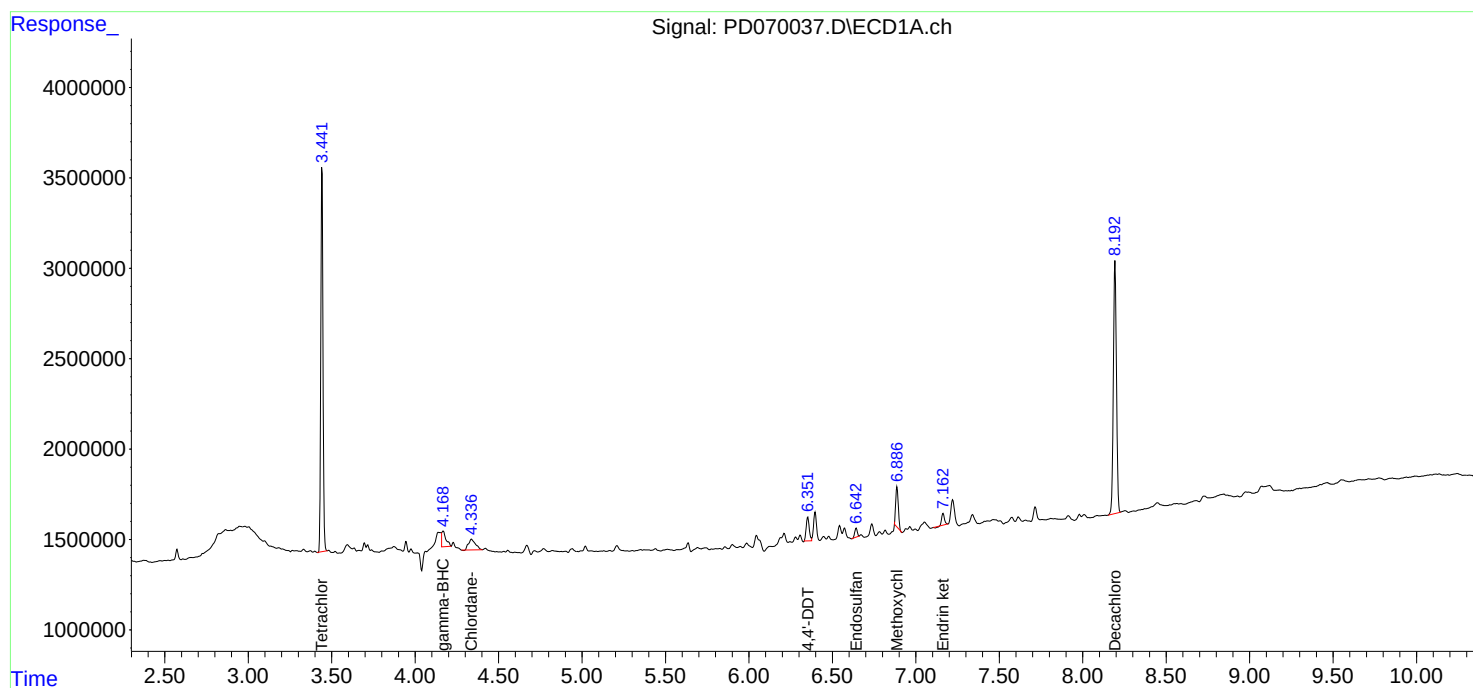


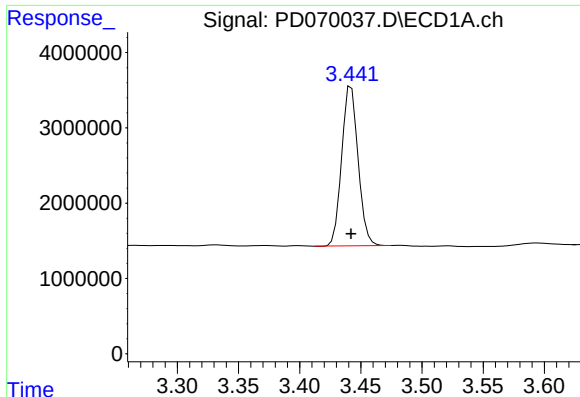

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 19790945
Conc: 18.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

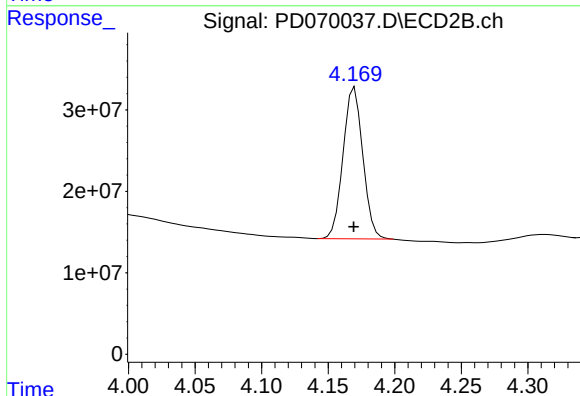


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 192499890
Conc: 21.85 ng/ml

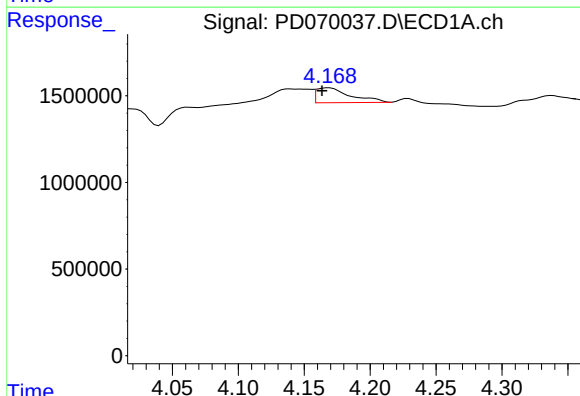


#3 gamma-BHC (Lindane)

R.T.: 4.169 min
Delta R.T.: 0.005 min
Response: 1563687
Conc: 0.91 ng/ml

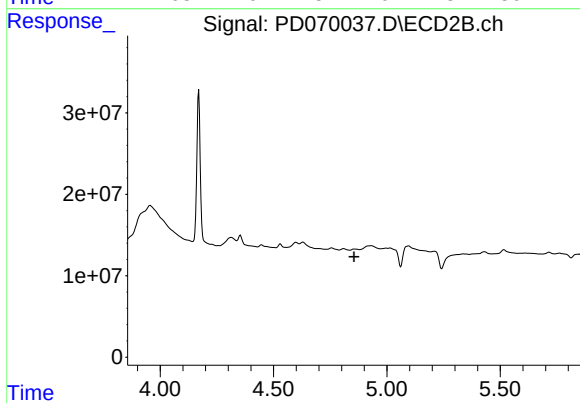

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

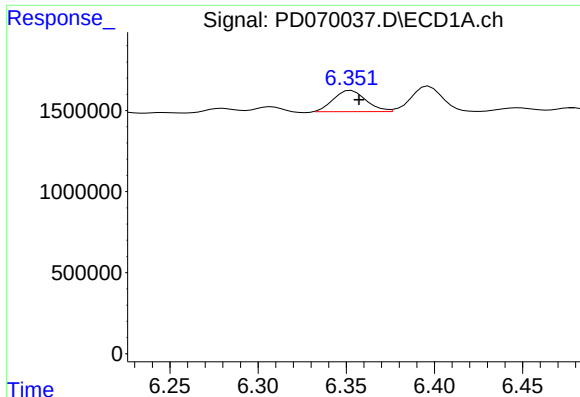

#17 4,4'-DDT


R.T.: 6.353 min
Delta R.T.: -0.005 min
Response: 1687146
Conc: 1.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

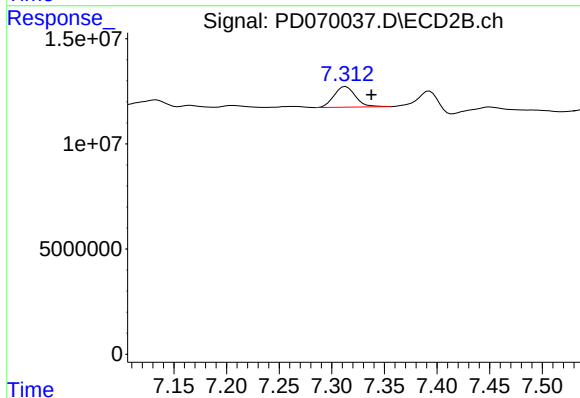


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: -0.024 min
Response: 13925866
Conc: 1.90 ng/ml

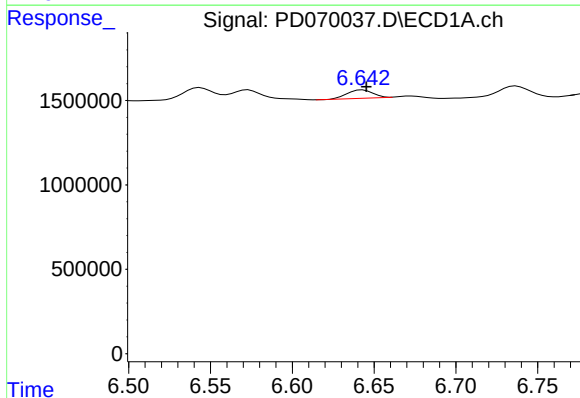


#19 Endosulfan Sulfate

R.T.: 6.643 min
Delta R.T.: -0.002 min
Response: 532135
Conc: 0.46 ng/ml

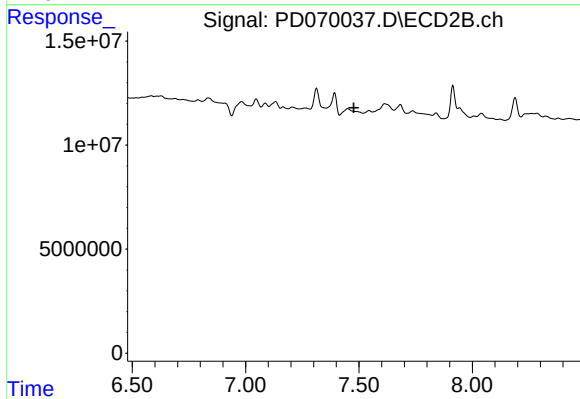

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.478 min
Response: 0
Conc: N.D.

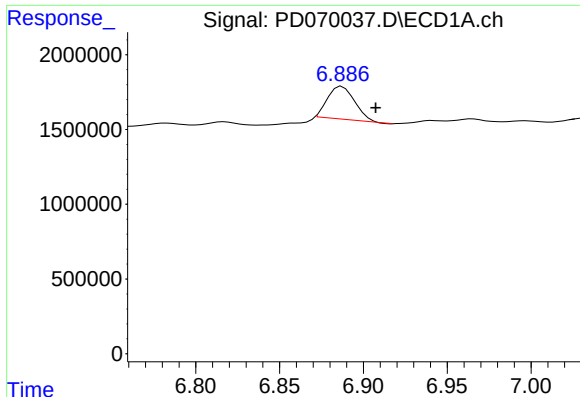

#20 Methoxychlor


R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 2456500
Conc: 4.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

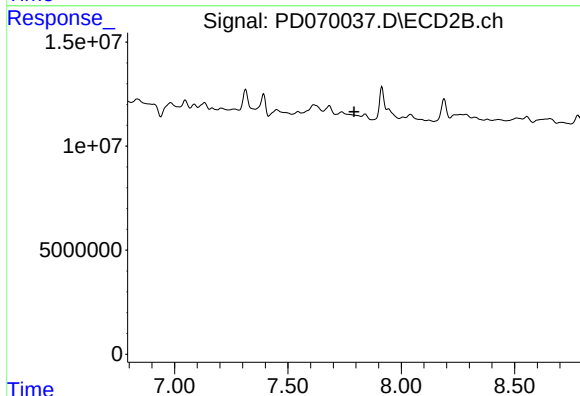


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

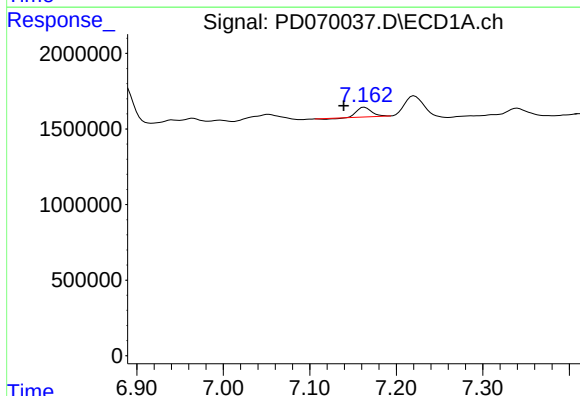


#21 Endrin ketone

R.T.: 7.163 min
Delta R.T.: 0.024 min
Response: 741732
Conc: 0.56 ng/ml

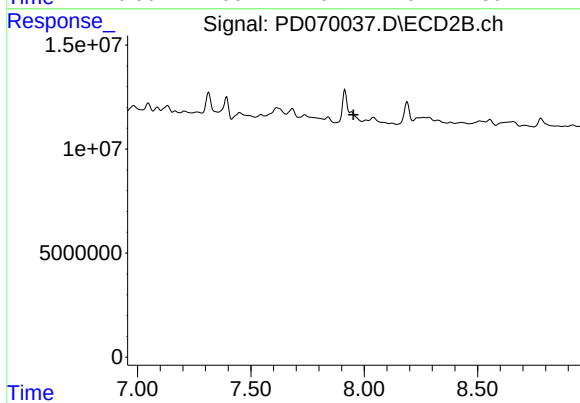

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

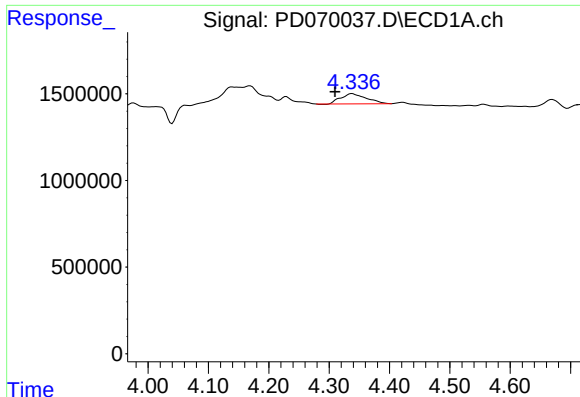

#23 Chlordane-1


R.T.: 4.338 min
Delta R.T.: 0.028 min
Response: 1725280
Conc: 44.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

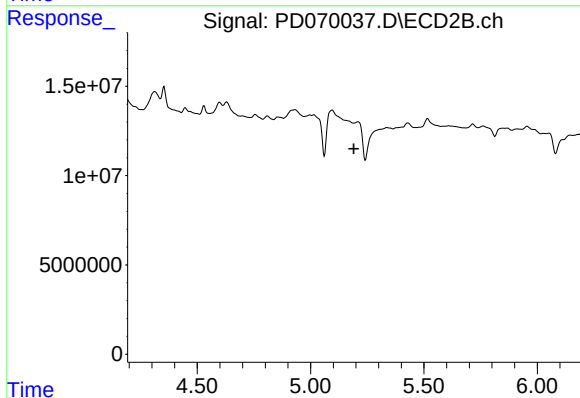


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

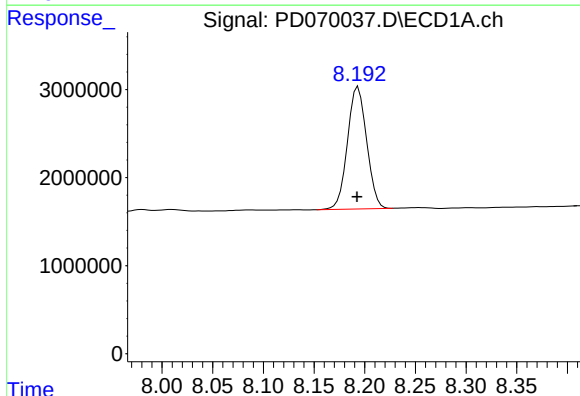

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.001 min
Response: 18288658
Conc: 16.77 ng/ml

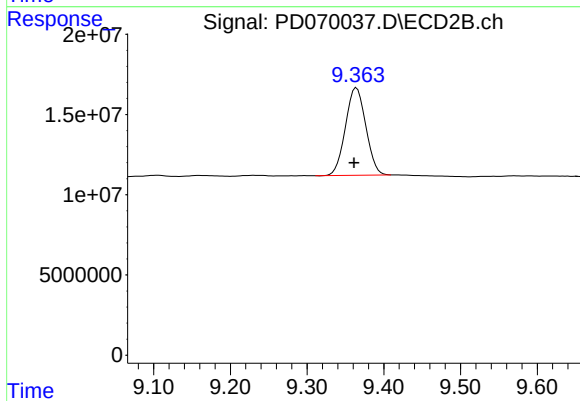

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.003 min
Response: 101465124
Conc: 18.76 ng/ml