

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
 Data File : PD070038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 19:42
 Operator : AR\AJ
 Sample : N2990-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:42:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	8992372	88338500	8.450	10.025
28)	SA Decachlor...	8.195	9.365	9275549	51055812	8.504	9.441
Target Compounds							
3)	MA gamma-BHC...	4.154	0.000	3577252	0	2.073	N.D. #
14)	MA Endrin	5.987	0.000	1139837	0	0.987	N.D. #
16)	A 4,4'-DDD	0.000	7.048	0	37983516	N.D.	5.129 #
17)	MA 4,4'-DDT	6.354	7.315f	8120713	70715077	8.194	9.663
18)	B Endrin al...	6.448	0.000	1534555	0	1.786	N.D. #
19)	B Endosulfa...	6.642	0.000	3054712	0	2.650	N.D. #
20)	A Methoxychlor	6.888f	0.000	14647843	0	25.820	N.D. #
21)	B Endrin ke...	7.164f	0.000	6689689	0	5.020	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
Data File : PD070038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 19:42
Operator : AR\AJ
Sample : N2990-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:42:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

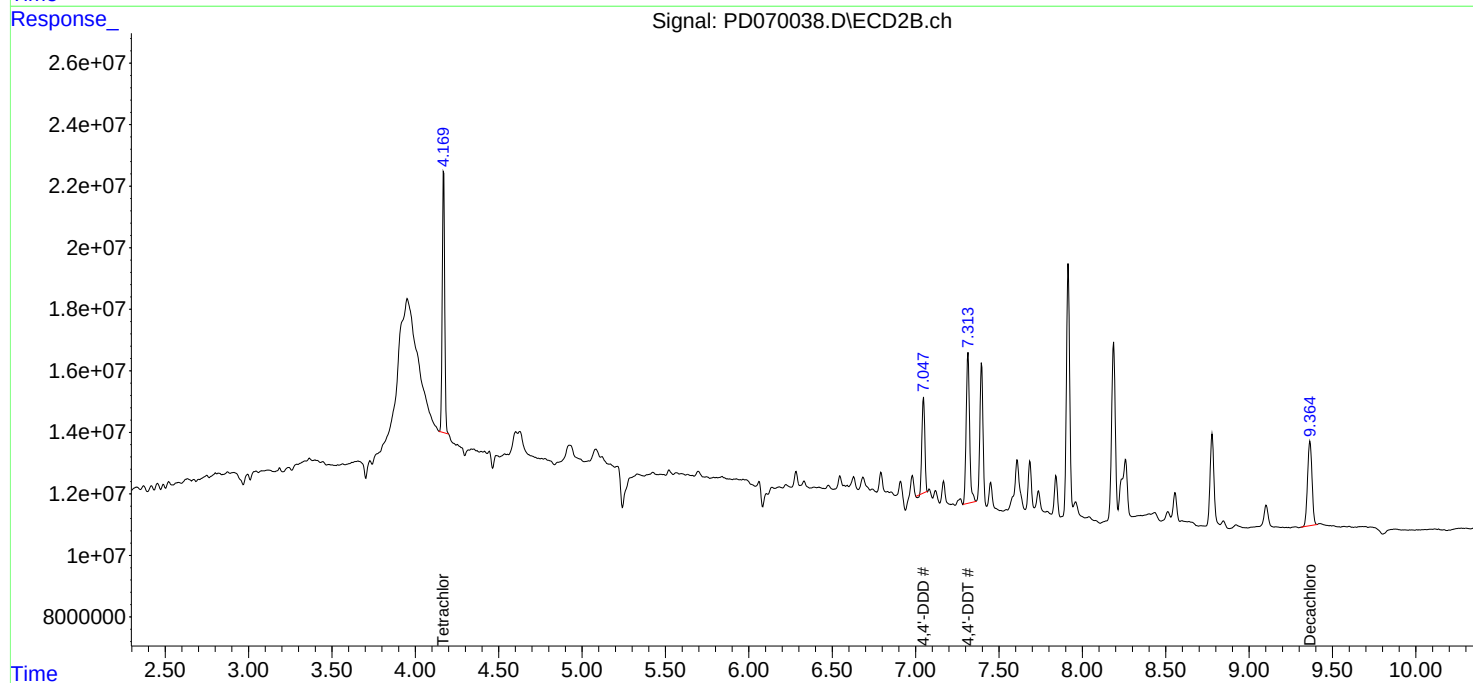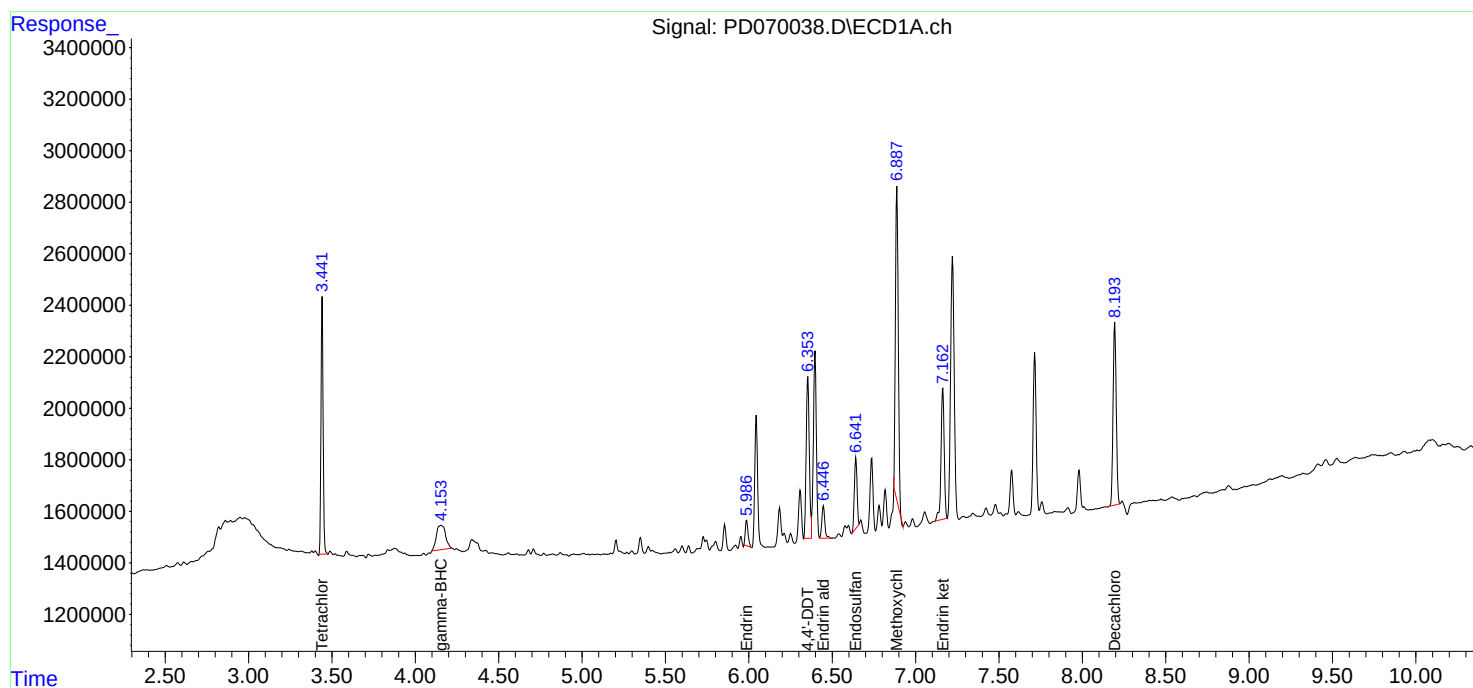


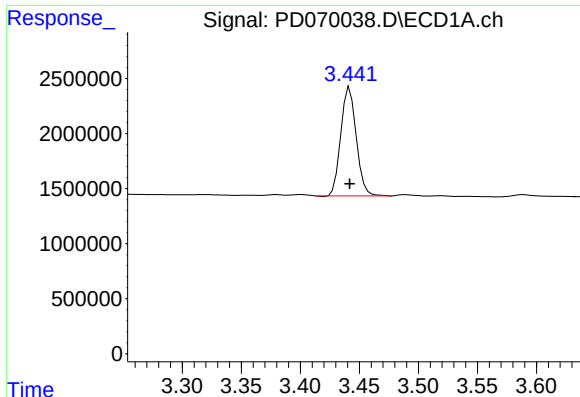

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 8992372
Conc: 8.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

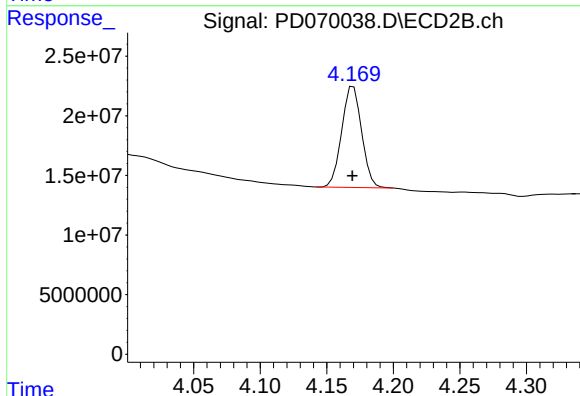


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 88338500
Conc: 10.03 ng/ml

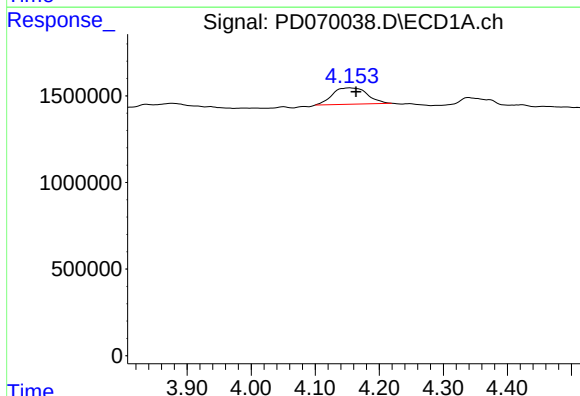


#3 gamma-BHC (Lindane)

R.T.: 4.154 min
Delta R.T.: -0.009 min
Response: 3577252
Conc: 2.07 ng/ml

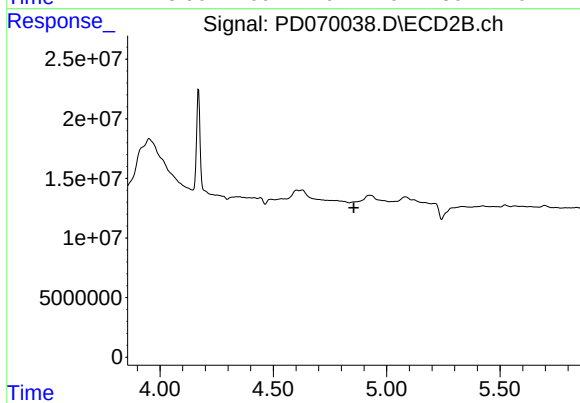

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

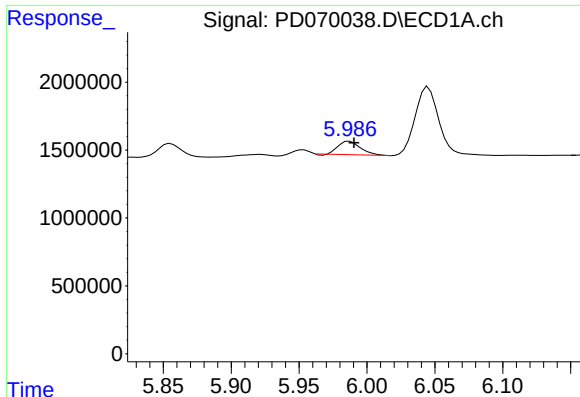

#14 Endrin


R.T.: 5.987 min
Delta R.T.: -0.003 min
Response: 1139837
Conc: 0.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

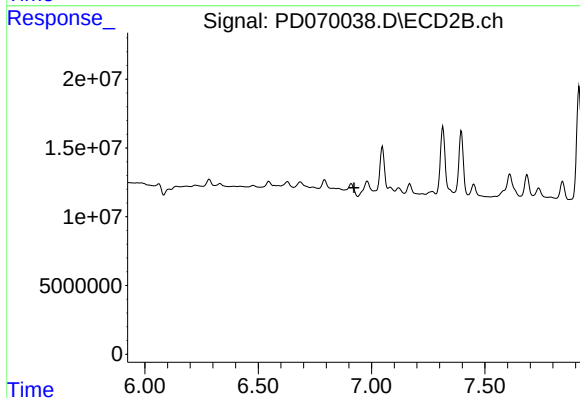


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

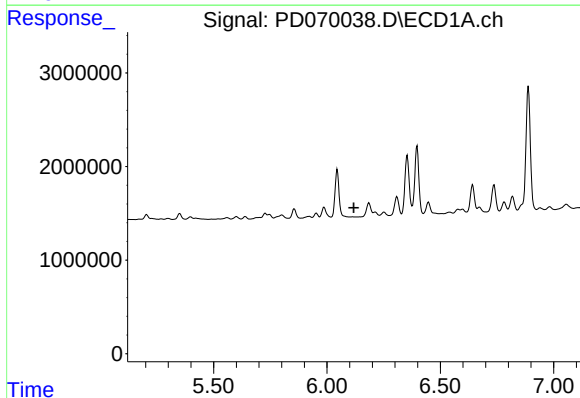


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

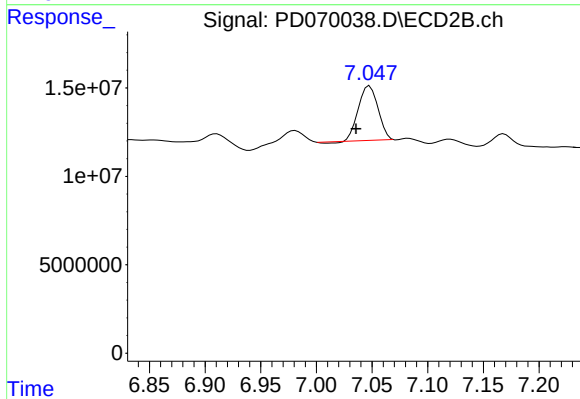

#16 4,4'-DDD


R.T.: 7.048 min
Delta R.T.: 0.012 min
Response: 37983516
Conc: 5.13 ng/ml

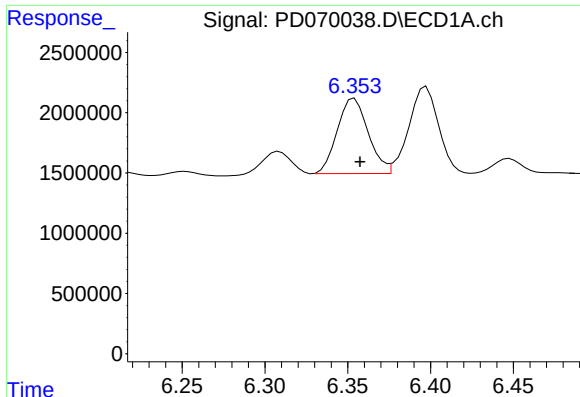

#17 4,4'-DDT


R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 8120713
Conc: 8.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

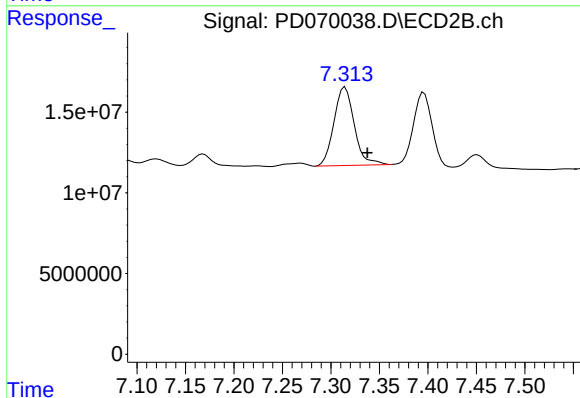


#17 4,4'-DDT

R.T.: 7.315 min
Delta R.T.: -0.023 min
Response: 70715077
Conc: 9.66 ng/ml

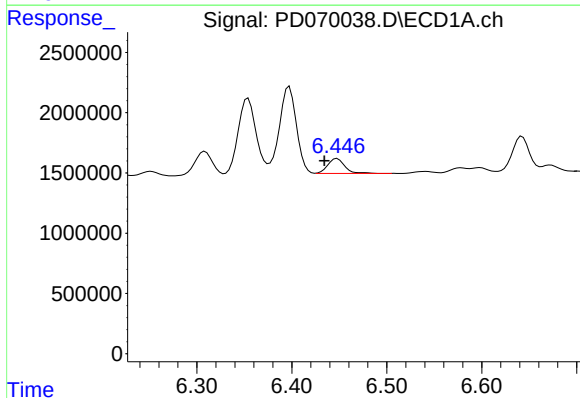


#18 Endrin aldehyde

R.T.: 6.448 min
Delta R.T.: 0.014 min
Response: 1534555
Conc: 1.79 ng/ml

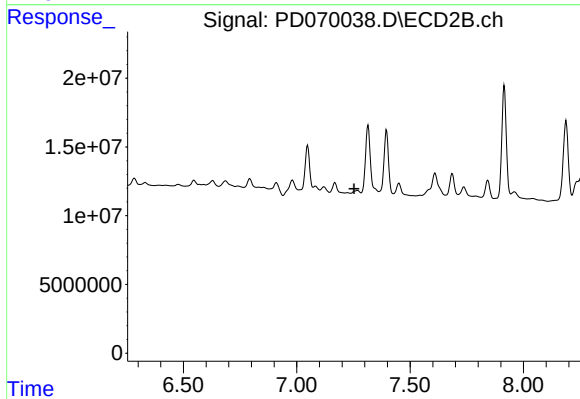

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

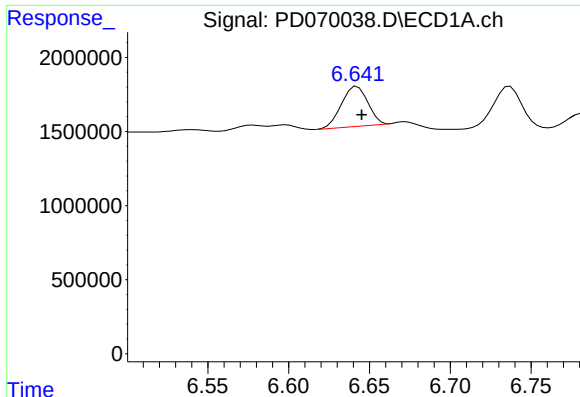

#19 Endosulfan Sulfate


R.T.: 6.642 min
Delta R.T.: -0.003 min
Response: 3054712
Conc: 2.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

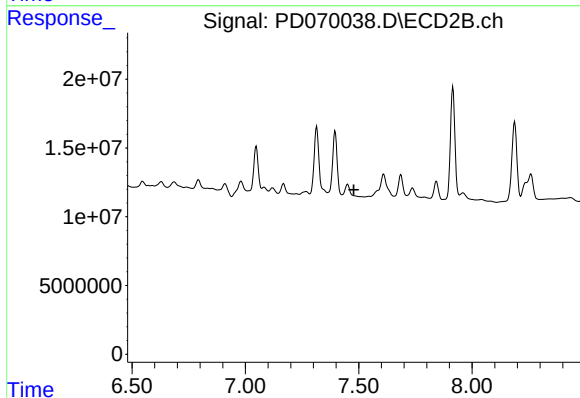


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

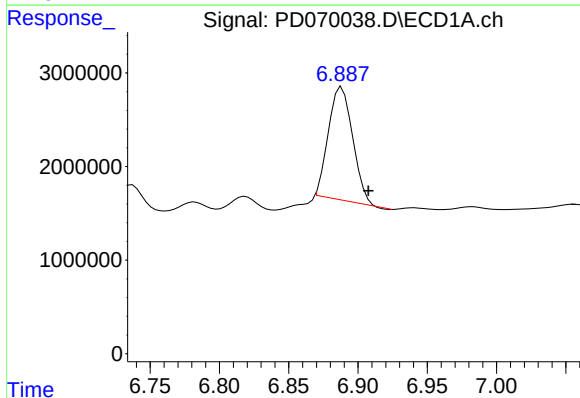


#20 Methoxychlor

R.T.: 6.888 min
Delta R.T.: -0.019 min
Response: 14647843
Conc: 25.82 ng/ml

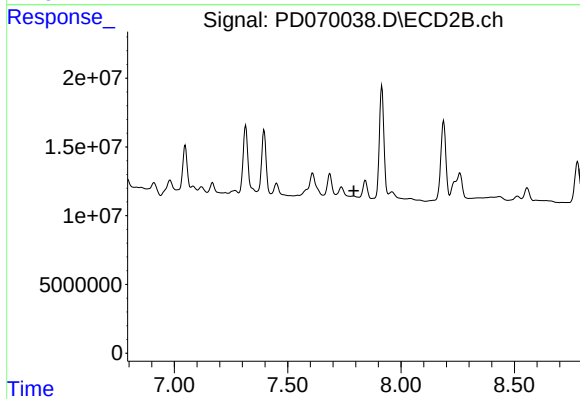

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

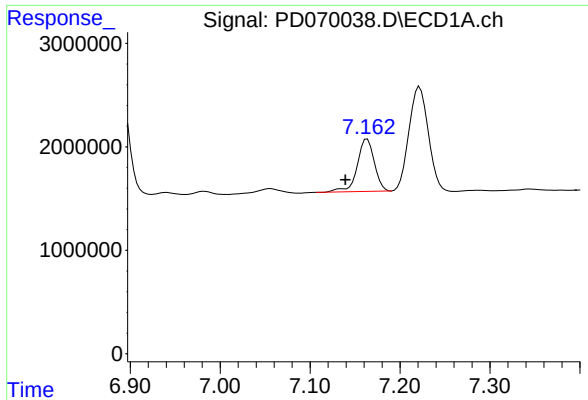

#21 Endrin ketone


R.T.: 7.164 min
Delta R.T.: 0.024 min
Response: 6689689
Conc: 5.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

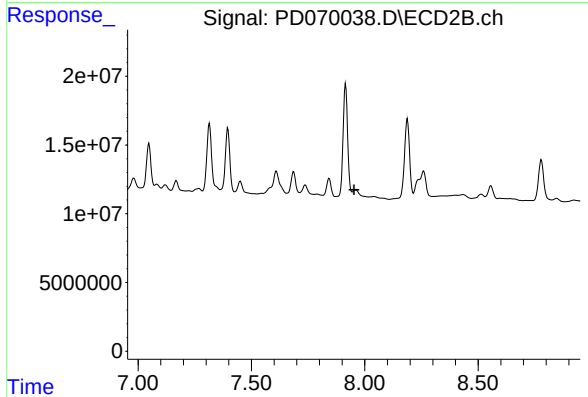


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

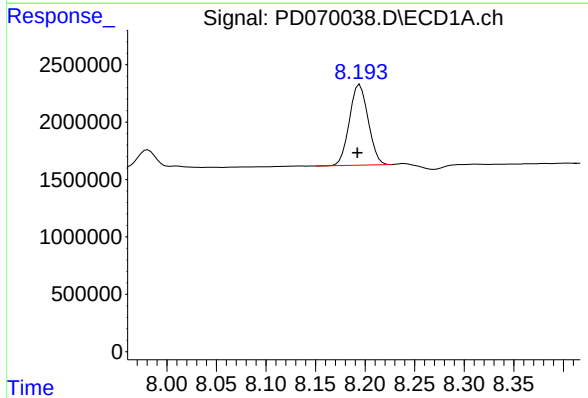

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.002 min
Response: 9275549
Conc: 8.50 ng/ml

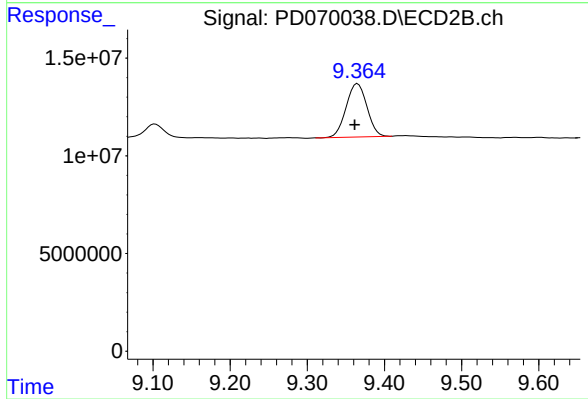

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.004 min
Response: 51055812
Conc: 9.44 ng/ml