

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
 Data File : PD070014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 13:02
 Operator : AR\AJ
 Sample : N2894-19RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P008-SS003-0006-01RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:33:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	21804706	211.9E6	20.489	24.047
28)	SA Decachlor...	8.195	9.363	33485377	194.9E6	30.700	36.042
Target Compounds							
12)	B 4,4'-DDE	5.601	6.545	1617505	14950690	1.277	1.652 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060422\
Data File : PD070014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 13:02
Operator : AR\AJ
Sample : N2894-19RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
P008-SS003-0006-01RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:33:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

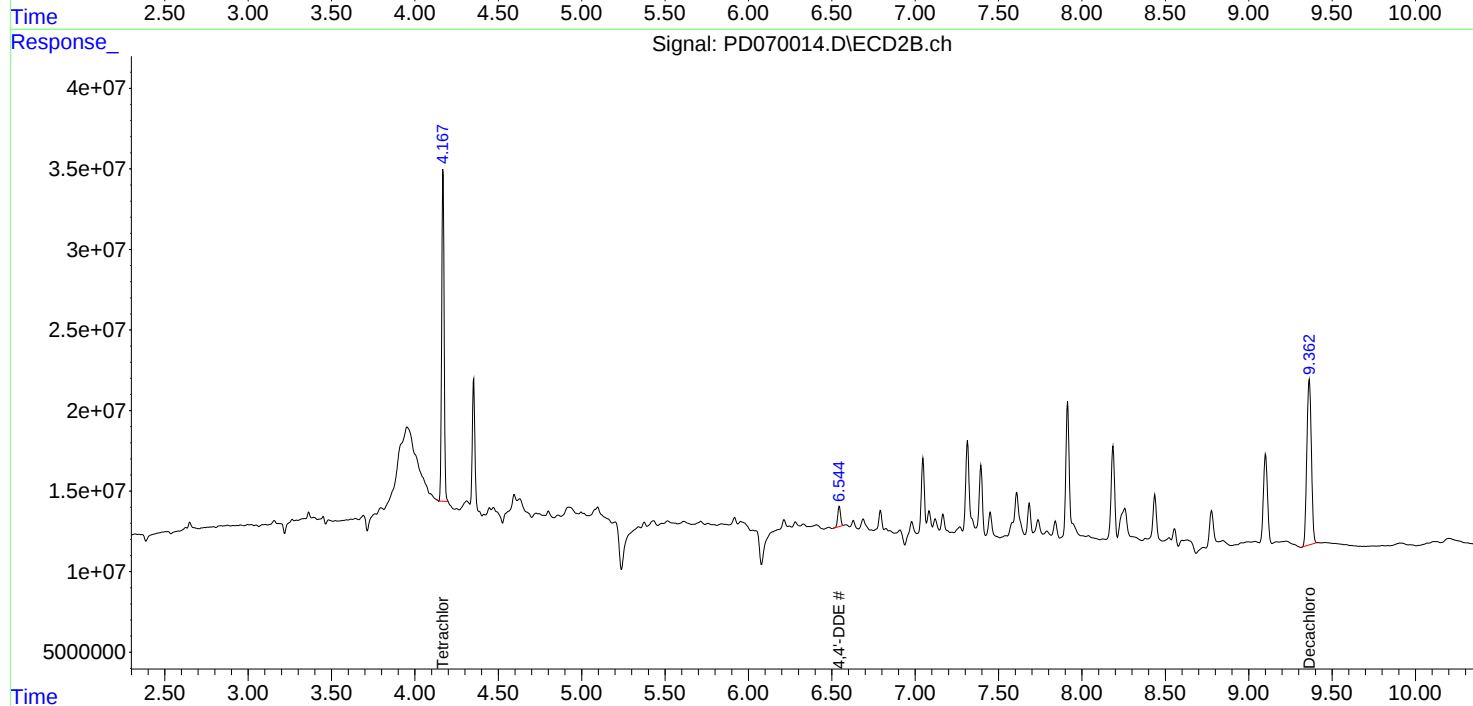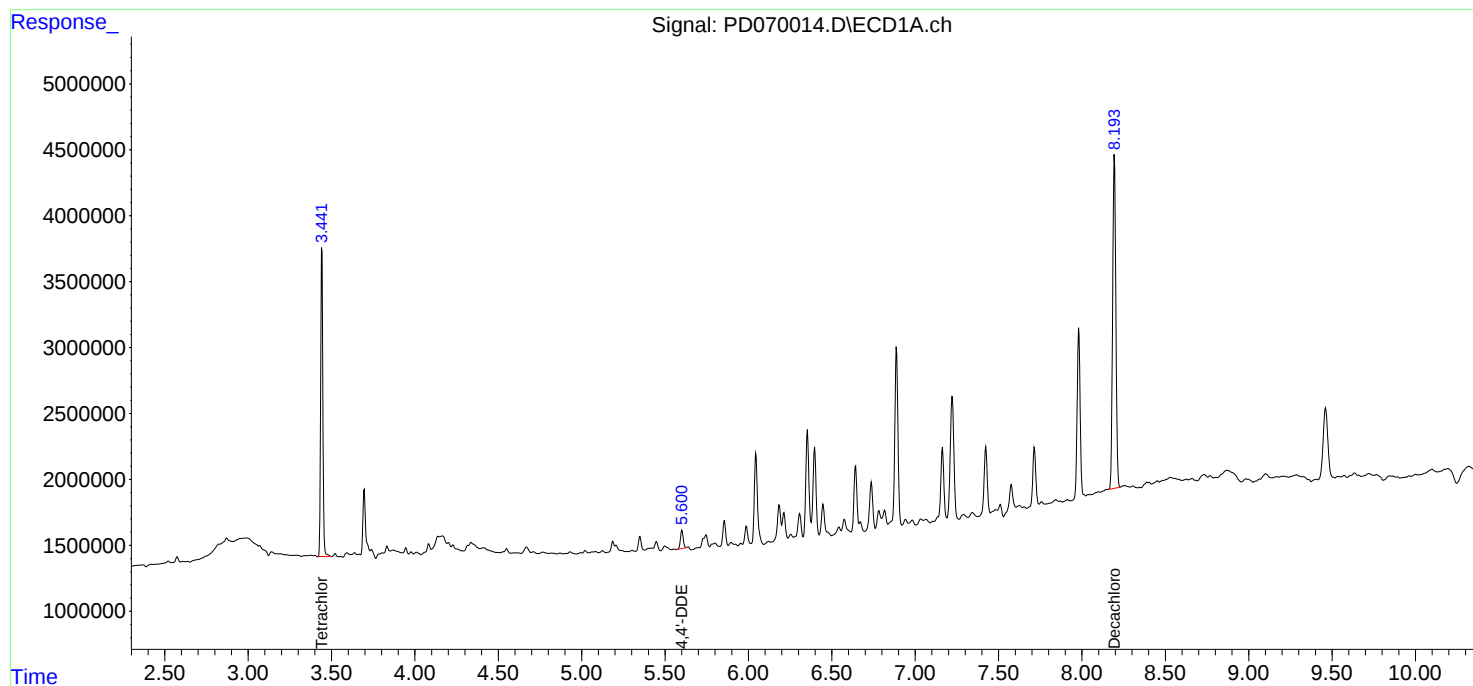


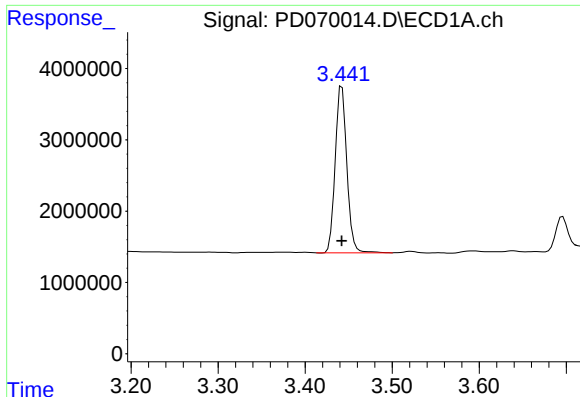

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 21804706
Conc: 20.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS003-0006-01RE

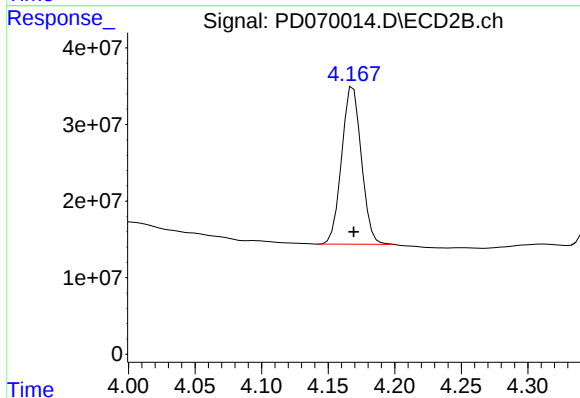


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 211895551
Conc: 24.05 ng/ml

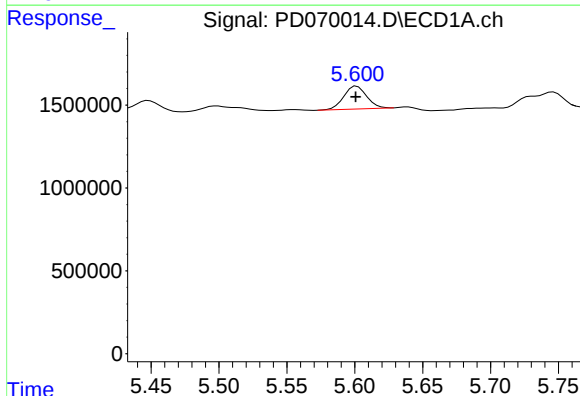


#12 4,4'-DDE

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 1617505
Conc: 1.28 ng/ml

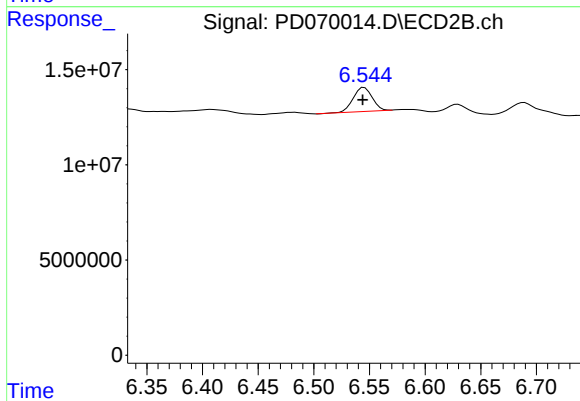

#12 4,4'-DDE


R.T.: 6.545 min
Delta R.T.: 0.001 min
Response: 14950690
Conc: 1.65 ng/ml

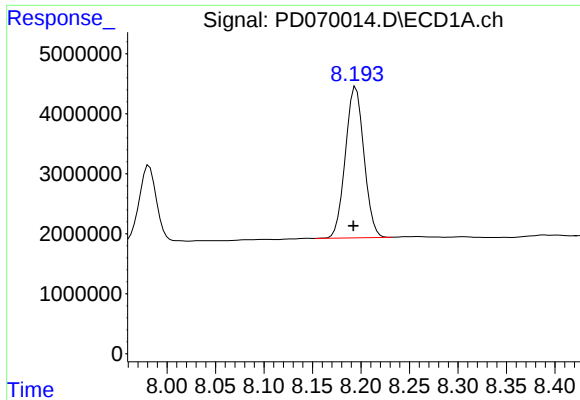

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.002 min
Response: 33485377
Conc: 30.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS003-0006-01RE

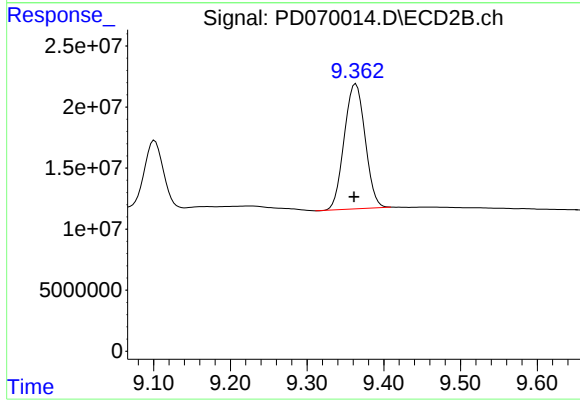

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.002 min
Response: 194921455
Conc: 36.04 ng/ml