

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 22:03
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:37:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 06:36:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.772	7197700	23900008	5.020	5.022
27)	SA Decachlor...	9.118	7.900	21499598	51767789	10.579	10.359
Target Compounds							
2)	A alpha-BHC	4.020	3.272	11496657	33696115	4.620	4.605
3)	MA gamma-BHC...	4.354	3.600	11430165	33099715	4.762	4.871
4)	MA Heptachlor	4.946	3.939	12113717	32949294	4.881	4.868
9)	A Endosulfan I	6.105	5.088	10328682	26997940	4.882	4.941
13)	MA Dieldrin	6.381	5.352	21470045	59060086	9.638	9.627
14)	MA Endrin	6.612	5.628	17838170	52407778	9.770	9.659
16)	A 4,4'-DDD	6.745	5.775	15063570	44337248	9.609	9.502
17)	MA 4,4'-DDT	7.060	6.026	15015557	41988312	9.395	8.830
20)	A Methoxychlor	7.537	6.601	46633677	131.2E6	51.384	52.371


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 22:03
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:37:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 06:36:45 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

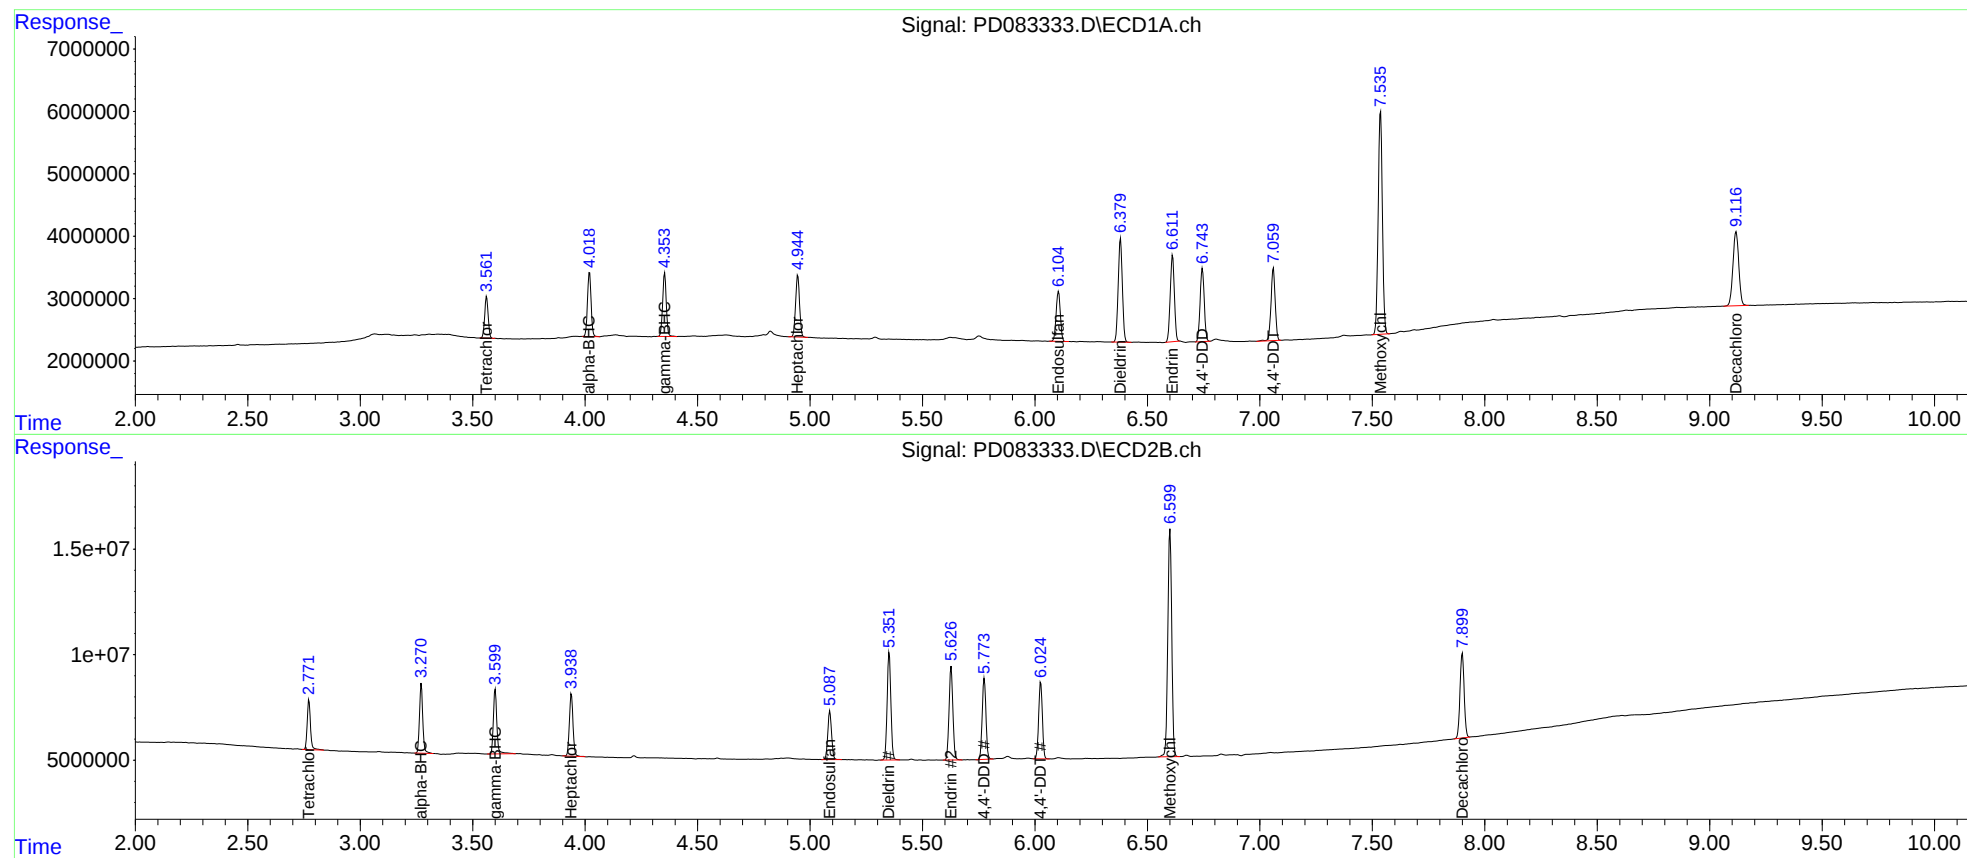

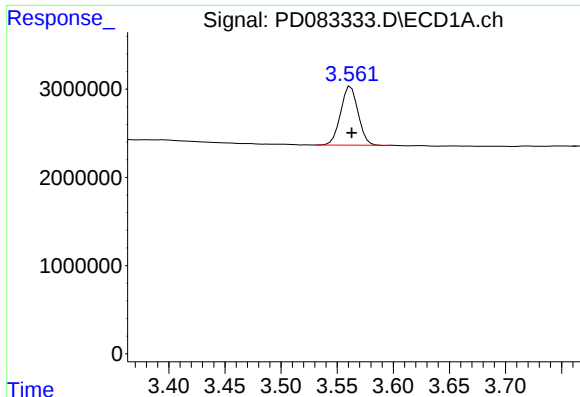


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 7197700
Conc: 5.02 ng/ml

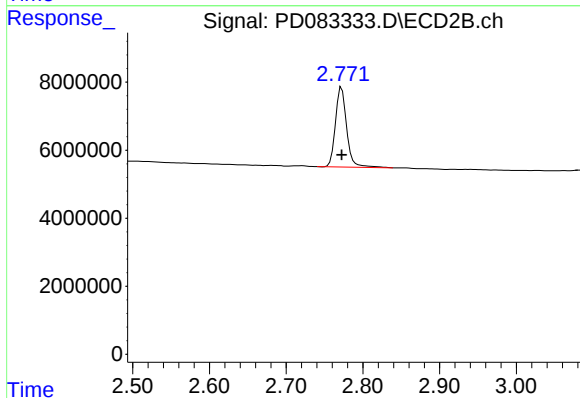


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 23900008
Conc: 5.02 ng/ml

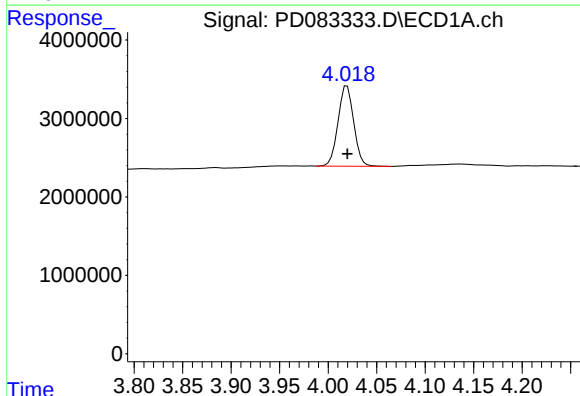


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 11496657
Conc: 4.62 ng/ml

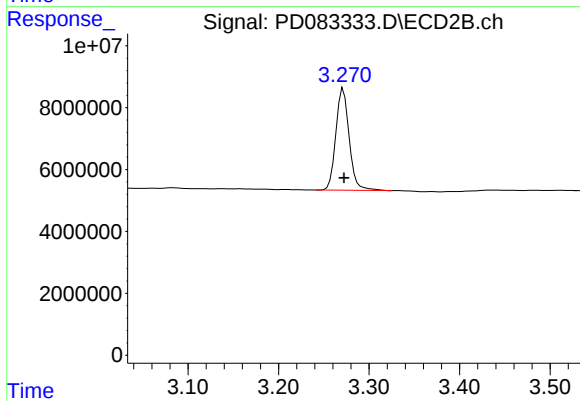


#2 alpha-BHC

R.T.: 3.272 min
Delta R.T.: 0.000 min
Response: 33696115
Conc: 4.60 ng/ml

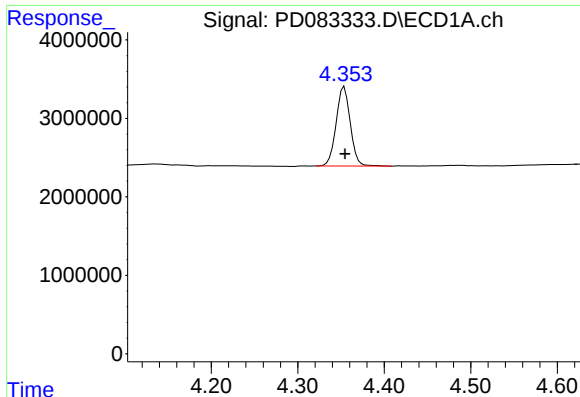


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 11430165
Conc: 4.76 ng/ml

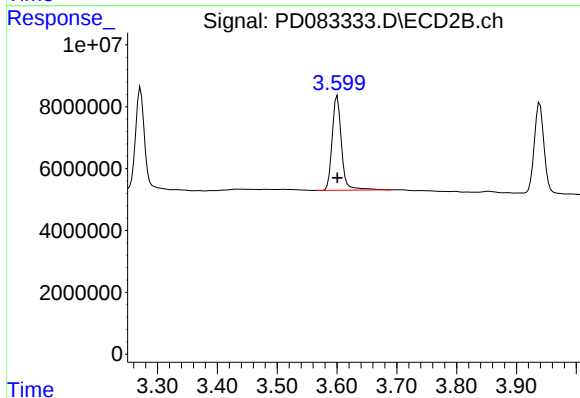


#3 gamma-BHC (Lindane)

R.T.: 3.600 min
Delta R.T.: 0.000 min
Response: 33099715
Conc: 4.87 ng/ml

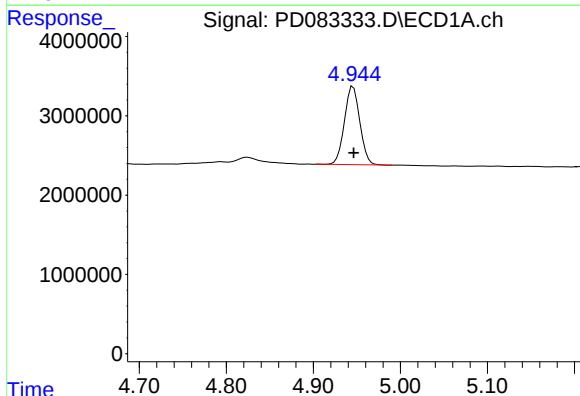


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 12113717
Conc: 4.88 ng/ml

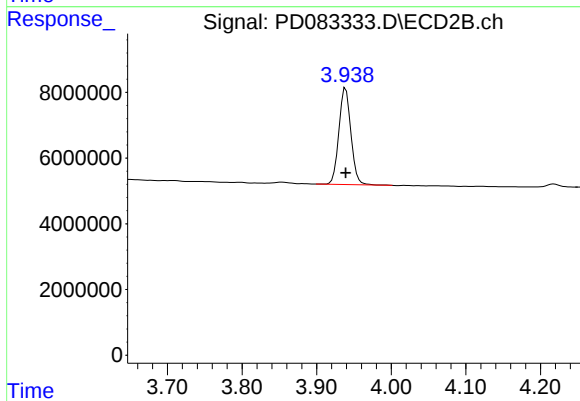


#4 Heptachlor

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 32949294
Conc: 4.87 ng/ml

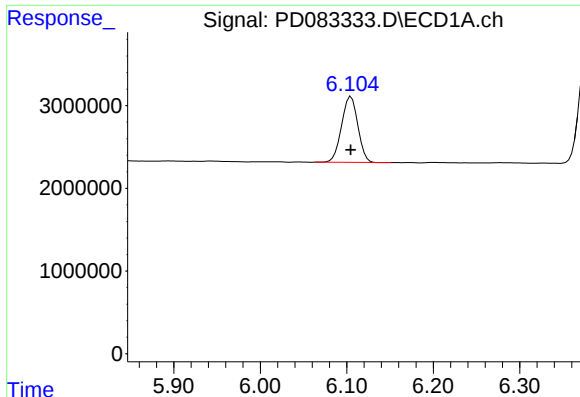


#9 Endosulfan I

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 10328682
Conc: 4.88 ng/ml

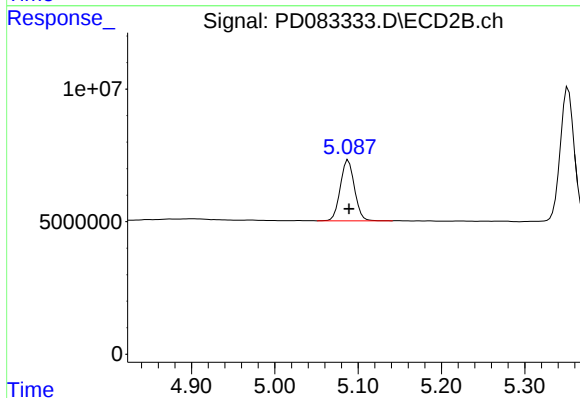


#9 Endosulfan I

R.T.: 5.088 min
Delta R.T.: 0.000 min
Response: 26997940
Conc: 4.94 ng/ml

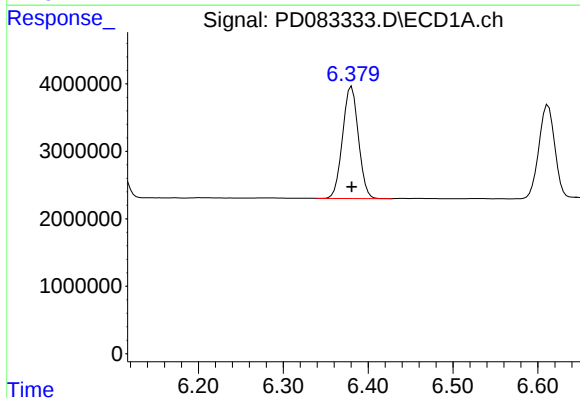


#13 Dieldrin

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 21470045
Conc: 9.64 ng/ml

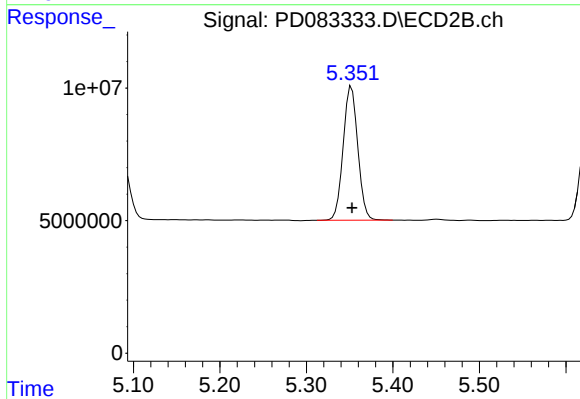


#13 Dieldrin

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 59060086
Conc: 9.63 ng/ml

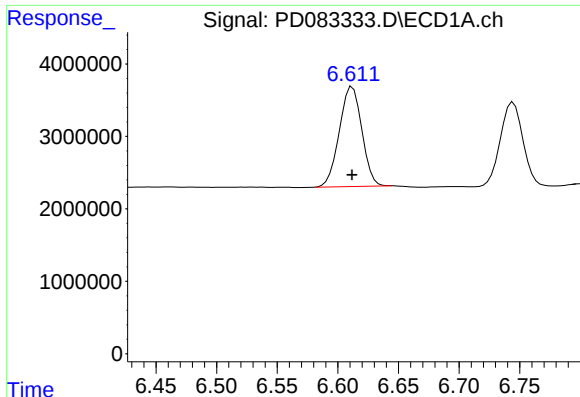


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 17838170
Conc: 9.77 ng/ml

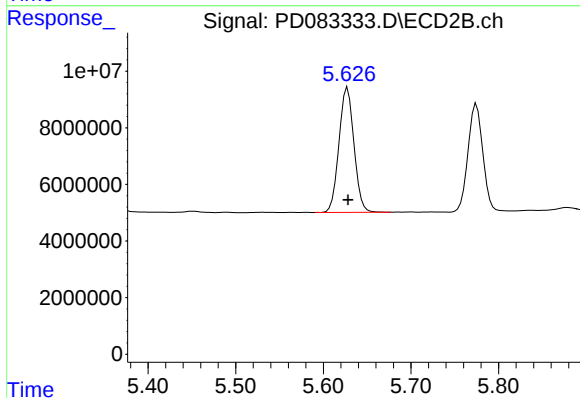


#14 Endrin

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 52407778
Conc: 9.66 ng/ml

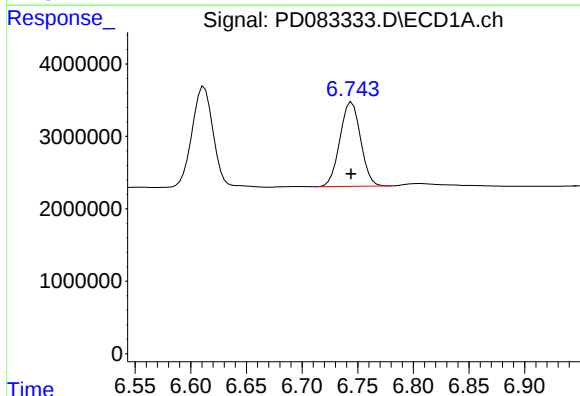


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 15063570
Conc: 9.61 ng/ml

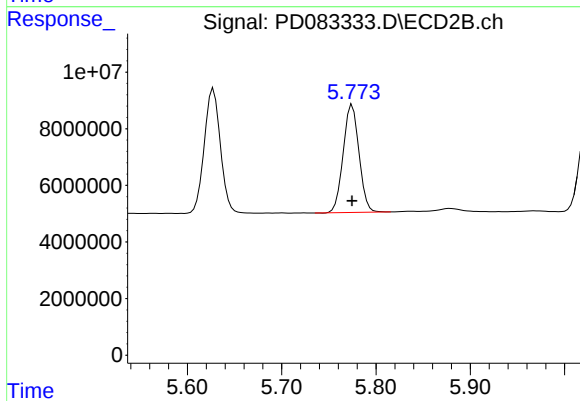


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 44337248
Conc: 9.50 ng/ml

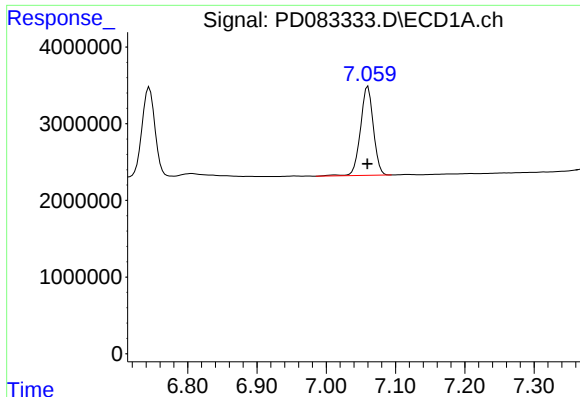


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 15015557
Conc: 9.40 ng/ml

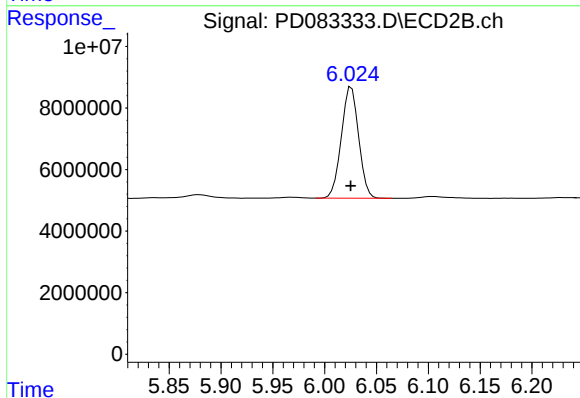


#17 4,4'-DDT

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 41988312
Conc: 8.83 ng/ml

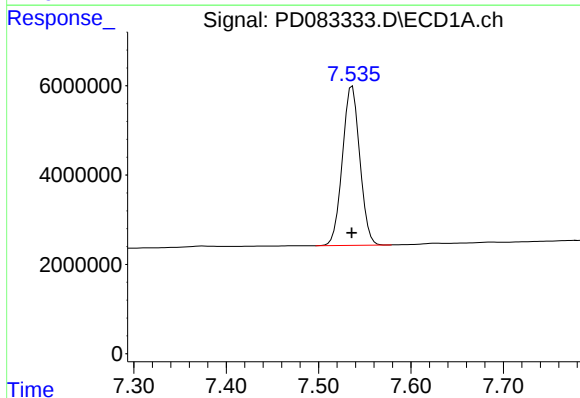


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 46633677
Conc: 51.38 ng/ml

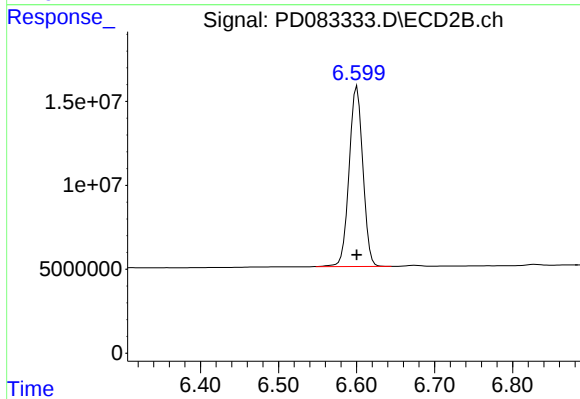


#20 Methoxychlor

R.T.: 6.601 min
Delta R.T.: 0.000 min
Response: 131232357
Conc: 52.37 ng/ml

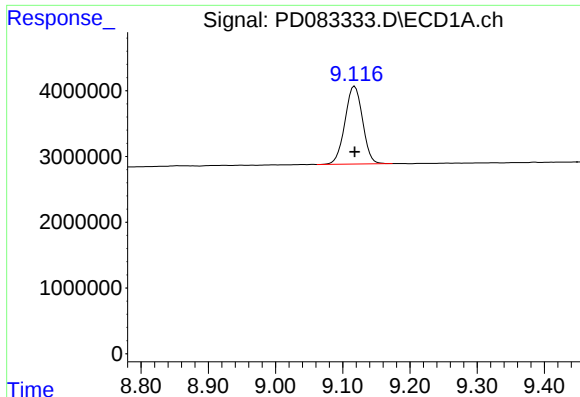

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 21499598
Conc: 10.58 ng/ml

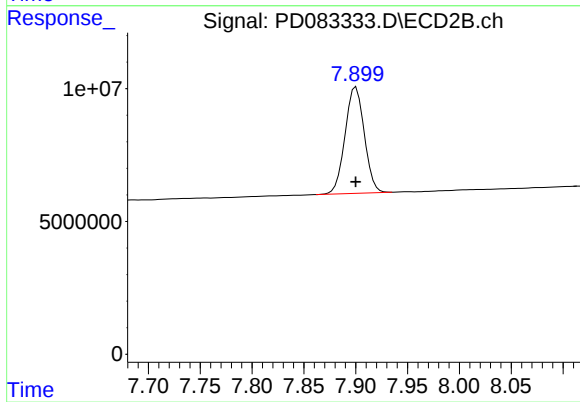

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 51767789
Conc: 10.36 ng/ml