

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 22:30
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:37:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 06:36:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.772	14608412	47998097	10.188	10.086
27)	SA Decachlor...	9.117	7.900	41996381	101.9E6	20.664	20.399
Target Compounds							
2)	A alpha-BHC	4.019	3.272	23752343	70974960	9.544	9.699
3)	MA gamma-BHC...	4.354	3.600	23214268	67229401	9.671	9.893
4)	MA Heptachlor	4.946	3.939	24491342	67328730	9.868	9.948
9)	A Endosulfan I	6.105	5.088	21314744	55018219	10.076	10.069
13)	MA Dieldrin	6.380	5.352	43540376	121.1E6	19.545	19.735
14)	MA Endrin	6.611	5.627	35878746	107.6E6	19.651	19.832
16)	A 4,4'-DDD	6.744	5.774	30580367	91998793	19.508	19.716
17)	MA 4,4'-DDT	7.060	6.025	31034578	90730275	19.418	19.080
20)	A Methoxychlor	7.536	6.600	92576101	261.4E6	102.006	104.336


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 22:30
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:37:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 06:36:45 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

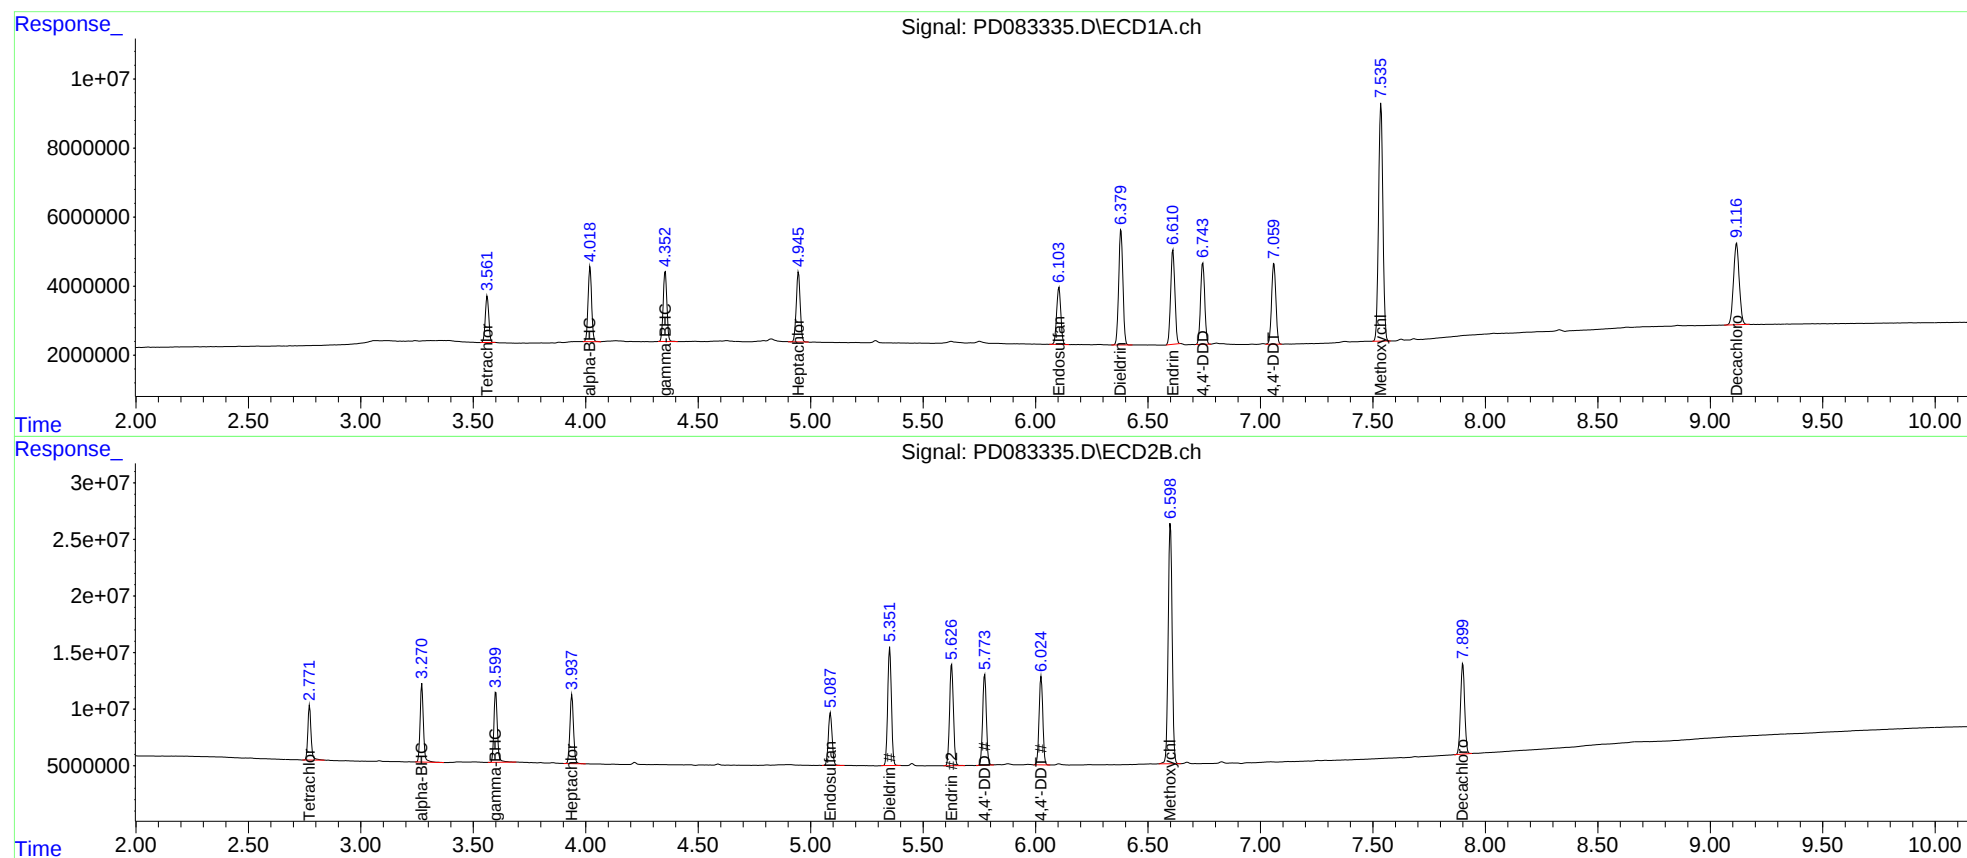

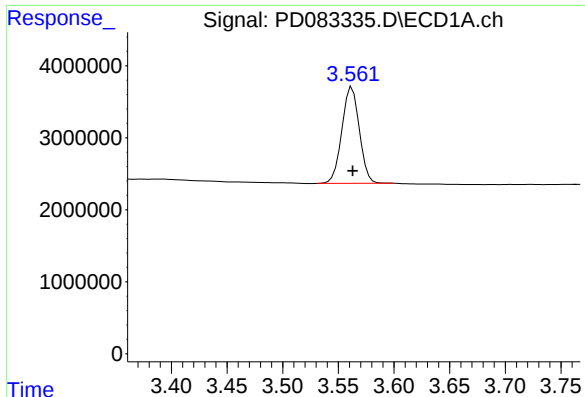


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 14608412
Conc: 10.19 ng/ml

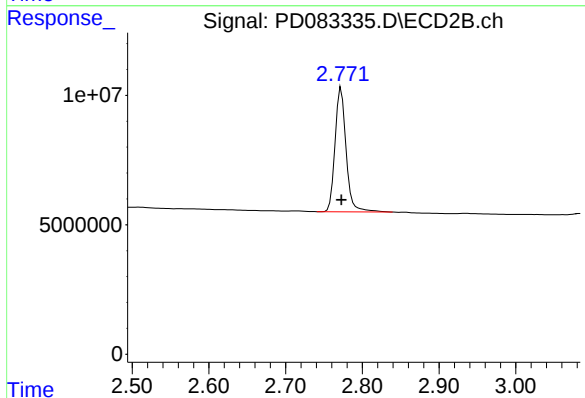


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 47998097
Conc: 10.09 ng/ml

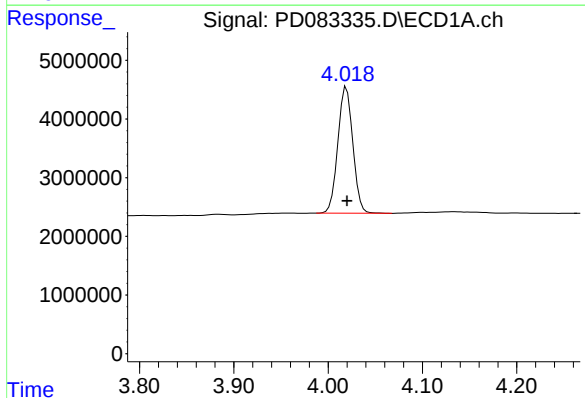


#2 alpha-BHC

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 23752343
Conc: 9.54 ng/ml

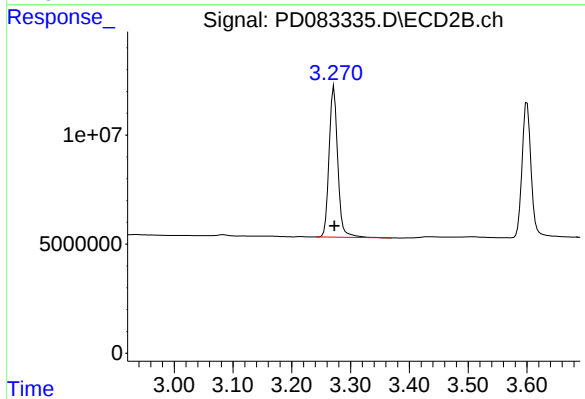


#2 alpha-BHC

R.T.: 3.272 min
Delta R.T.: 0.000 min
Response: 70974960
Conc: 9.70 ng/ml

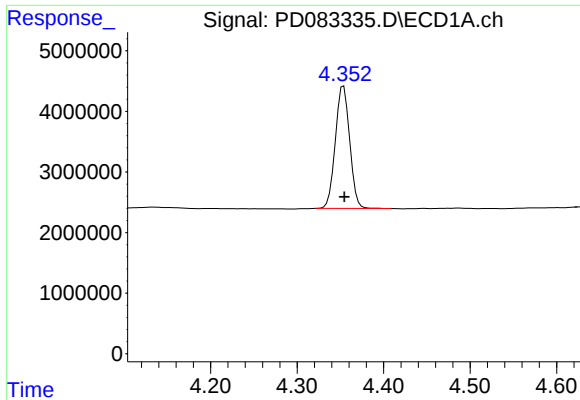


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 23214268
Conc: 9.67 ng/ml

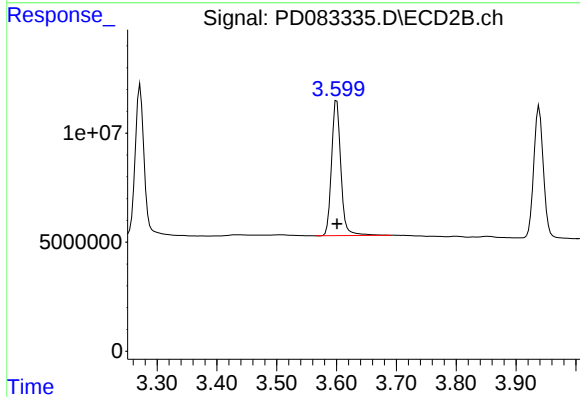


#3 gamma-BHC (Lindane)

R.T.: 3.600 min
Delta R.T.: 0.000 min
Response: 67229401
Conc: 9.89 ng/ml

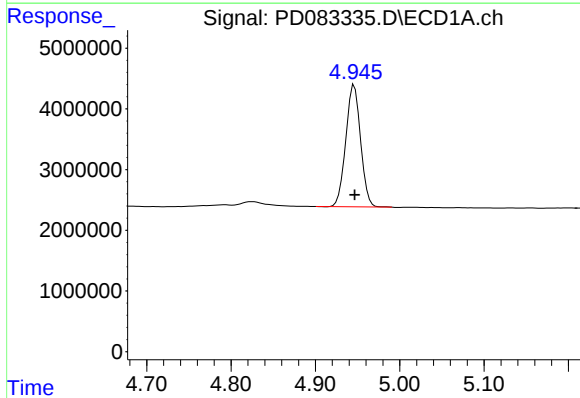


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 24491342
Conc: 9.87 ng/ml

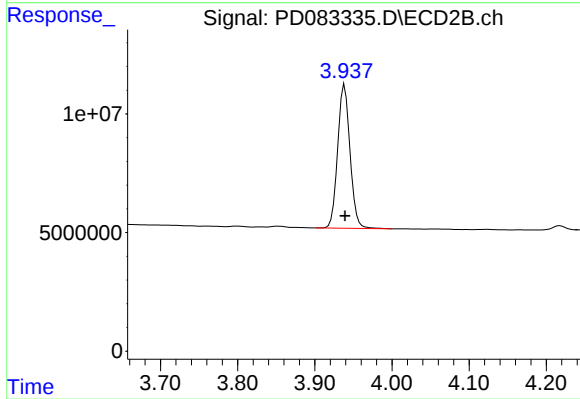


#4 Heptachlor

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 67328730
Conc: 9.95 ng/ml

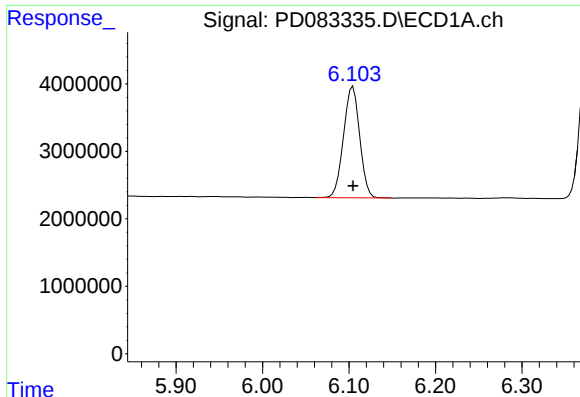


#9 Endosulfan I

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 21314744
Conc: 10.08 ng/ml

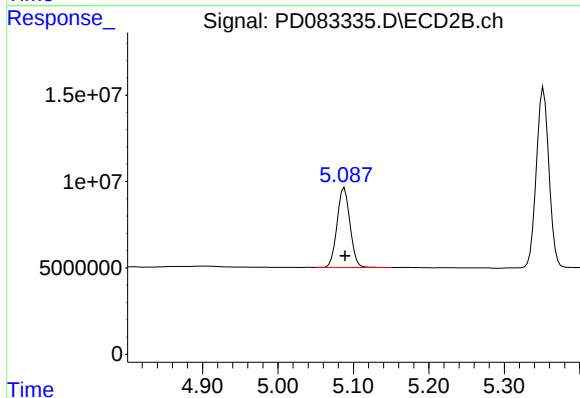


#9 Endosulfan I

R.T.: 5.088 min
Delta R.T.: 0.000 min
Response: 55018219
Conc: 10.07 ng/ml

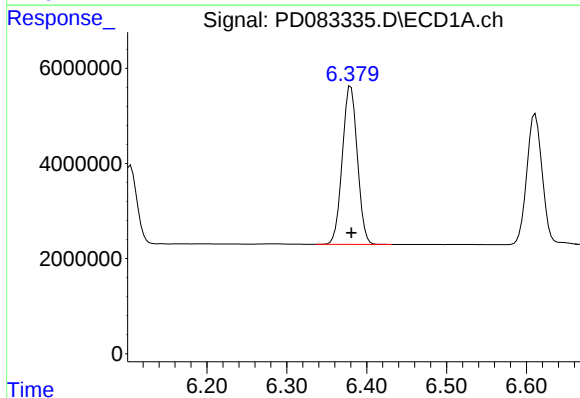


#13 Dieldrin

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 43540376
Conc: 19.54 ng/ml

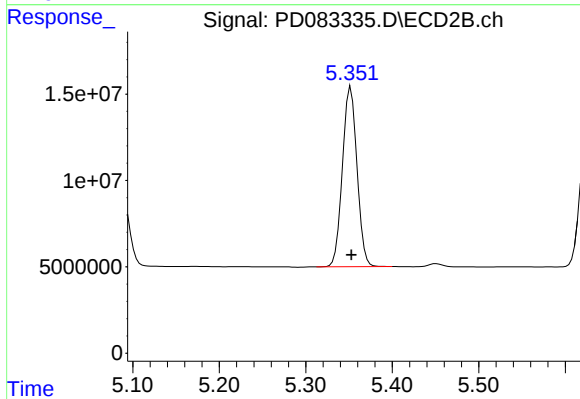


#13 Dieldrin

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 121070245
Conc: 19.74 ng/ml

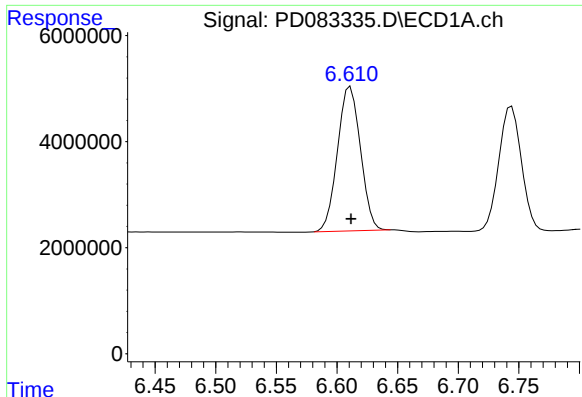


#14 Endrin

R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 35878746
Conc: 19.65 ng/ml

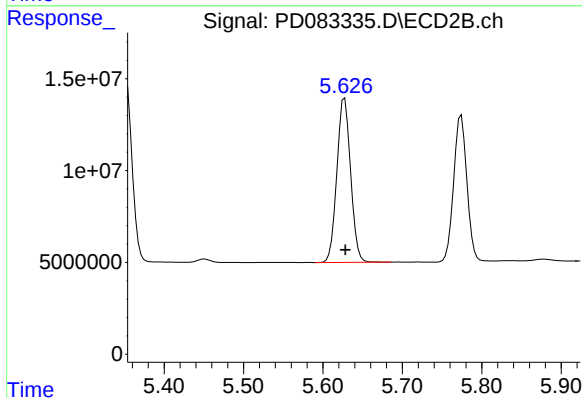


#14 Endrin

R.T.: 5.627 min
Delta R.T.: 0.000 min
Response: 107599165
Conc: 19.83 ng/ml

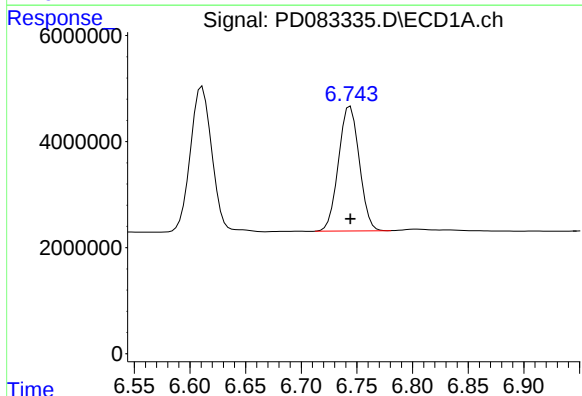


#16 4,4'-DDD

R.T.: 6.744 min
Delta R.T.: 0.000 min
Response: 30580367
Conc: 19.51 ng/ml

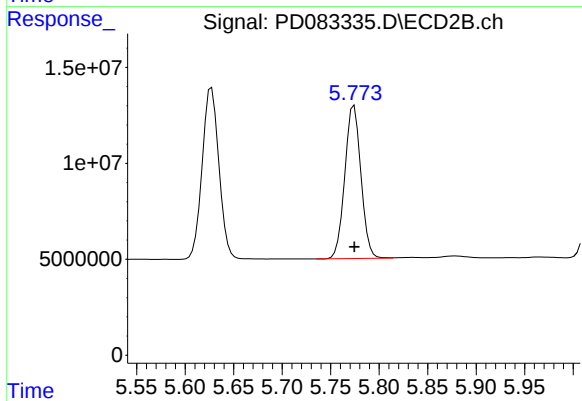


#16 4,4'-DDD

R.T.: 5.774 min
Delta R.T.: 0.000 min
Response: 91998793
Conc: 19.72 ng/ml

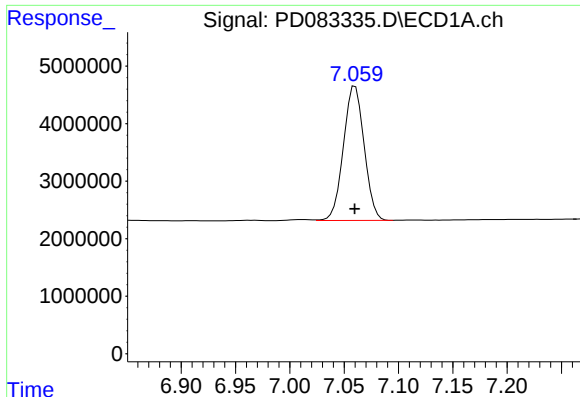


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 31034578
Conc: 19.42 ng/ml

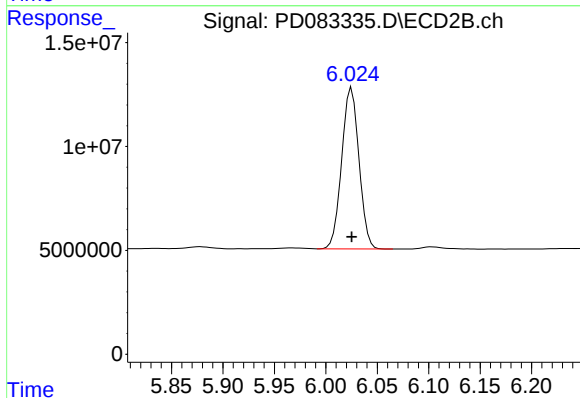


#17 4,4'-DDT

R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 90730275
Conc: 19.08 ng/ml

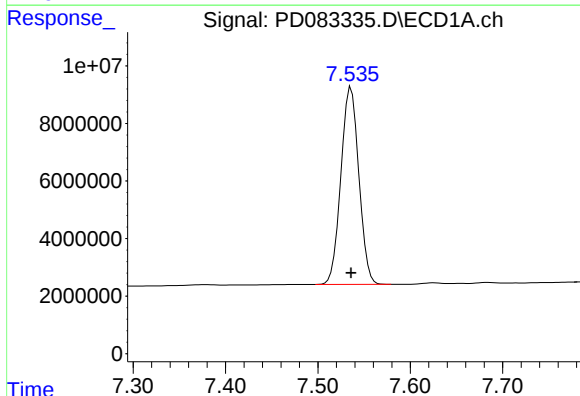


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 92576101
Conc: 102.01 ng/ml

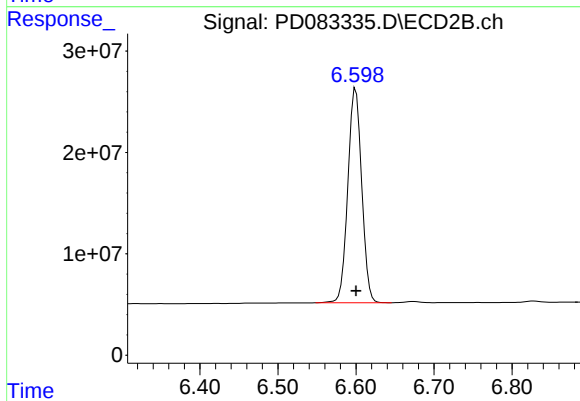


#20 Methoxychlor

R.T.: 6.600 min
Delta R.T.: 0.000 min
Response: 261446144
Conc: 104.34 ng/ml

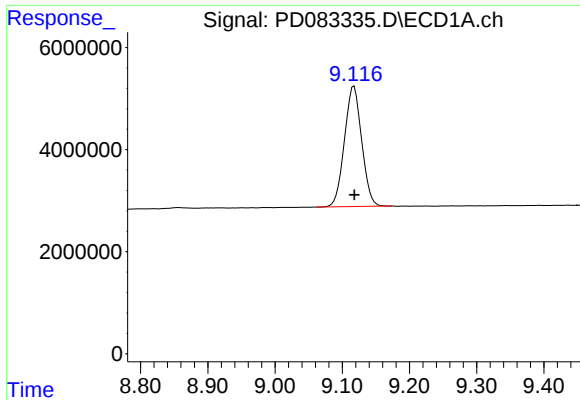

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 41996381
Conc: 20.66 ng/ml

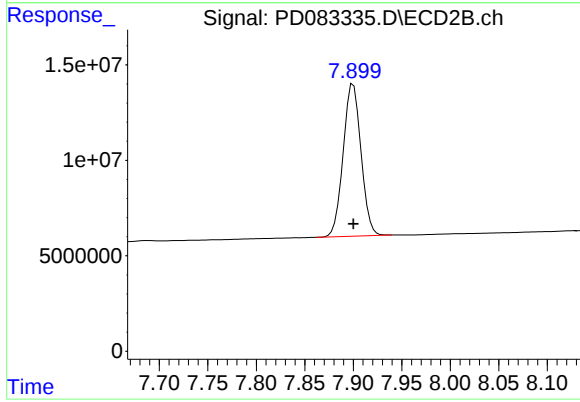

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 101944431
Conc: 20.40 ng/ml