

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 22:56
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:37:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 06:36:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	28678898	95177450	20.000	20.000
27)	SA Decachlor...	9.118	7.900	81294937	199.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.020	3.272	49773857	146.3E6	20.000	20.000
3)	MA gamma-BHC...	4.354	3.601	48009311	135.9E6	20.000	20.000
4)	MA Heptachlor	4.947	3.939	49639877	135.4E6	20.000	20.000
9)	A Endosulfan I	6.104	5.089	42309299	109.3E6	20.000	20.000
13)	MA Dieldrin	6.381	5.353	89109744	245.4E6	40.000	40.000
14)	MA Endrin	6.612	5.628	73030565	217.0E6	40.000	40.000
16)	A 4,4'-DDD	6.744	5.775	62704073	186.6E6	40.000	40.000
17)	MA 4,4'-DDT	7.060	6.025	63929760	190.2E6	40.000	40.000
20)	A Methoxychlor	7.536	6.600	181.5E6	501.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 22:56
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:37:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 06:36:45 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

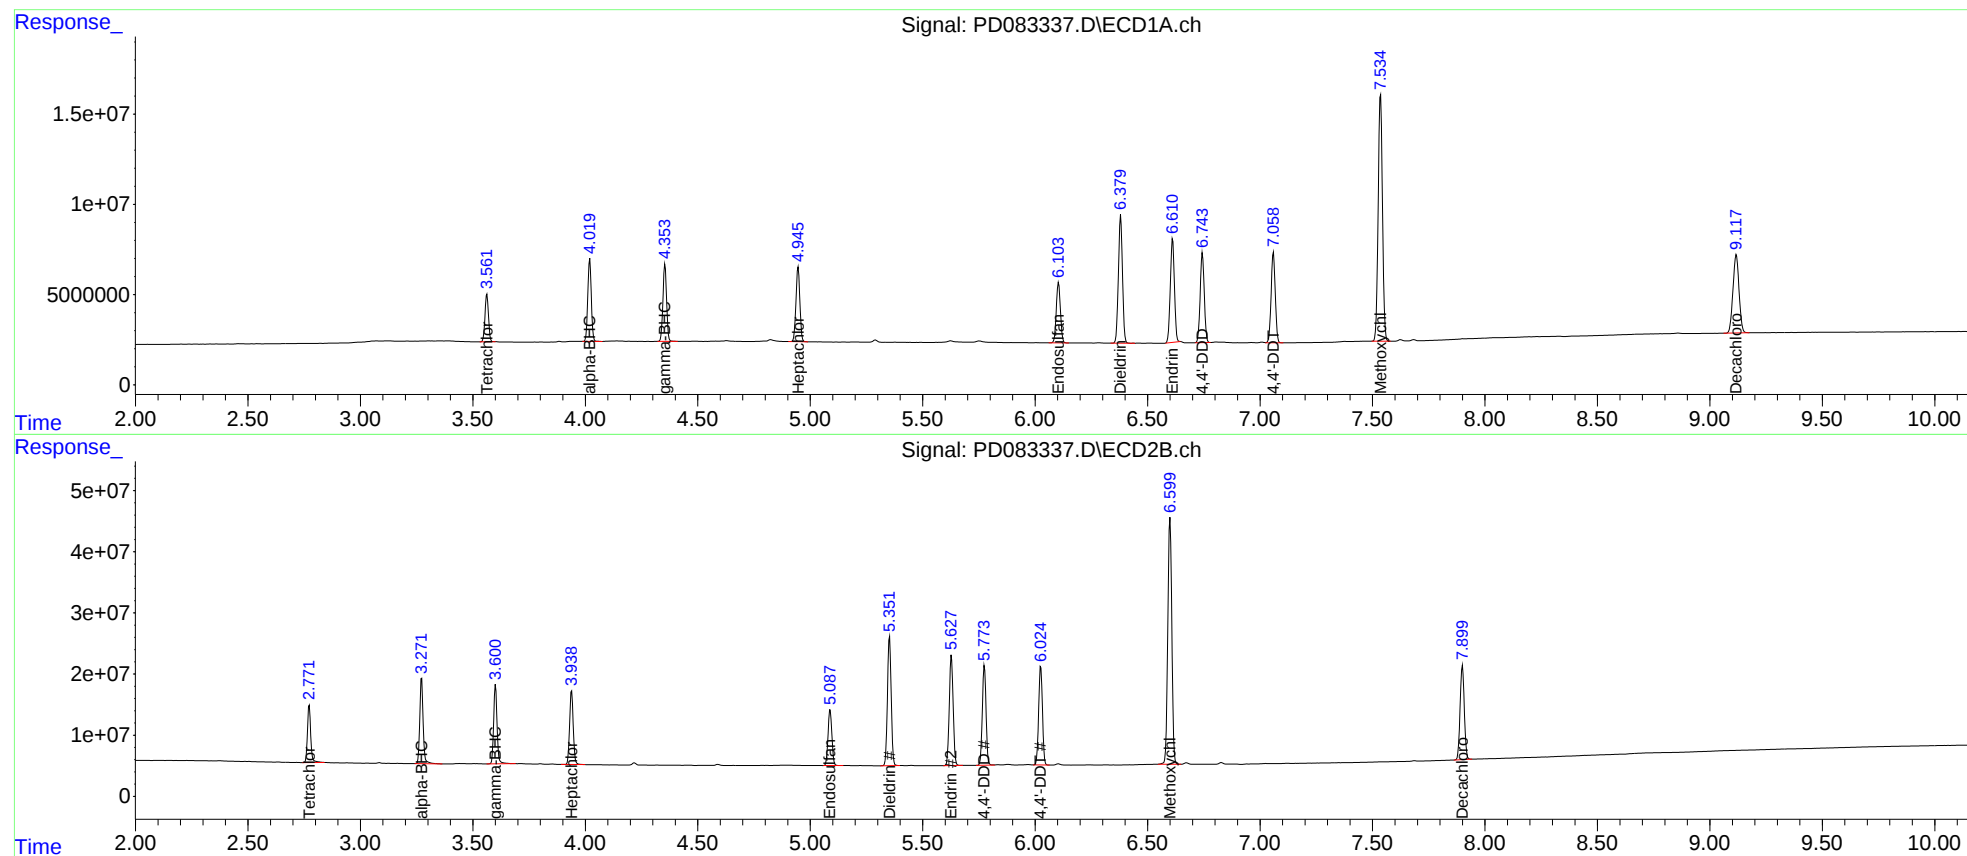

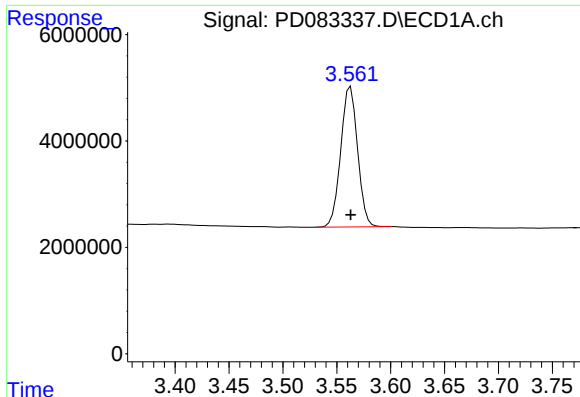


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 28678898
Conc: 20.00 ng/ml

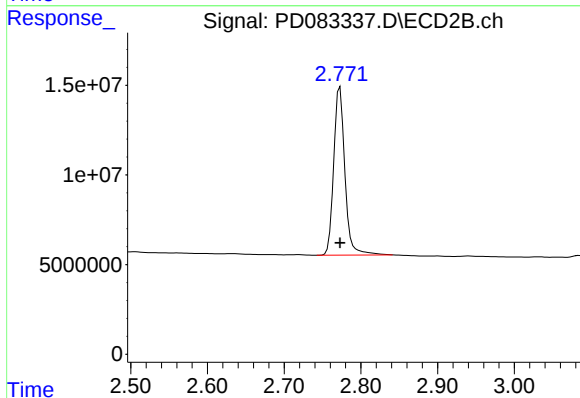


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 95177450
Conc: 20.00 ng/ml

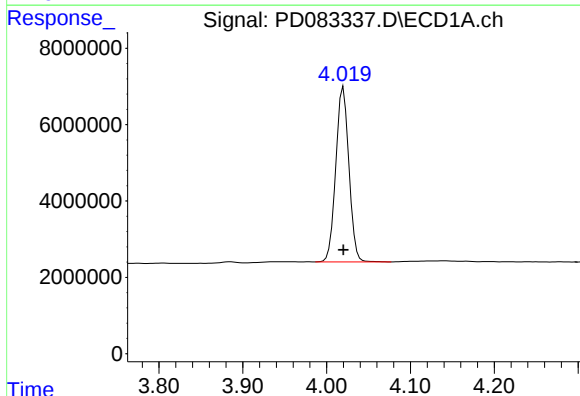


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 49773857
Conc: 20.00 ng/ml

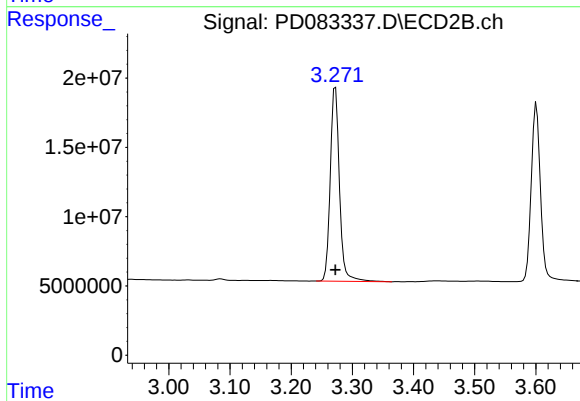


#2 alpha-BHC

R.T.: 3.272 min
Delta R.T.: 0.000 min
Response: 146348782
Conc: 20.00 ng/ml

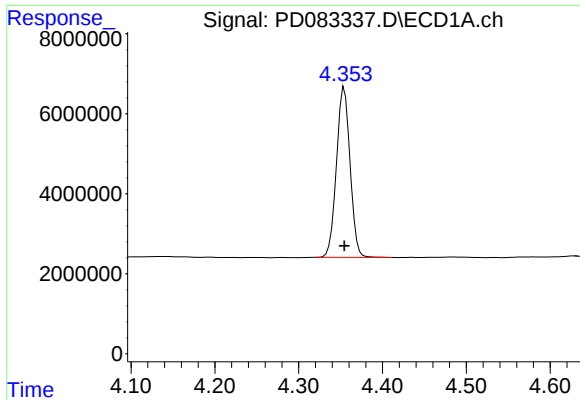


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 48009311
Conc: 20.00 ng/ml

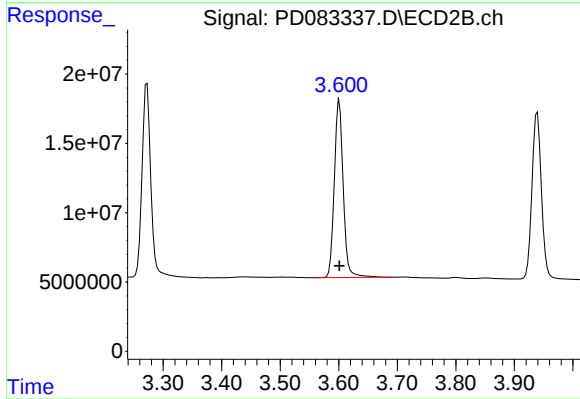


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 135917935
Conc: 20.00 ng/ml

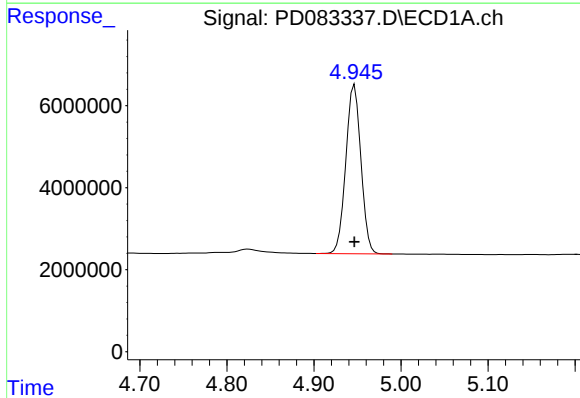


#4 Heptachlor

R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 49639877
Conc: 20.00 ng/ml

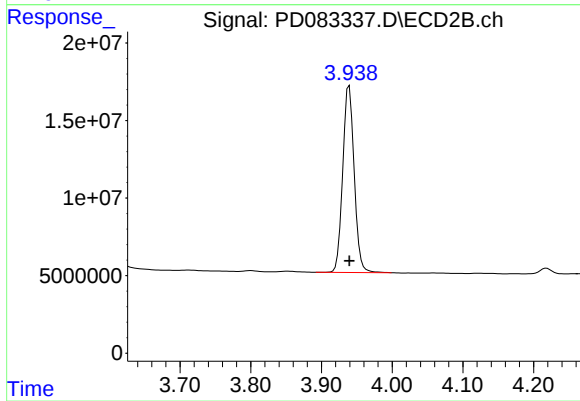


#4 Heptachlor

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 135362297
Conc: 20.00 ng/ml

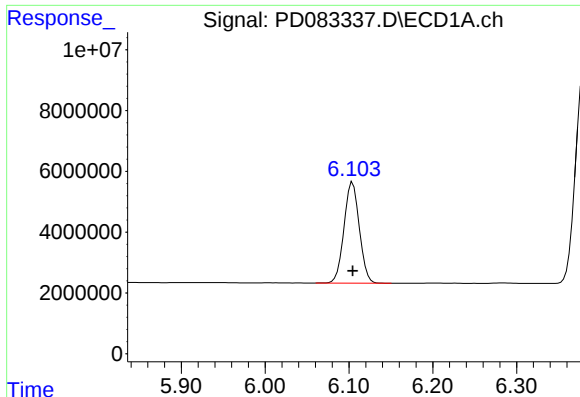


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 42309299
Conc: 20.00 ng/ml

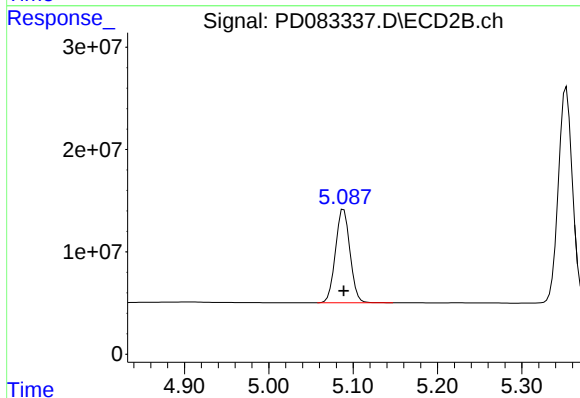


#9 Endosulfan I

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 109285195
Conc: 20.00 ng/ml

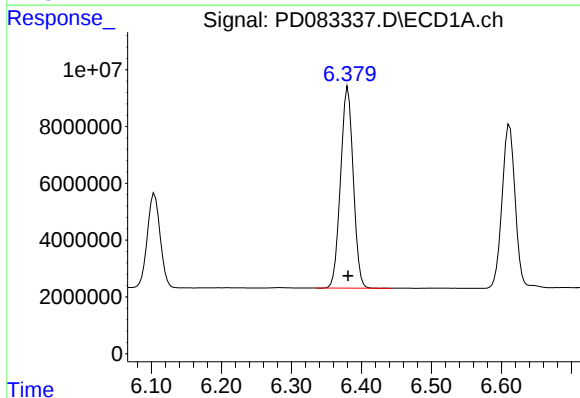


#13 Dieldrin

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 89109744
Conc: 40.00 ng/ml

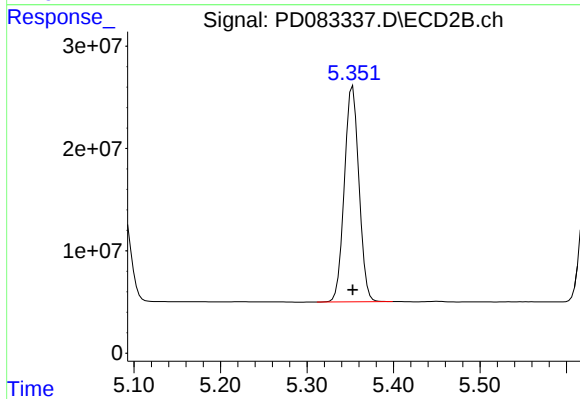


#13 Dieldrin

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 245387856
Conc: 40.00 ng/ml

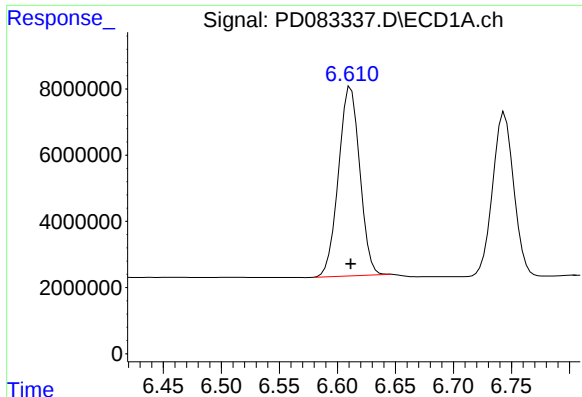


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 73030565
Conc: 40.00 ng/ml

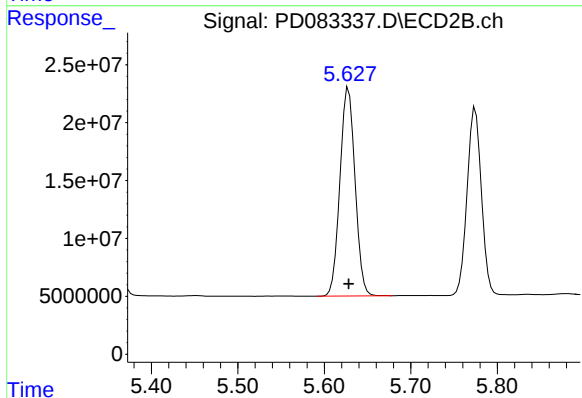


#14 Endrin

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 217026078
Conc: 40.00 ng/ml

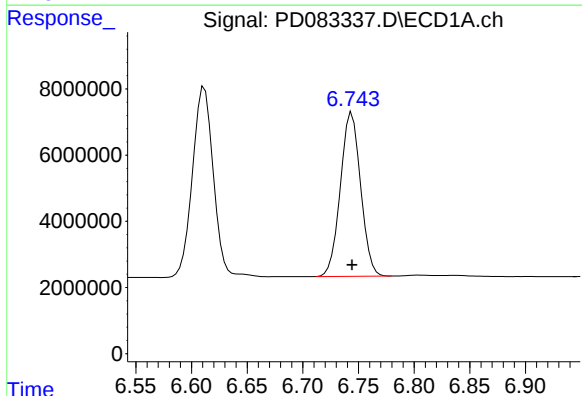


#16 4,4'-DDD

R.T.: 6.744 min
Delta R.T.: 0.000 min
Response: 62704073
Conc: 40.00 ng/ml

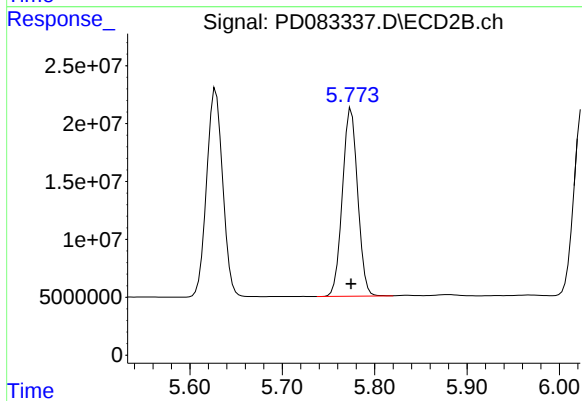


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 186647411
Conc: 40.00 ng/ml

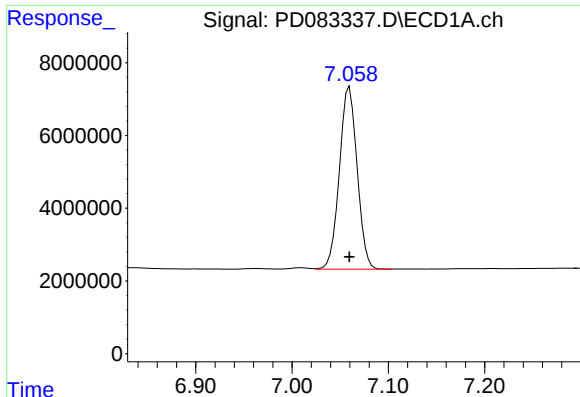


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 63929760
Conc: 40.00 ng/ml

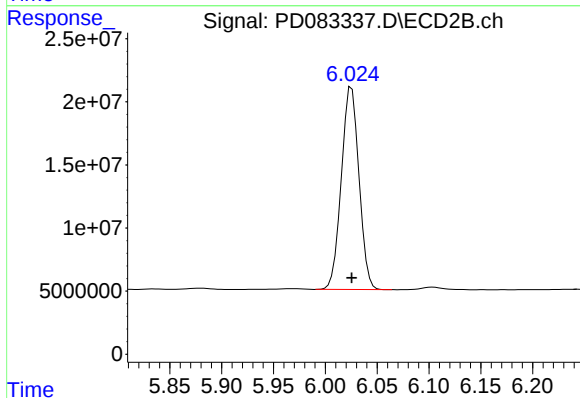


#17 4,4'-DDT

R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 190207045
Conc: 40.00 ng/ml

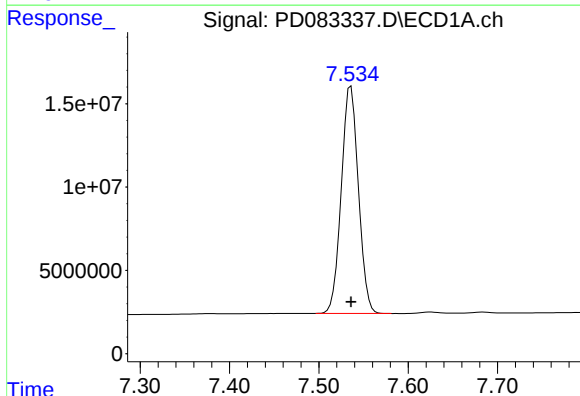


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 181511863
Conc: 200.00 ng/ml

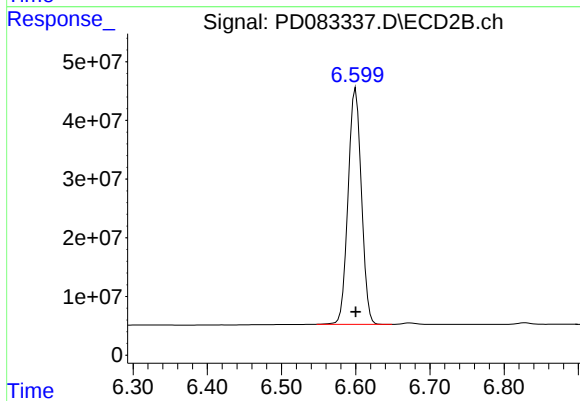


#20 Methoxychlor

R.T.: 6.600 min
Delta R.T.: 0.000 min
Response: 501163290
Conc: 200.00 ng/ml

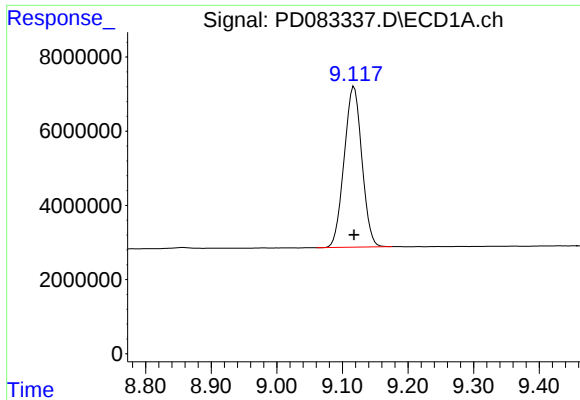

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 81294937
Conc: 40.00 ng/ml

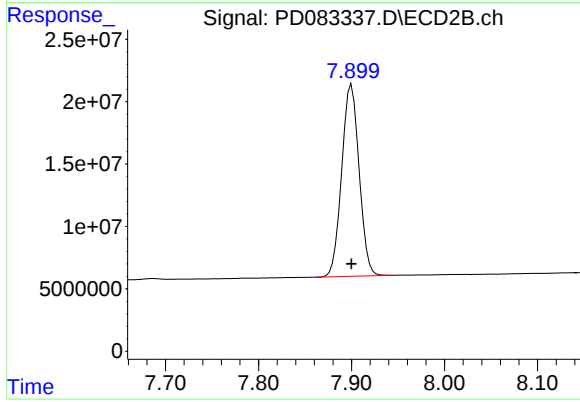

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 199902085
Conc: 40.00 ng/ml