

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 23:23
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:38:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 06:36:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.772	56889945	185.7E6	39.674	39.023
27)	SA Decachlor...	9.117	7.900	157.6E6	387.6E6	77.525	77.566
Target Compounds							
2)	A alpha-BHC	4.020	3.272	104.5E6	296.4E6	41.977	40.510
3)	MA gamma-BHC...	4.354	3.601	99821762	272.4E6	41.584	40.080
4)	MA Heptachlor	4.947	3.939	103.2E6	270.0E6	41.585	39.886
9)	A Endosulfan I	6.104	5.088	85252533	216.9E6	40.300	39.695
13)	MA Dieldrin	6.380	5.353	185.7E6	488.7E6	83.363	79.655
14)	MA Endrin	6.611	5.628	152.7E6	429.9E6	83.650	79.235
16)	A 4,4'-DDD	6.745	5.775	133.6E6	375.6E6	85.247	80.487
17)	MA 4,4'-DDT	7.060	6.025	137.9E6	387.8E6	86.293	81.555
20)	A Methoxychlor	7.536	6.600	367.4E6	930.3E6	404.776	371.250


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 23:23
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:38:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 06:36:45 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

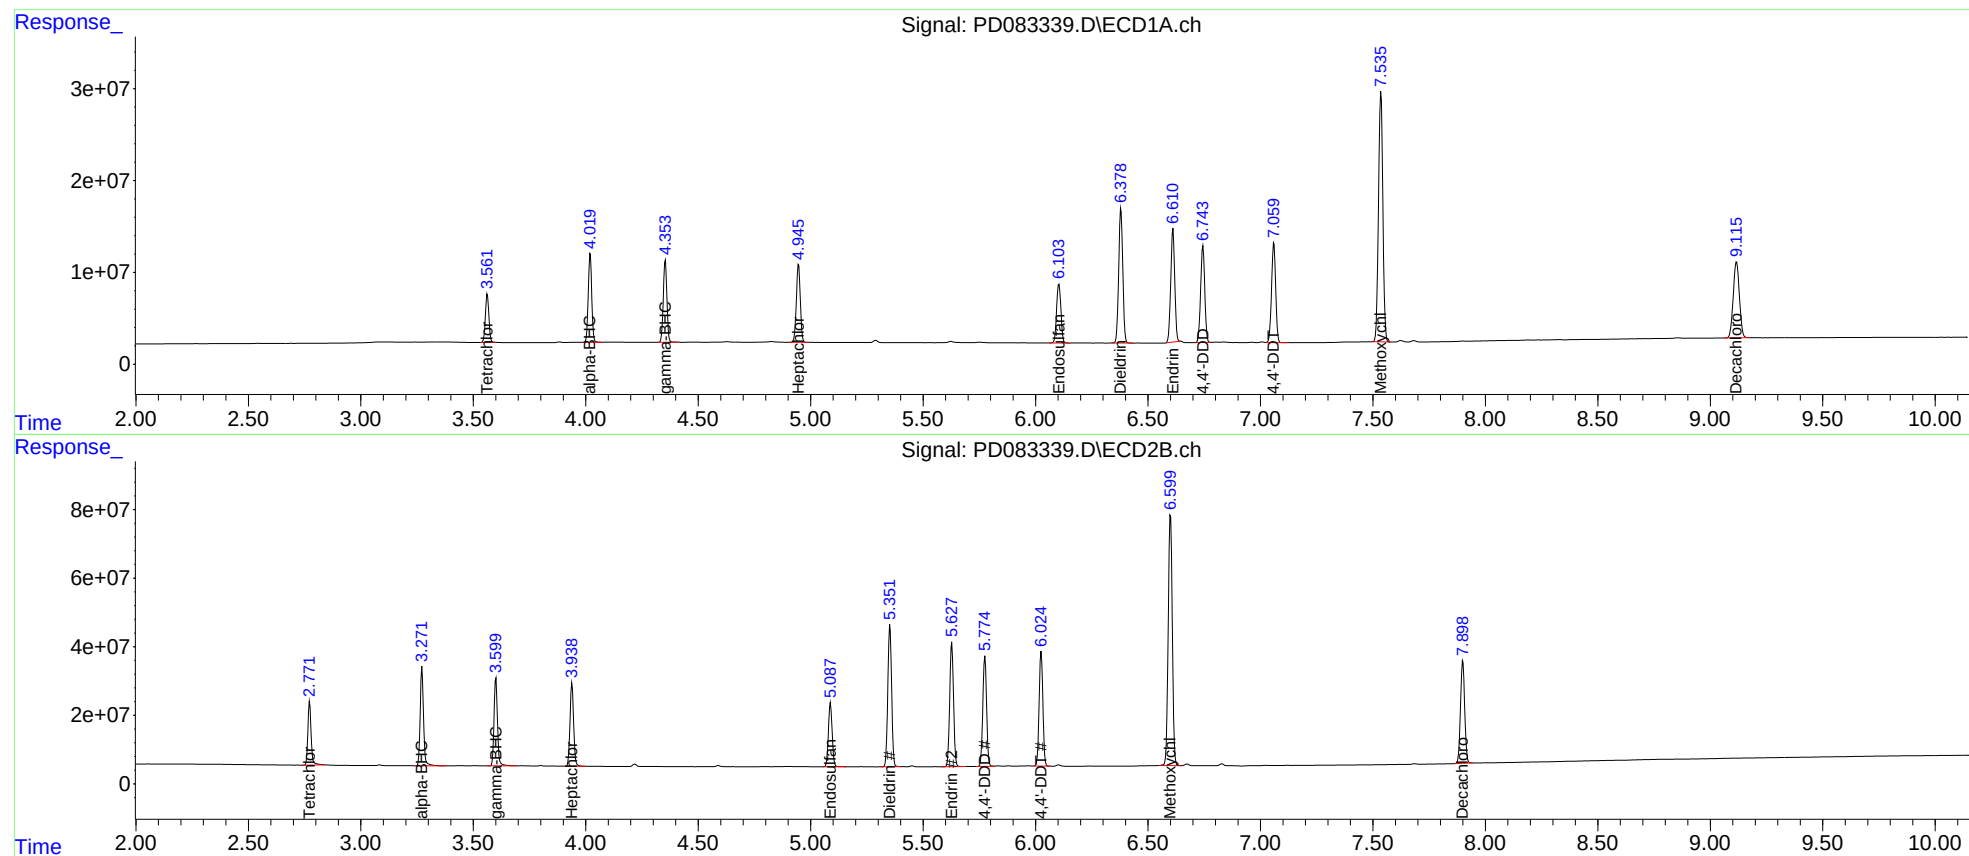

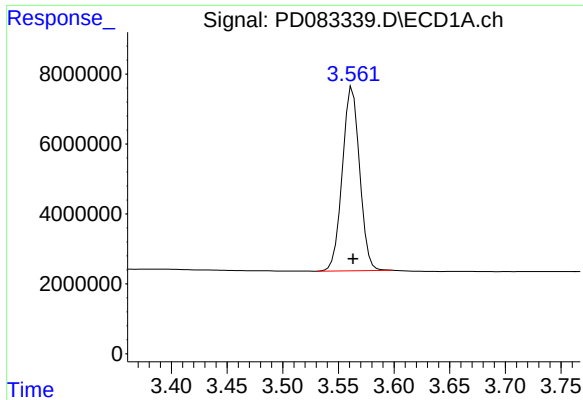


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 56889945
Conc: 39.67 ng/ml

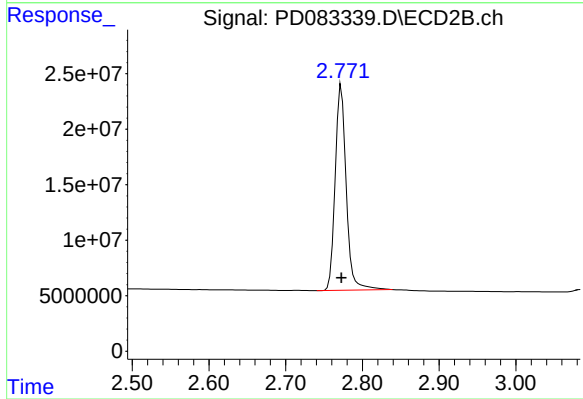


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 185706780
Conc: 39.02 ng/ml

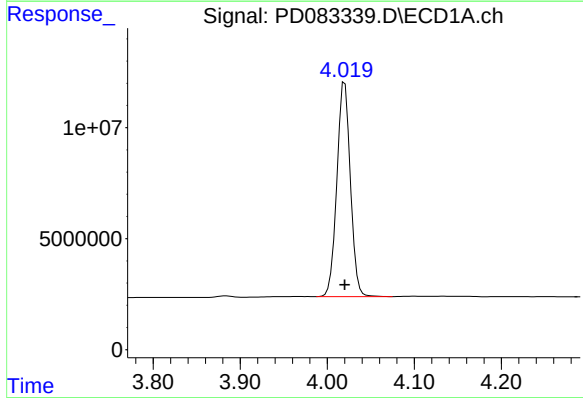


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 104469079
Conc: 41.98 ng/ml

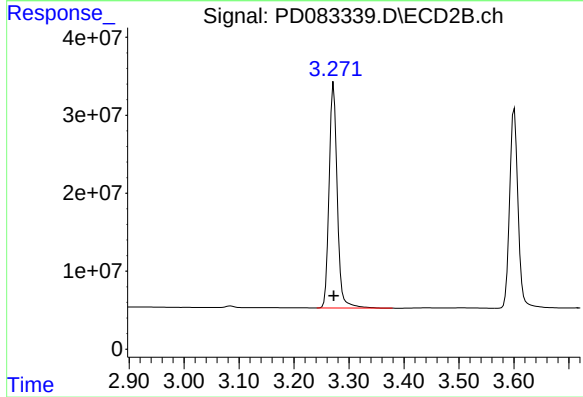


#2 alpha-BHC

R.T.: 3.272 min
Delta R.T.: 0.000 min
Response: 296426737
Conc: 40.51 ng/ml

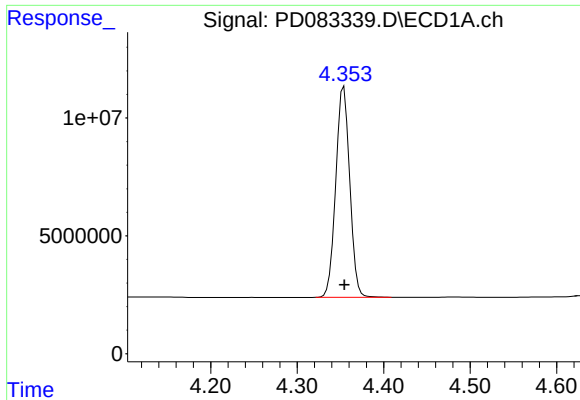


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 99821762
Conc: 41.58 ng/ml

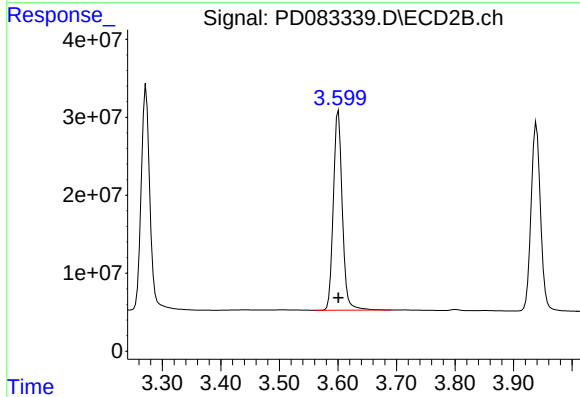


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 272382914
Conc: 40.08 ng/ml

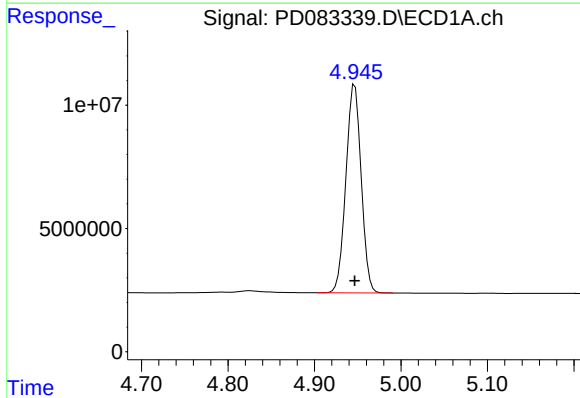


#4 Heptachlor

R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 103212590
Conc: 41.58 ng/ml

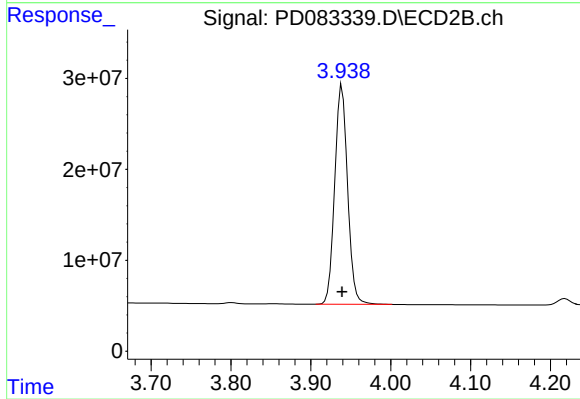


#4 Heptachlor

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 269955392
Conc: 39.89 ng/ml

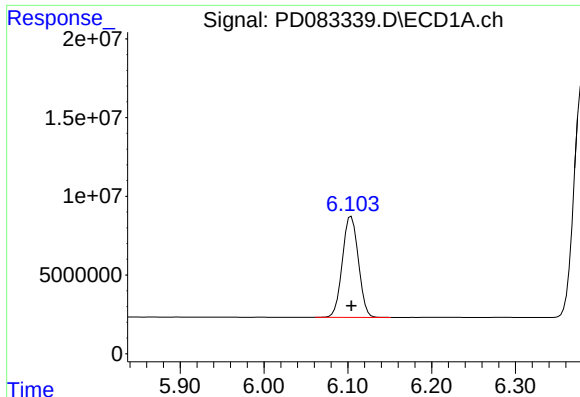


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 85252533
Conc: 40.30 ng/ml

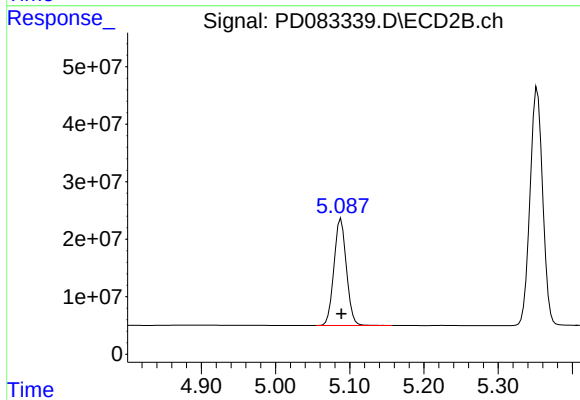


#9 Endosulfan I

R.T.: 5.088 min
Delta R.T.: 0.000 min
Response: 216901742
Conc: 39.69 ng/ml

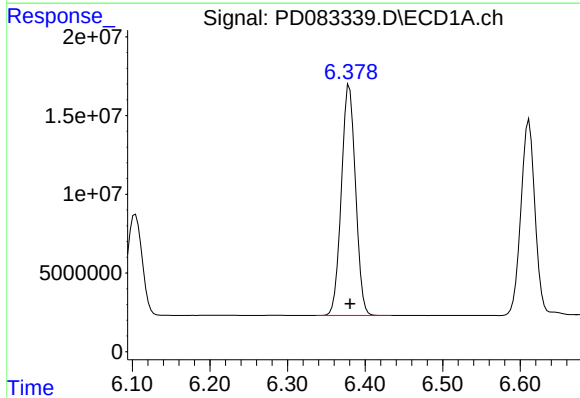


#13 Dieldrin

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 185711451
Conc: 83.36 ng/ml

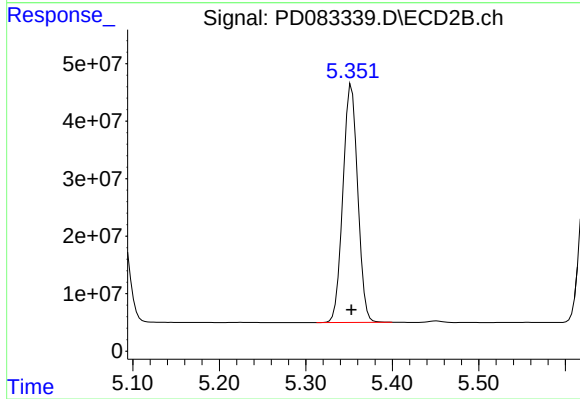


#13 Dieldrin

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 488658834
Conc: 79.65 ng/ml

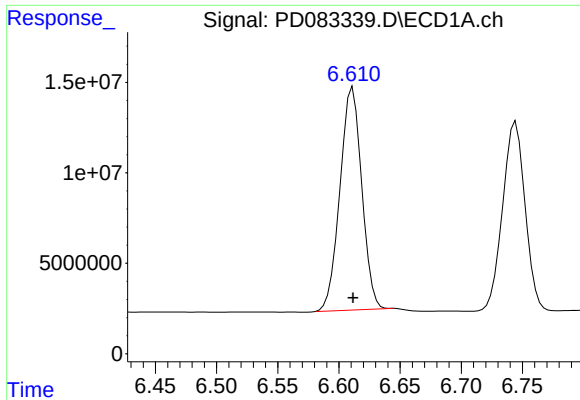


#14 Endrin

R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 152725492
Conc: 83.65 ng/ml

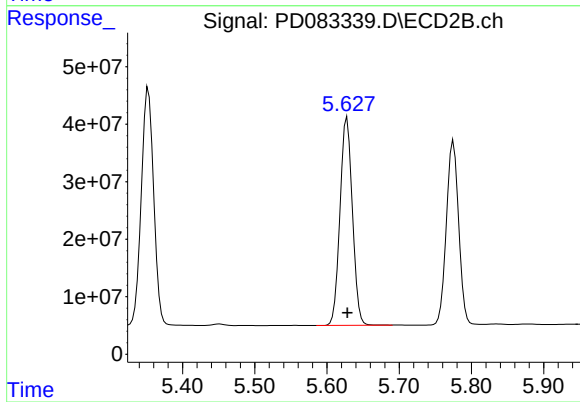


#14 Endrin

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 429902944
Conc: 79.24 ng/ml

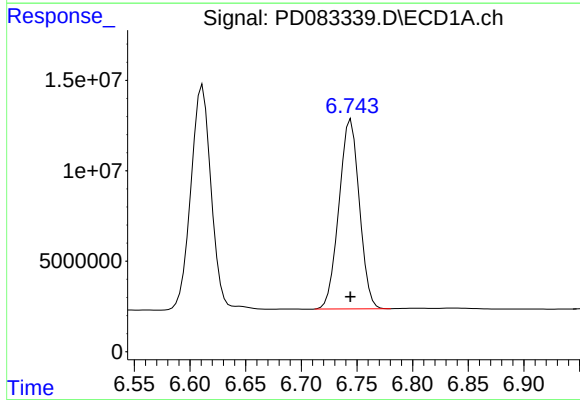


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 133632877
Conc: 85.25 ng/ml

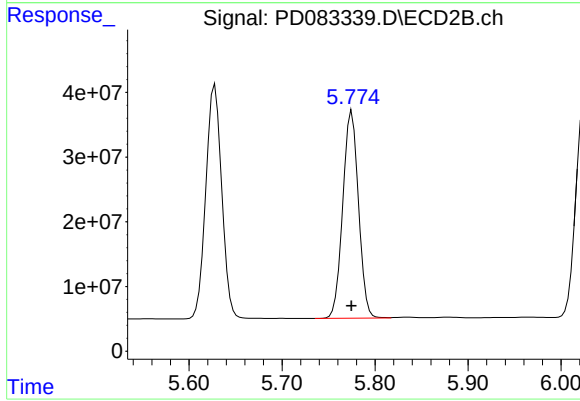


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 375566029
Conc: 80.49 ng/ml

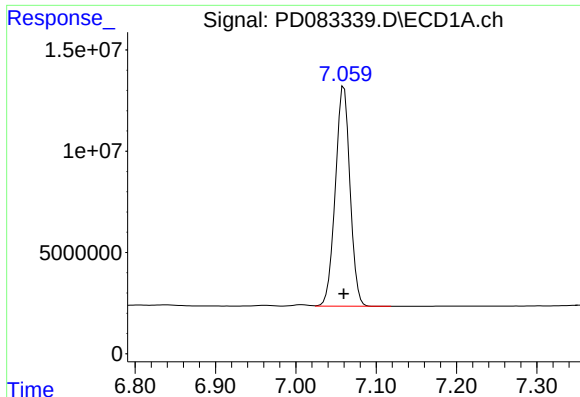


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 137917088
Conc: 86.29 ng/ml

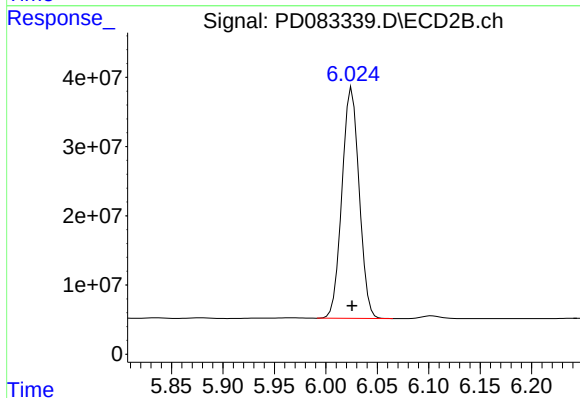


#17 4,4'-DDT

R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 387809883
Conc: 81.56 ng/ml

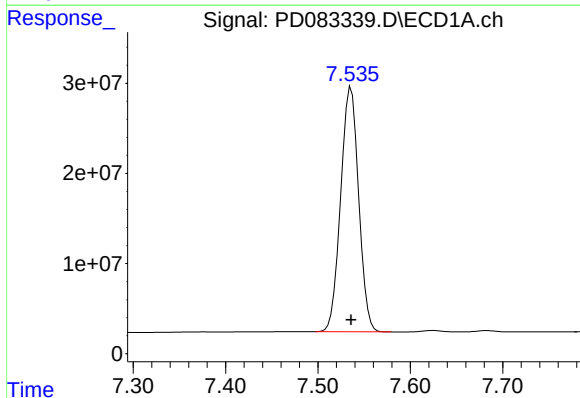


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 367358207
Conc: 404.78 ng/ml

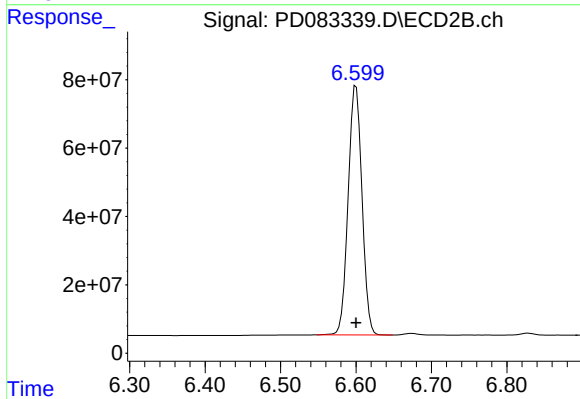


#20 Methoxychlor

R.T.: 6.600 min
Delta R.T.: 0.000 min
Response: 930283287
Conc: 371.25 ng/ml

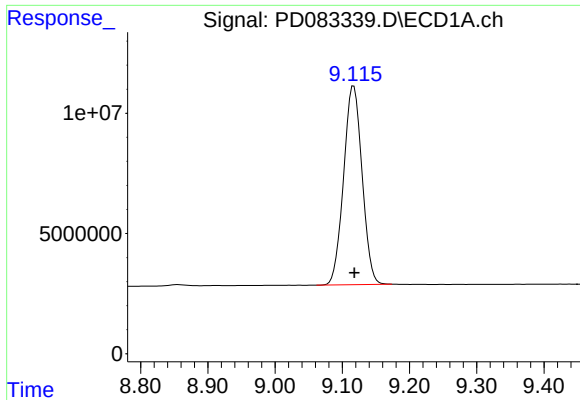

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: -0.001 min
Response: 157560074
Conc: 77.53 ng/ml

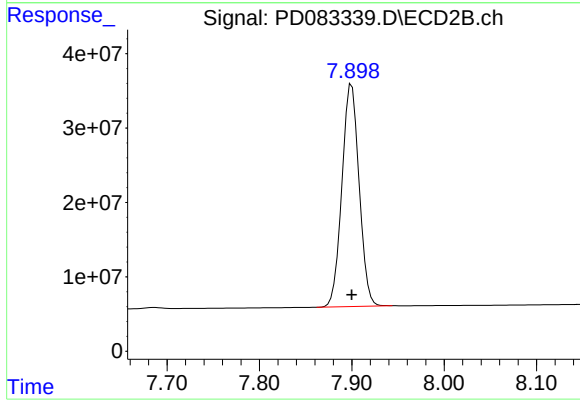

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 387639488
Conc: 77.57 ng/ml