

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 23:36
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:20:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 06:18:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.772	57031484	188.5E6	39.363	39.234
27)	SA Decachlor...	9.116	7.900	157.0E6	389.5E6	76.702	77.558
Target Compounds							
5)	MB Aldrin	5.289	4.218	96800006	260.9E6	40.051	40.386
6)	B beta-BHC	4.550	3.897	42378045	115.4E6	39.002	39.188
7)	B delta-BHC	4.800	4.126	106.2E6	286.1E6	40.680	40.561
8)	B Heptachlo...	5.717	4.719	88044184	236.5E6	40.109	39.656
10)	B trans-Chl...	5.974	4.968	85908458	233.1E6	39.567	39.987
11)	B cis-Chlor...	6.053	5.032	87449976	236.5E6	39.374	39.740
12)	B 4,4'-DDE	6.225	5.221	176.3E6	461.9E6	79.776	80.231
15)	B Endosulfa...	6.831	5.921	149.3E6	400.3E6	76.867	79.185
18)	B Endrin al...	6.961	6.101	110.2E6	299.6E6	76.205	78.139
19)	B Endosulfa...	7.196	6.323	140.6E6	385.8E6	76.763	78.681
21)	B Endrin ke...	7.684	6.828	150.1E6	427.1E6	77.949	79.058


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 23:36
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:20:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 06:18:40 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

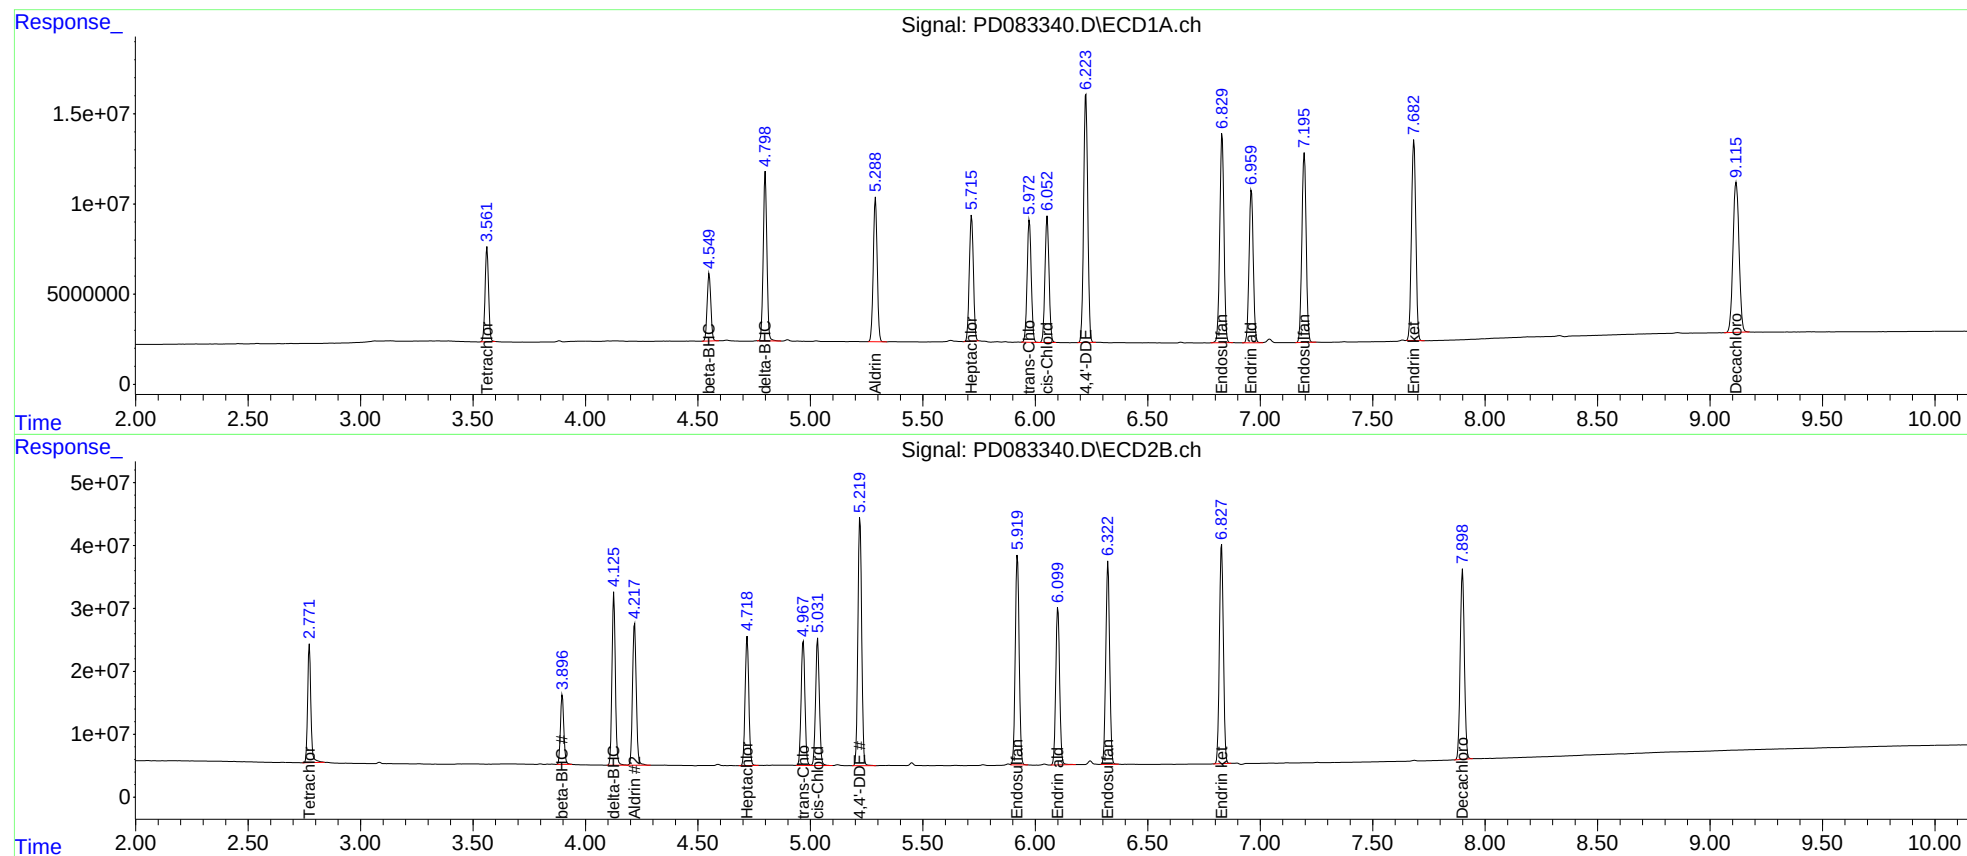

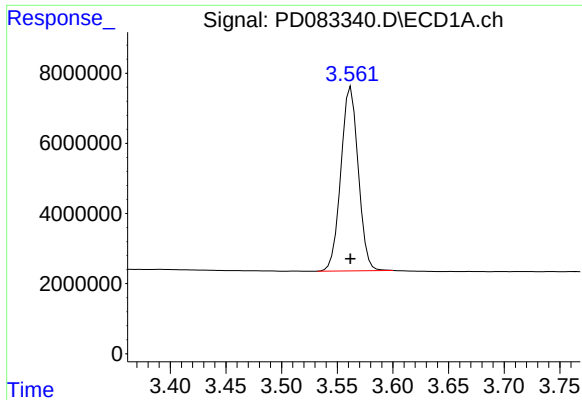


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 57031484
Conc: 39.36 ng/ml

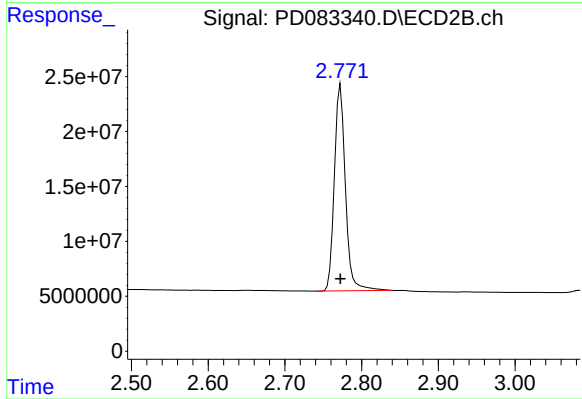


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 188459327
Conc: 39.23 ng/ml

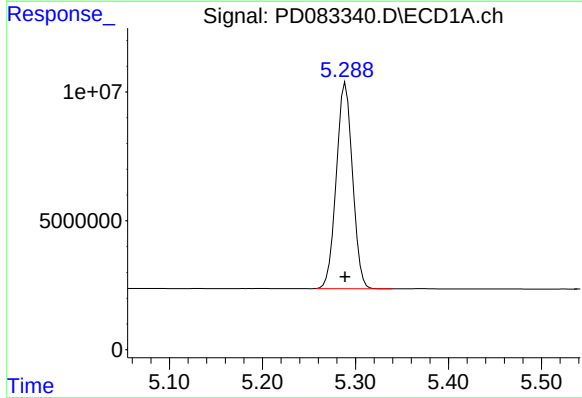


#5 Aldrin

R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 96800006
Conc: 40.05 ng/ml

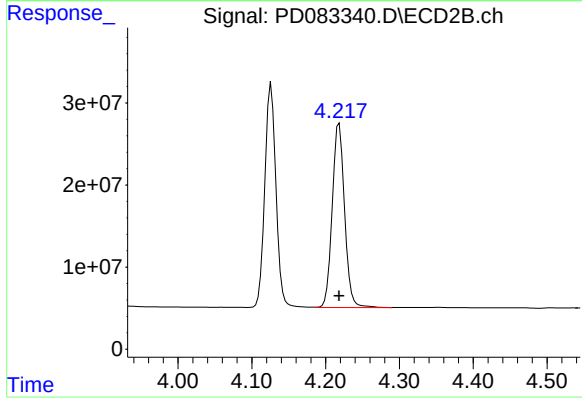


#5 Aldrin

R.T.: 4.218 min
Delta R.T.: 0.000 min
Response: 260867427
Conc: 40.39 ng/ml

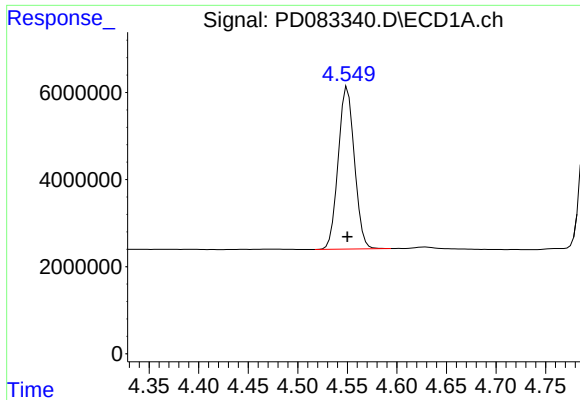


#6 beta-BHC

R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 42378045
Conc: 39.00 ng/ml

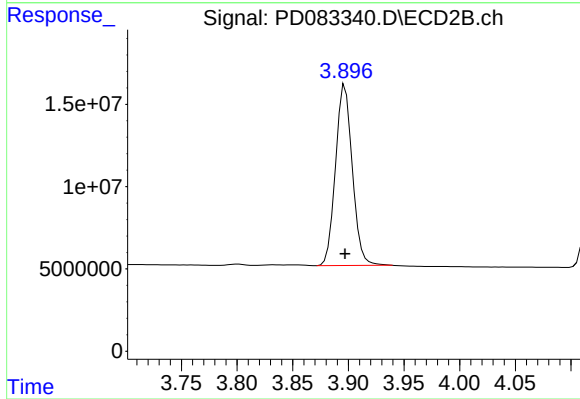


#6 beta-BHC

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 115444762
Conc: 39.19 ng/ml

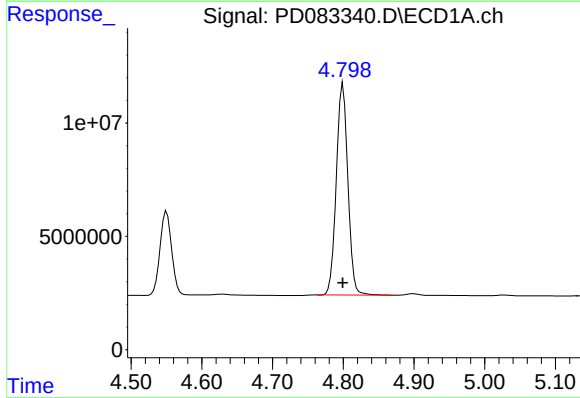


#7 delta-BHC

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 106232281
Conc: 40.68 ng/ml

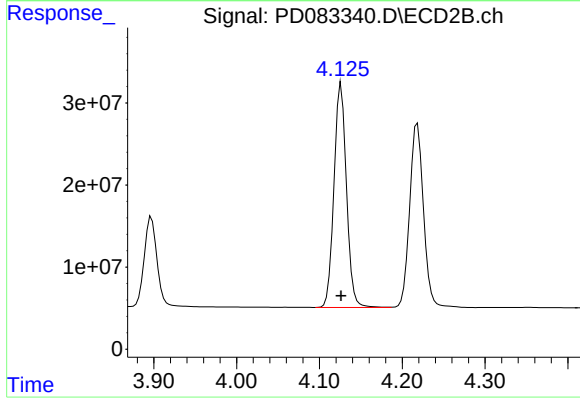


#7 delta-BHC

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 286142081
Conc: 40.56 ng/ml

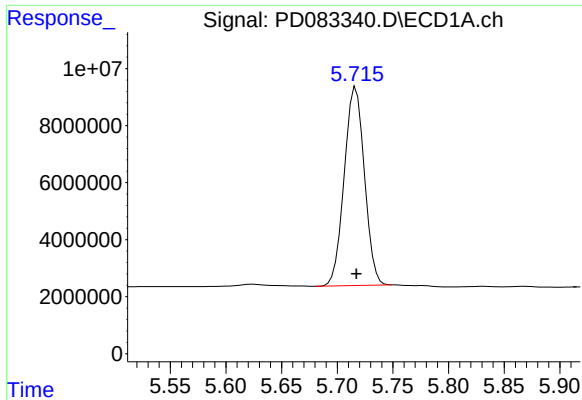


#8 Heptachlor epoxide

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 88044184
Conc: 40.11 ng/ml

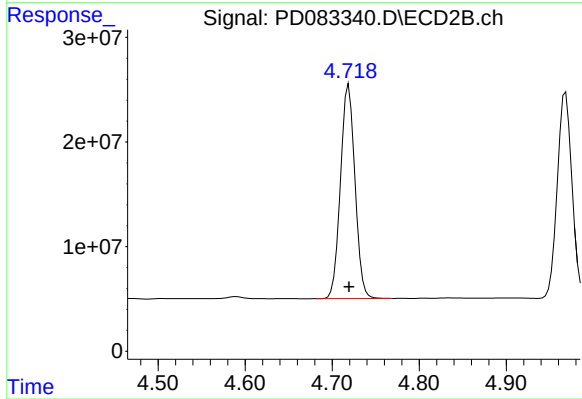


#8 Heptachlor epoxide

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 236490317
Conc: 39.66 ng/ml

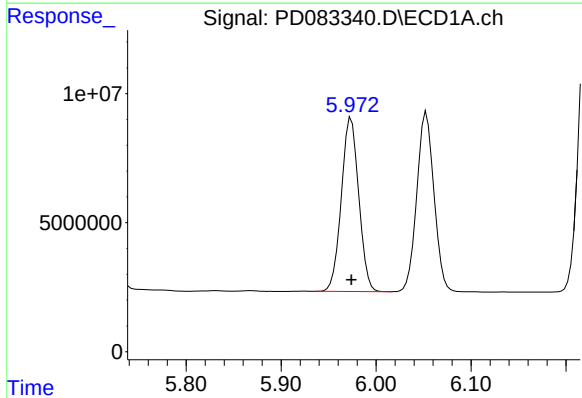


#10 trans-Chlordane

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 85908458
Conc: 39.57 ng/ml

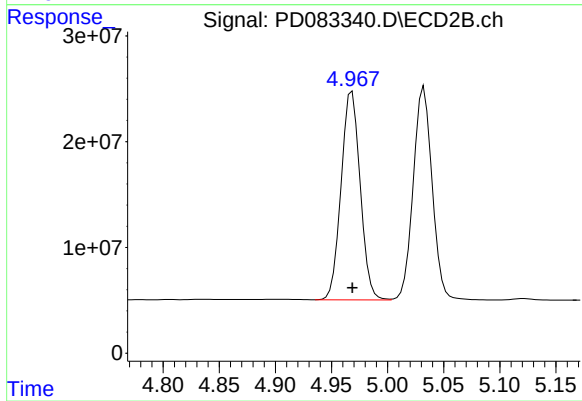


#10 trans-Chlordane

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 233070331
Conc: 39.99 ng/ml

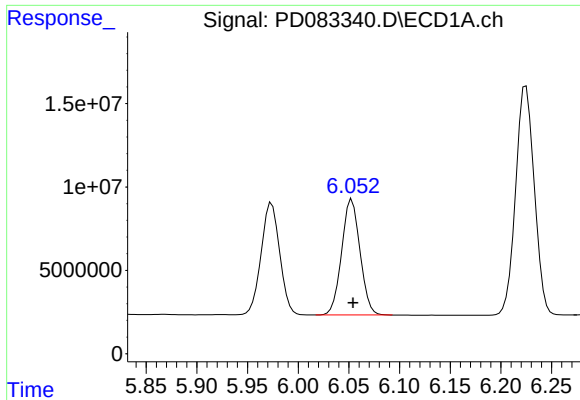


#11 cis-Chlordane

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 87449976
Conc: 39.37 ng/ml

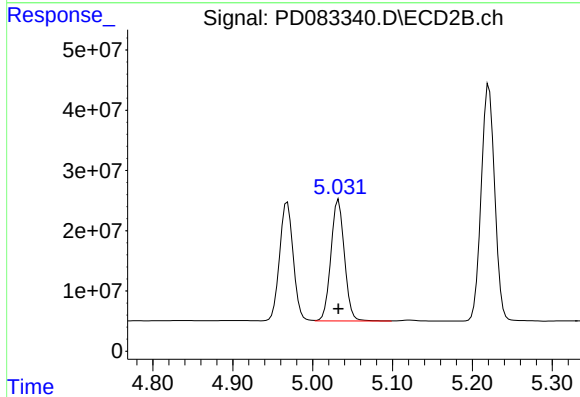


#11 cis-Chlordane

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 236455540
Conc: 39.74 ng/ml

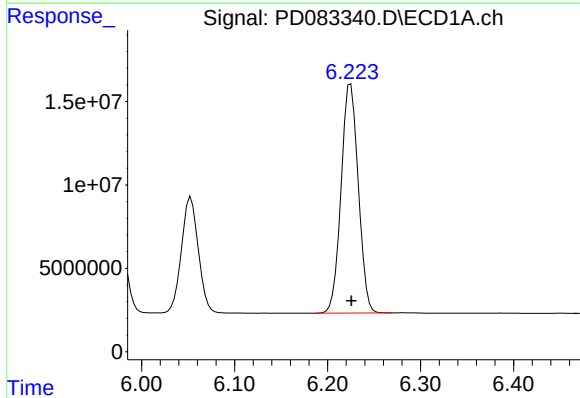


#12 4,4'-DDE

R.T.: 6.225 min
Delta R.T.: 0.000 min
Response: 176298876
Conc: 79.78 ng/ml

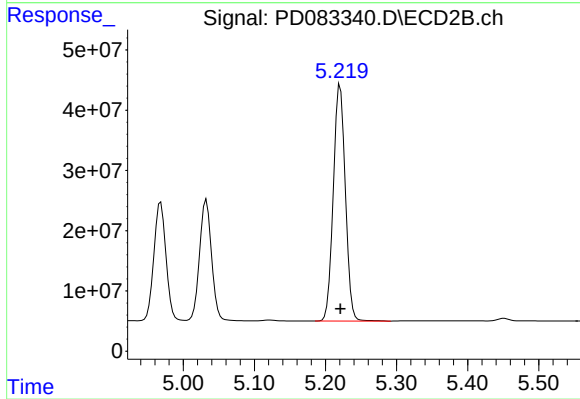


#12 4,4'-DDE

R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 461859824
Conc: 80.23 ng/ml

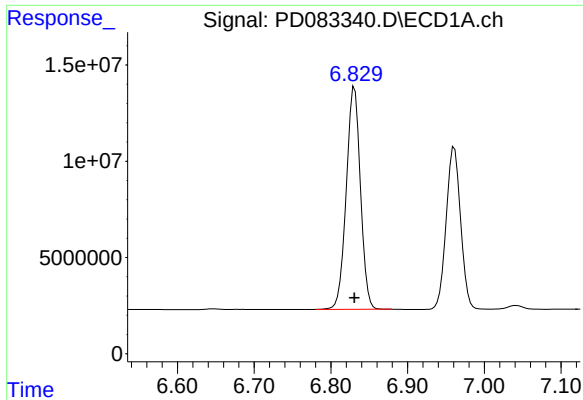


#15 Endosulfan II

R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 149317358
Conc: 76.87 ng/ml

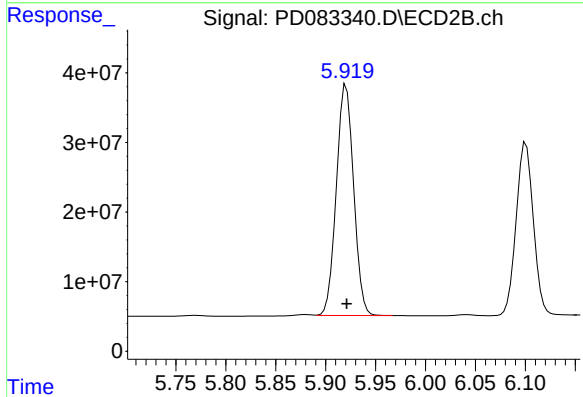


#15 Endosulfan II

R.T.: 5.921 min
Delta R.T.: 0.000 min
Response: 400251447
Conc: 79.18 ng/ml

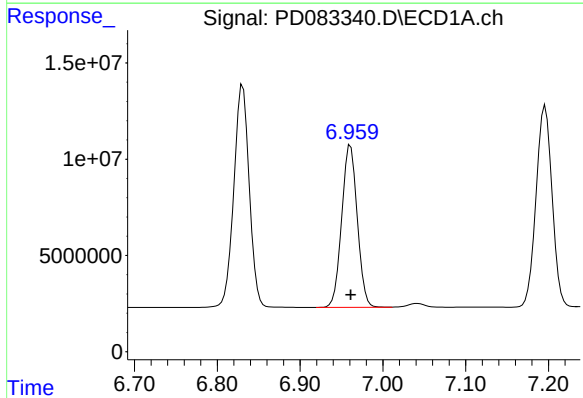


#18 Endrin aldehyde

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 110175221
Conc: 76.21 ng/ml

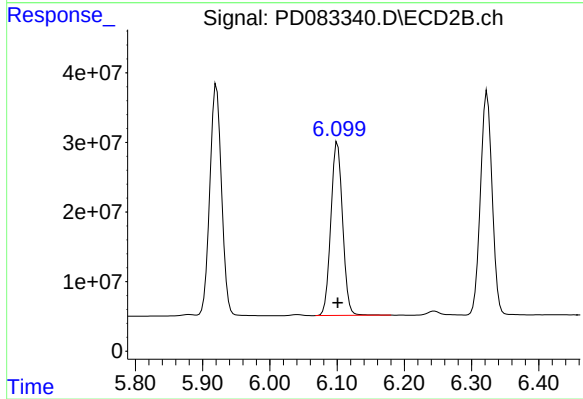


#18 Endrin aldehyde

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 299636196
Conc: 78.14 ng/ml

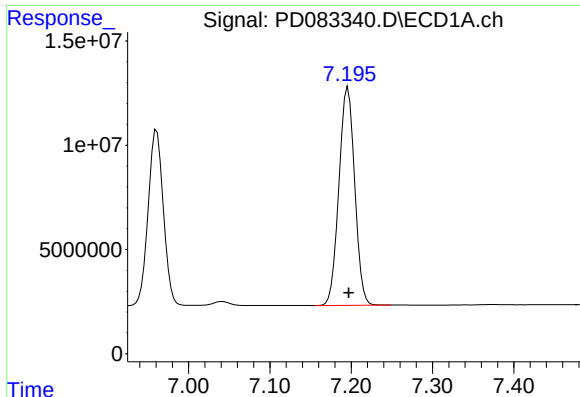


#19 Endosulfan Sulfate

R.T.: 7.196 min
Delta R.T.: 0.000 min
Response: 140632743
Conc: 76.76 ng/ml

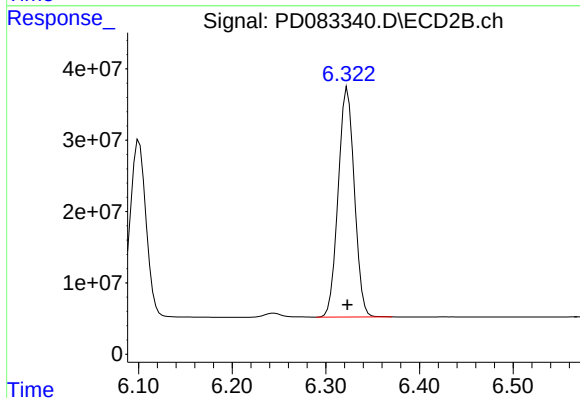


#19 Endosulfan Sulfate

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 385825806
Conc: 78.68 ng/ml

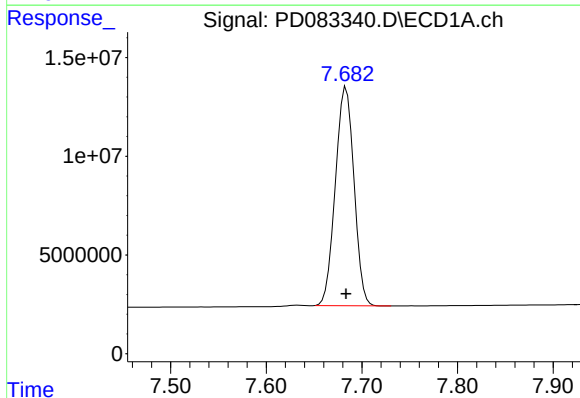


#21 Endrin ketone

R.T.: 7.684 min
Delta R.T.: 0.000 min
Response: 150070388
Conc: 77.95 ng/ml

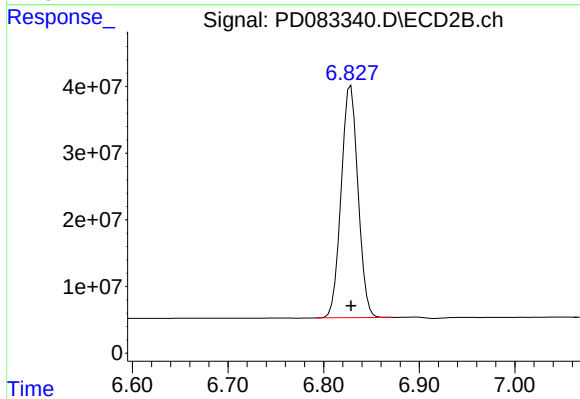


#21 Endrin ketone

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 427115071
Conc: 79.06 ng/ml

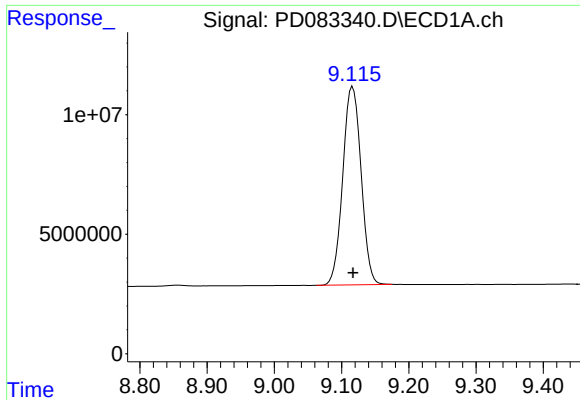

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 157003270
Conc: 76.70 ng/ml

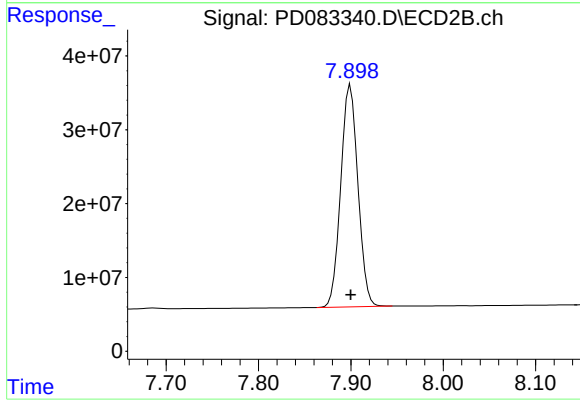

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 389457144
Conc: 77.56 ng/ml