

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 23:50
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 06:38:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 06:36:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.772	113.3E6	376.1E6	79.034	79.032
27)	SA Decachlor...	9.116	7.899	314.5E6	771.2E6	154.760	154.312
Target Compounds							
2)	A alpha-BHC	4.020	3.272	223.4E6	613.3E6	89.771	83.812
3)	MA gamma-BHC...	4.354	3.601	212.3E6	558.9E6	88.434	82.247
4)	MA Heptachlor	4.946	3.939	215.2E6	548.3E6	86.717	81.010
9)	A Endosulfan I	6.104	5.088	174.2E6	437.6E6	82.364	80.078
13)	MA Dieldrin	6.380	5.353	389.3E6	980.1E6	174.766	159.763
14)	MA Endrin	6.611	5.628	318.9E6	862.1E6	174.685	158.891
16)	A 4,4'-DDD	6.745	5.775	281.5E6	763.1E6	179.605	163.541
17)	MA 4,4'-DDT	7.060	6.025	291.0E6	802.0E6	182.074	168.651
20)	A Methoxychlor	7.537	6.600	729.7E6	1721.8E6	803.987	687.119


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 23:50
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 06:38:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 06:36:45 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

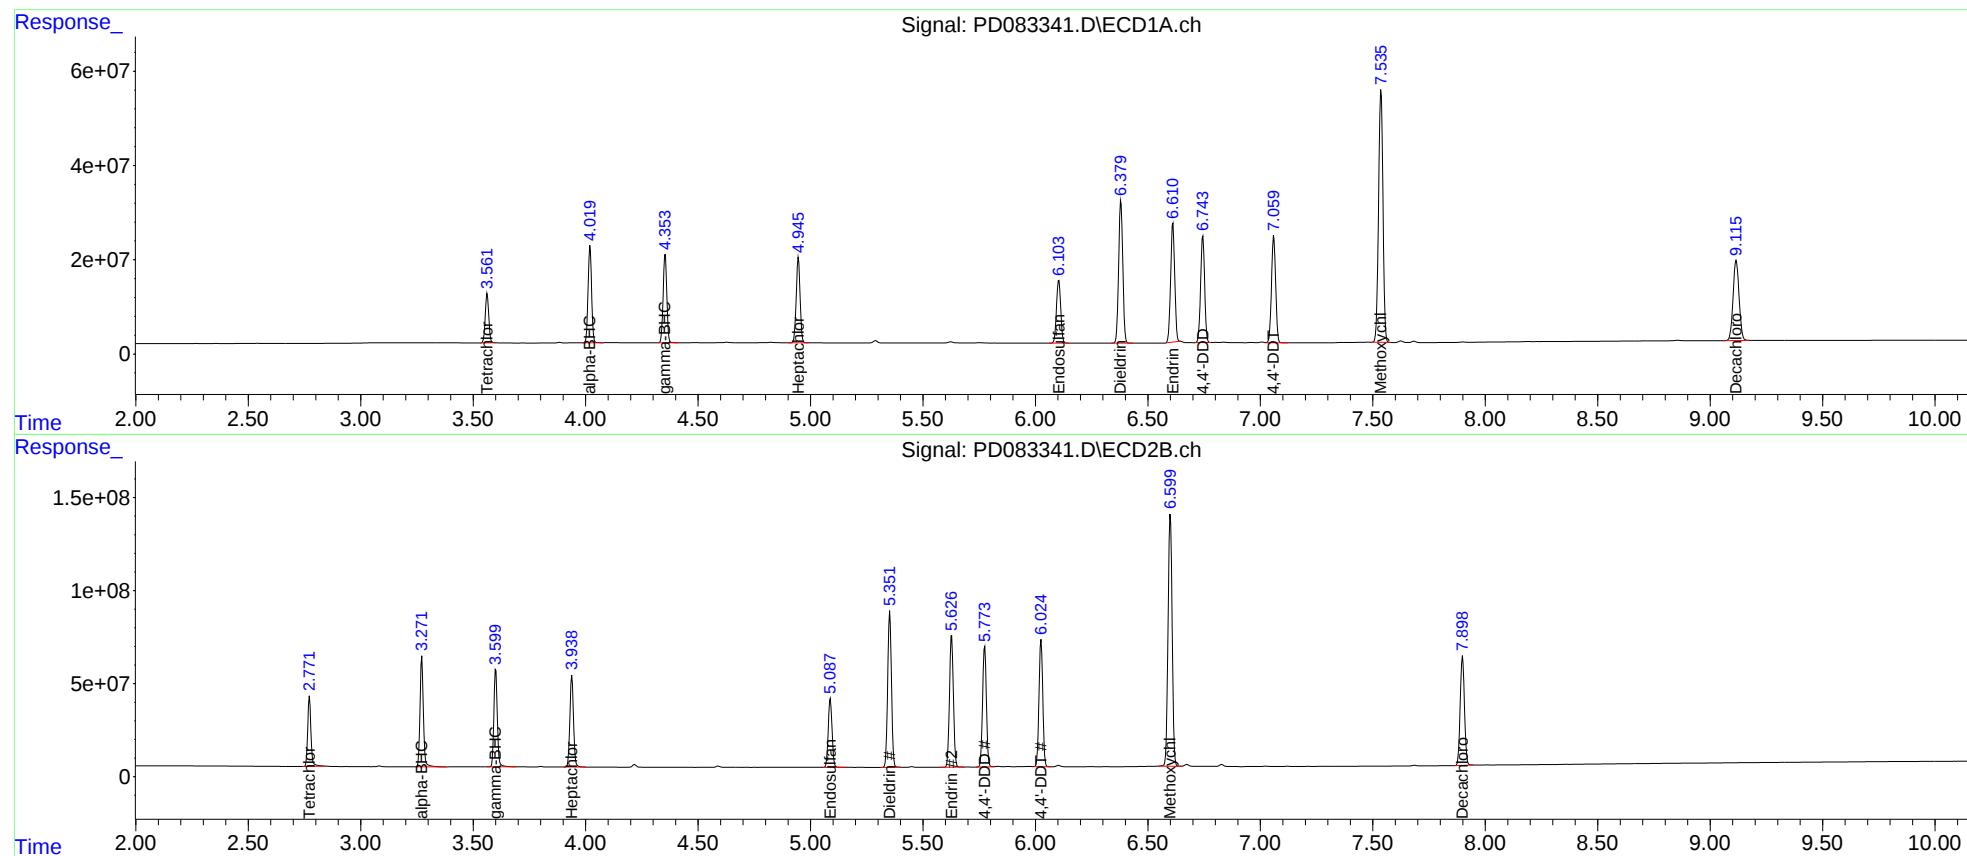

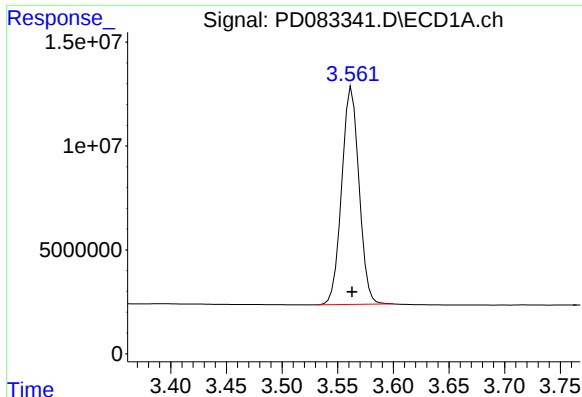


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 113329718
Conc: 79.03 ng/ml

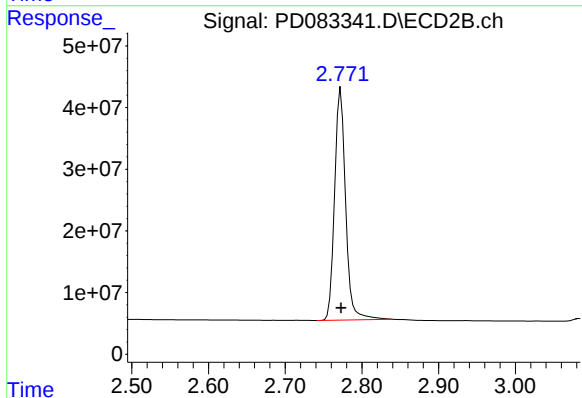


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 376101760
Conc: 79.03 ng/ml

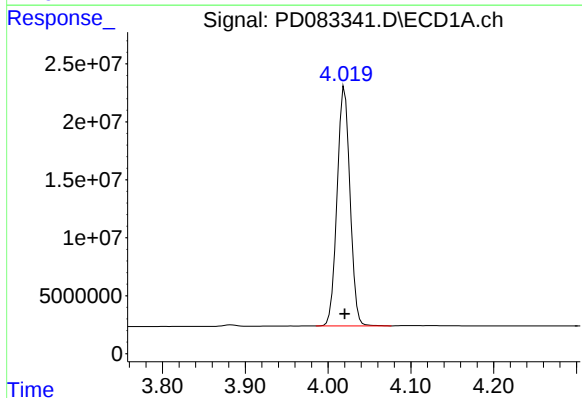


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 223412695
Conc: 89.77 ng/ml

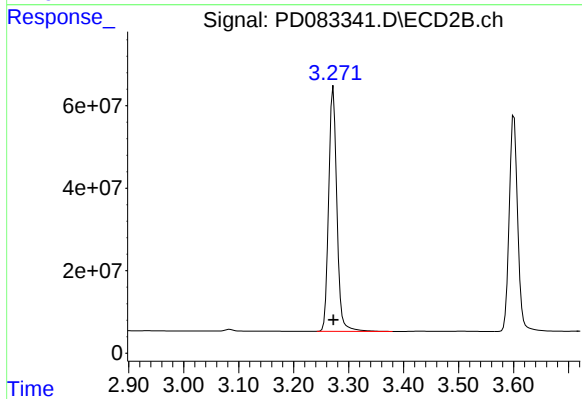


#2 alpha-BHC

R.T.: 3.272 min
Delta R.T.: 0.000 min
Response: 613287507
Conc: 83.81 ng/ml

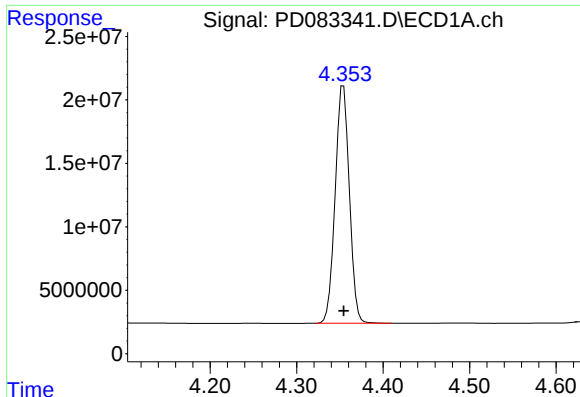


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 212283788
Conc: 88.43 ng/ml

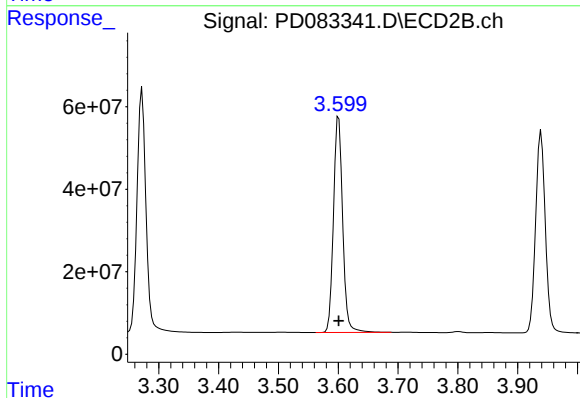


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 558942847
Conc: 82.25 ng/ml

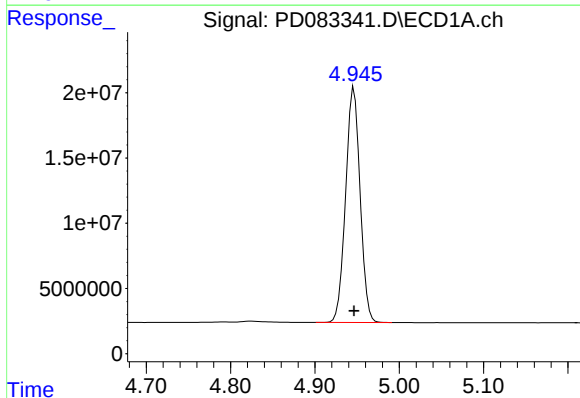


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 215231166
Conc: 86.72 ng/ml

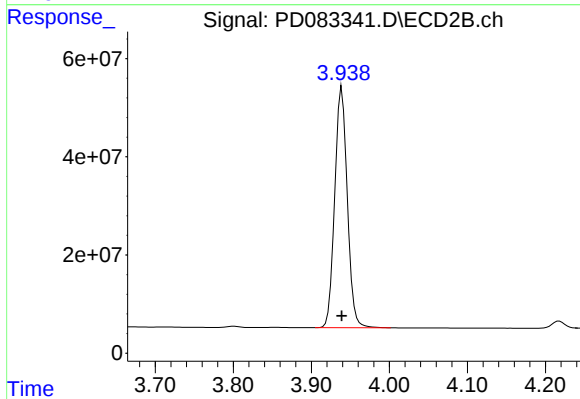


#4 Heptachlor

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 548282023
Conc: 81.01 ng/ml

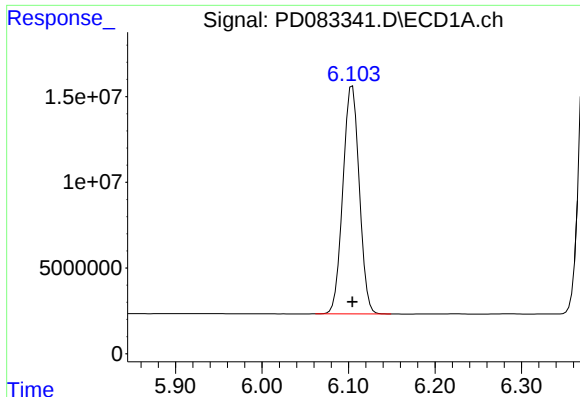


#9 Endosulfan I

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 174237381
Conc: 82.36 ng/ml

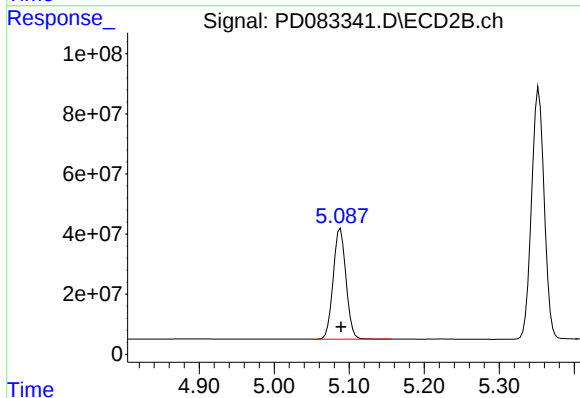


#9 Endosulfan I

R.T.: 5.088 min
Delta R.T.: 0.000 min
Response: 437565792
Conc: 80.08 ng/ml

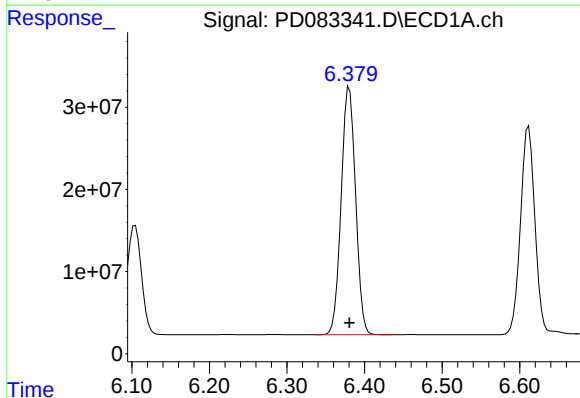


#13 Dieldrin

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 389333511
Conc: 174.77 ng/ml

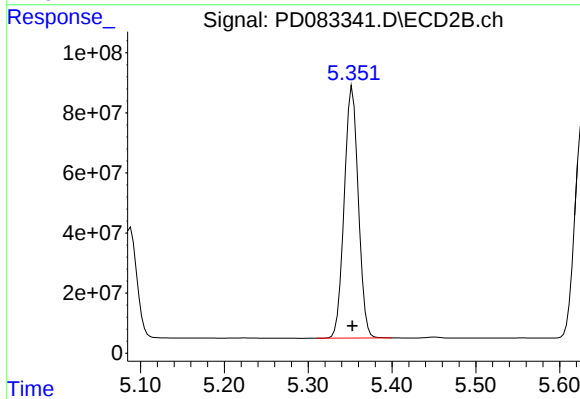


#13 Dieldrin

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 980098344
Conc: 159.76 ng/ml

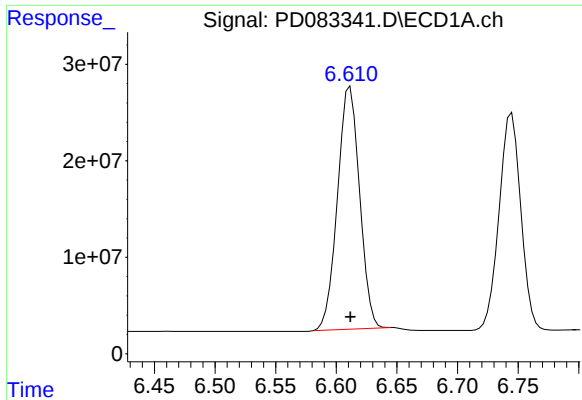


#14 Endrin

R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 318933763
Conc: 174.69 ng/ml

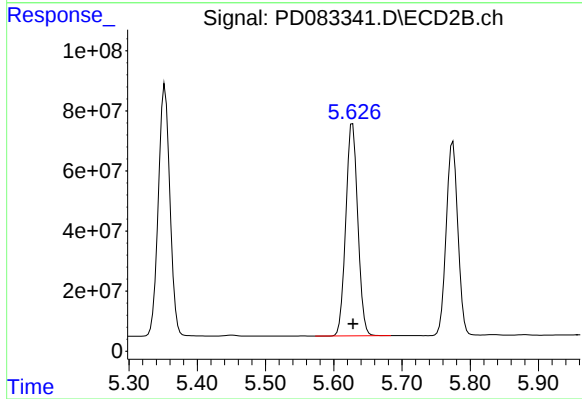


#14 Endrin

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 862089897
Conc: 158.89 ng/ml

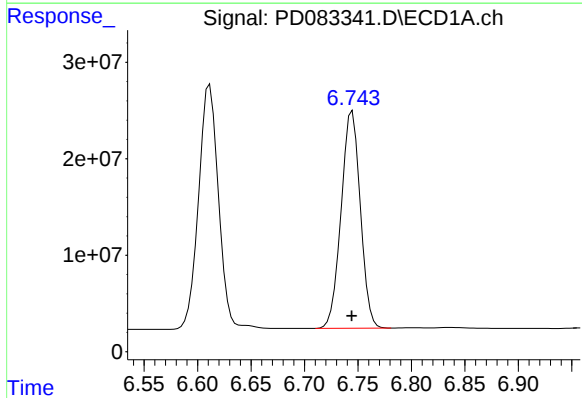


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 281549711
Conc: 179.61 ng/ml

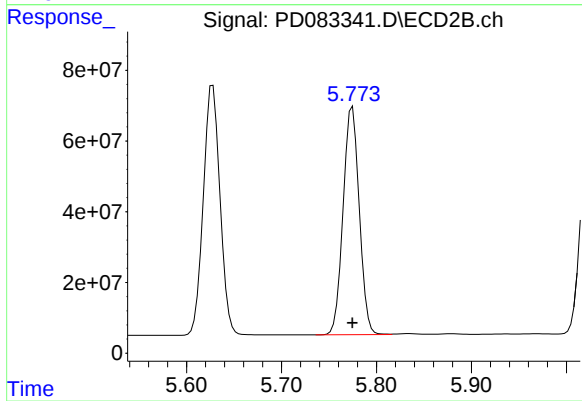


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 763112202
Conc: 163.54 ng/ml

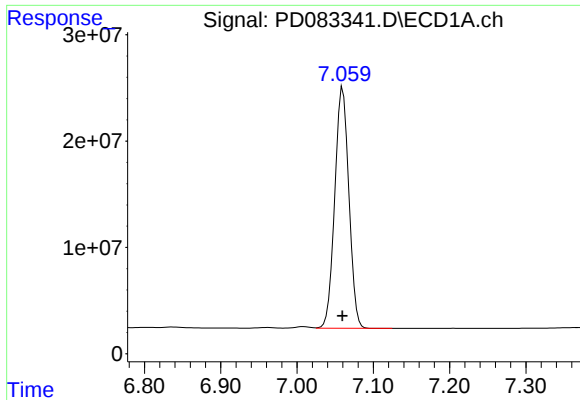


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 290998719
Conc: 182.07 ng/ml

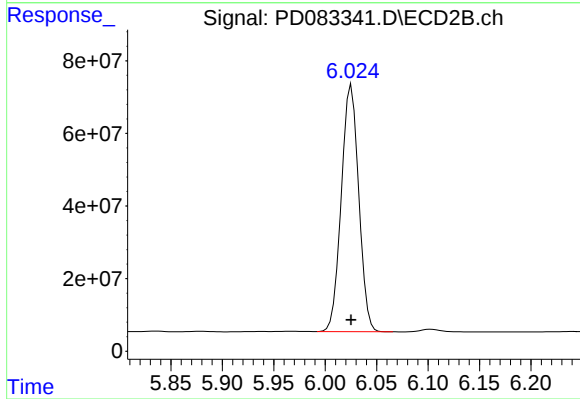


#17 4,4'-DDT

R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 801966003
Conc: 168.65 ng/ml

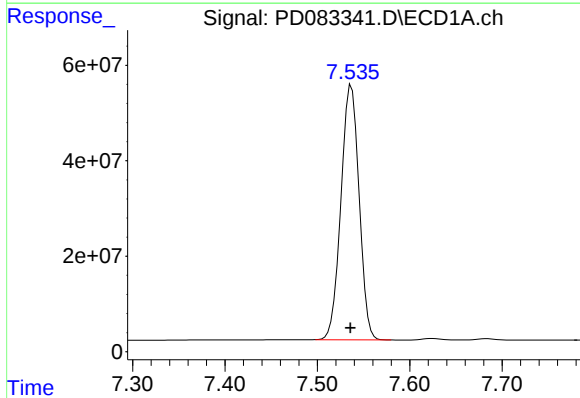


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.001 min
Response: 729665863
Conc: 803.99 ng/ml

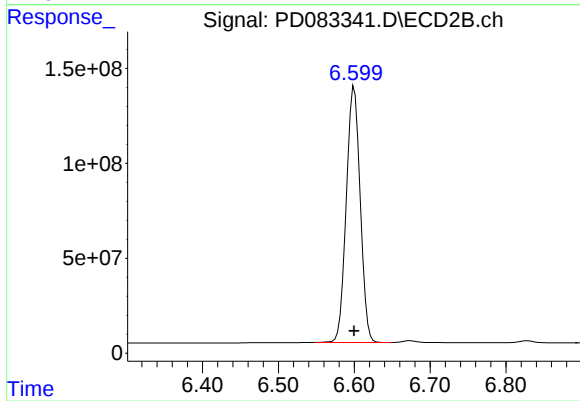


#20 Methoxychlor

R.T.: 6.600 min
Delta R.T.: 0.000 min
Response: 1721793851
Conc: 687.12 ng/ml

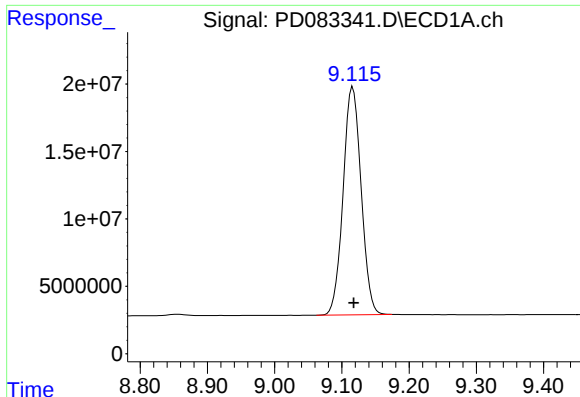

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.002 min
Response: 314530185
Conc: 154.76 ng/ml

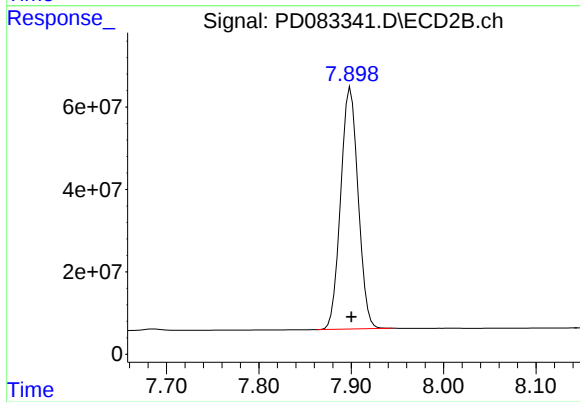

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: 0.000 min
Response: 771184240
Conc: 154.31 ng/ml