

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 00:16
 Operator : AR\AJ
 Sample : PIBLK158
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 07:09:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	26908262	88824123	18.756	18.753
27)	SA Decachlor...	9.116	7.900	43135297	106.3E6	21.109	21.308
Target Compounds							
2)	A alpha-BHC	0.000	3.301f	0	262025	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.578	0	134754	N.D.	<MDL
5)	MB Aldrin	0.000	4.261f	0	464167	N.D.	<MDL
6)	B beta-BHC	0.000	3.853f	0	2451548	N.D.	0.833
7)	B delta-BHC	4.791	4.124	1390533	361152	0.526	<MDL #
8)	B Heptachlo...	0.000	4.743	0	1195422	N.D.	0.201
9)	A Endosulfan I	0.000	5.090	0	114788	N.D.	<MDL
10)	B trans-Chl...	0.000	4.904f	0	2376462	N.D.	0.406
11)	B cis-Chlor...	0.000	5.090f	0	114788	N.D.	<MDL
12)	B 4,4'-DDE	0.000	5.168f	0	158540	N.D.	<MDL
14)	MA Endrin	0.000	5.645	0	298920	N.D.	<MDL
15)	B Endosulfa...	0.000	5.880f	0	229328	N.D.	<MDL
18)	B Endrin al...	0.000	6.110	0	609108	N.D.	0.159
19)	B Endosulfa...	0.000	6.320	0	79204	N.D.	<MDL
20)	A Methoxychlor	0.000	6.575	0	298801	N.D.	0.122
21)	B Endrin ke...	0.000	6.836	0	48513	N.D.	<MDL
23)	Toxaphene-2	0.000	5.664	0	74799	N.D.	2.245
24)	Toxaphene-3	0.000	6.575	0	298801	N.D.	2.846
25)	Toxaphene-4	0.000	6.722	0	295095	N.D.	1.981
26)	Toxaphene-5	0.000	7.044	0	255195	N.D.	4.634


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 00:16
Operator : AR\AJ
Sample : PIBLK158
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 07:09:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

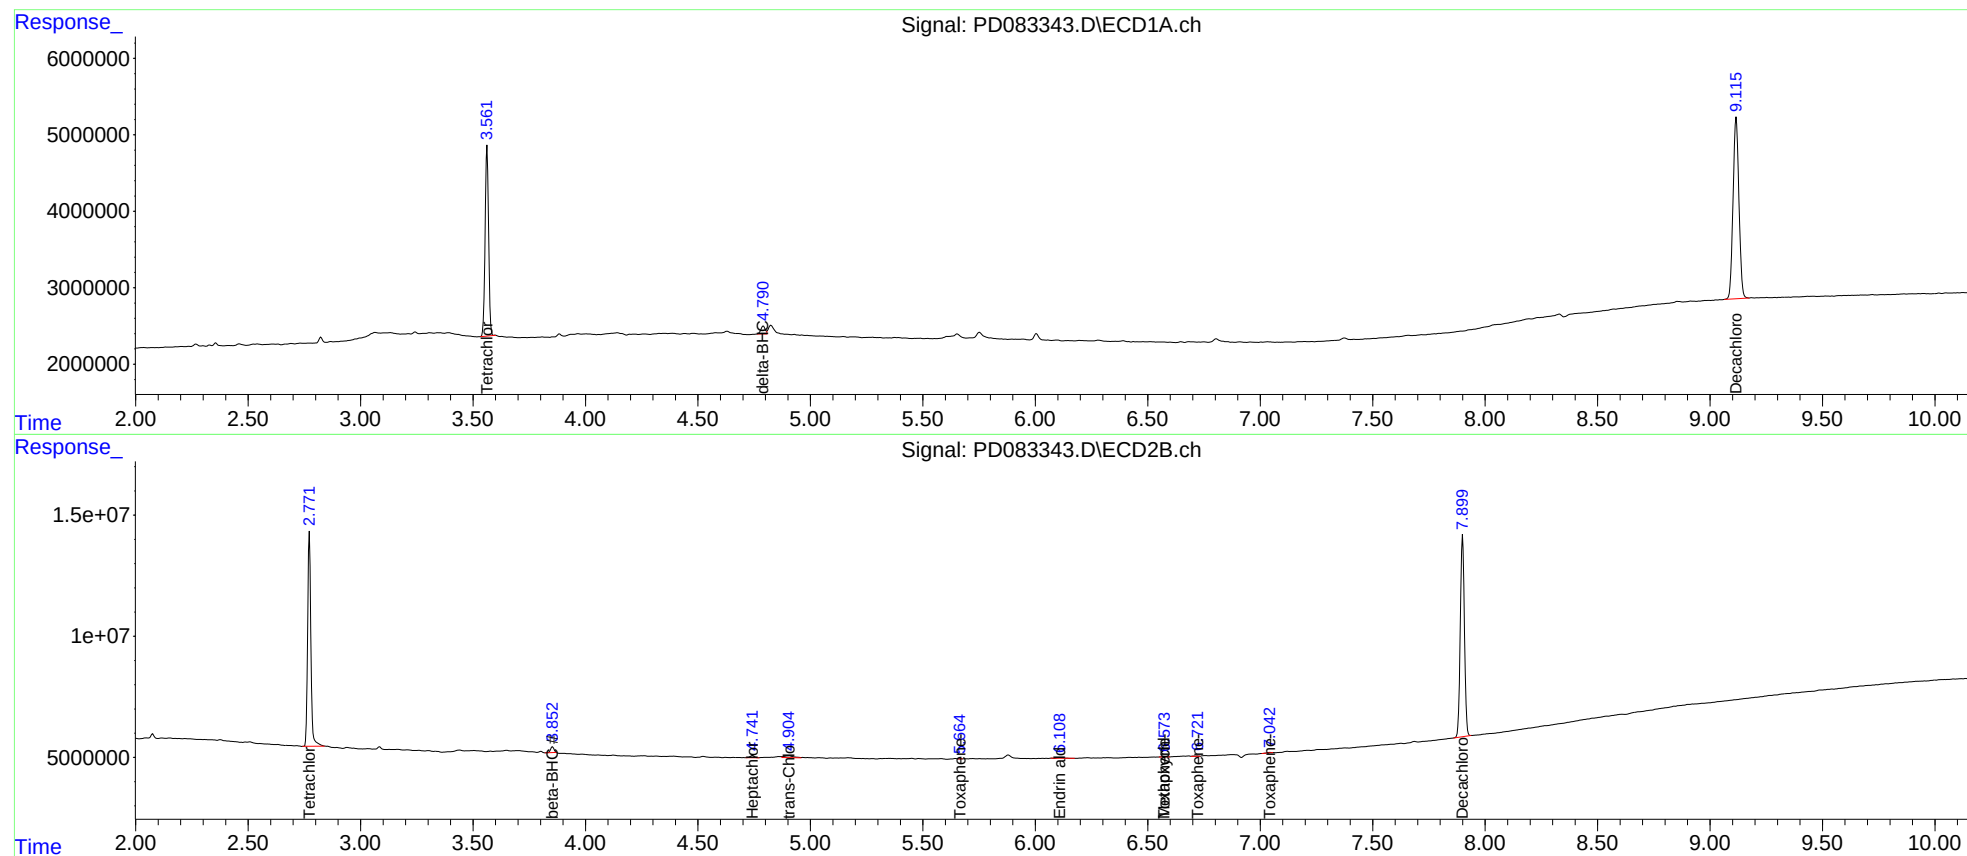

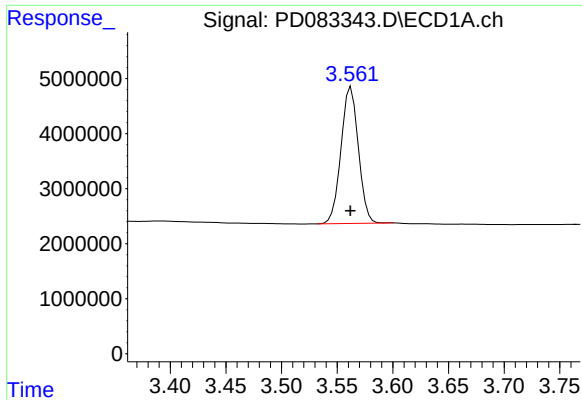


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 26908262
Conc: 18.76 ng/ml

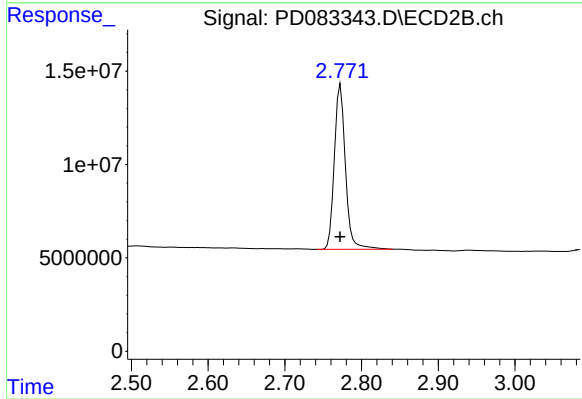


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 88824123
Conc: 18.75 ng/ml

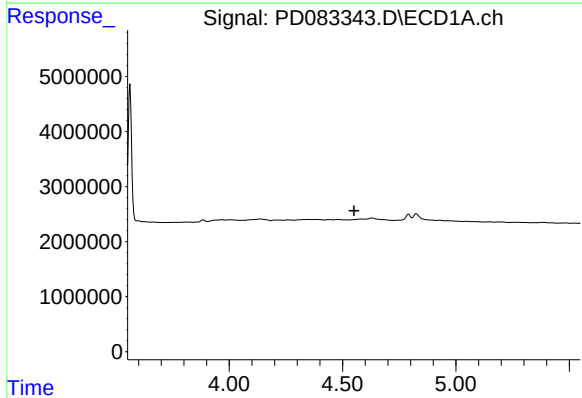


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

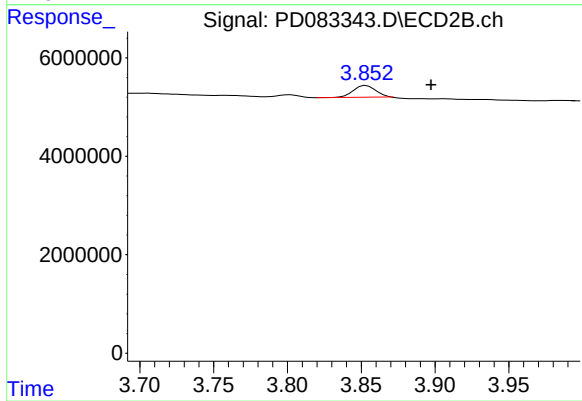


#6 beta-BHC

R.T.: 3.853 min
Delta R.T.: -0.044 min
Response: 2451548
Conc: 0.83 ng/ml

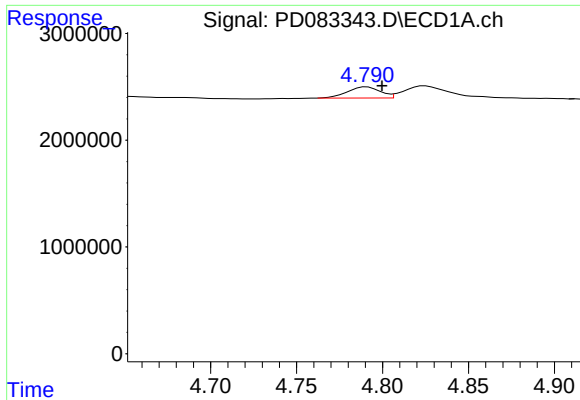


#7 delta-BHC

R.T.: 4.791 min
Delta R.T.: -0.009 min
Response: 1390533
Conc: 0.53 ng/ml

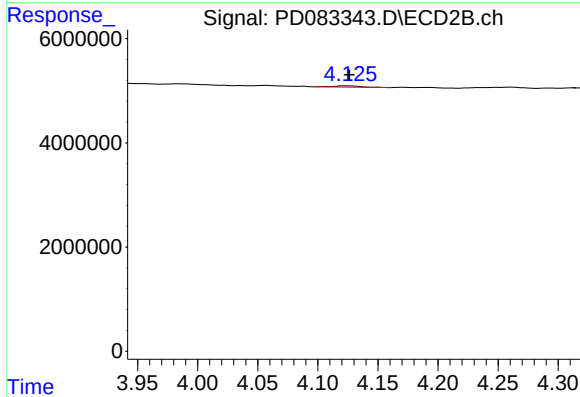


#7 delta-BHC

R.T.: 4.124 min
Delta R.T.: -0.002 min
Response: 361152
Conc: N.D.

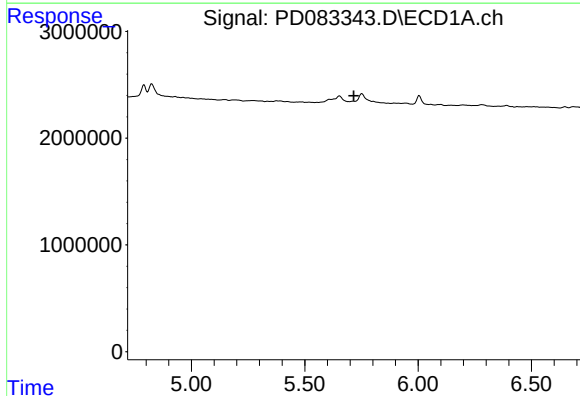


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.717 min
Response: 0
Conc: N.D.

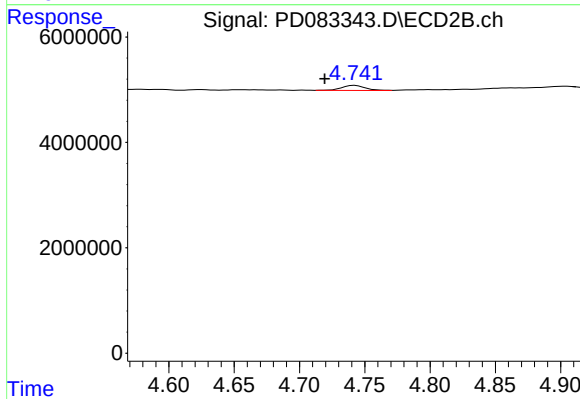


#8 Heptachlor epoxide

R.T.: 4.743 min
Delta R.T.: 0.023 min
Response: 1195422
Conc: 0.20 ng/ml

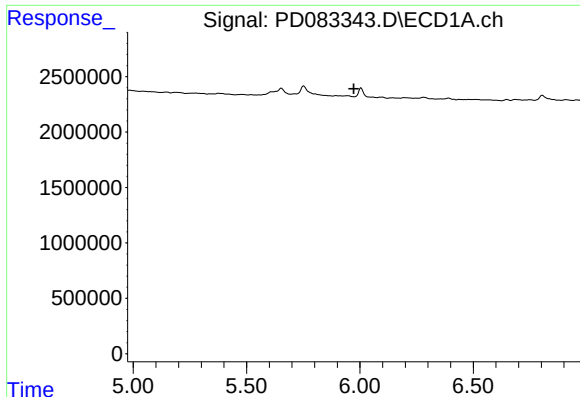


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

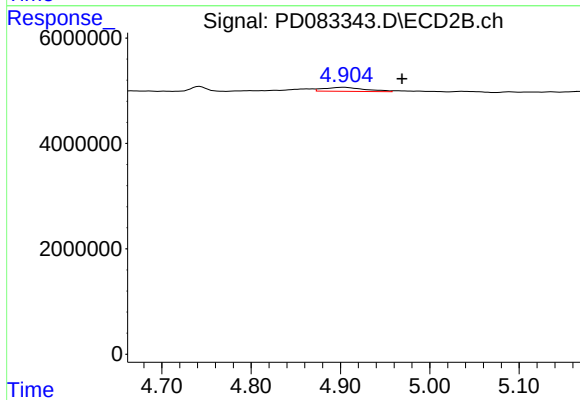


#10 trans-Chlordane

R.T.: 4.904 min
Delta R.T.: -0.065 min
Response: 2376462
Conc: 0.41 ng/ml

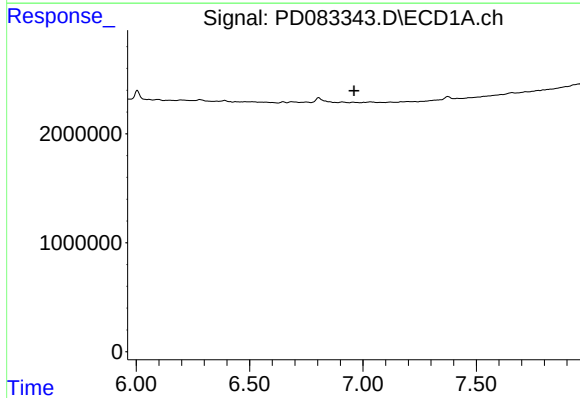


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.961 min
Response: 0
Conc: N.D.

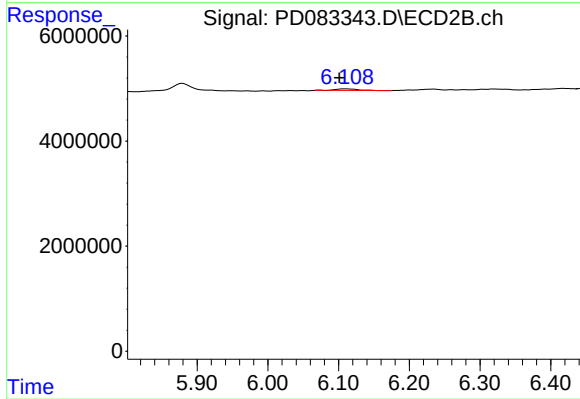


#18 Endrin aldehyde

R.T.: 6.110 min
Delta R.T.: 0.009 min
Response: 609108
Conc: 0.16 ng/ml

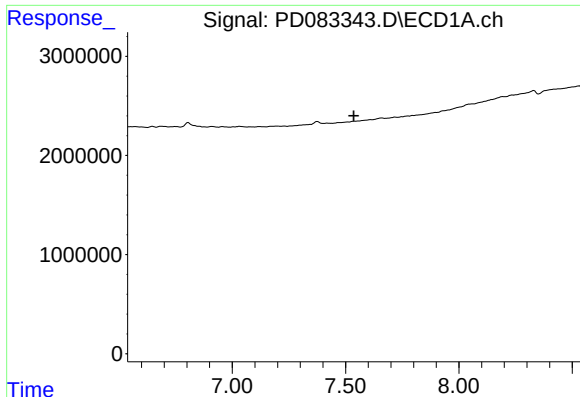


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.537 min
Response: 0
Conc: N.D.

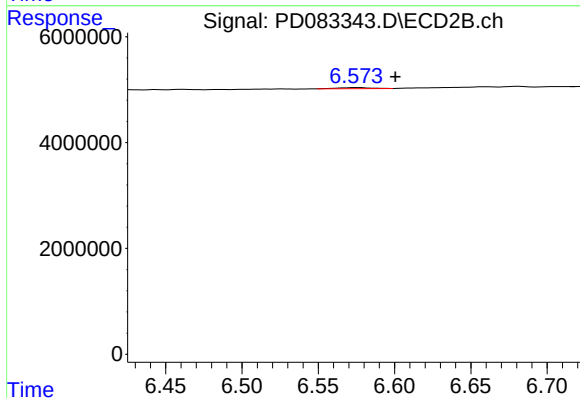


#20 Methoxychlor

R.T.: 6.575 min
Delta R.T.: -0.025 min
Response: 298801
Conc: 0.12 ng/ml

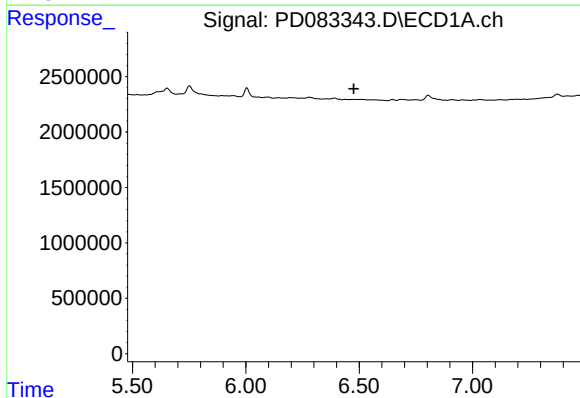


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.477 min
Response: 0
Conc: N.D.

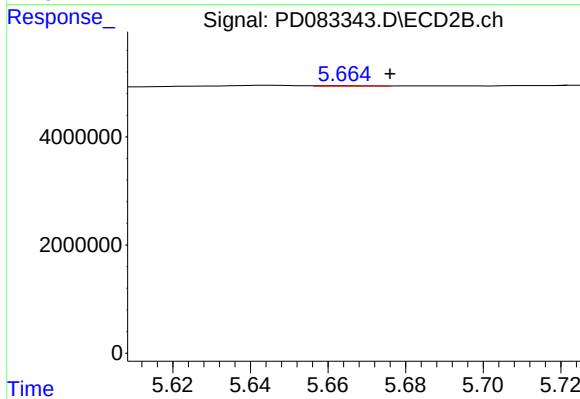


#23 Toxaphene-2

R.T.: 5.664 min
Delta R.T.: -0.012 min
Response: 74799
Conc: 2.24 ng/ml

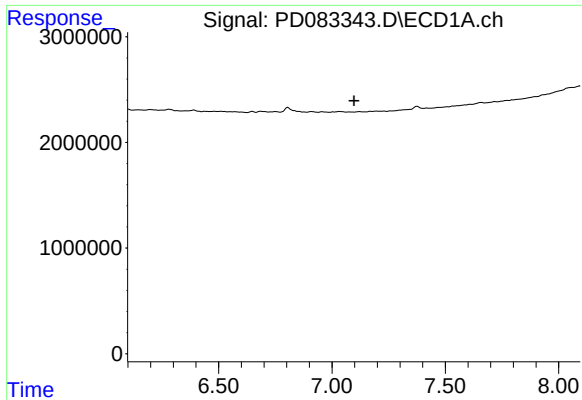


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 7.097 min
Response: 0
Conc: N.D.

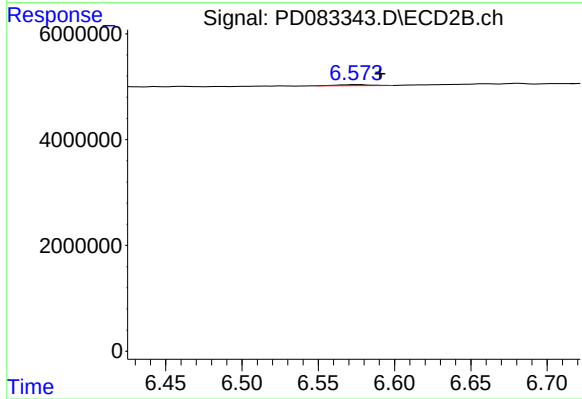


#24 Toxaphene-3

R.T.: 6.575 min
Delta R.T.: -0.015 min
Response: 298801
Conc: 2.85 ng/ml

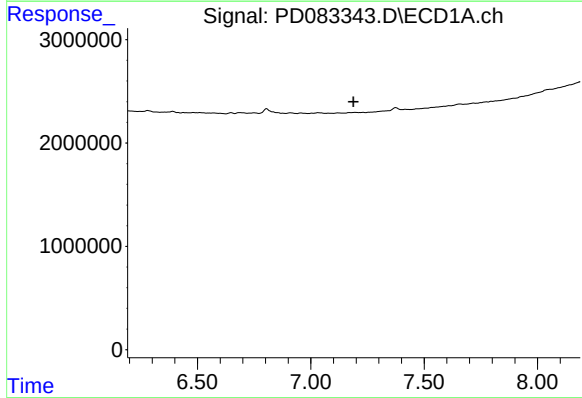


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.189 min
Response: 0
Conc: N.D.

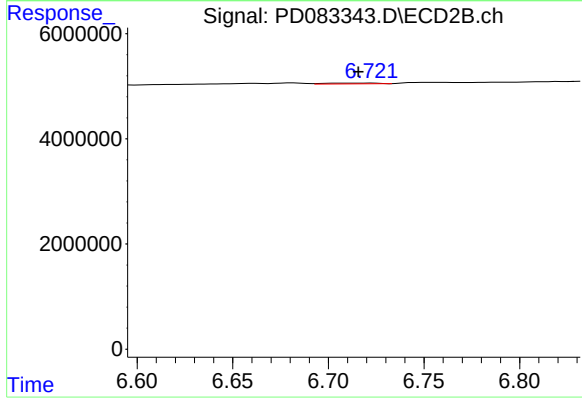


#25 Toxaphene-4

R.T.: 6.722 min
Delta R.T.: 0.006 min
Response: 295095
Conc: 1.98 ng/ml

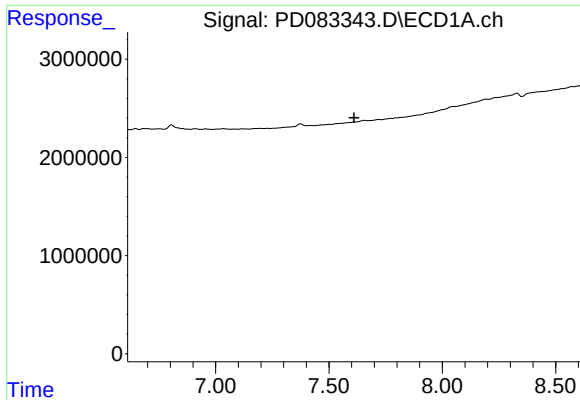


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.611 min
Response: 0
Conc: N.D.

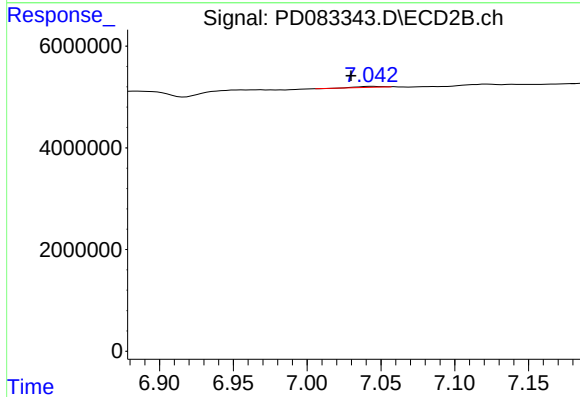


#26 Toxaphene-5

R.T.: 7.044 min
Delta R.T.: 0.015 min
Response: 255195
Conc: 4.63 ng/ml

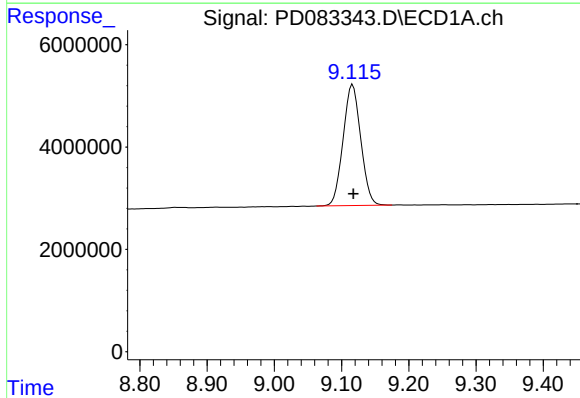

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.001 min
Response: 43135297
Conc: 21.11 ng/ml

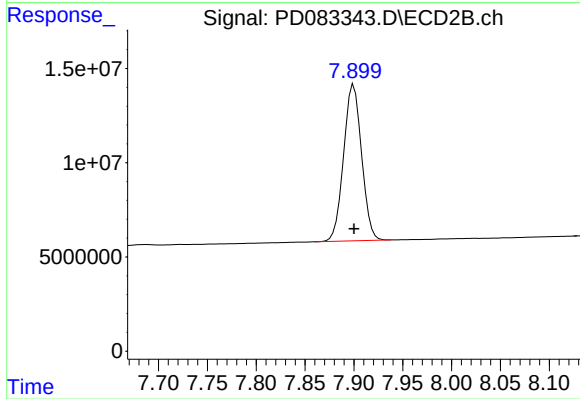

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 106268907
Conc: 21.31 ng/ml