

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2024 20:30
 Operator : AR\AJ
 Sample : RESC032
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC034

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 07:08:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.772	28497782	94821860	19.864	20.019
2)	SA Decachlor...	9.117	7.900	81090958	193.3E6	39.683	38.761
Target Compounds							
2)	A alpha-BHC	4.020	3.272	22565493	68752689	8.978	9.488
3)	MA gamma-BHC...	4.354	3.601	22089705	63026682	9.085	9.286
4)	MA Heptachlor	4.947	3.939	23114097	63649431	9.154	9.445
5)	MB Aldrin	5.290	4.218	24723186	67444999	10.206	10.416
6)	B beta-BHC	4.551	3.897	11004666	30681458	10.267	10.423
7)	B delta-BHC	4.800	4.126	26340004	72049877	9.962	10.226
8)	B Heptachlo...	5.718	4.719	21923942	61158851	9.982	10.270
9)	A Endosulfan I	6.105	5.089	20199468	52934955	9.508	9.710
10)	B trans-Chl...	5.975	4.969	21865028	59471598	10.078	10.169
11)	B cis-Chlor...	6.054	5.033	22420777	60721023	10.106	10.187
12)	B 4,4'-DDE	6.227	5.221	44391709	116.9E6	19.989	20.469
13)	MA Dieldrin	6.381	5.352	41612842	114.3E6	18.402	18.838
14)	MA Endrin	6.612	5.629	34355074	101.7E6	18.459	18.971
15)	B Endosulfa...	6.832	5.922	39878933	102.4E6	20.504	20.450
16)	A 4,4'-DDD	6.745	5.775	29594068	87245101	18.420	18.832
17)	MA 4,4'-DDT	7.061	6.025	31167800	85909202	19.084	18.396
18)	B Endrin al...	6.962	6.101	28310020	76450865	19.614	19.939
19)	B Endosulfa...	7.198	6.323	38039079	100.7E6	20.821	20.707
20)	A Methoxychlor	7.537	6.600	89344861	245.3E6	97.189	100.364
21)	B Endrin ke...	7.685	6.829	39453450	112.5E6	20.544	21.080

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 20:30
Operator : AR\AJ
Sample : RESC032
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 07:08:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

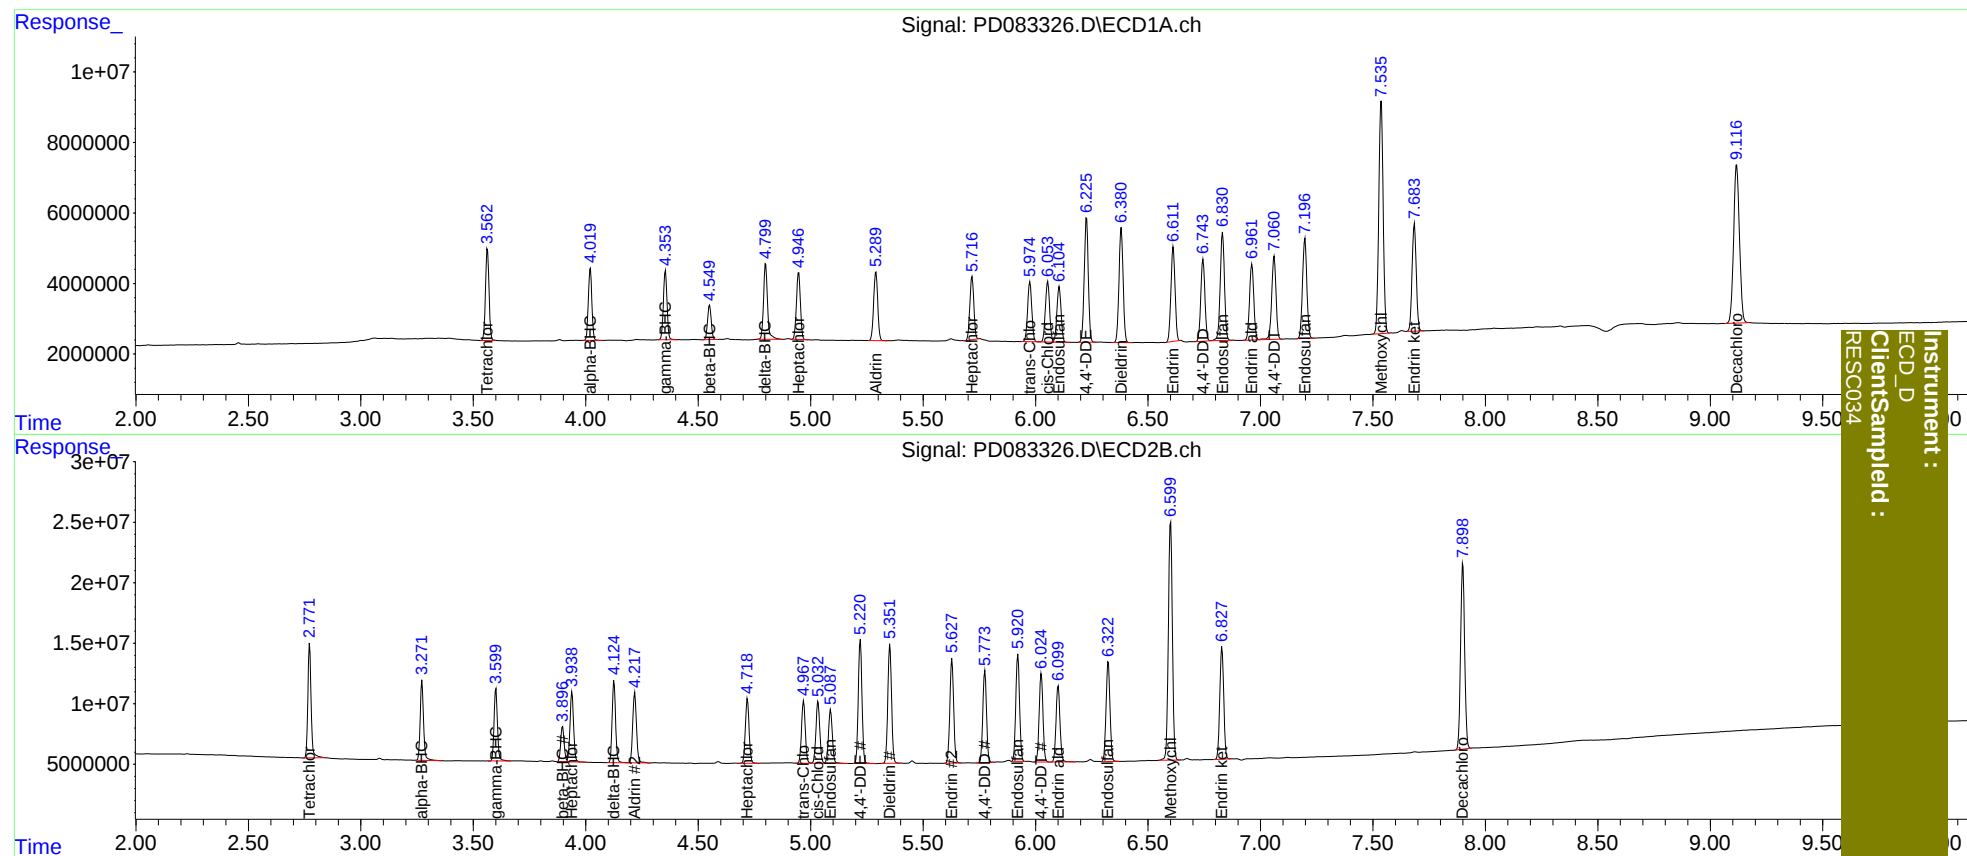

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083326.D
Acq On : 03 Jun 2024 20:30
Operator : AR\AJ
Sample : RESC032
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC034

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Title : GC Extractables
Last Update : Tue Jun 04 07:04:40 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.563	4.020	100.00%
4.020	4.354	100.00%
4.354	4.551	100.00%
4.551	4.800	100.00%
4.800	4.947	100.00%
4.947	5.290	100.00%
5.290	5.718	100.00%
5.718	5.975	100.00%
5.975	6.054	100.00%
6.054	6.105	97.63%
6.105	6.227	100.00%
6.227	6.381	100.00%
6.381	6.612	100.00%
6.612	6.745	100.00%
6.745	6.832	100.00%
6.832	6.962	100.00%
6.962	7.061	100.00%
7.061	7.198	100.00%
7.198	7.537	100.00%
7.537	7.685	100.00%
7.685	9.117	100.00%

Signal #2


2.772	3.272	100.00%
3.272	3.601	100.00%
3.601	3.897	100.00%
3.897	3.939	94.85%
3.939	4.126	100.00%
4.126	4.218	100.00%
4.218	4.719	100.00%
4.719	4.969	100.00%
4.969	5.033	100.00%
5.033	5.089	100.00%
5.089	5.221	100.00%
5.221	5.352	100.00%
5.352	5.629	100.00%
5.629	5.775	100.00%
5.775	5.922	100.00%
5.922	6.025	100.00%
6.025	6.101	100.00%
6.101	6.323	100.00%
6.323	6.600	100.00%
6.600	6.829	100.00%
6.829	7.900	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 20:30
Operator : AR\AJ
Sample : RESC032
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC034

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 07:08:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

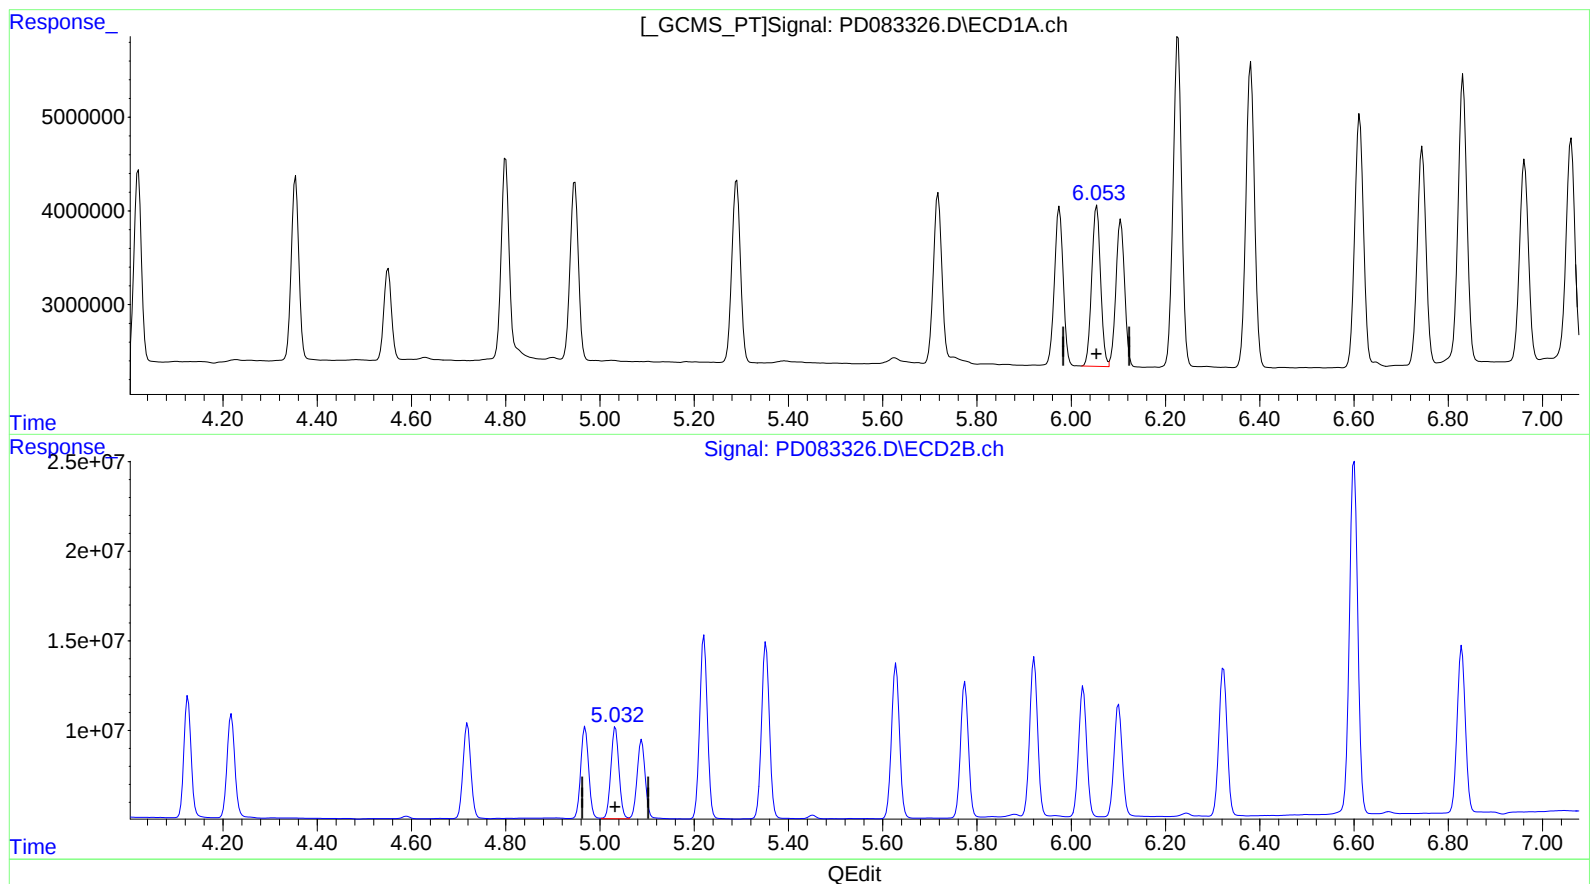

(11) cis-Chlordane (B)

6.054min 10.106 ng/ml

response 22420777

(11) cis-Chlordane #2 (B)

5.033min 10.187 ng/ml


response 60721023

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2024 20:30
Operator : AR\AJ
Sample : RESC032
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC034

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 07:08:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

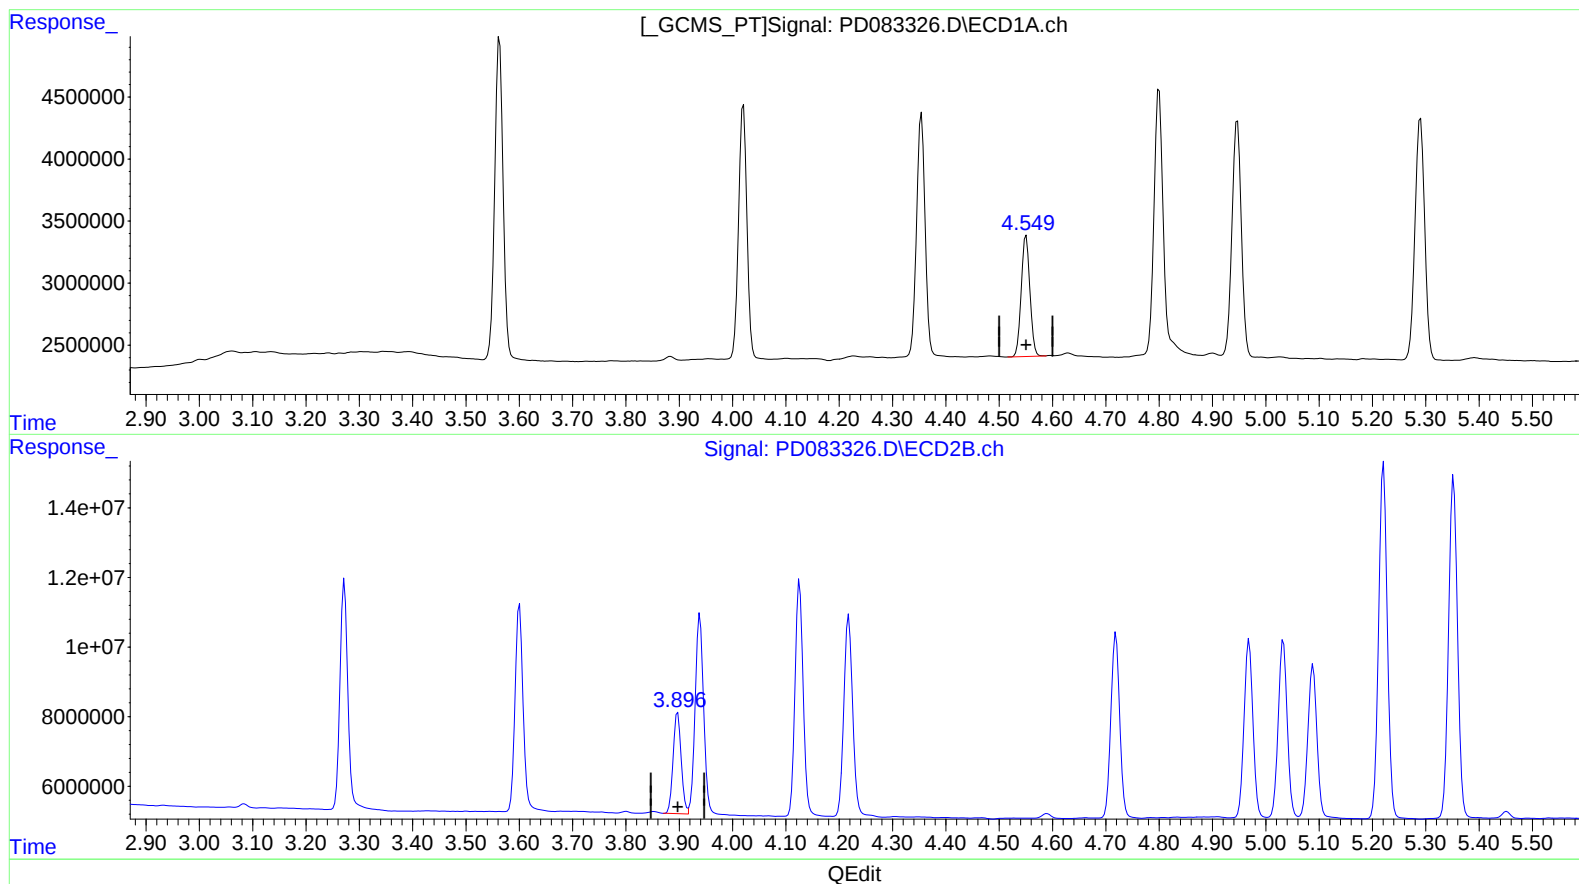

(6) beta-BHC (B)

4.551min 10.267 ng/ml

response 11004666

(6) beta-BHC #2 (B)

3.897min 10.423 ng/ml

response 30681458