

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 12:57
 Operator : AR\AJ
 Sample : P2647-01DL2 50X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5T4DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2024
 Supervised By : Ankita Jodhani 06/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 21:33:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
10) B	trans-Chl...	5.972	4.967	2193176	4942167	1.011m 0.845m
12) B	4,4'-DDE	6.225	5.221	27110068	78804749	12.207 13.793
14) MA	Endrin	6.644	5.636	37053140	103.3E6	19.908m 19.263m
17) MA	4,4'-DDT	7.058	6.025	206.2E6	602.2E6	126.277m 128.951

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 12:57
Operator : AR\AJ
Sample : P2647-01DL2 50X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 21:33:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

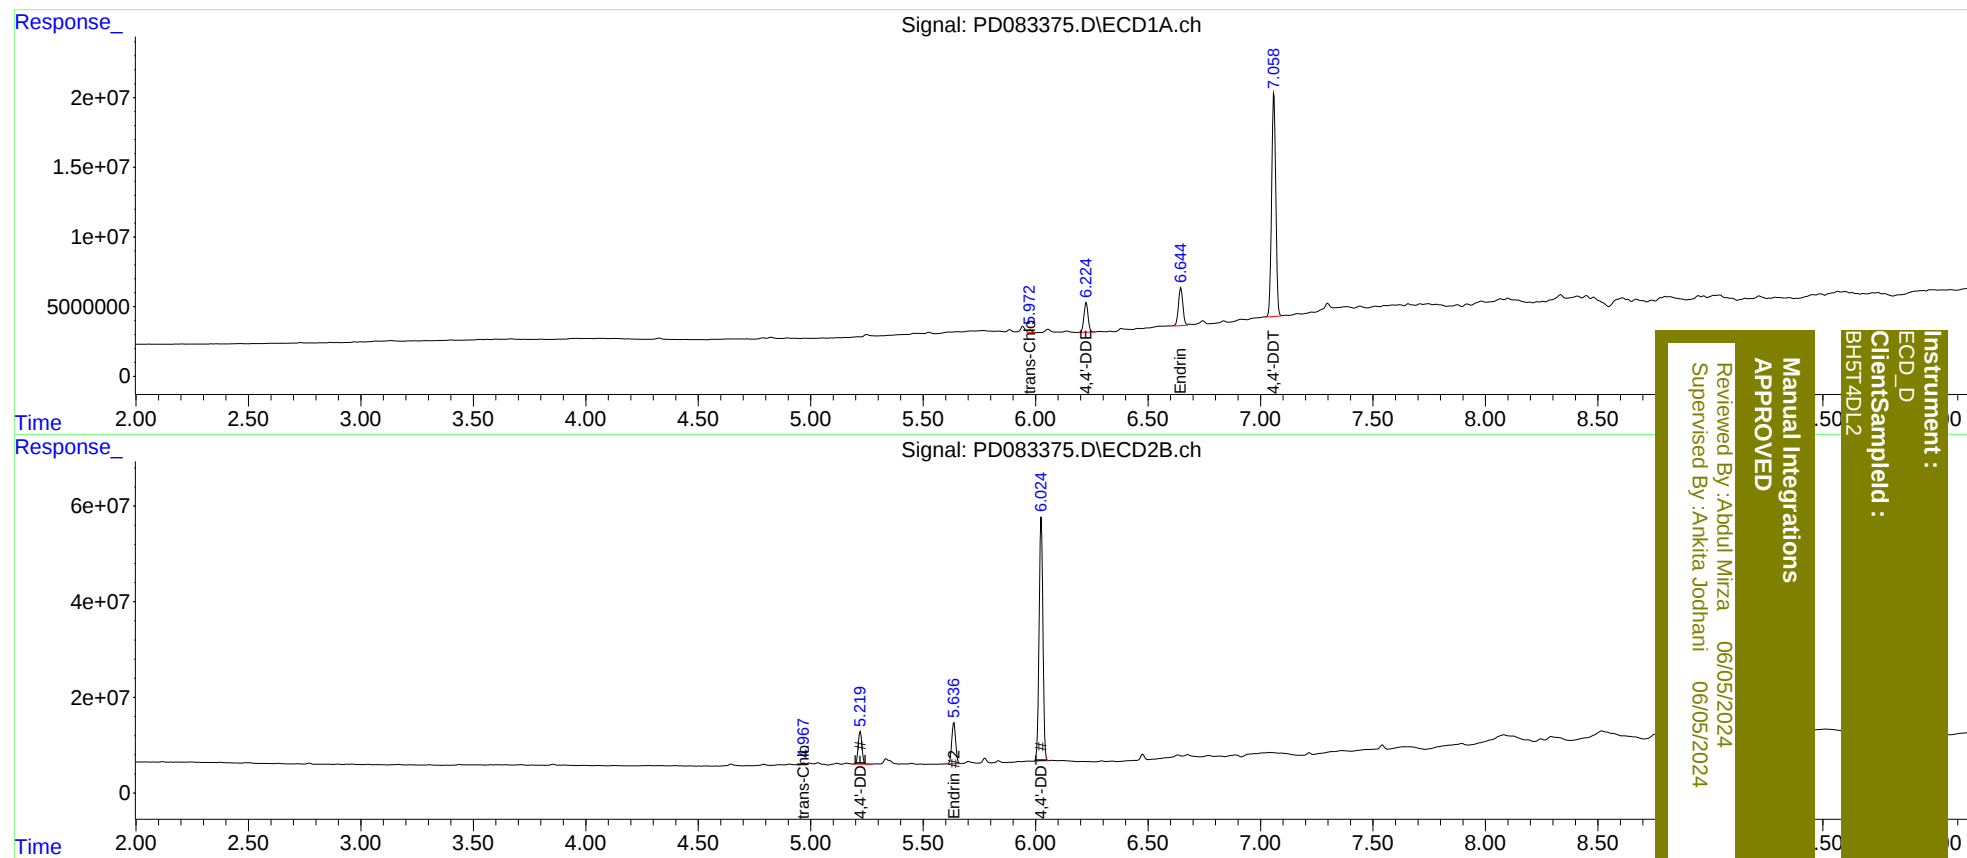

Instrument :
ECD_D
Client Sampled :
BH5T4DL2

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/05/2024
Supervised By : Ankita Jodhani 06/05/2024