

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
 Data File : PD083380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 15:10
 Operator : AR\AJ
 Sample : P2647-13DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHBS7DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/05/2024
 Supervised By : Ankita Jodhani 06/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 21:35:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.564	2.772	5252492	29468217	3.661m	6.221m#
27) SA Decachlor...	9.106	7.898	23454599	69242389	11.478m	13.883
Target Compounds						
12) B 4,4'-DDE	6.225	5.221	220.3E6	740.6E6	99.217	129.620 #
16) A 4,4'-DDD	6.731	5.775	17282408	40692916	10.757m	8.784m
17) MA 4,4'-DDT	7.060	6.024	161.3E6	442.9E6	98.789	94.827

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060424\
Data File : PD083380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 15:10
Operator : AR\AJ
Sample : P2647-13DL 2X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 21:35:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

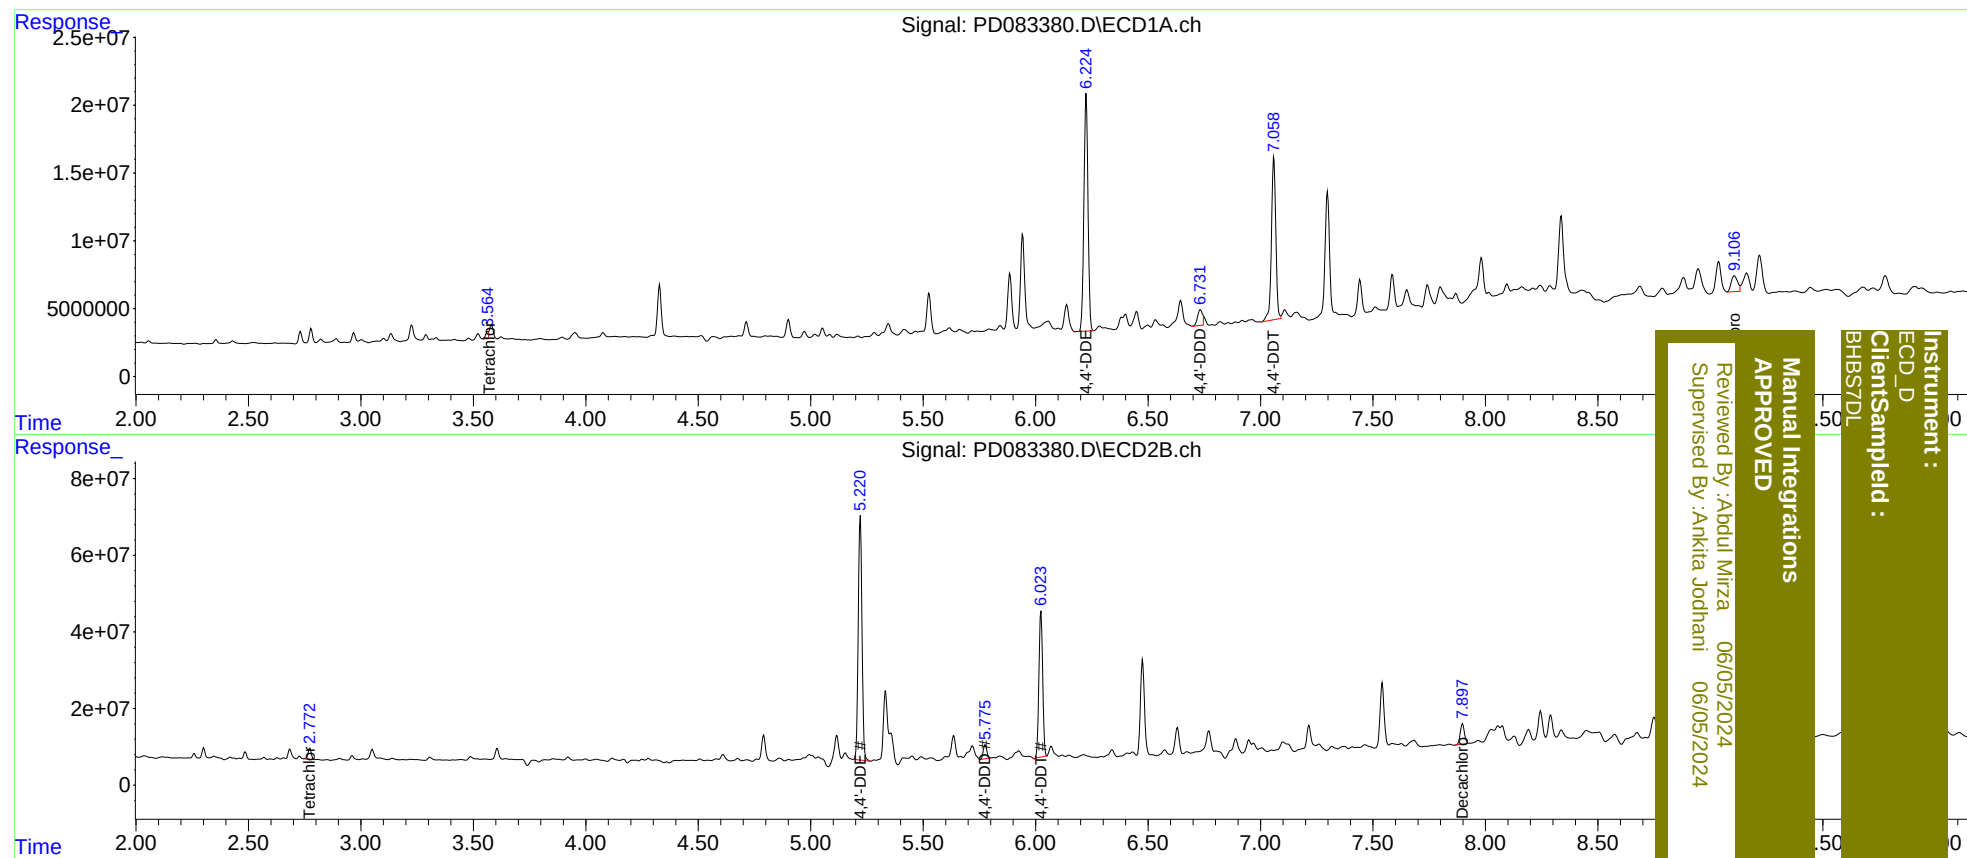

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/05/2024
Supervised By: Ankita Jodhani 06/05/2024

Instrument :
ECD_D
Client Sampled :
BHBSTDL