

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060521\
 Data File : PD063470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2021 13:59
 Operator : AR\AJ
 Sample : M2598-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 23

Manual Integrations
 APPROVED

Ankita
 6/7/2021 8:42:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:43:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	17257364	178.7E6	12.472	13.338
28)	SA Decachlor...	8.195	9.024	21918982	172.2E6	13.937m	12.461m
Target Compounds							
12)	B 4,4'-DDE	5.599	6.304	2785916	32972143	1.602m	1.814
17)	MA 4,4'-DDT	6.356	7.094	2672797	15654028	1.850m	1.040 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060521\
Data File : PD063470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2021 13:59
Operator : AR\AJ
Sample : M2598-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
23


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:43:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

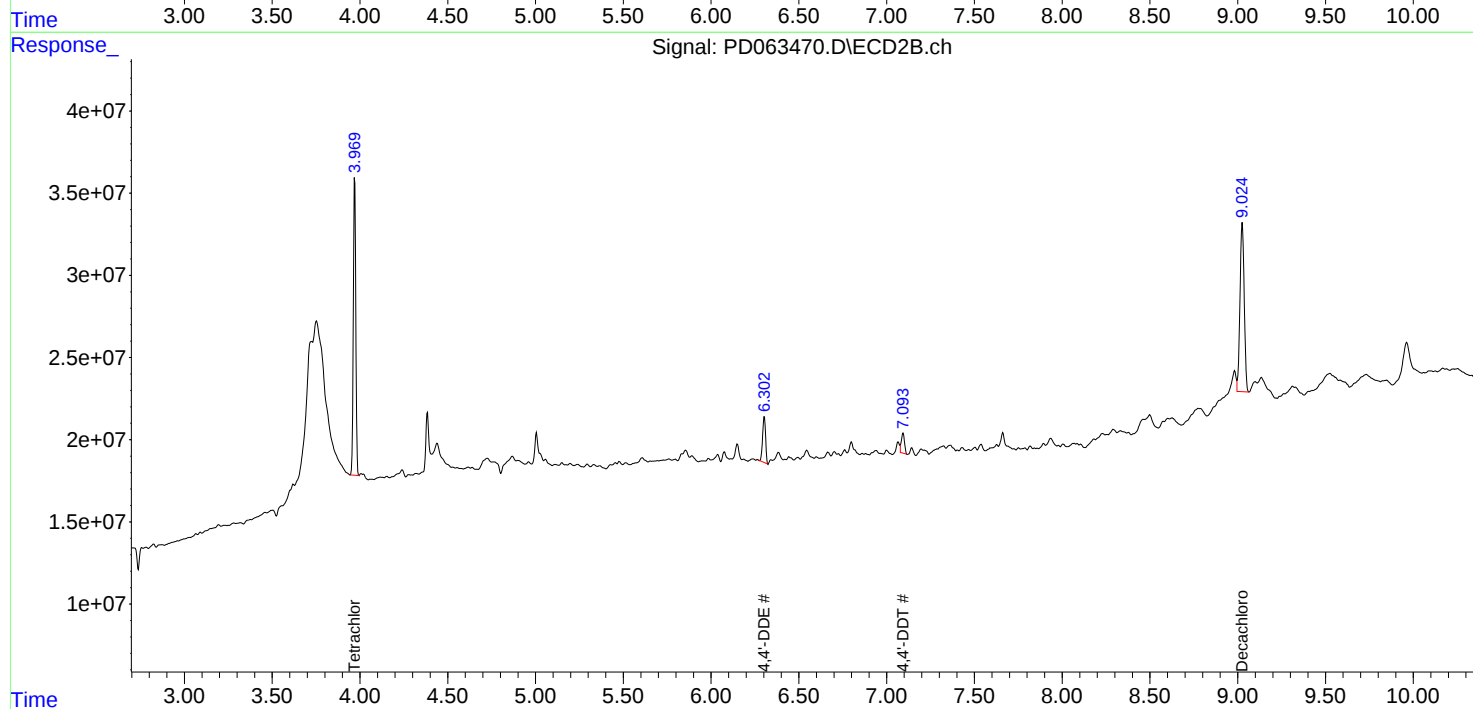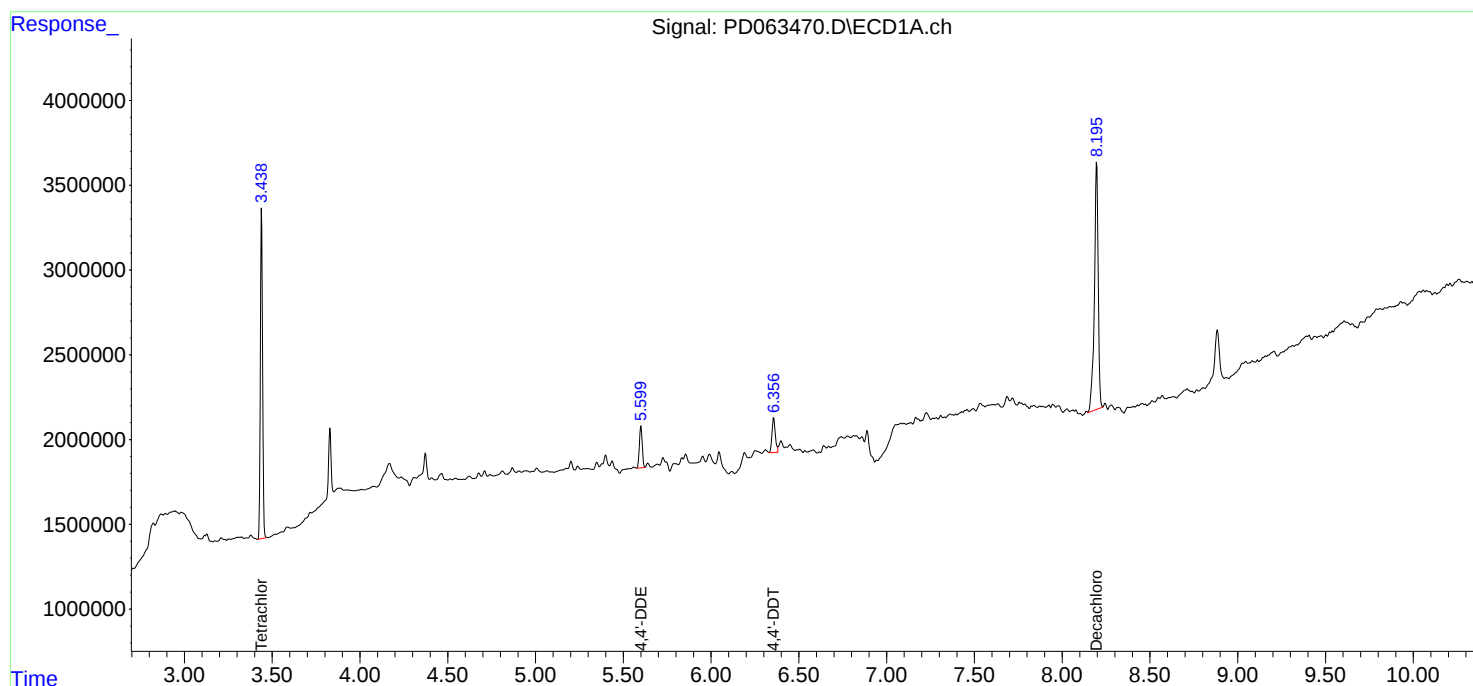

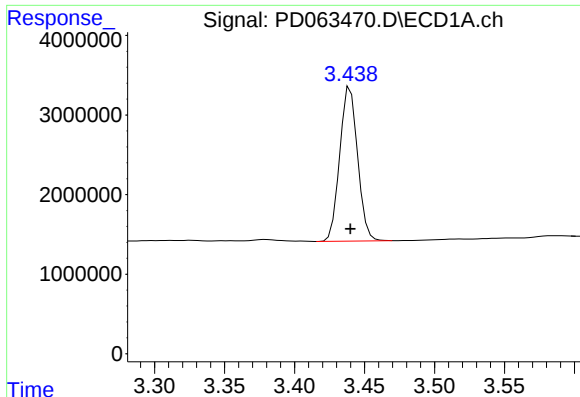


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 17257364
Conc: 12.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
23


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:04 AM

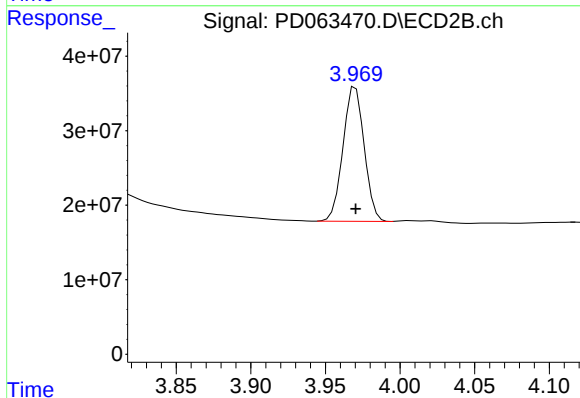


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 178712277
Conc: 13.34 ng/ml

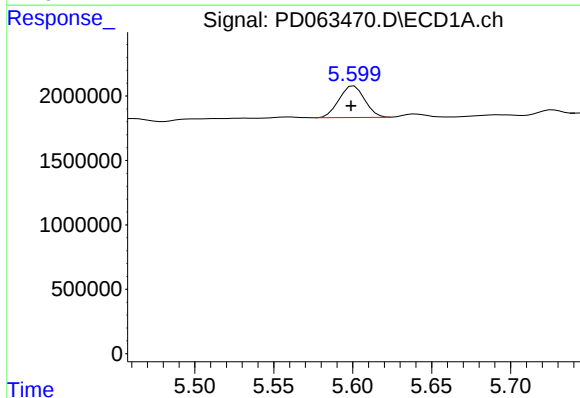


#12 4,4'-DDE

R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 2785916
Conc: 1.60 ng/ml m

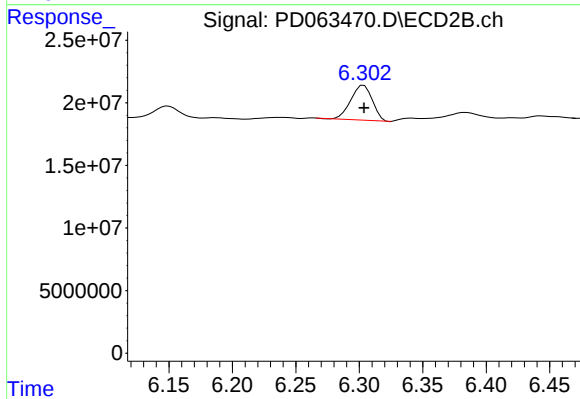

#12 4,4'-DDE

R.T.: 6.304 min
Delta R.T.: 0.000 min
Response: 32972143
Conc: 1.81 ng/ml

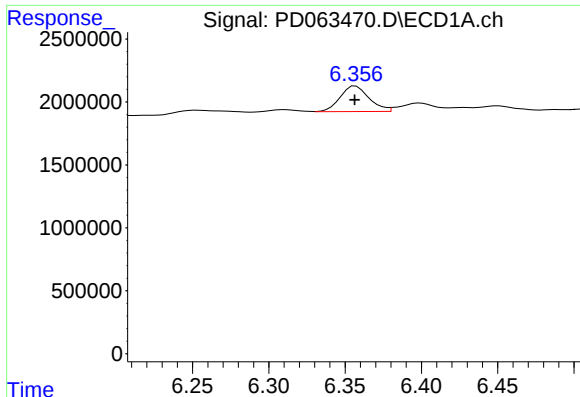


#17 4,4'-DDT

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 2672797
Conc: 1.85 ng/ml m

Instrument :
ECD_D
ClientSampleId :
23


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:04 AM

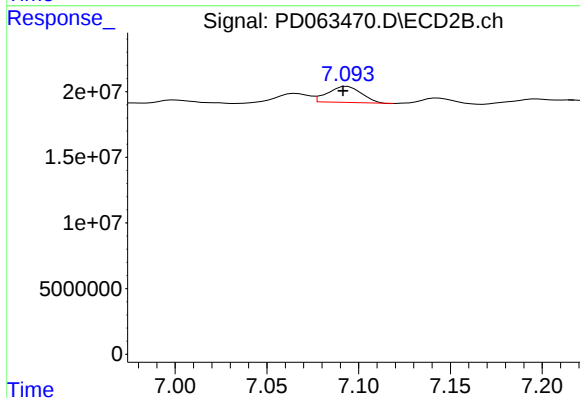


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.002 min
Response: 15654028
Conc: 1.04 ng/ml

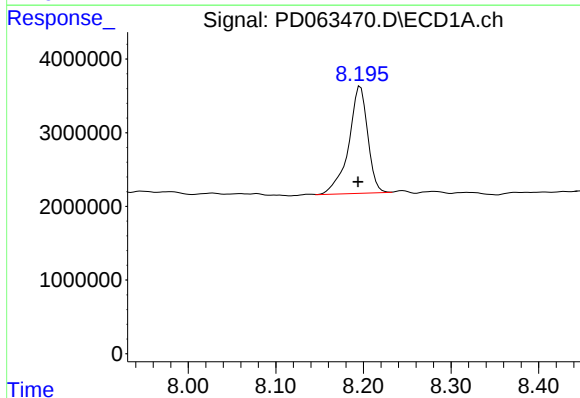

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.001 min
Response: 21918982
Conc: 13.94 ng/ml m

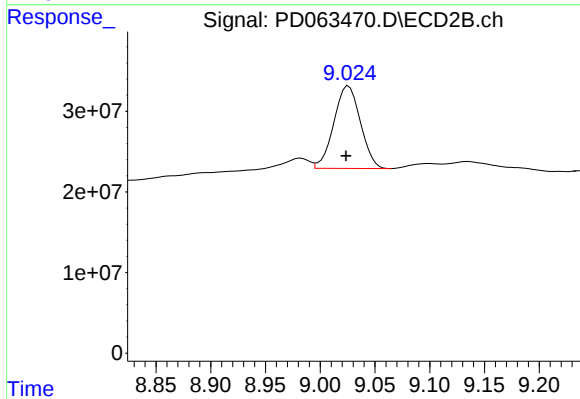

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 172192747
Conc: 12.46 ng/ml m