

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060521\
 Data File : PD063476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2021 15:23
 Operator : AR\AJ
 Sample : M2599-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 339

Manual Integrations
 APPROVED

Ankita
 6/7/2021 8:42:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:46:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	23182731	234.0E6	16.754	17.464
28)	SA Decachlor...	8.197	9.028	26453795	243.4E6	16.821	17.614
Target Compounds							
17)	MA 4,4'-DDT	6.356	7.093	4528224	22710305	3.134m	1.509 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060521\
Data File : PD063476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2021 15:23
Operator : AR\AJ
Sample : M2599-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
339


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:46:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

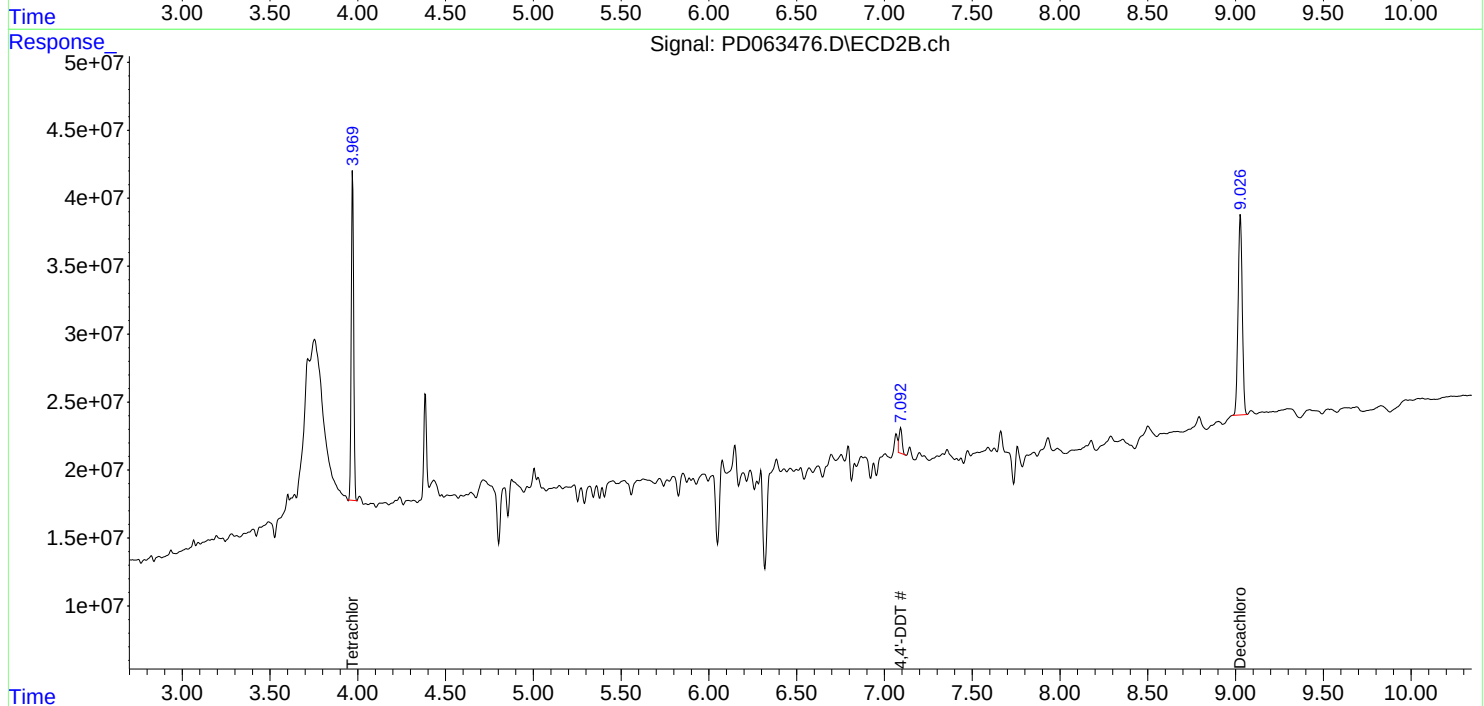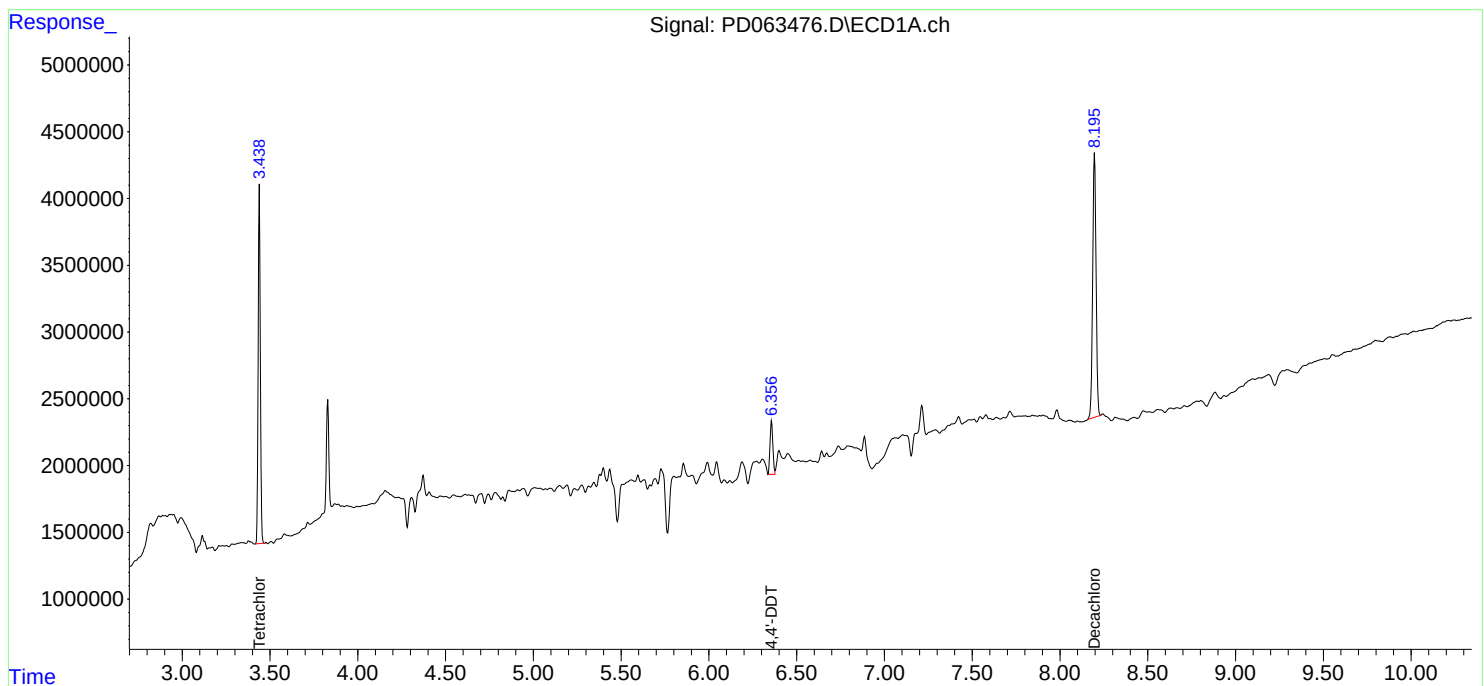

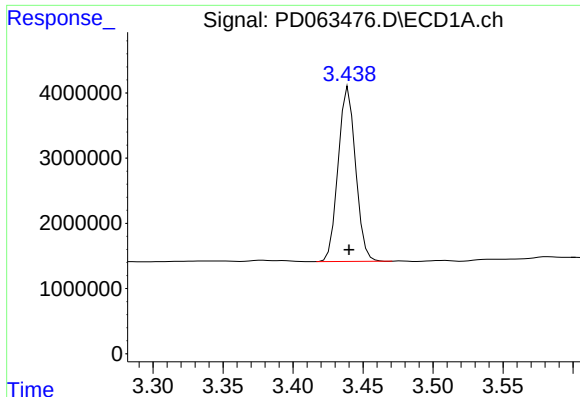


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 23182731
Conc: 16.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
339


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:15 AM

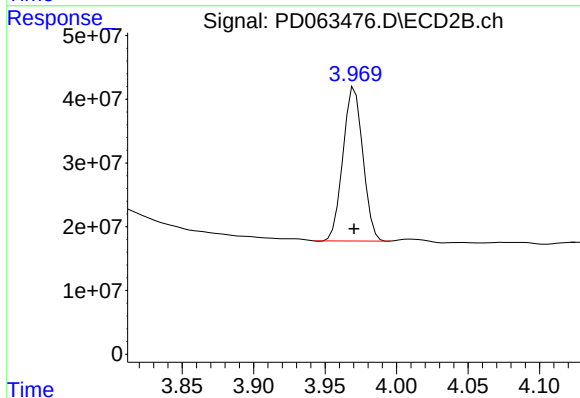


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 233994543
Conc: 17.46 ng/ml

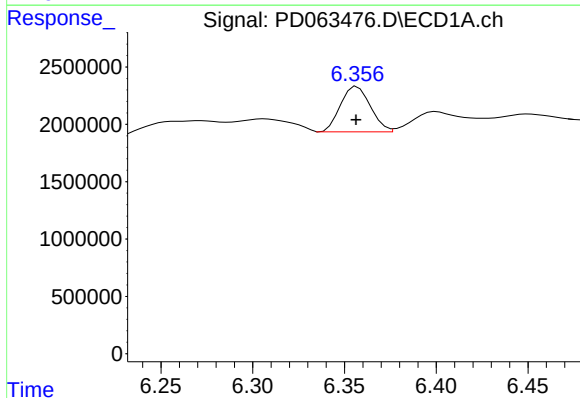


#17 4,4'-DDT

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 4528224
Conc: 3.13 ng/ml m

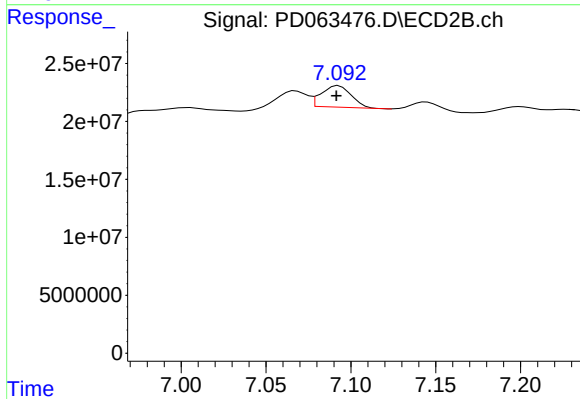

#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.001 min
Response: 22710305
Conc: 1.51 ng/ml

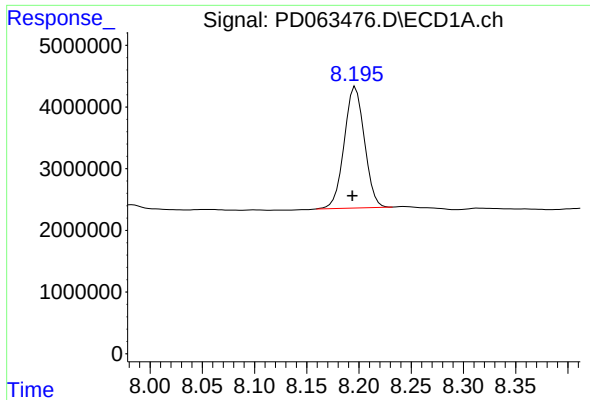


#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: 0.003 min
Response: 26453795
Conc: 16.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
339

Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:15 AM

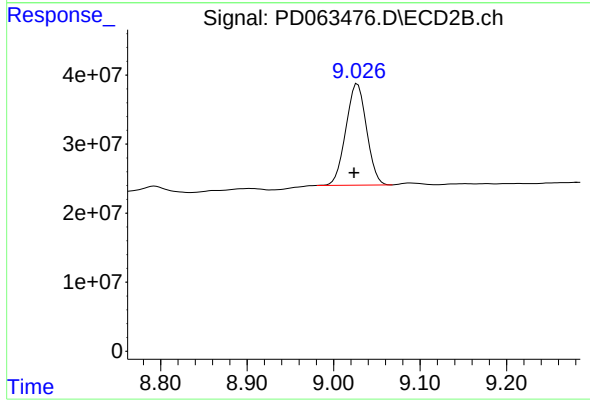

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: 0.004 min
Response: 243396193
Conc: 17.61 ng/ml