

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060521\
 Data File : PD063479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2021 16:05
 Operator : AR\AJ
 Sample : M2602-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-02-060321

Manual Integrations
 APPROVED

Ankita
 6/7/2021 8:42:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:48:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.971	16730334	161.3E6	12.091	12.041
28) SA Decachlor...	8.197	9.027	16038157	176.4E6	10.198	12.765 #
Target Compounds						
12) B 4,4'-DDE	5.598	6.295	1293269	19179566	0.744m	1.055m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060521\
Data File : PD063479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2021 16:05
Operator : AR\AJ
Sample : M2602-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
SU-02-060321


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:48:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

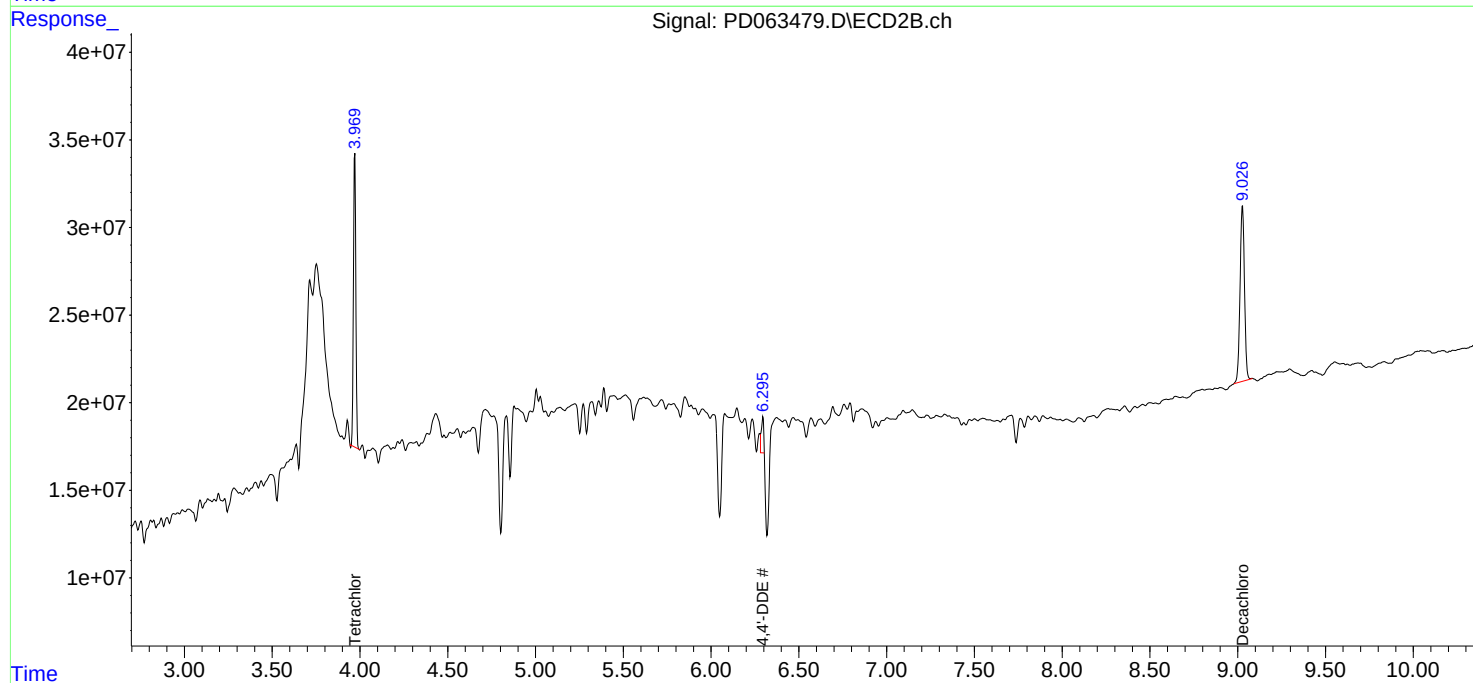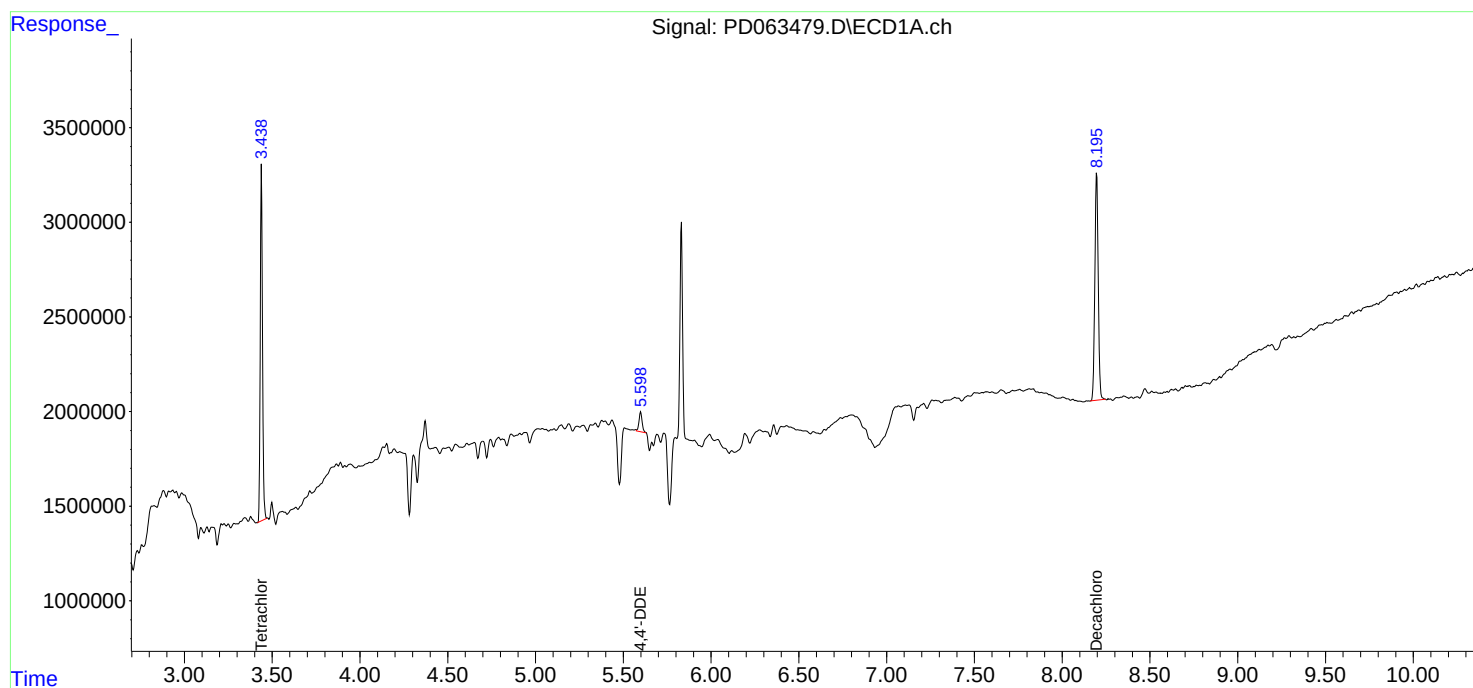

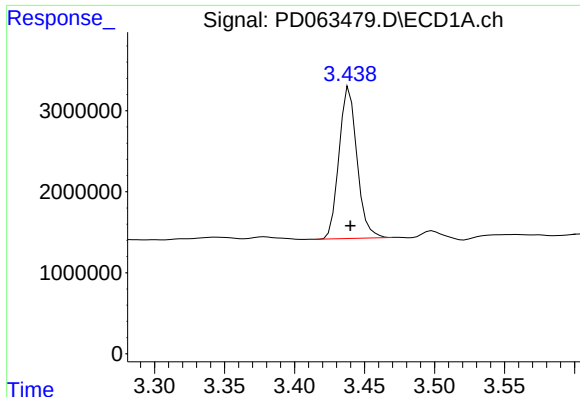


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 16730334
Conc: 12.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-02-060321


Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:20 AM

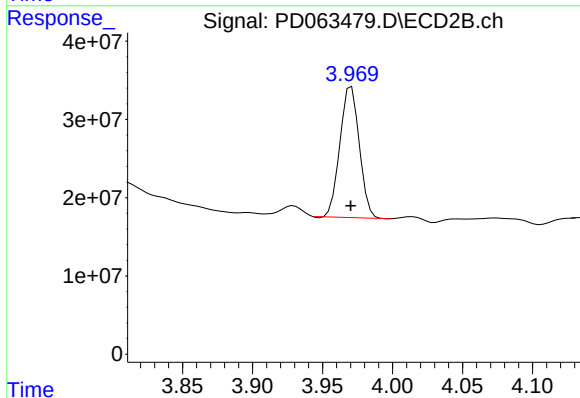


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 161334613
Conc: 12.04 ng/ml

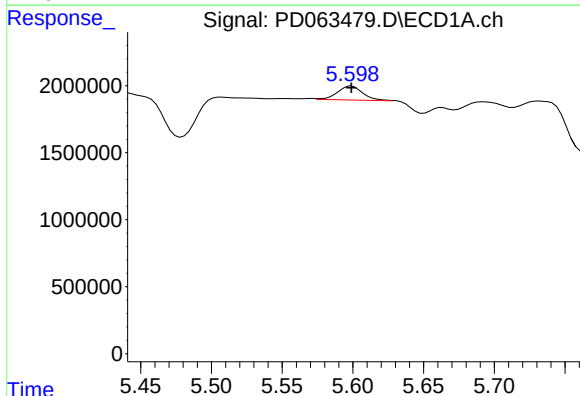


#12 4,4'-DDE

R.T.: 5.598 min
Delta R.T.: -0.001 min
Response: 1293269
Conc: 0.74 ng/ml m

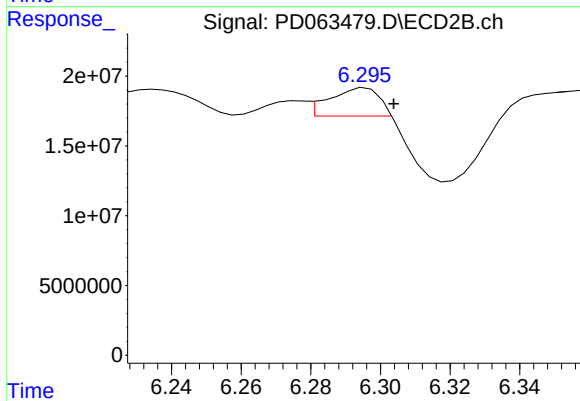

#12 4,4'-DDE

R.T.: 6.295 min
Delta R.T.: -0.009 min
Response: 19179566
Conc: 1.06 ng/ml m

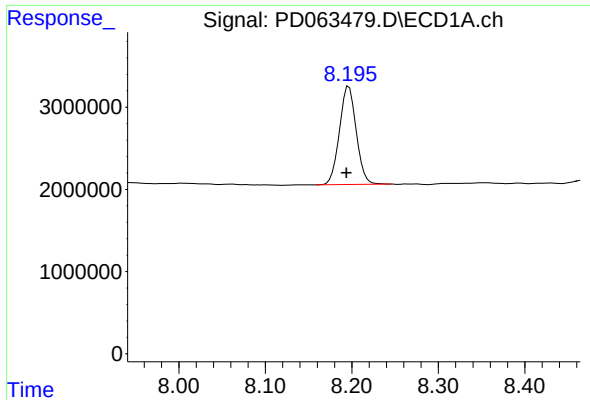


#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: 0.003 min
Response: 16038157
Conc: 10.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-02-060321

Manual Integrations
APPROVED

Ankita
6/7/2021 8:42:20 AM

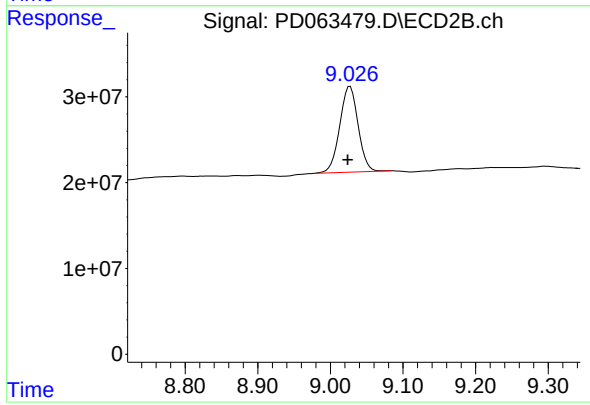

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.003 min
Response: 176400370
Conc: 12.77 ng/ml