

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 11:09
 Operator : AR\AJ
 Sample : N3143-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:34:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.168	20735248	177.5E6	19.484	20.141
28)	SA Decachlor...	8.194	9.363	18760697	114.0E6	17.200	21.080
Target Compounds							
3)	MA gamma-BHC...	4.161	0.000	3300138	0	1.912	N.D. #
6)	B beta-BHC	4.425	5.015	223867	22564736	0.322	4.296 #
9)	A Endosulfan I	5.500	0.000	1115567	0	0.890	N.D. #
10)	B gamma-Chl...	5.400f	6.318	3793303	54309499	2.803	5.480 #
19)	B Endosulfa...	0.000	7.503f	0	4441013	N.D.	0.602 #
20)	A Methoxychlor	6.915	0.000	494568	0	0.872	N.D. #
25)	Chlordane-3	5.400f	6.318	3793303	54309499	29.913	42.114 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 11:09
Operator : AR\AJ
Sample : N3143-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:34:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

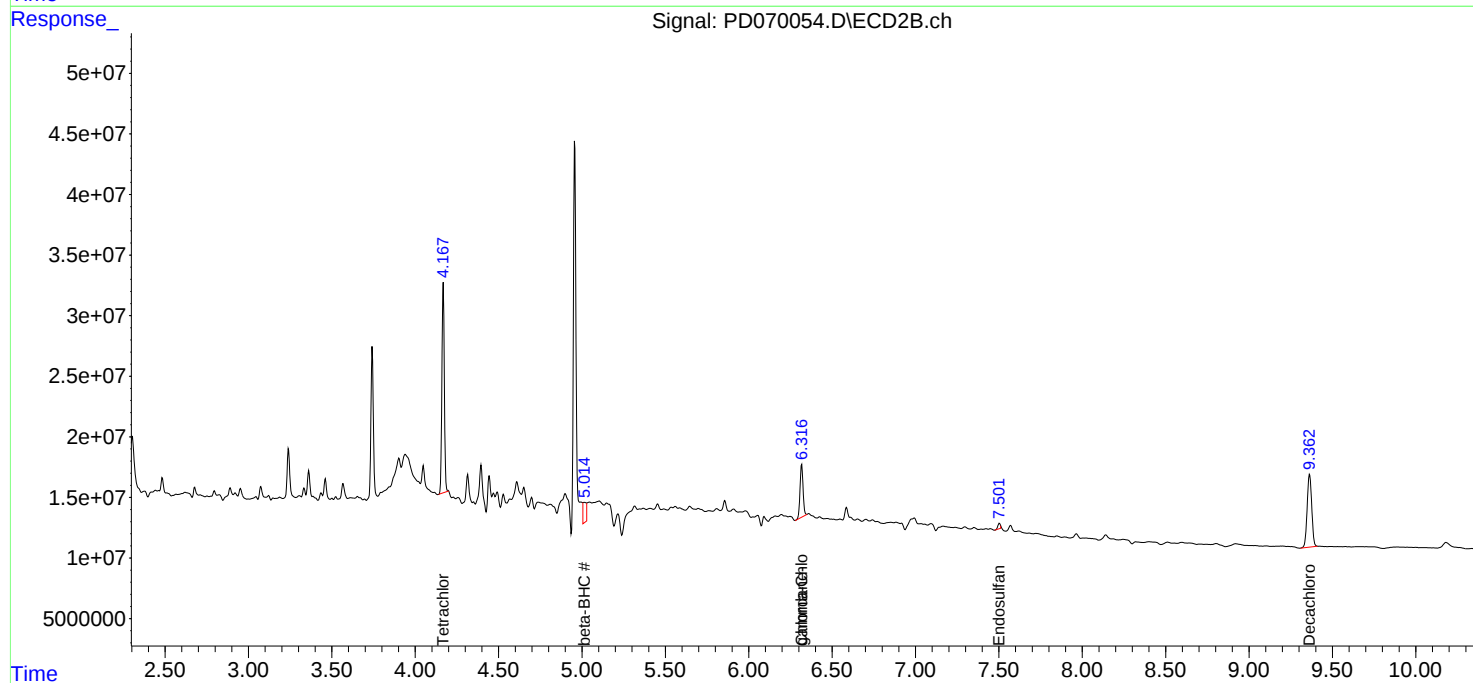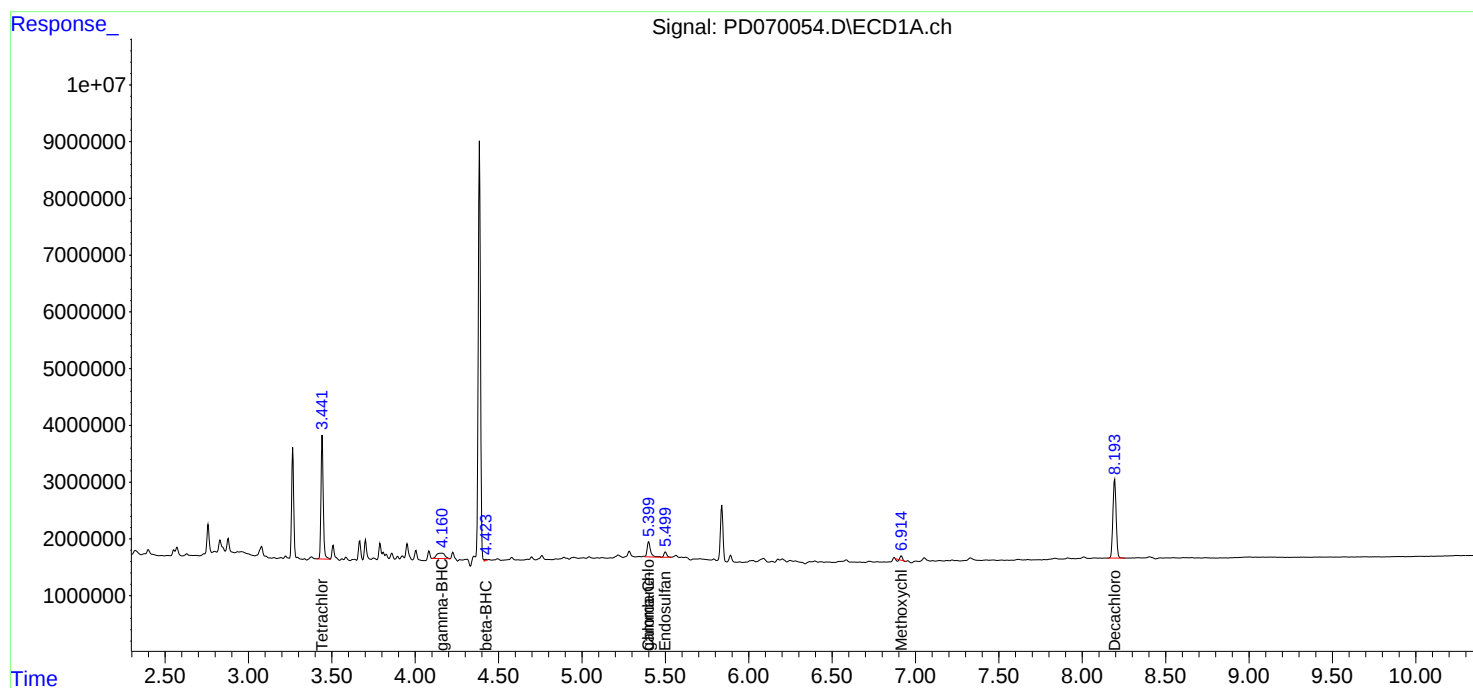


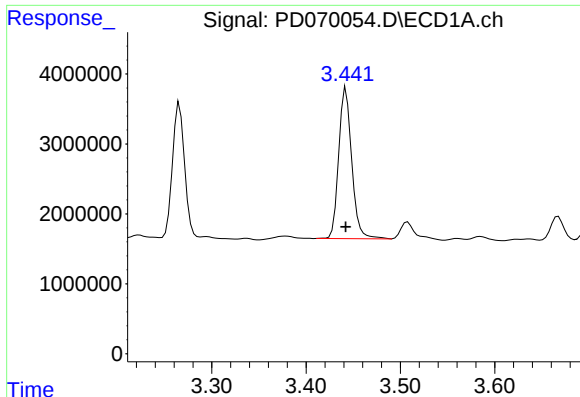

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 20735248
Conc: 19.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

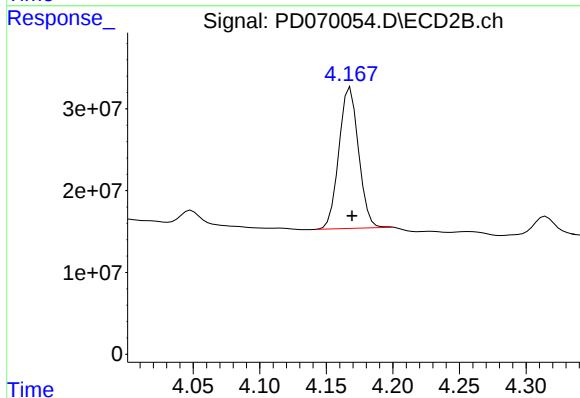


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: -0.001 min
Response: 177480338
Conc: 20.14 ng/ml

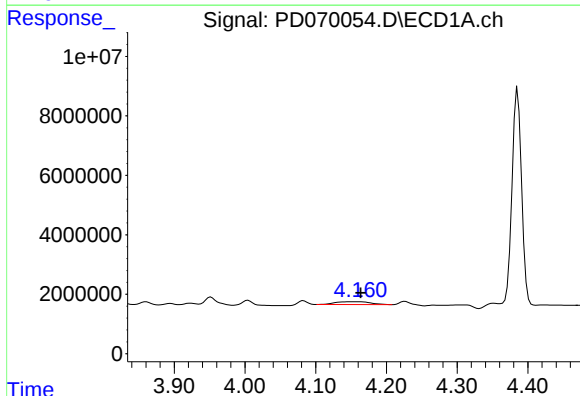


#3 gamma-BHC (Lindane)

R.T.: 4.161 min
Delta R.T.: -0.003 min
Response: 3300138
Conc: 1.91 ng/ml

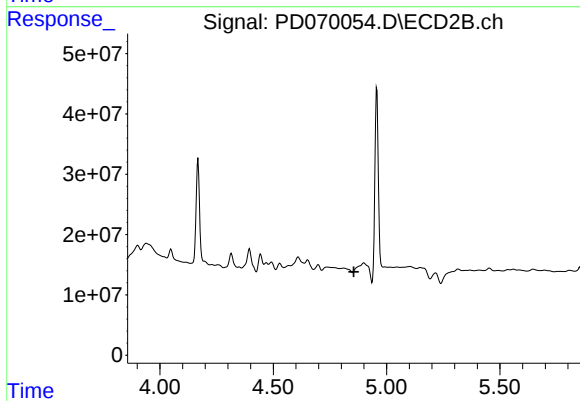

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

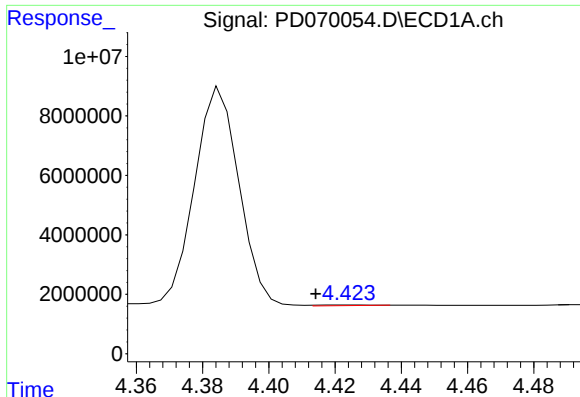

#6 beta-BHC


R.T.: 4.425 min
Delta R.T.: 0.011 min
Response: 223867
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

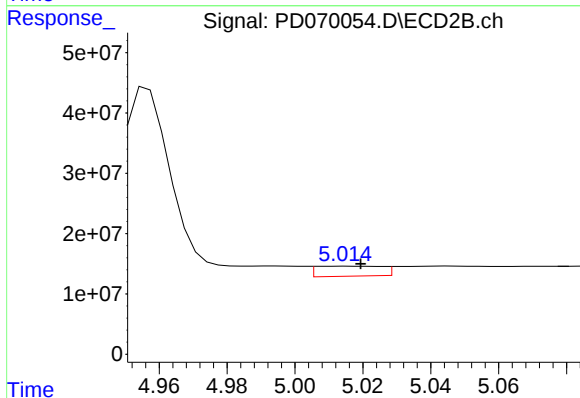


#6 beta-BHC

R.T.: 5.015 min
Delta R.T.: -0.004 min
Response: 22564736
Conc: 4.30 ng/ml

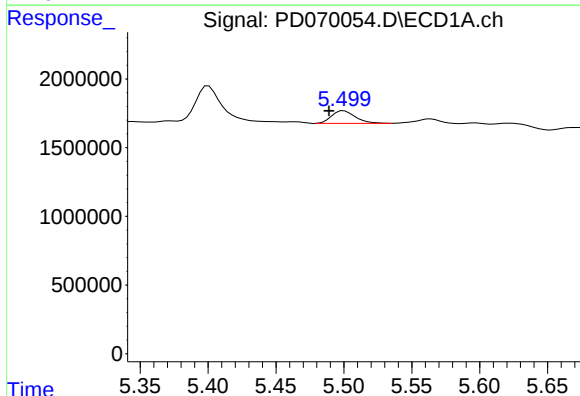


#9 Endosulfan I

R.T.: 5.500 min
Delta R.T.: 0.011 min
Response: 1115567
Conc: 0.89 ng/ml

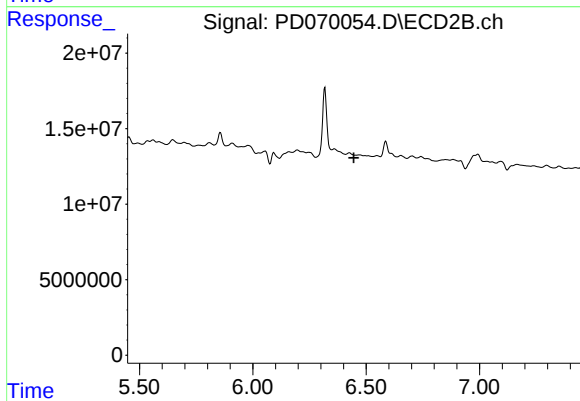

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.445 min
Response: 0
Conc: N.D.

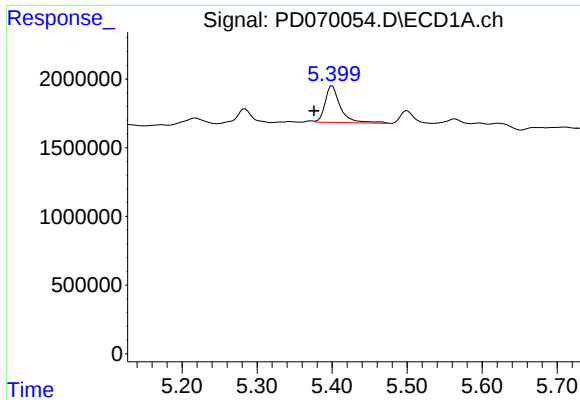

#10 gamma-Chlordane


R.T.: 5.400 min
Delta R.T.: 0.024 min
Response: 3793303
Conc: 2.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

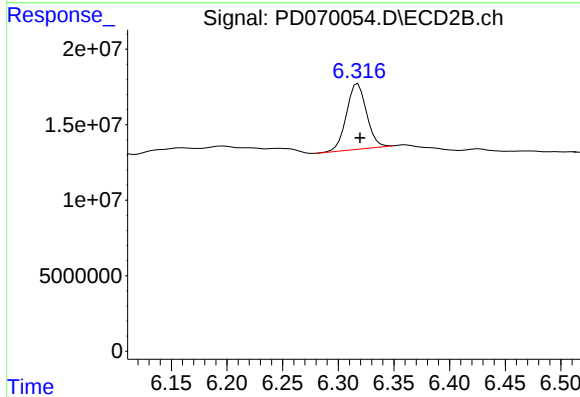


#10 gamma-Chlordane

R.T.: 6.318 min
Delta R.T.: -0.002 min
Response: 54309499
Conc: 5.48 ng/ml

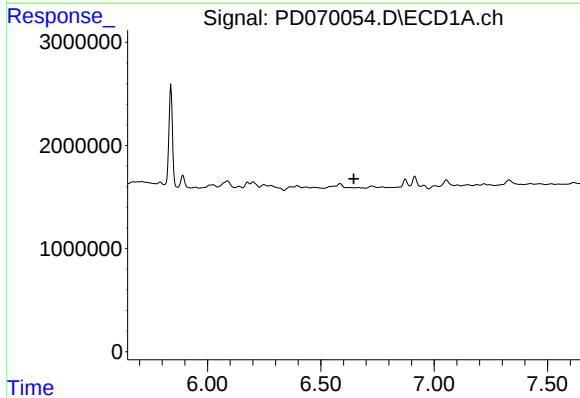


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

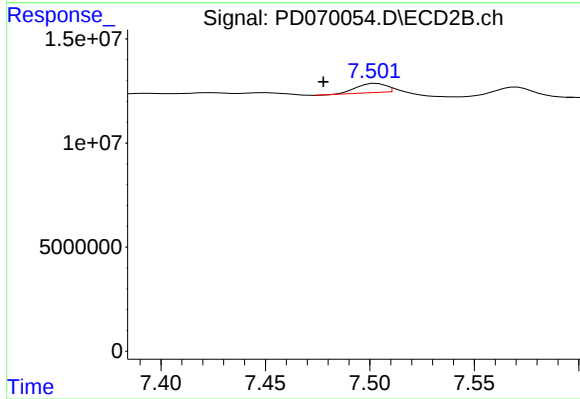

#19 Endosulfan Sulfate


R.T.: 7.503 min
Delta R.T.: 0.025 min
Response: 4441013
Conc: 0.60 ng/ml

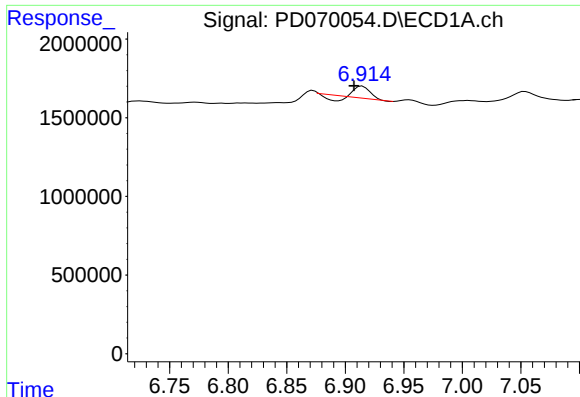

#20 Methoxychlor


R.T.: 6.915 min
Delta R.T.: 0.007 min
Response: 494568
Conc: 0.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

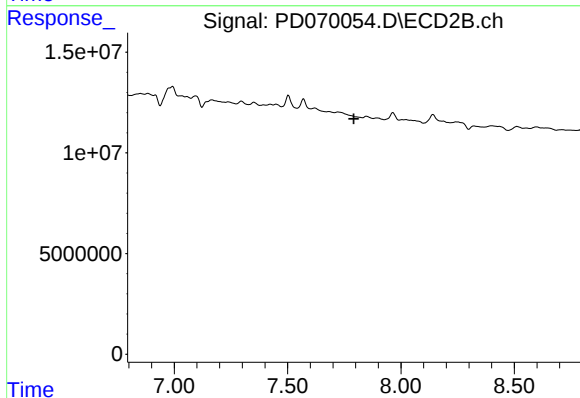


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

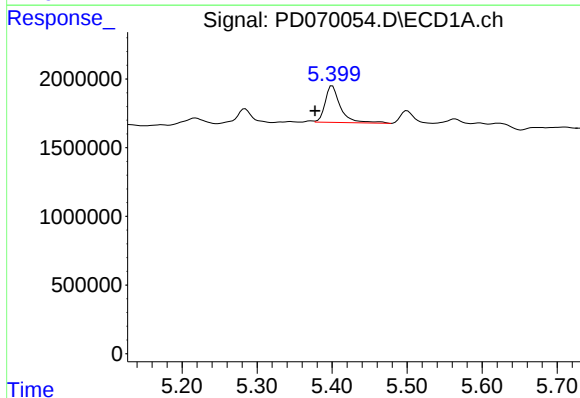


#25 Chlordane-3

R.T.: 5.400 min
Delta R.T.: 0.023 min
Response: 3793303
Conc: 29.91 ng/ml

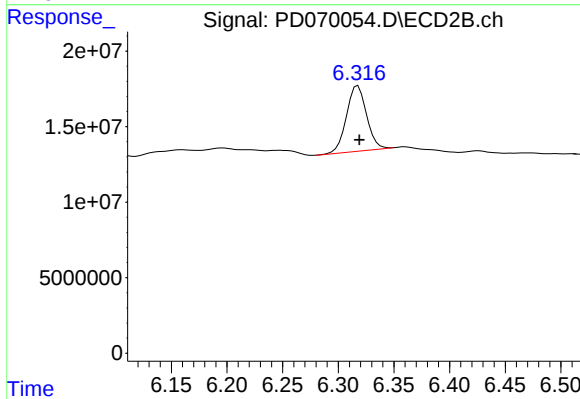

#25 Chlordane-3


R.T.: 6.318 min
Delta R.T.: -0.001 min
Response: 54309499
Conc: 42.11 ng/ml

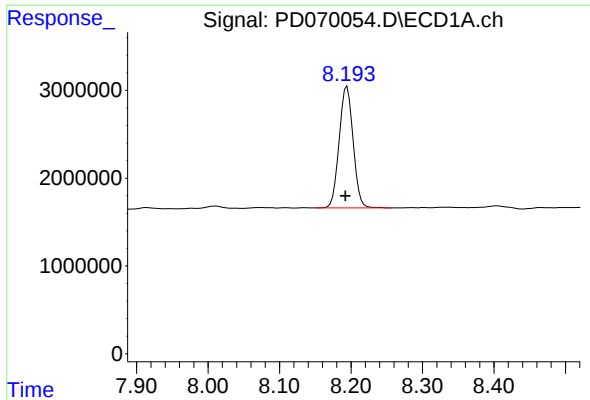

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 18760697
Conc: 17.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

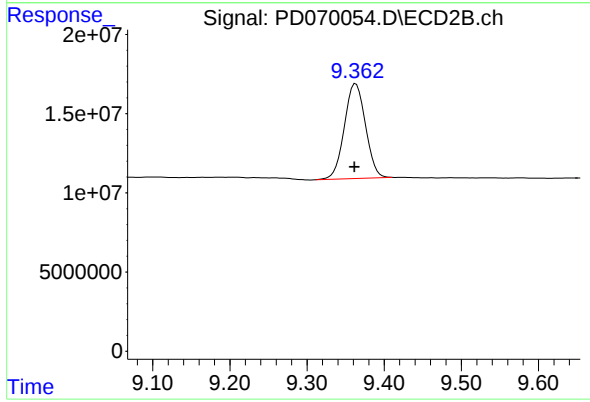

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.002 min
Response: 114003748
Conc: 21.08 ng/ml