

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 19:46
 Operator : AR\AJ
 Sample : PB145234BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:06:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	20119670	187.9E6	18.906	21.323
28)	SA Decachlor...	8.194	9.364	21050380	121.9E6	19.299	22.533
Target Compounds							
3)	MA gamma-BHC...	4.167	0.000	727454	0	0.421	N.D. #
8)	B Heptachlo...	5.158	6.068	4239766	50425821	3.175	6.408 #
14)	MA Endrin	6.002	0.000	3924273	0	3.399	N.D. #
22)	Mirex	0.000	8.418	0	81272151	N.D.	15.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 19:46
Operator : AR\AJ
Sample : PB145234BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:06:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

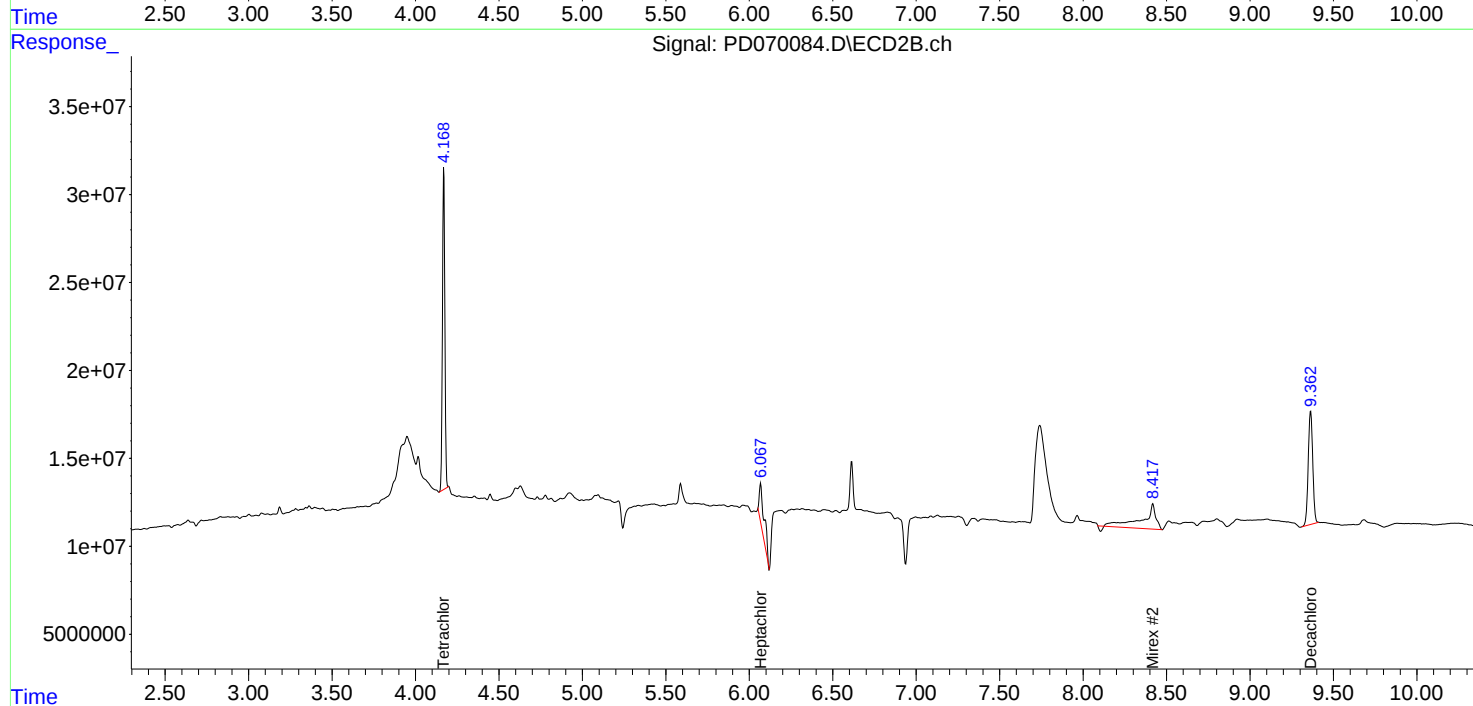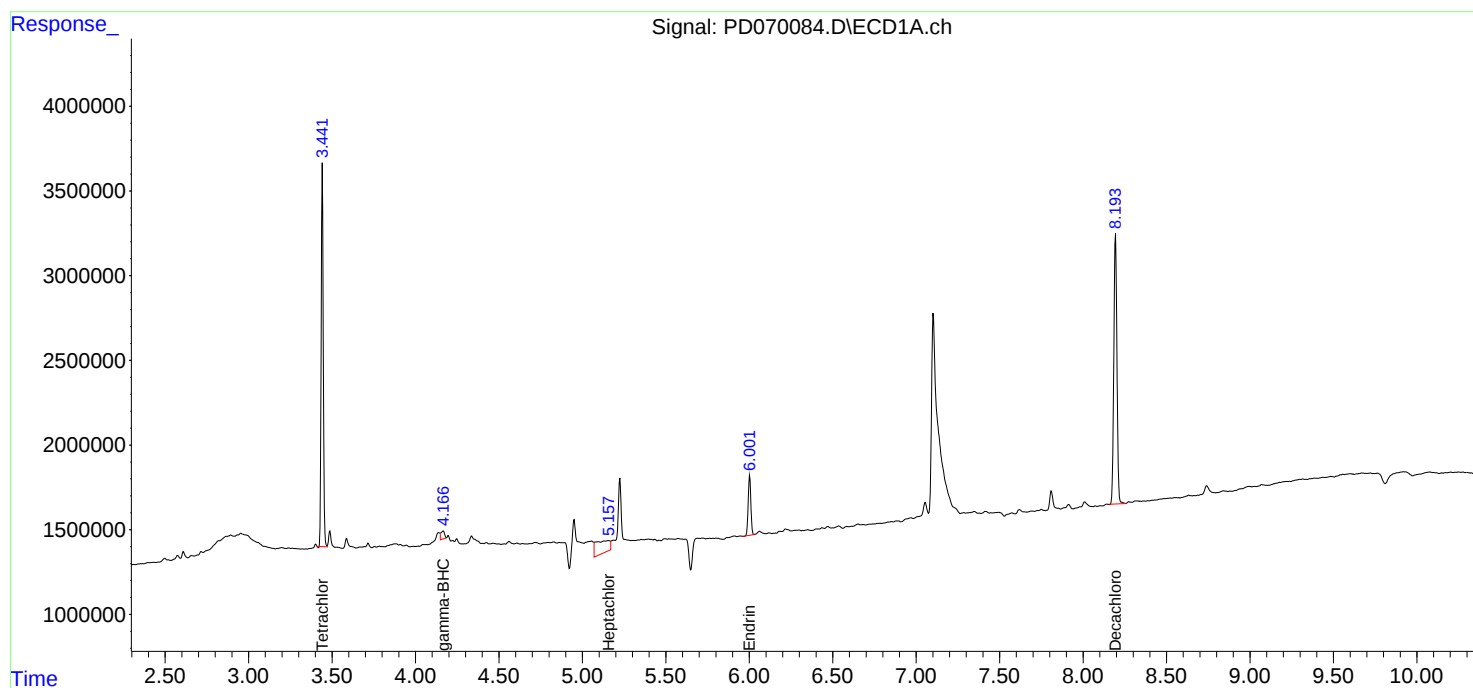


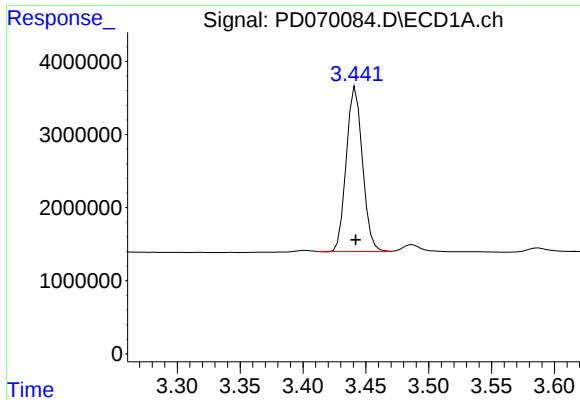

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 20119670
Conc: 18.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

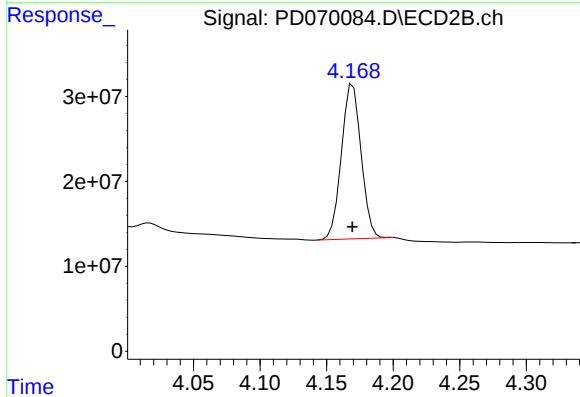


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 187890160
Conc: 21.32 ng/ml

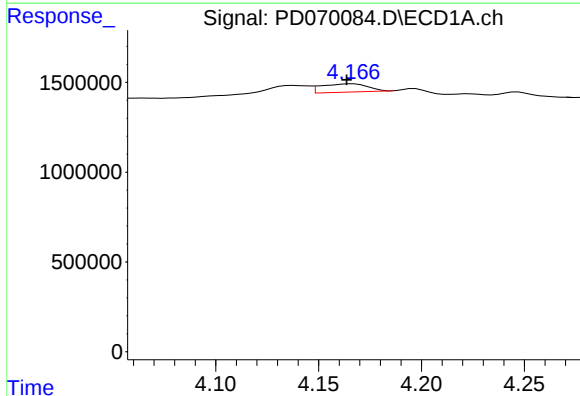


#3 gamma-BHC (Lindane)

R.T.: 4.167 min
Delta R.T.: 0.003 min
Response: 727454
Conc: 0.42 ng/ml

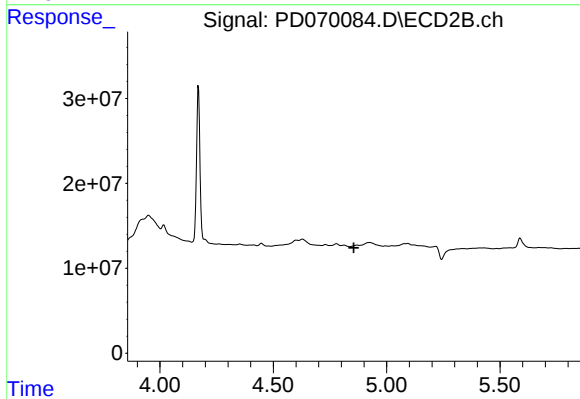

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

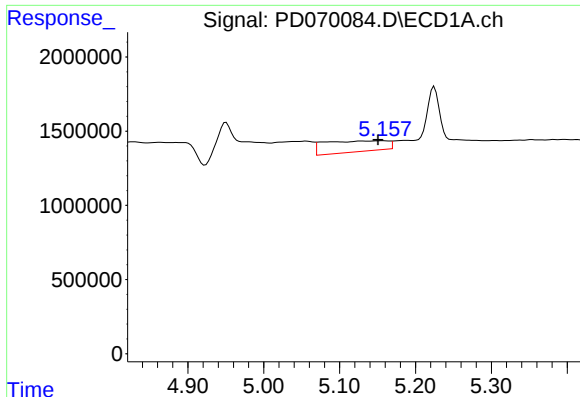

#8 Heptachlor epoxide


R.T.: 5.158 min
Delta R.T.: 0.007 min
Response: 4239766
Conc: 3.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

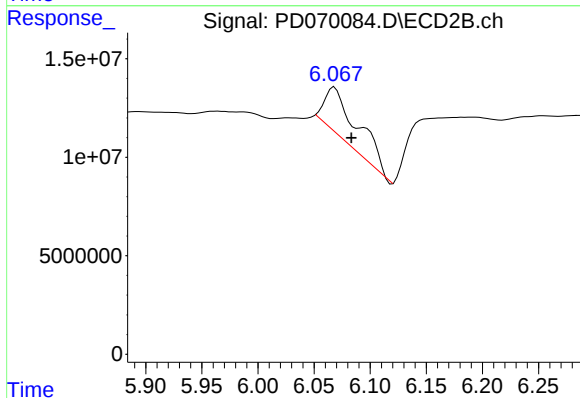


#8 Heptachlor epoxide

R.T.: 6.068 min
Delta R.T.: -0.015 min
Response: 50425821
Conc: 6.41 ng/ml

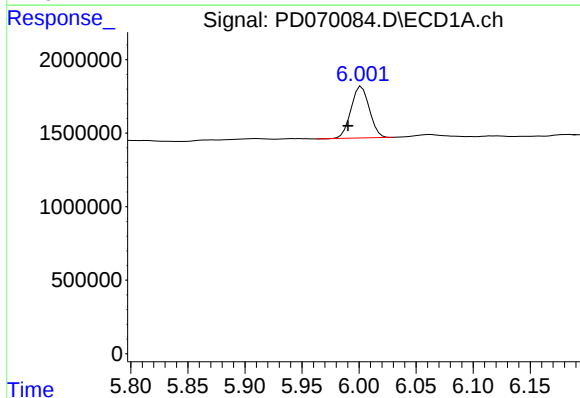


#14 Endrin

R.T.: 6.002 min
Delta R.T.: 0.012 min
Response: 3924273
Conc: 3.40 ng/ml

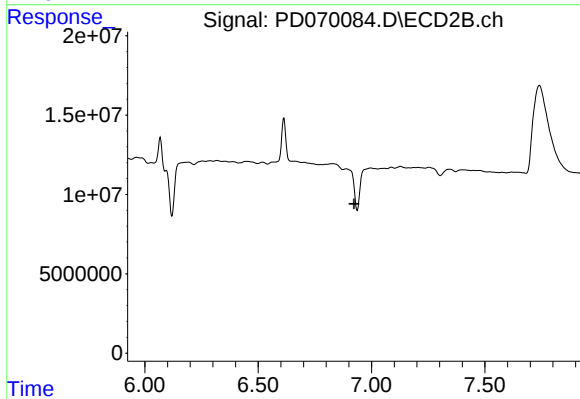

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.924 min
Response: 0
Conc: N.D.

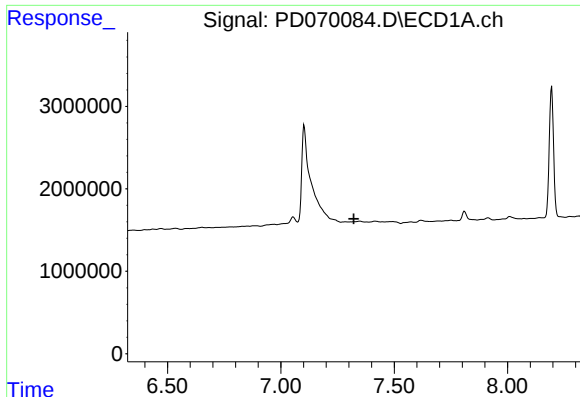

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.321 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

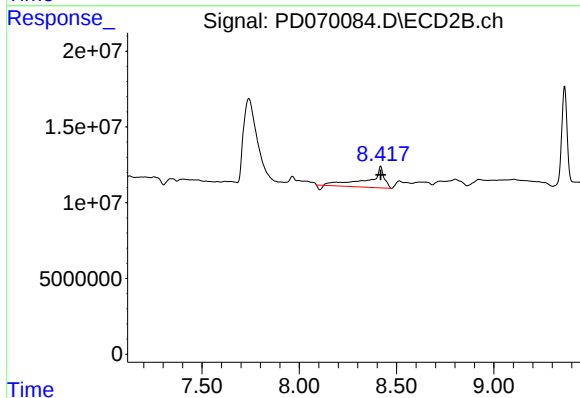


#22 Mirex

R.T.: 8.418 min
Delta R.T.: 0.000 min
Response: 81272151
Conc: 15.21 ng/ml

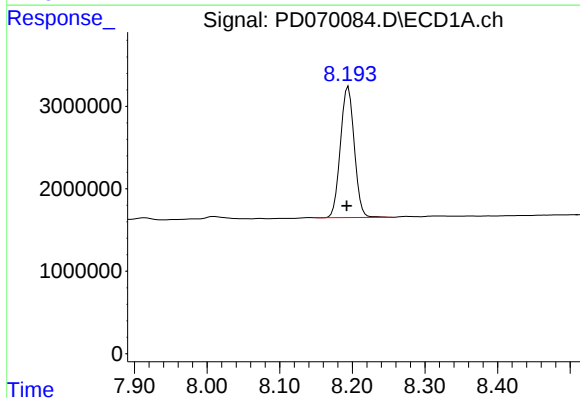

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 21050380
Conc: 19.30 ng/ml

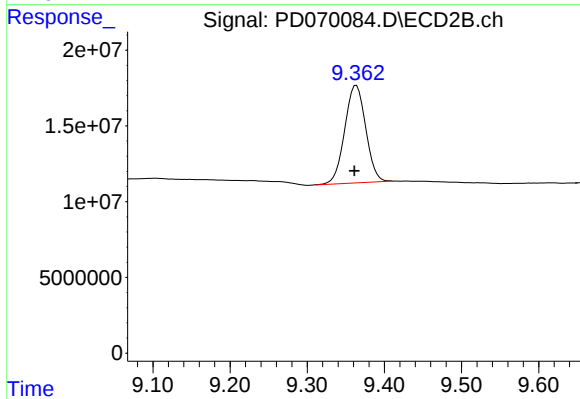

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.002 min
Response: 121858448
Conc: 22.53 ng/ml