

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 20:56
 Operator : AR\AJ
 Sample : N2952-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:07:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	10331031	101.7E6	9.708	11.546
28)	SA Decachlor...	8.194	9.364	11937279	67822090	10.944	12.541
Target Compounds							
3)	MA gamma-BHC...	4.159	0.000	2583167	0	1.497	N.D. #
8)	B Heptachlo...	0.000	6.069	0	65541184	N.D.	8.329 #
12)	B 4,4'-DDE	5.600	6.545	14569869	103.3E6	11.500	11.420
14)	MA Endrin	6.000	0.000	1600994	0	1.387	N.D. #
16)	A 4,4'-DDD	0.000	7.048	0	9900339	N.D.	1.337 #
17)	MA 4,4'-DDT	6.355	7.340	2357111	9370011	2.378	1.280 #
19)	B Endosulfa...	6.642	0.000	864951	0	0.750	N.D. #
20)	A Methoxychlor	6.887f	0.000	2639914	0	4.653	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 20:56
Operator : AR\AJ
Sample : N2952-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:07:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

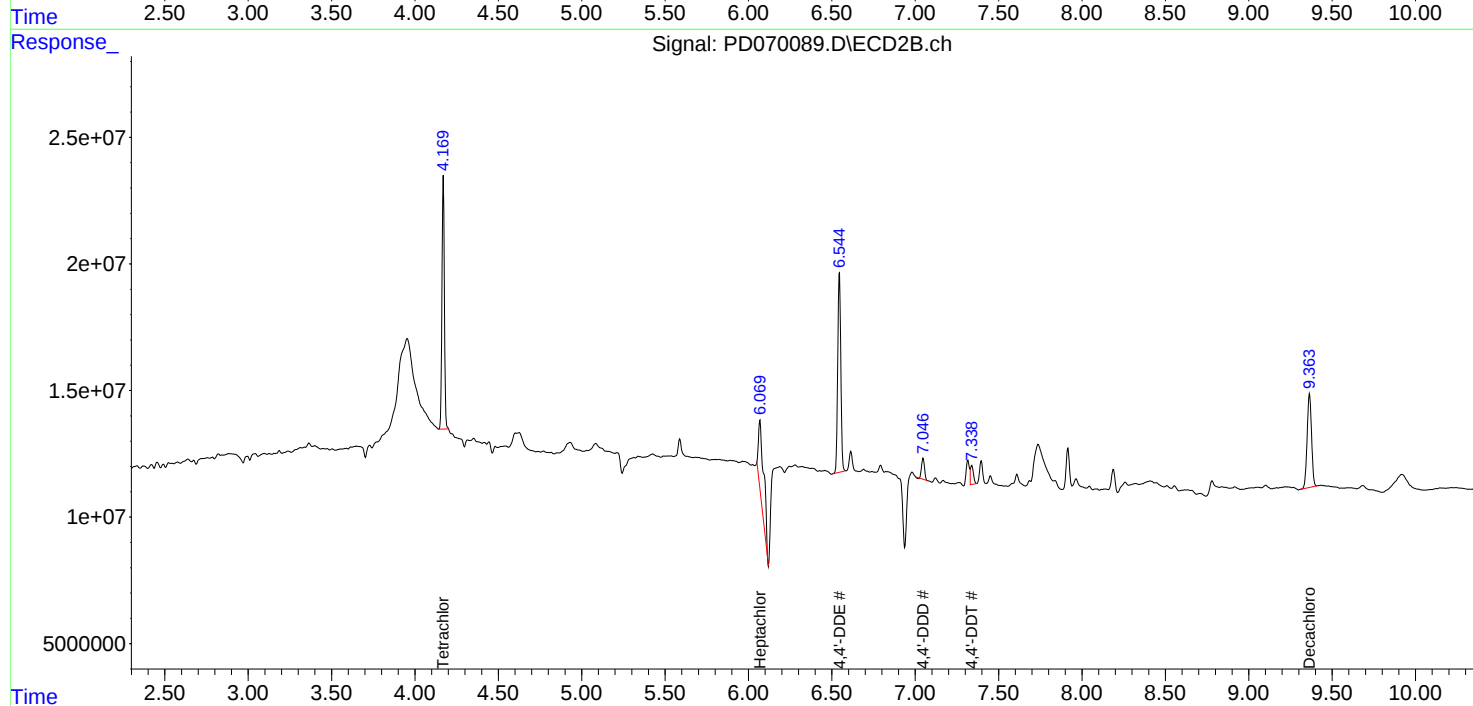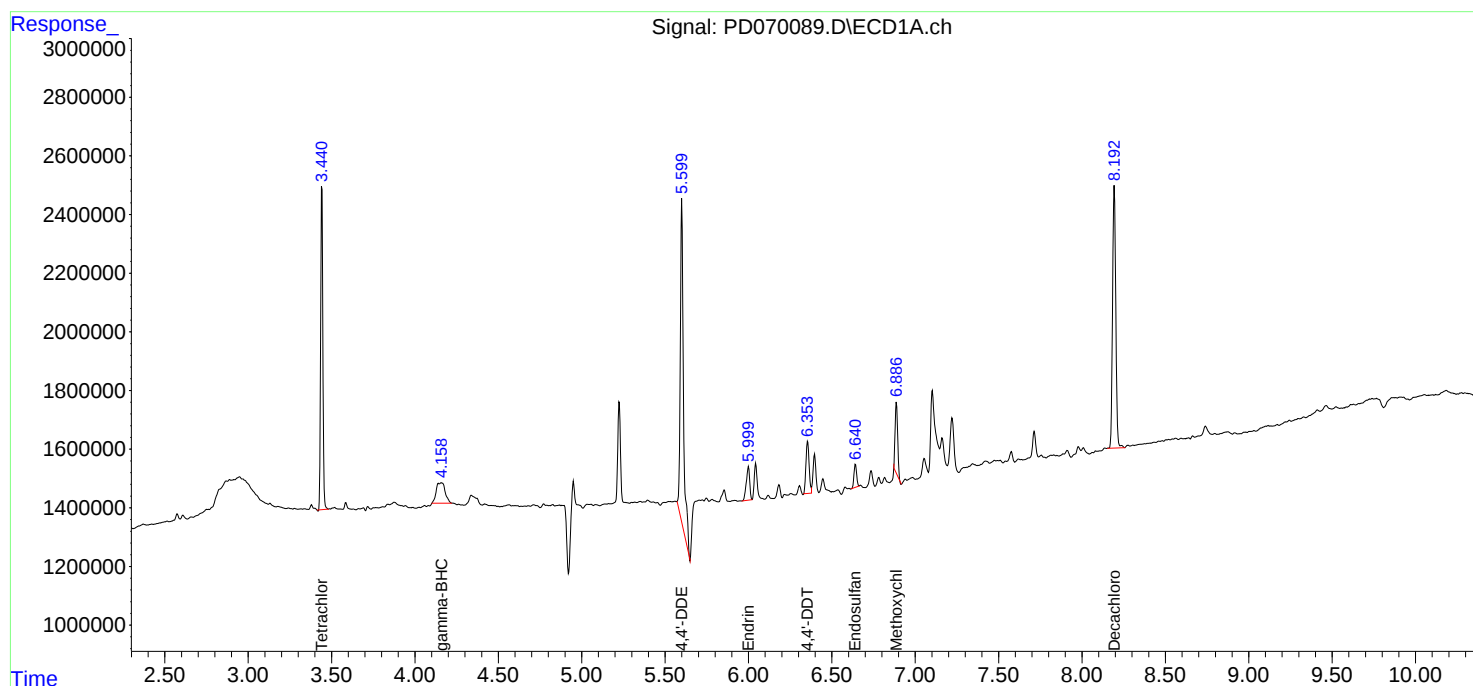


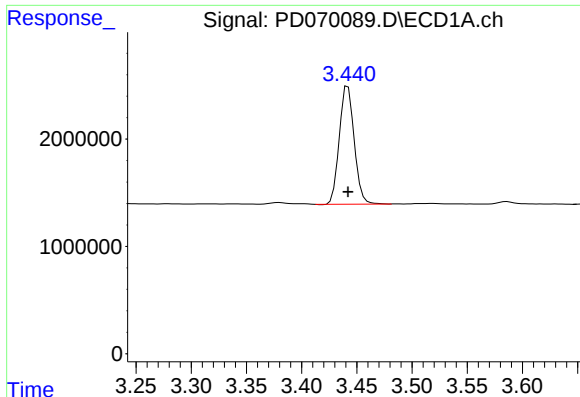

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 10331031
Conc: 9.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

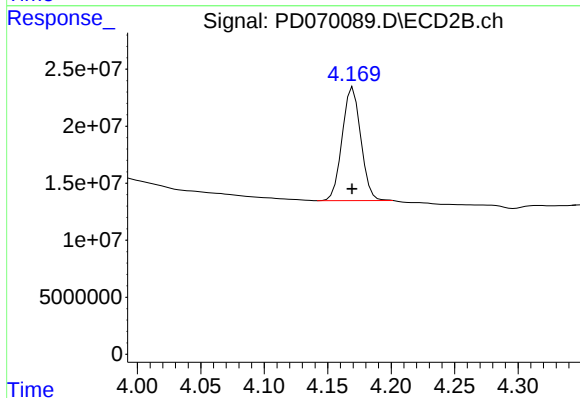


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 101738802
Conc: 11.55 ng/ml

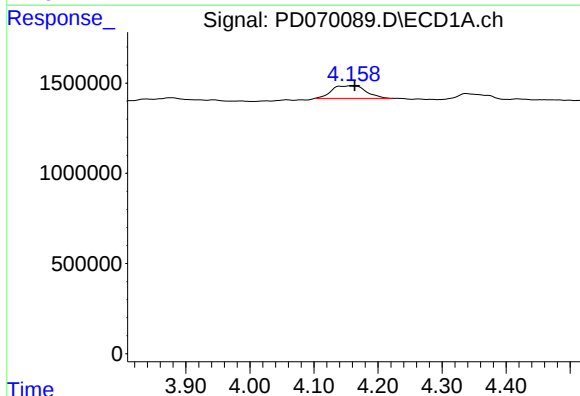


#3 gamma-BHC (Lindane)

R.T.: 4.159 min
Delta R.T.: -0.005 min
Response: 2583167
Conc: 1.50 ng/ml

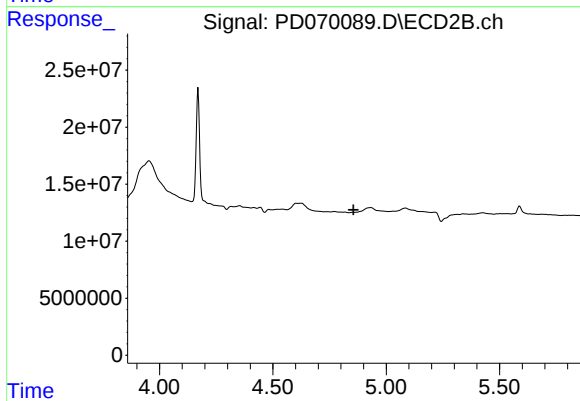

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

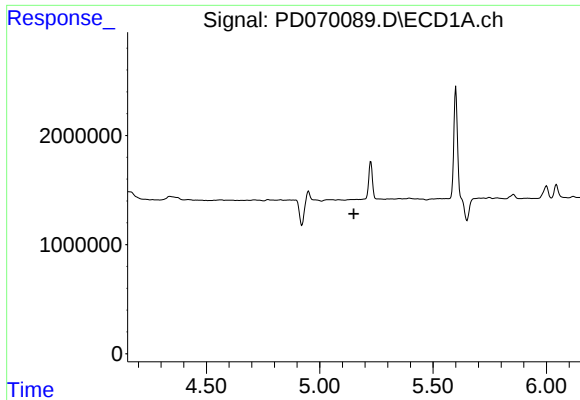

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

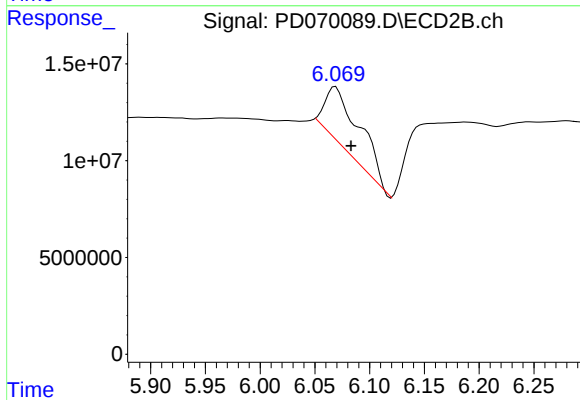


#8 Heptachlor epoxide

R.T.: 6.069 min
Delta R.T.: -0.014 min
Response: 65541184
Conc: 8.33 ng/ml

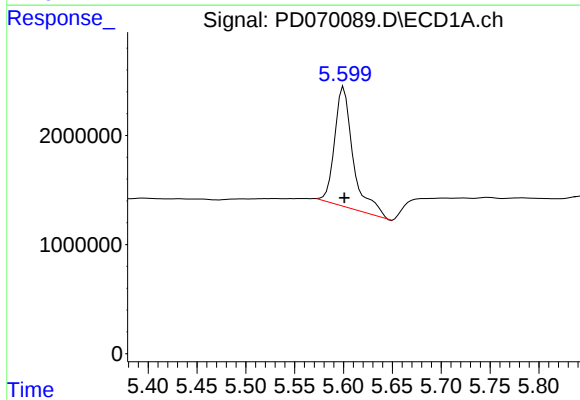


#12 4,4'-DDE

R.T.: 5.600 min
Delta R.T.: 0.000 min
Response: 14569869
Conc: 11.50 ng/ml

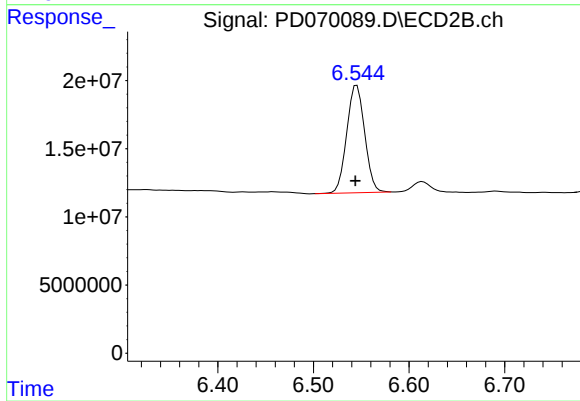

#12 4,4'-DDE


R.T.: 6.545 min
Delta R.T.: 0.001 min
Response: 103327786
Conc: 11.42 ng/ml

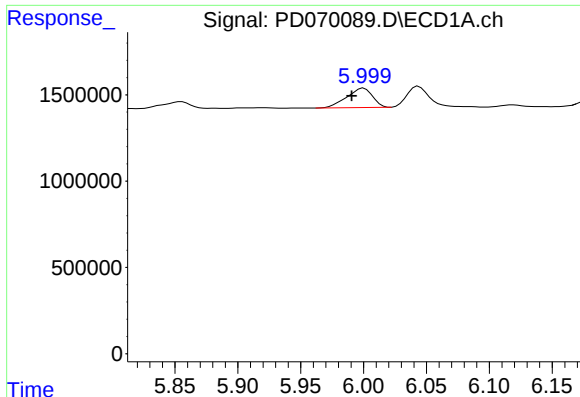

#14 Endrin


R.T.: 6.000 min
Delta R.T.: 0.010 min
Response: 1600994
Conc: 1.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

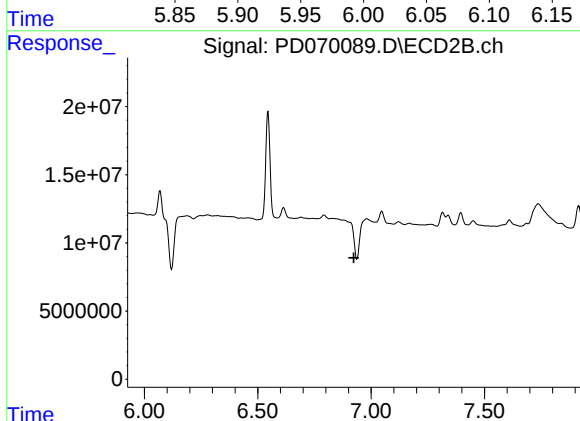


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

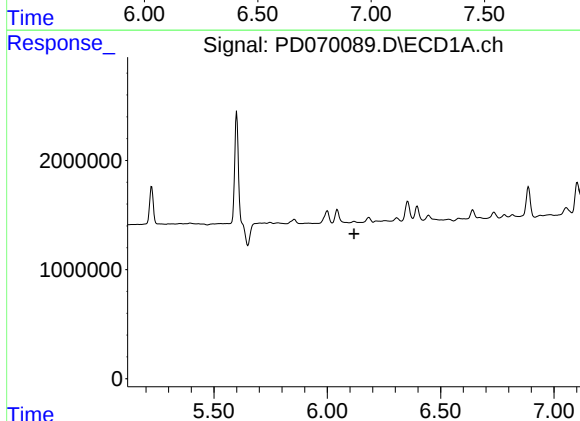


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

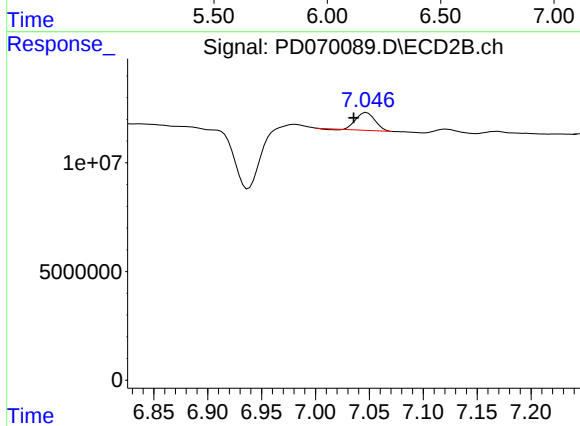

#16 4,4'-DDD


R.T.: 7.048 min
Delta R.T.: 0.012 min
Response: 9900339
Conc: 1.34 ng/ml

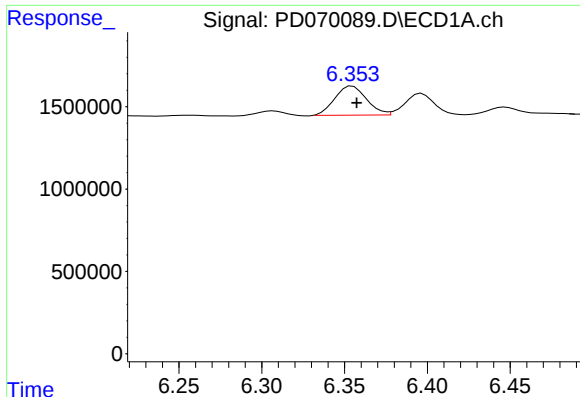

#17 4,4'-DDT


R.T.: 6.355 min
Delta R.T.: -0.003 min
Response: 2357111
Conc: 2.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

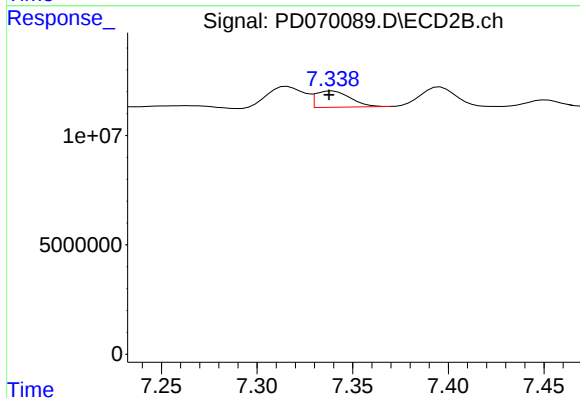


#17 4,4'-DDT

R.T.: 7.340 min
Delta R.T.: 0.002 min
Response: 9370011
Conc: 1.28 ng/ml

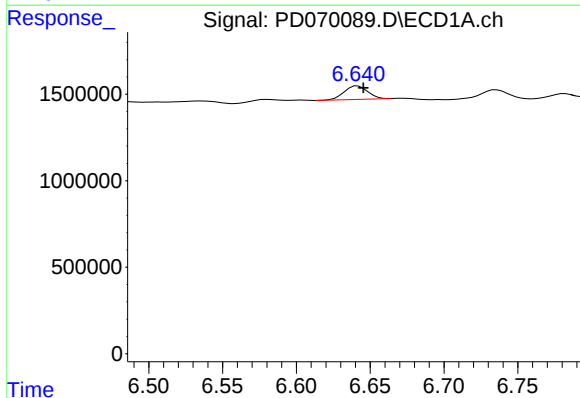


#19 Endosulfan Sulfate

R.T.: 6.642 min
Delta R.T.: -0.004 min
Response: 864951
Conc: 0.75 ng/ml

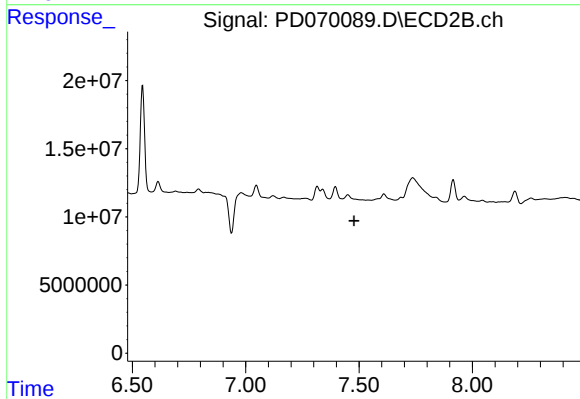

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

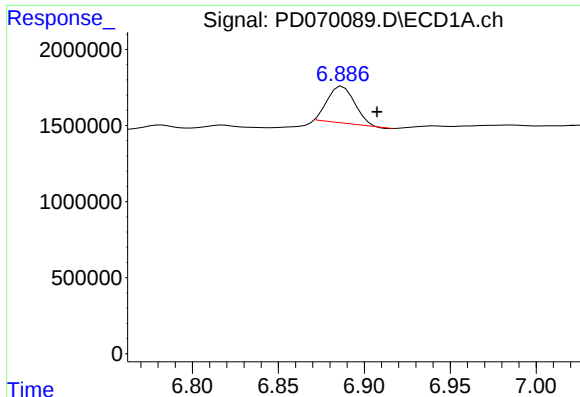

#20 Methoxychlor


R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 2639914
Conc: 4.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

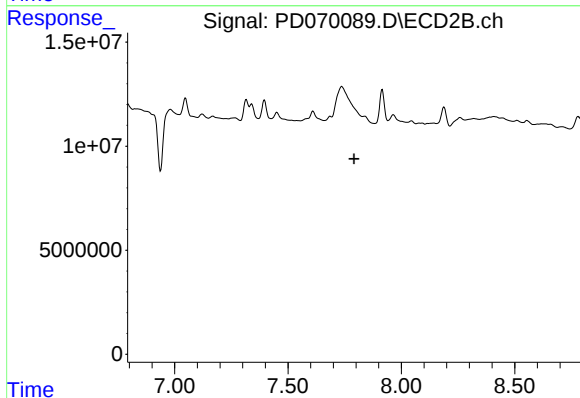


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.792 min
Response: 0
Conc: N.D.

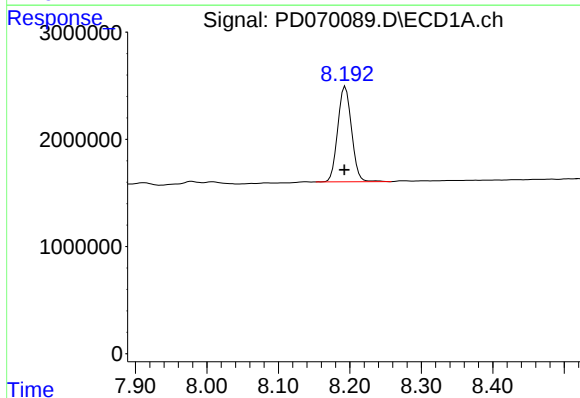

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.001 min
Response: 11937279
Conc: 10.94 ng/ml

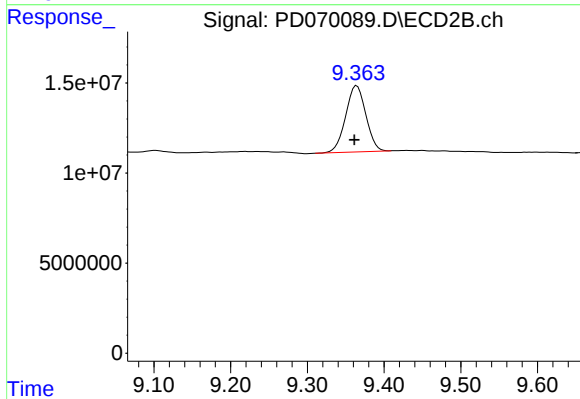

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.003 min
Response: 67822090
Conc: 12.54 ng/ml