

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2022 00:43
 Operator : AR\AJ
 Sample : N2952-14
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:10:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.170	20260815	194.7E6	19.038	22.096
28)	SA Decachlor...	8.193	9.363	17732735	100.9E6	16.258	18.658
Target Compounds							
23)	Chlordane-1	4.314	0.000	265680	0	6.783	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2022 00:43
Operator : AR\AJ
Sample : N2952-14
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:10:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

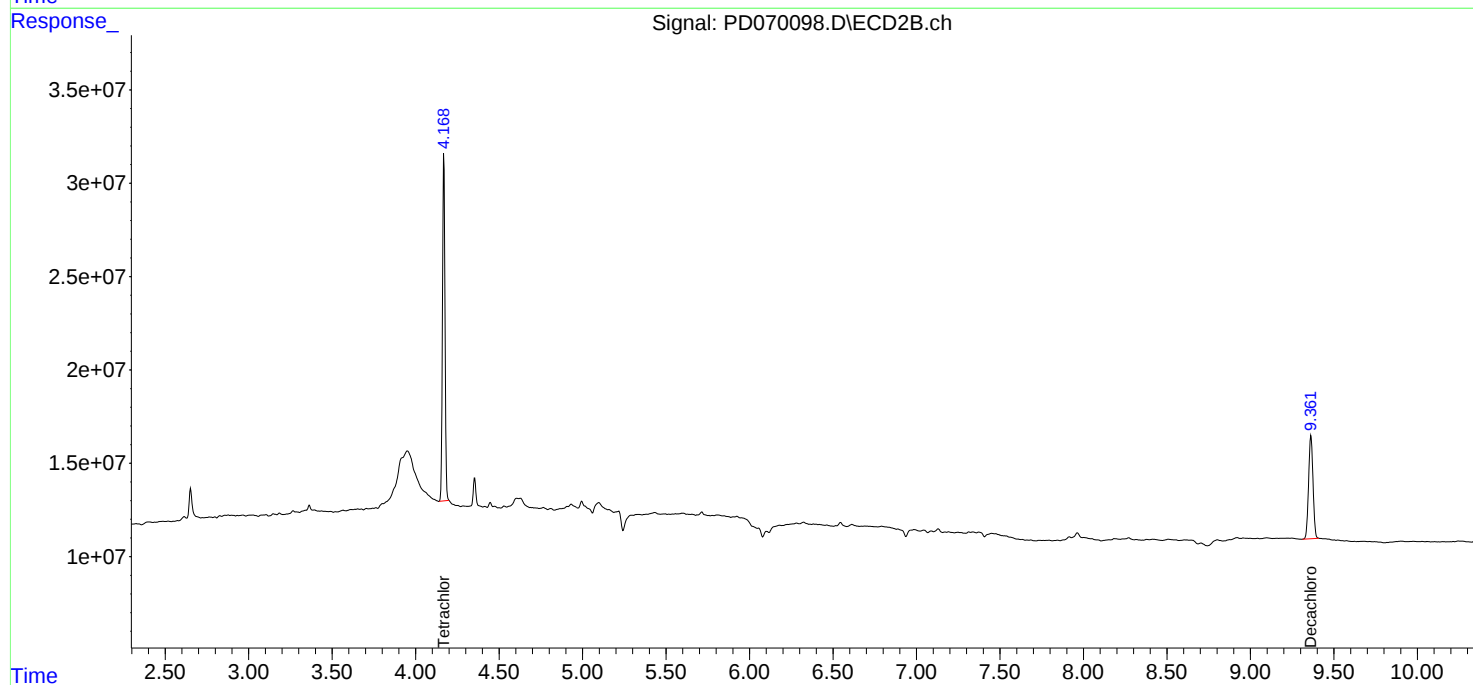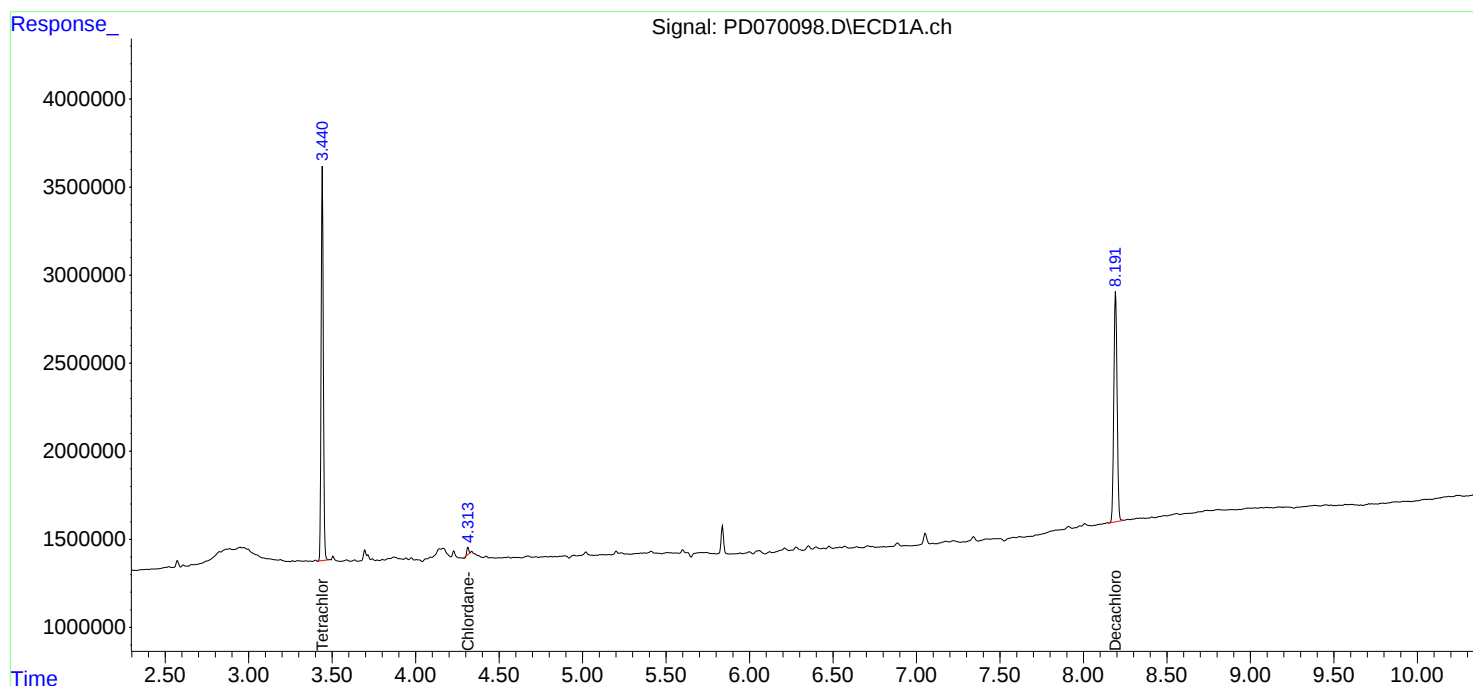


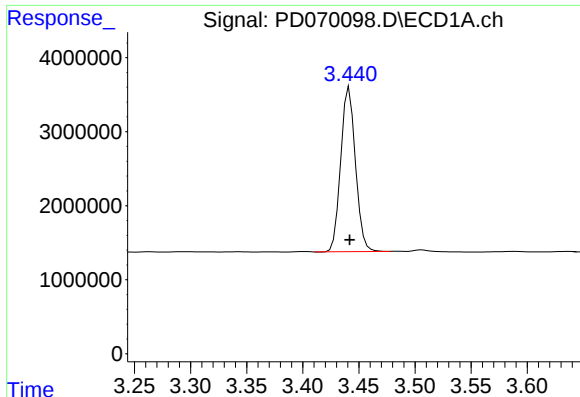

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 20260815
Conc: 19.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

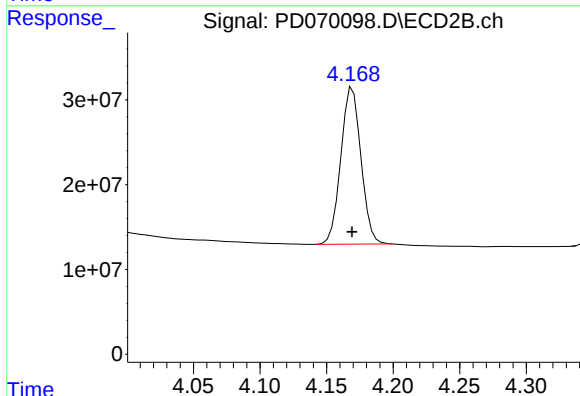


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 194700686
Conc: 22.10 ng/ml

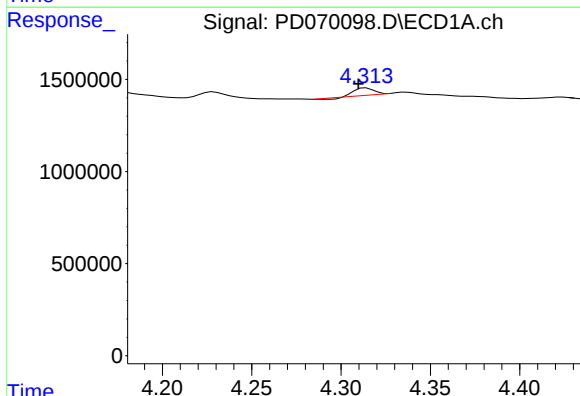


#23 Chlordane-1

R.T.: 4.314 min
Delta R.T.: 0.004 min
Response: 265680
Conc: 6.78 ng/ml

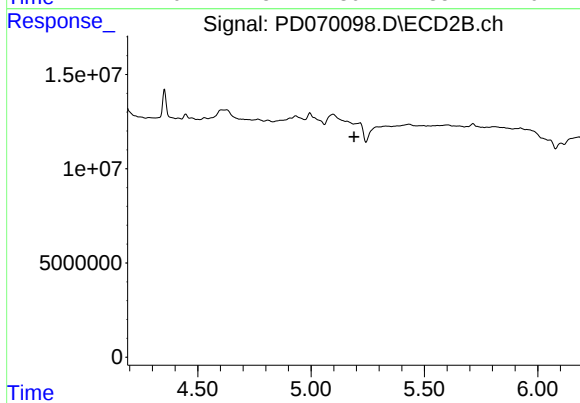

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

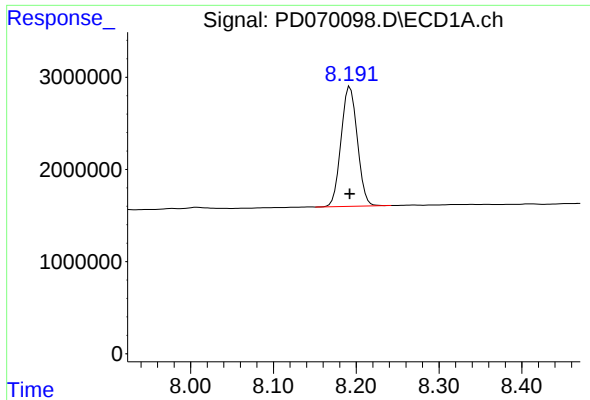

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 17732735
Conc: 16.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

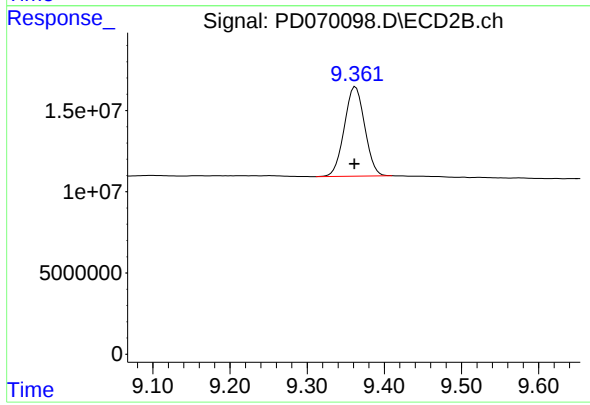

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.001 min
Response: 100906144
Conc: 18.66 ng/ml