

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2022 02:07
 Operator : AR\AJ
 Sample : N2953-04 5X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:11:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	2860109	29451125	2.688	3.342
28)	SA Decachlor...	8.193	9.363	3533864	20618110	3.240	3.812
Target Compounds							
13)	MA Dieldrin	5.746	6.690	927450	10434398	0.705	1.106 #
14)	MA Endrin	5.986	0.000	1152985	0	0.999	N.D. #
16)	A 4,4'-DDD	0.000	7.047	0	27327899	N.D.	3.690 #
17)	MA 4,4'-DDT	6.352	7.314f	2939138	24329681	2.966	3.325
18)	B Endrin al...	6.446	0.000	1170041	0	1.362	N.D. #
19)	B Endosulfa...	6.641	0.000	2217442	0	1.924	N.D. #
20)	A Methoxychlor	6.886f	0.000	4388663	0	7.736	N.D. #
21)	B Endrin ke...	7.162f	0.000	1273046	0	0.955	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2022 02:07
Operator : AR\AJ
Sample : N2953-04 5X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:11:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

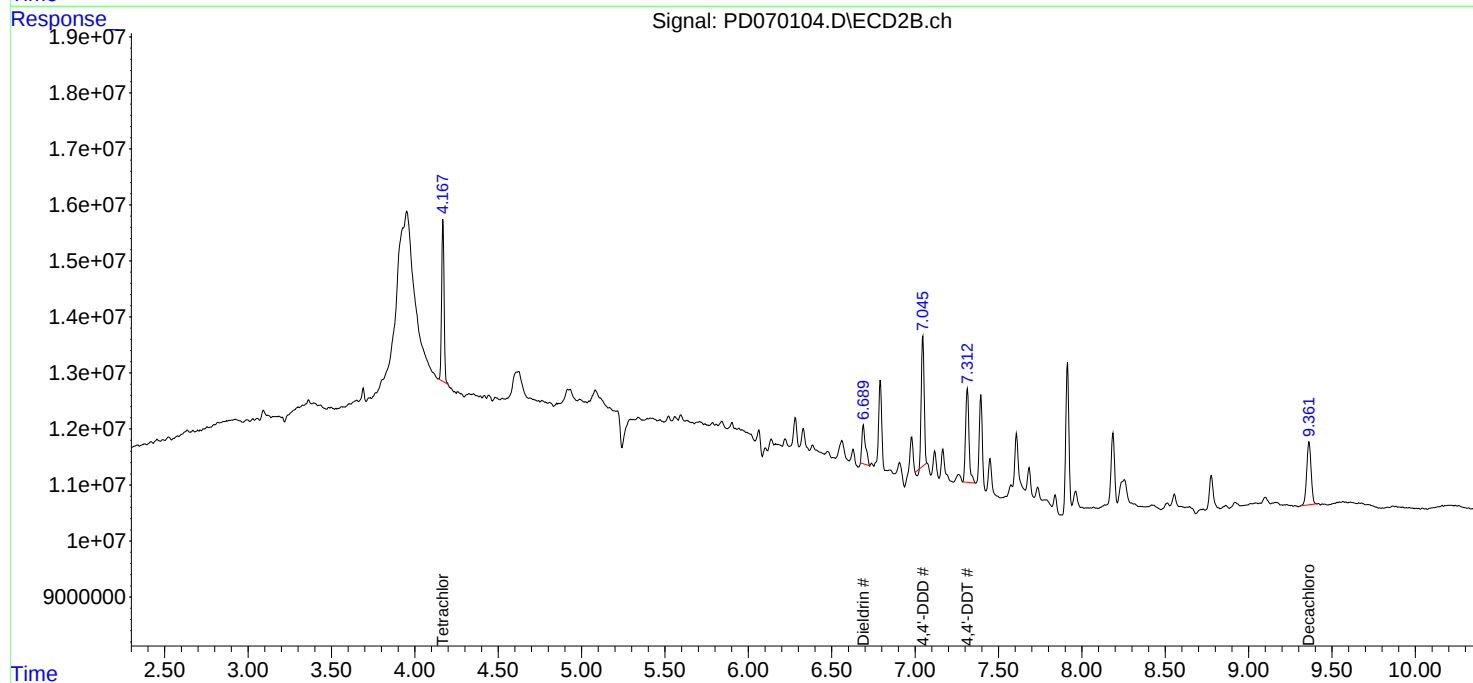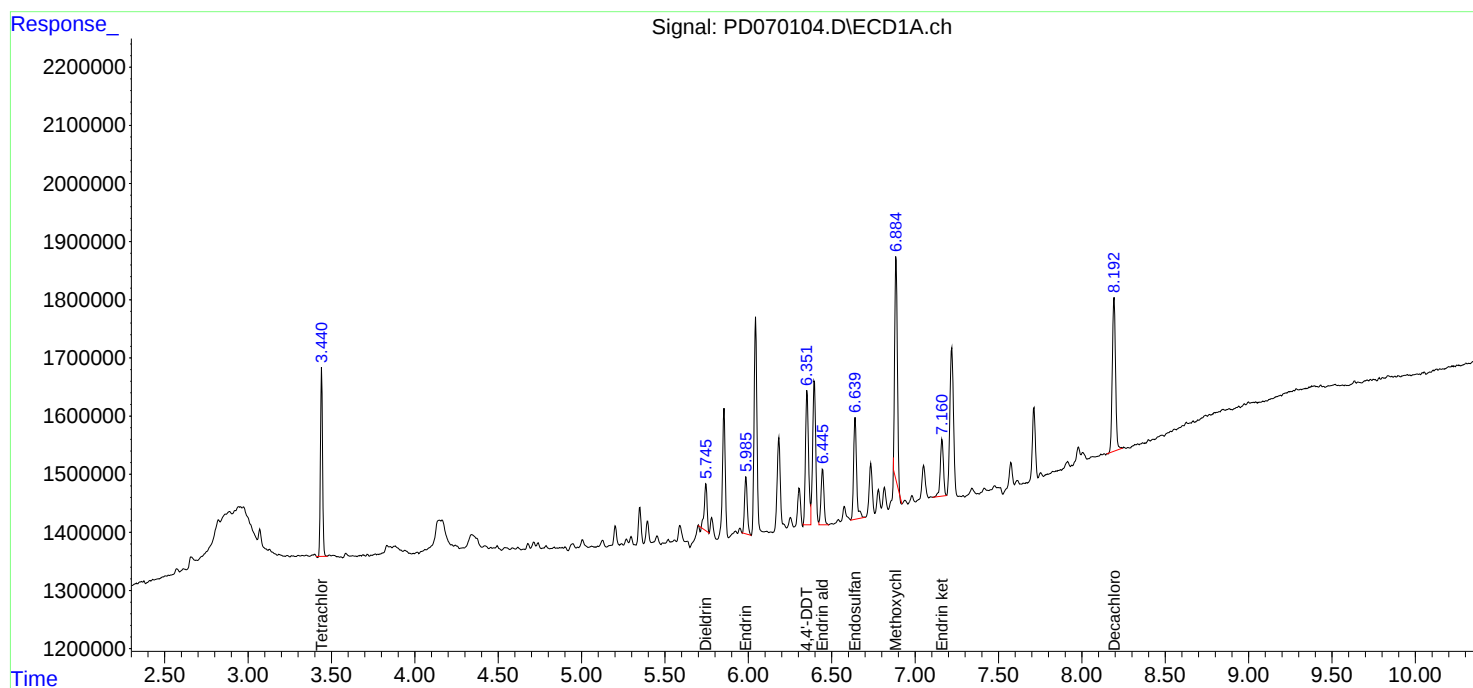


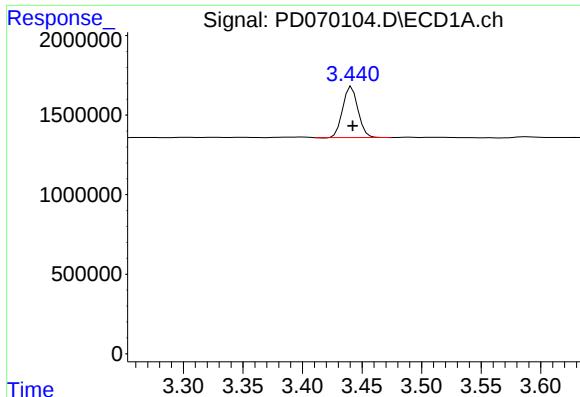

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 2860109
Conc: 2.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

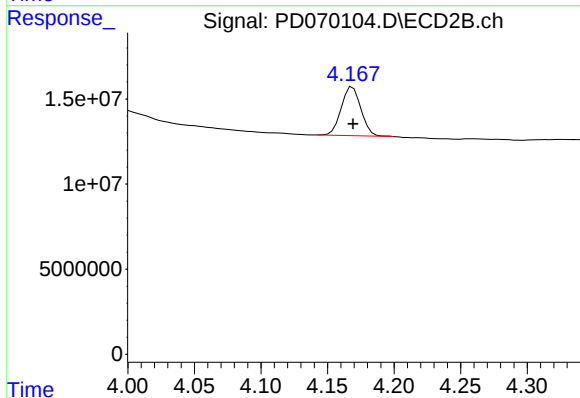


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 29451125
Conc: 3.34 ng/ml

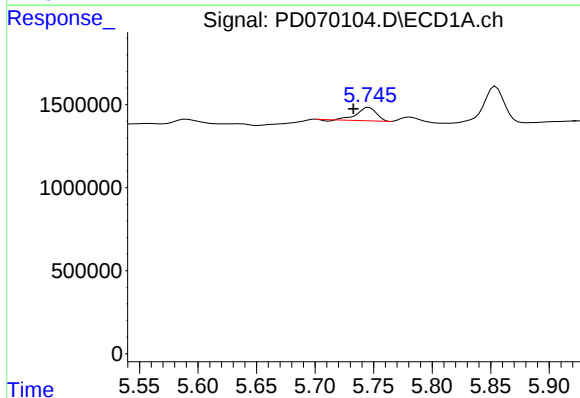


#13 Dieldrin

R.T.: 5.746 min
Delta R.T.: 0.013 min
Response: 927450
Conc: 0.70 ng/ml

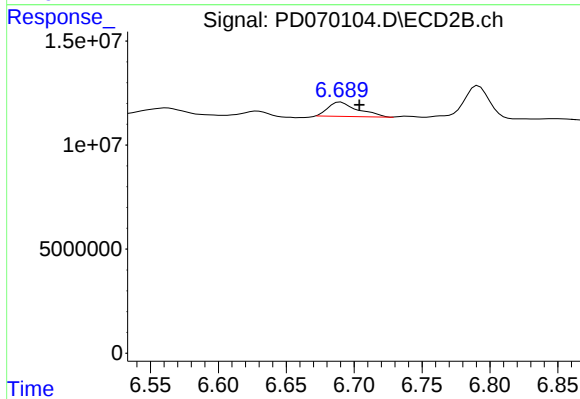

#13 Dieldrin


R.T.: 6.690 min
Delta R.T.: -0.014 min
Response: 10434398
Conc: 1.11 ng/ml

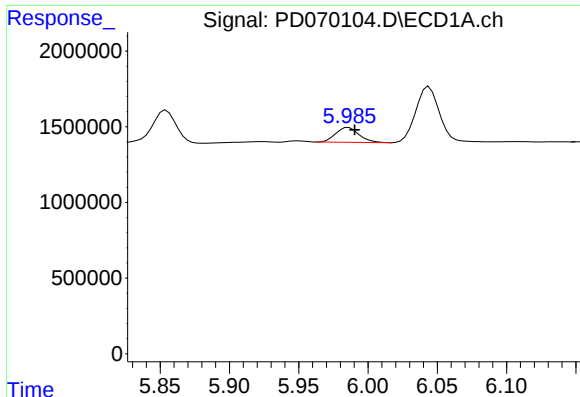

#14 Endrin


R.T.: 5.986 min
Delta R.T.: -0.004 min
Response: 1152985
Conc: 1.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

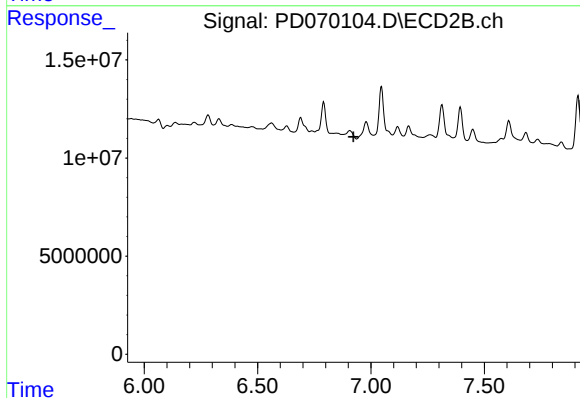


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

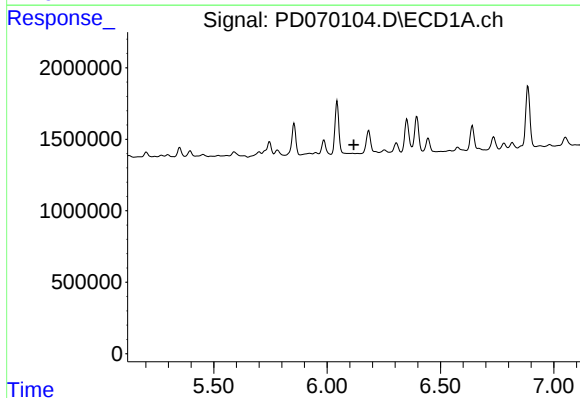


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

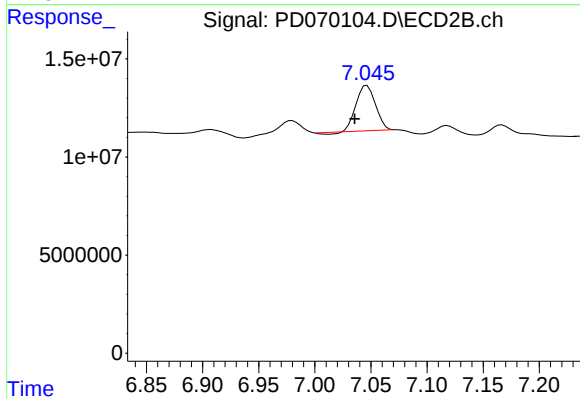

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: 0.011 min
Response: 27327899
Conc: 3.69 ng/ml

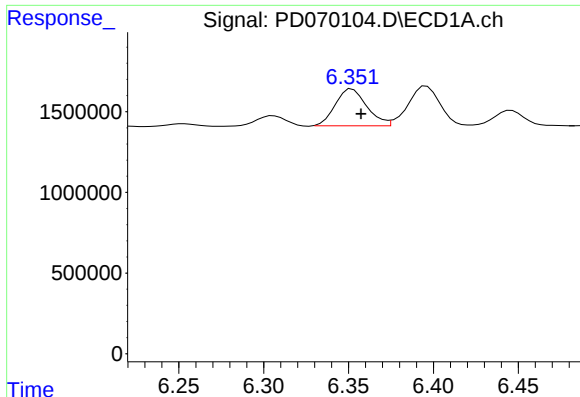

#17 4,4'-DDT


R.T.: 6.352 min
Delta R.T.: -0.005 min
Response: 2939138
Conc: 2.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

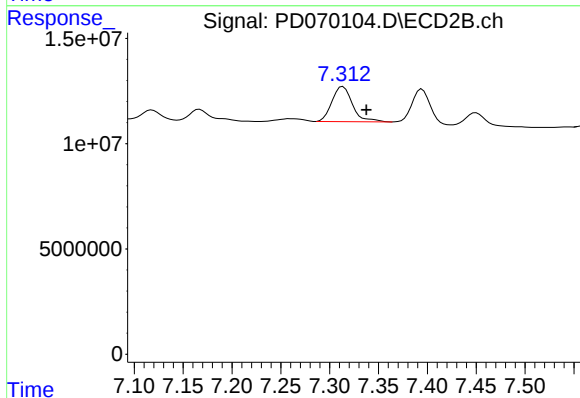


#17 4,4'-DDT

R.T.: 7.314 min
Delta R.T.: -0.024 min
Response: 24329681
Conc: 3.32 ng/ml

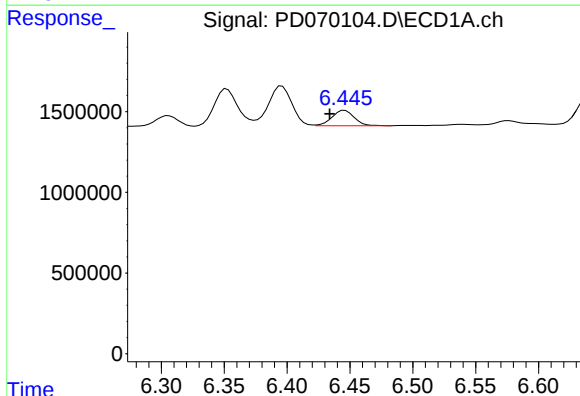


#18 Endrin aldehyde

R.T.: 6.446 min
Delta R.T.: 0.012 min
Response: 1170041
Conc: 1.36 ng/ml

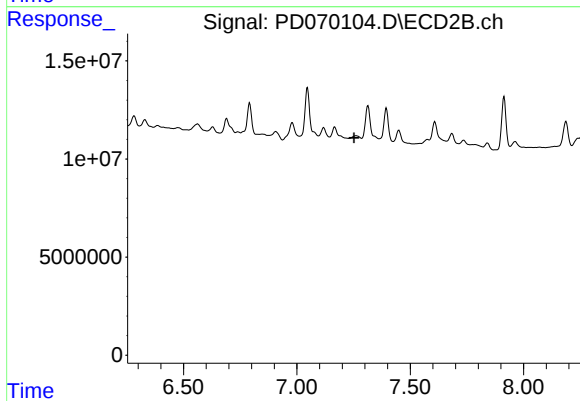

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

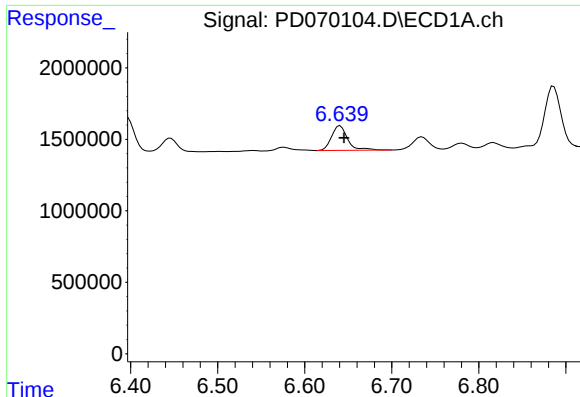

#19 Endosulfan Sulfate


R.T.: 6.641 min
Delta R.T.: -0.005 min
Response: 2217442
Conc: 1.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

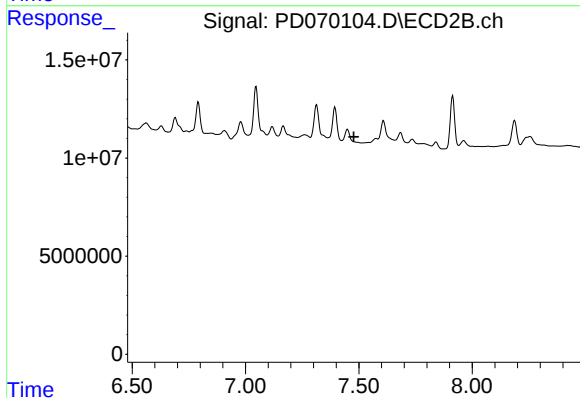


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

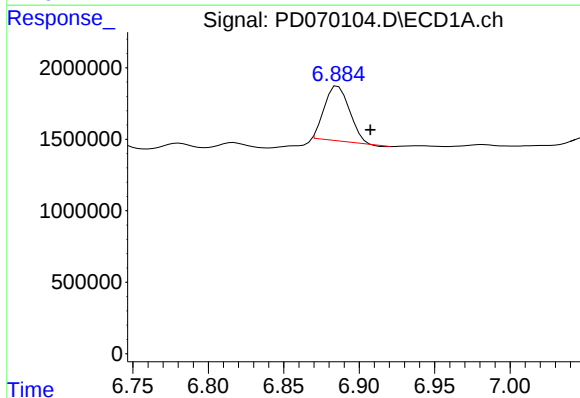


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: -0.022 min
Response: 4388663
Conc: 7.74 ng/ml

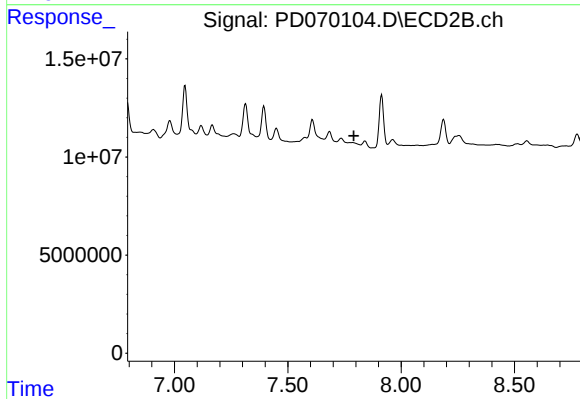

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

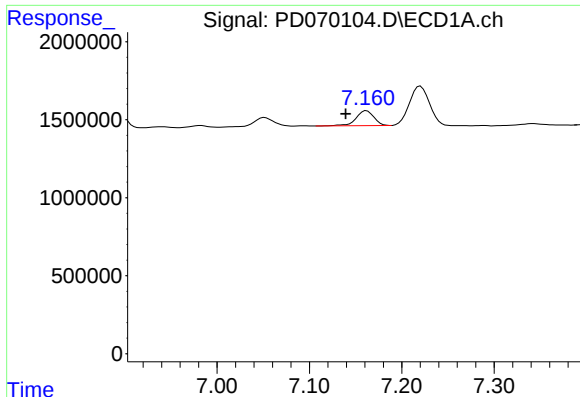

#21 Endrin ketone


R.T.: 7.162 min
Delta R.T.: 0.023 min
Response: 1273046
Conc: 0.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

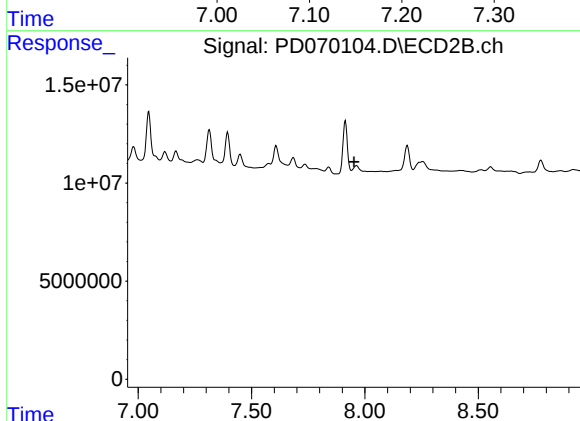


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

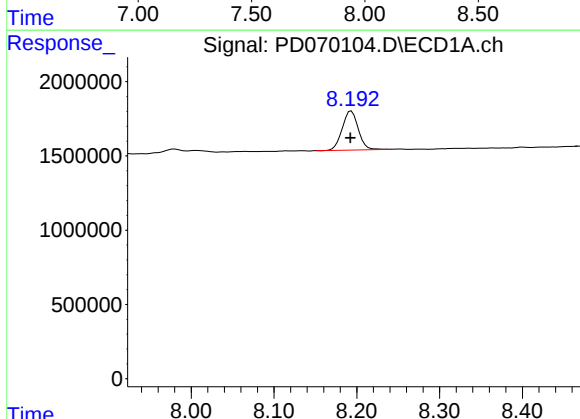

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.001 min
Response: 3533864
Conc: 3.24 ng/ml

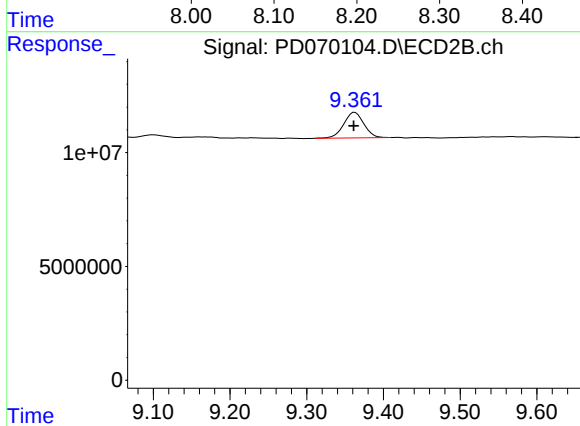

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.001 min
Response: 20618110
Conc: 3.81 ng/ml