

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2022 03:03
 Operator : AR\AJ
 Sample : N2953-08
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:12:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	10448084	105.8E6	9.818	12.009
28)	SA Decachlor...	8.194	9.364	10844918	63695984	9.943	11.778
Target Compounds							
12)	B 4,4'-DDE	5.599	6.547	990901	7869417	0.782	0.870
14)	MA Endrin	5.987	0.000	1033368	0	0.895	N.D. #
16)	A 4,4'-DDD	0.000	7.047	0	24146802	N.D.	3.261 #
17)	MA 4,4'-DDT	6.353	7.313f	2483008	20909755	2.505	2.857
18)	B Endrin al...	6.446	0.000	1005101	0	1.170	N.D. #
19)	B Endosulfa...	6.642	0.000	1438246	0	1.248	N.D. #
20)	A Methoxychlor	6.887f	0.000	3981592	0	7.018	N.D. #
21)	B Endrin ke...	7.163f	0.000	1246086	0	0.935	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2022 03:03
Operator : AR\AJ
Sample : N2953-08
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:12:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

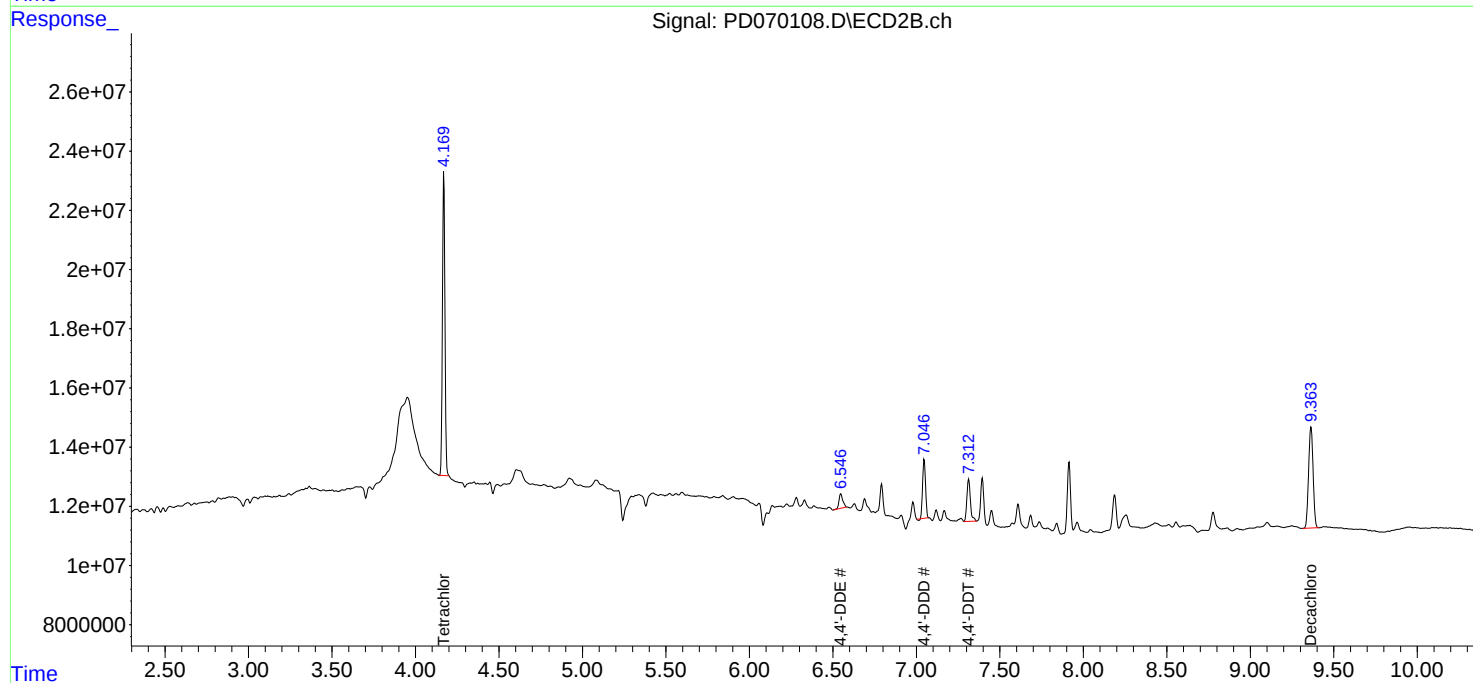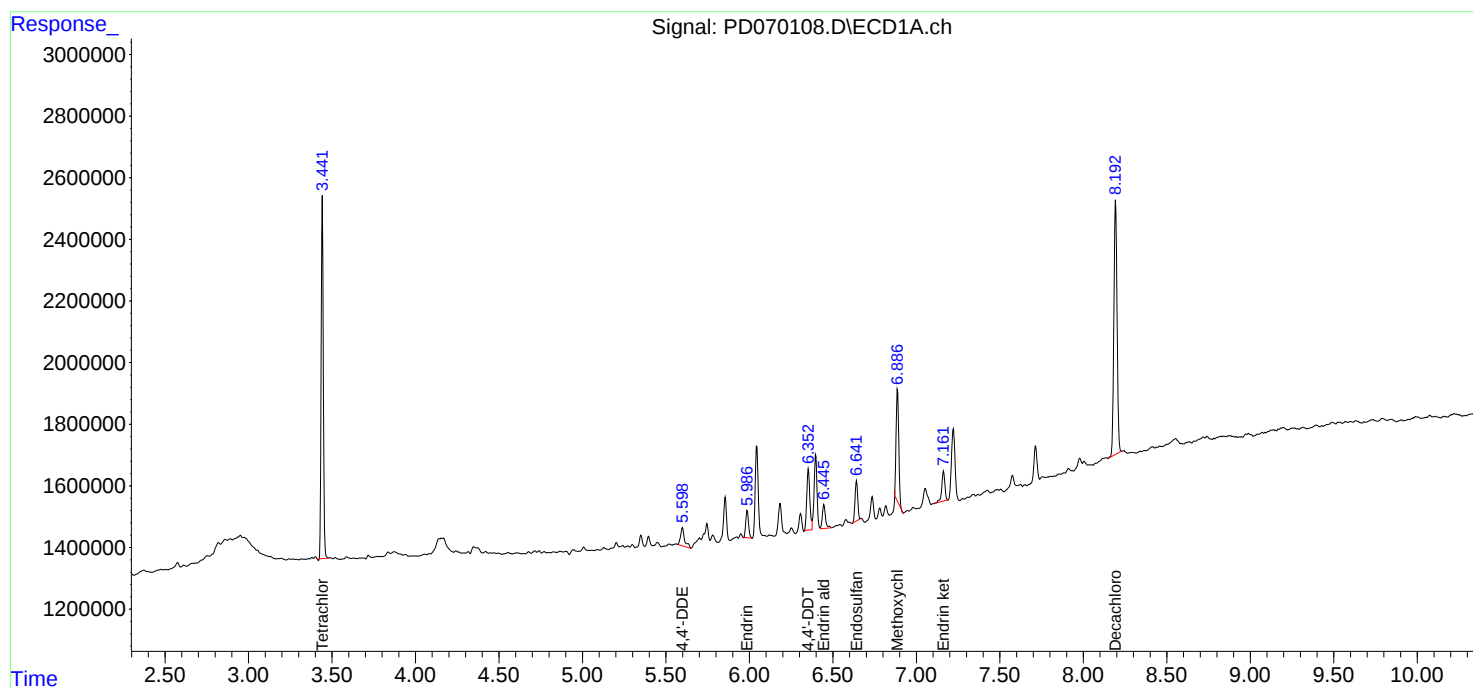


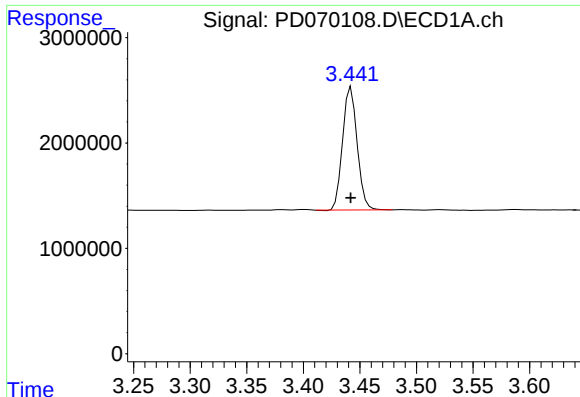

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 10448084
Conc: 9.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

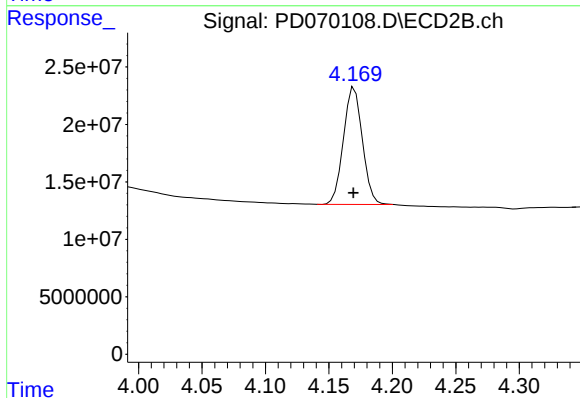


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 105821924
Conc: 12.01 ng/ml

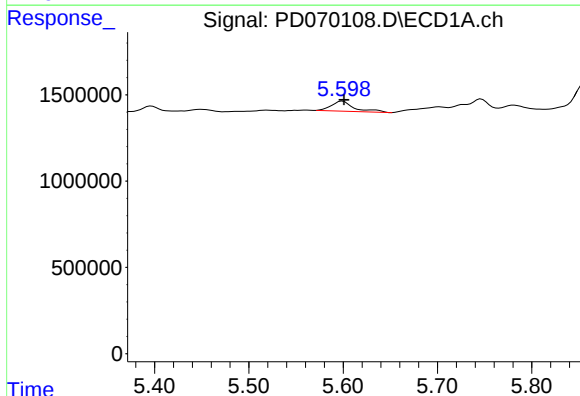


#12 4,4'-DDE

R.T.: 5.599 min
Delta R.T.: -0.002 min
Response: 990901
Conc: 0.78 ng/ml

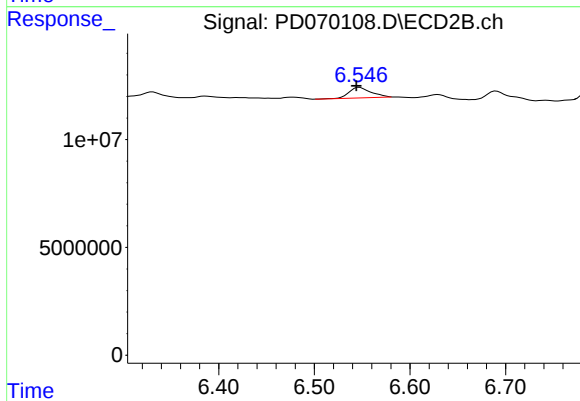

#12 4,4'-DDE


R.T.: 6.547 min
Delta R.T.: 0.003 min
Response: 7869417
Conc: 0.87 ng/ml

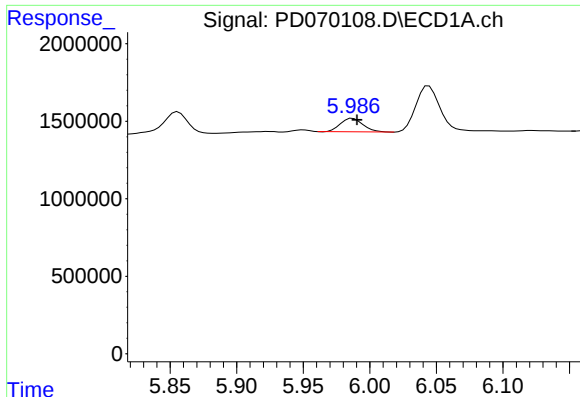

#14 Endrin


R.T.: 5.987 min
Delta R.T.: -0.003 min
Response: 1033368
Conc: 0.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

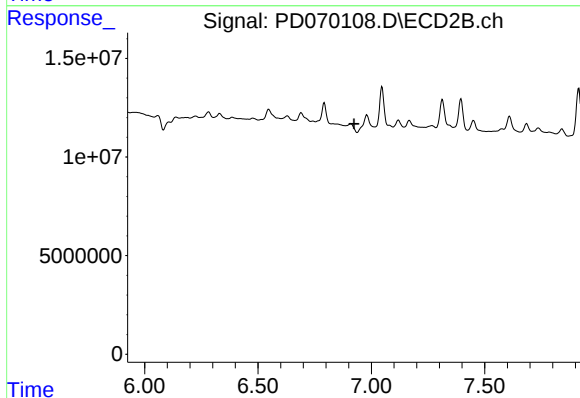


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

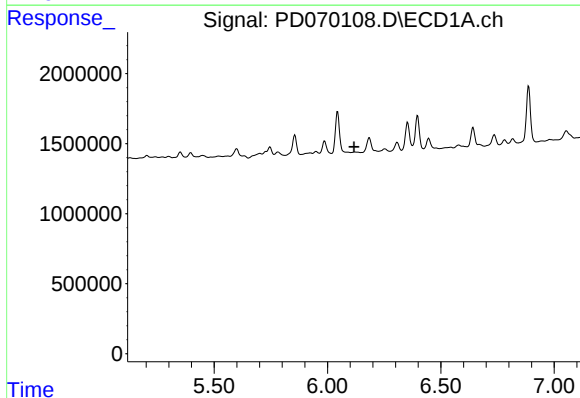


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

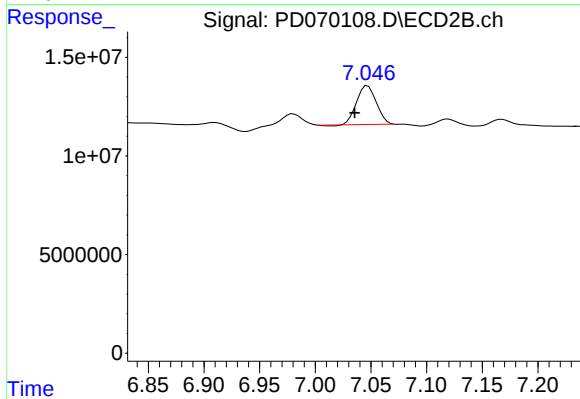

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: 0.011 min
Response: 24146802
Conc: 3.26 ng/ml

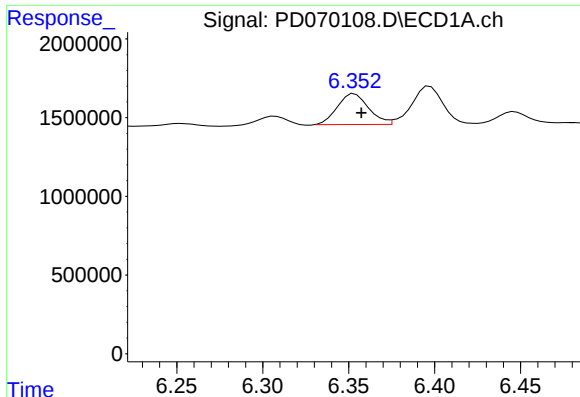

#17 4,4'-DDT


R.T.: 6.353 min
Delta R.T.: -0.004 min
Response: 2483008
Conc: 2.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

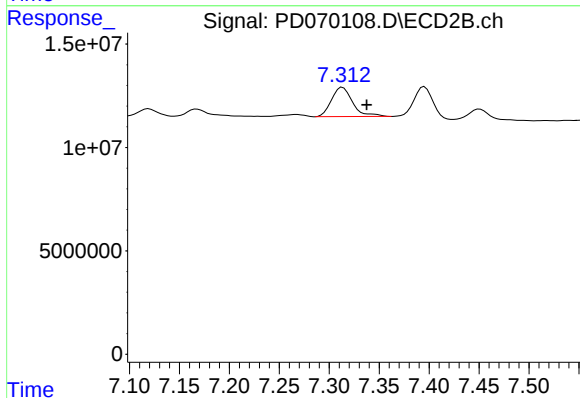


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: -0.024 min
Response: 20909755
Conc: 2.86 ng/ml

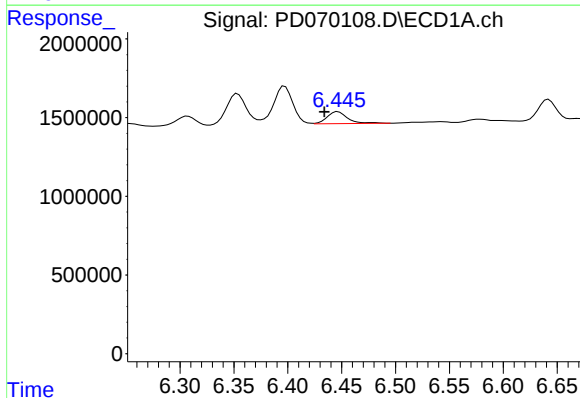


#18 Endrin aldehyde

R.T.: 6.446 min
Delta R.T.: 0.012 min
Response: 1005101
Conc: 1.17 ng/ml

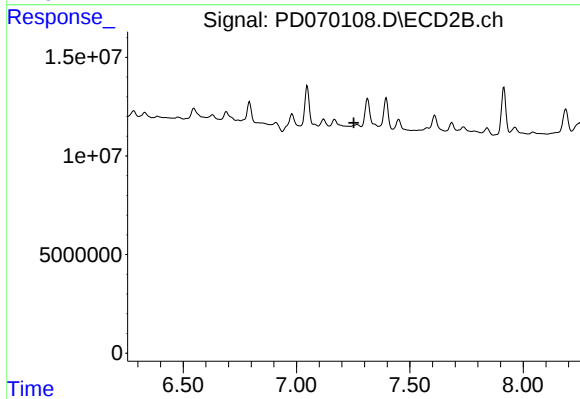

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

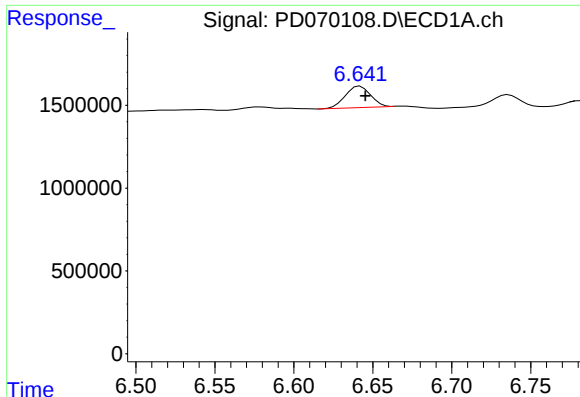

#19 Endosulfan Sulfate


R.T.: 6.642 min
Delta R.T.: -0.003 min
Response: 1438246
Conc: 1.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

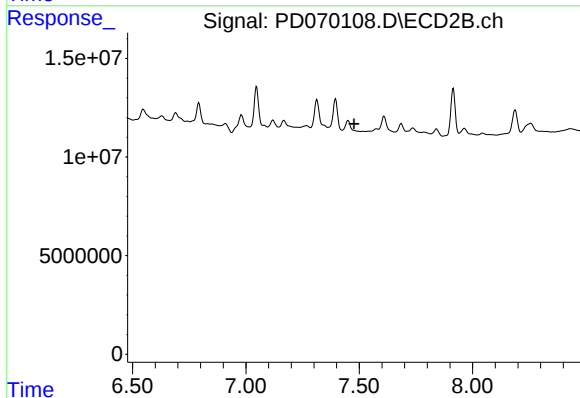


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

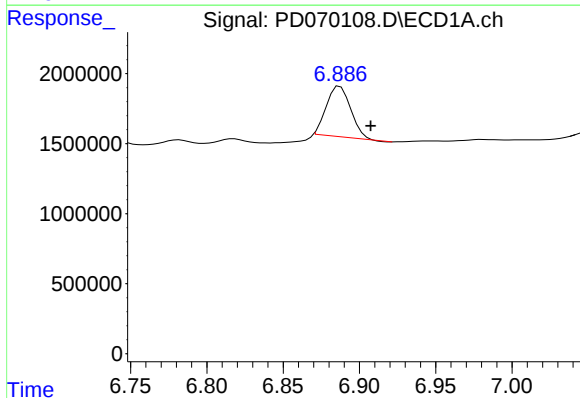


#20 Methoxychlor

R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 3981592
Conc: 7.02 ng/ml

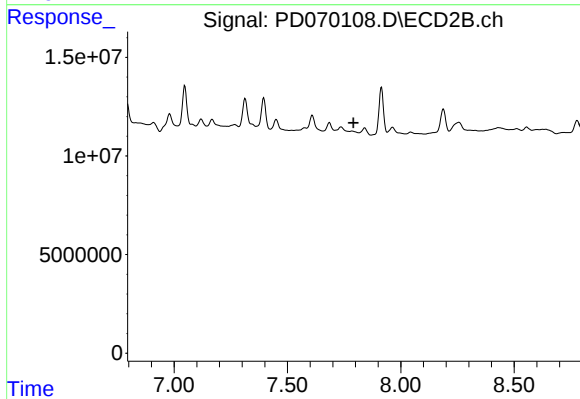

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

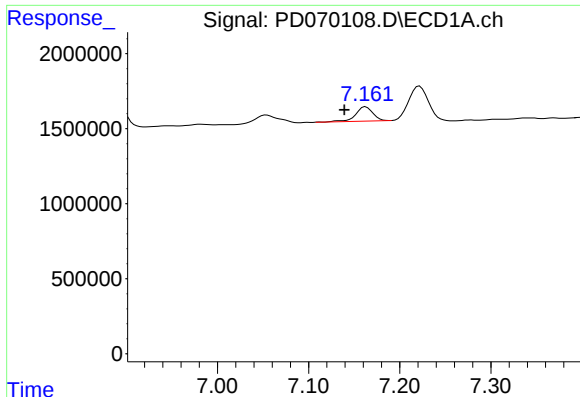

#21 Endrin ketone


R.T.: 7.163 min
Delta R.T.: 0.023 min
Response: 1246086
Conc: 0.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

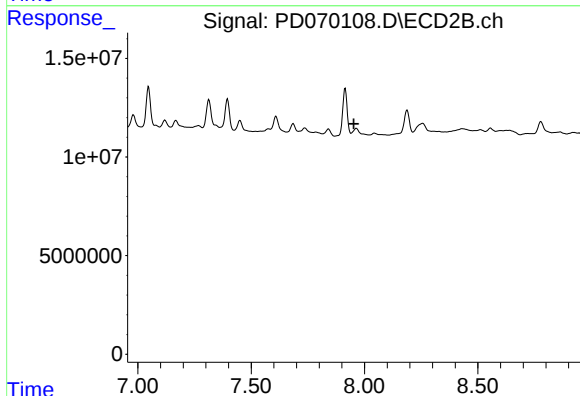


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

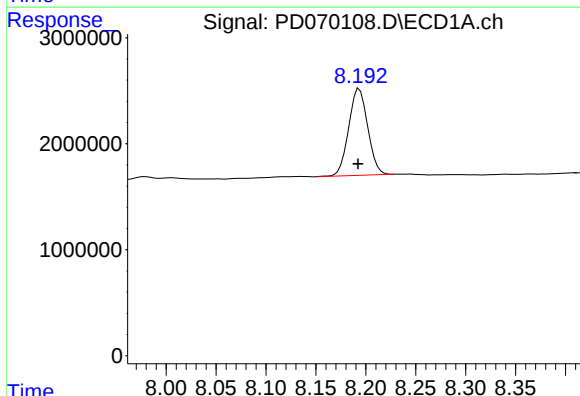

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.001 min
Response: 10844918
Conc: 9.94 ng/ml

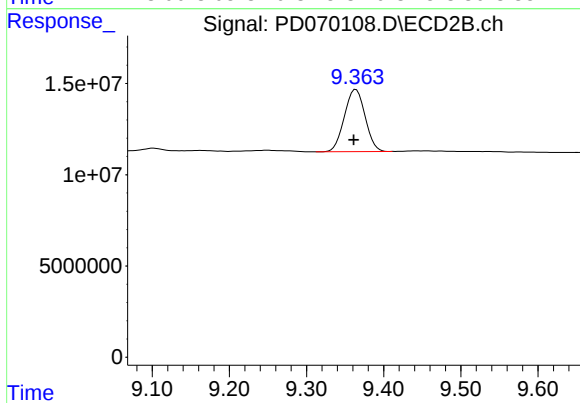

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.003 min
Response: 63695984
Conc: 11.78 ng/ml