

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 12:20
 Operator : AR\AJ
 Sample : N3170-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20220424-SPLP-AMENDED-COMPOSITE-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:35:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	22047734	177.1E6	20.717	20.094
28)	SA Decachlor...	8.193	9.362	18911170	116.1E6	17.338	21.471

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 12:20
Operator : AR\AJ
Sample : N3170-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20220424-SPLP-AMENDED-COMPOSITE-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:35:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

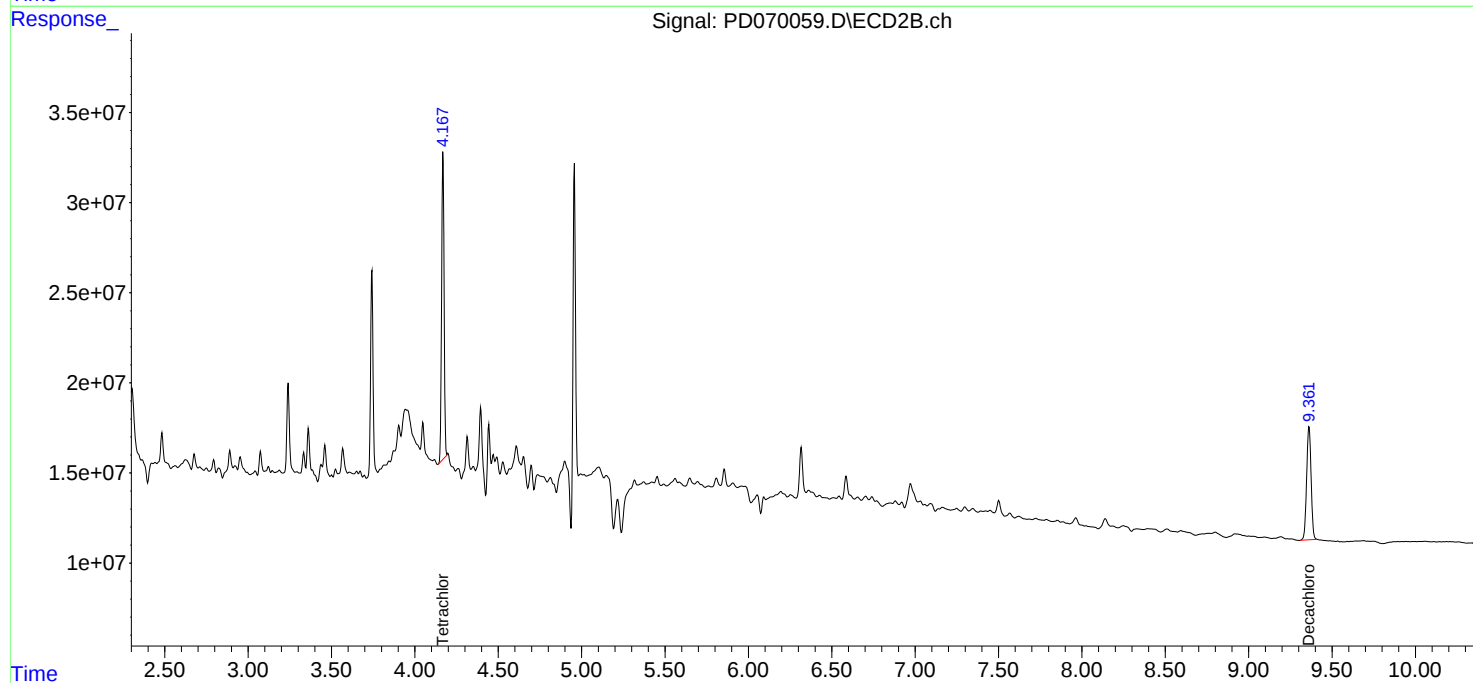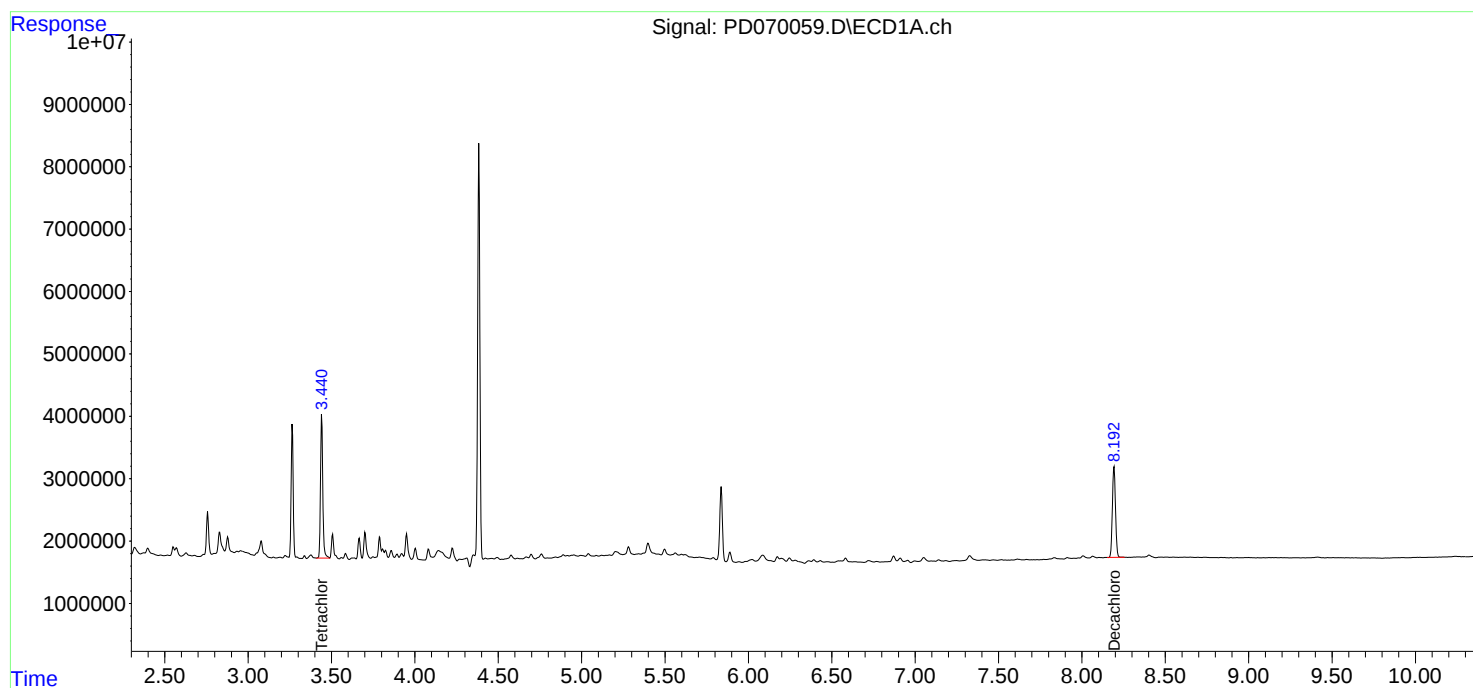

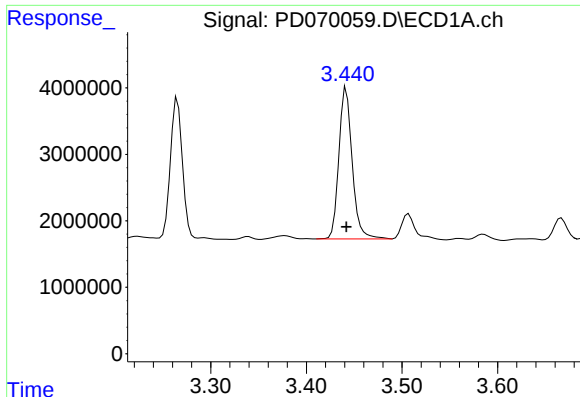

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 22047734
Conc: 20.72 ng/ml

Instrument :

ECD_D


ClientSampleId :

20220424-SPLP-AMENDED-COMPOSITE-D

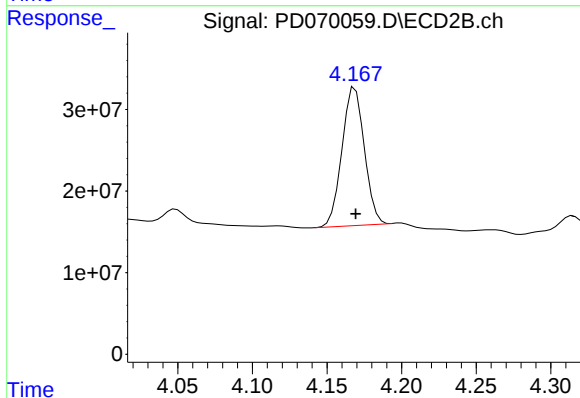


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 177063271
Conc: 20.09 ng/ml

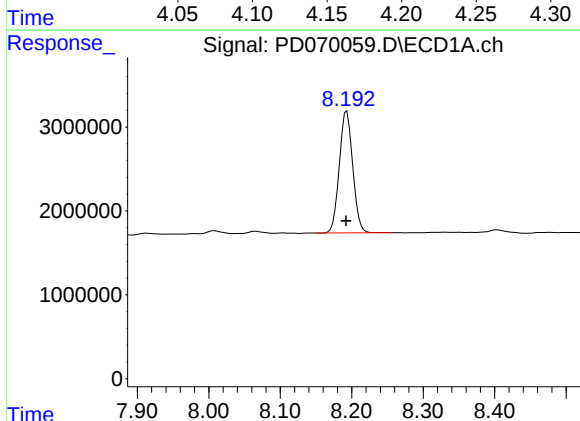

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 18911170
Conc: 17.34 ng/ml

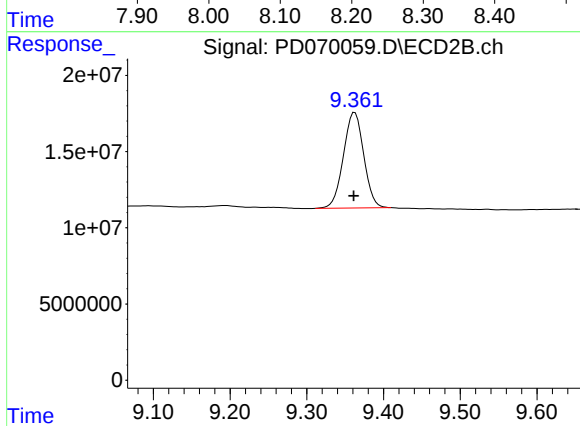

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: 0.001 min
Response: 116118862
Conc: 21.47 ng/ml