

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 14:38
 Operator : AR\AJ
 Sample : N2986-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P027-SS001-2430-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/06/2022
 Supervised By : Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 12:37:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.169	20427189	196.6E6	19.195	22.306
28)	SA Decachlor...	8.197	9.366	16528458	111.1E6	15.153m	20.548 #
Target Compounds							
12)	B 4,4'-DDE	5.605	6.544	7005502	84367571	5.529m	9.325m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 14:38
Operator : AR\AJ
Sample : N2986-08
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P027-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/06/2022
Supervised By : Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 12:37:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

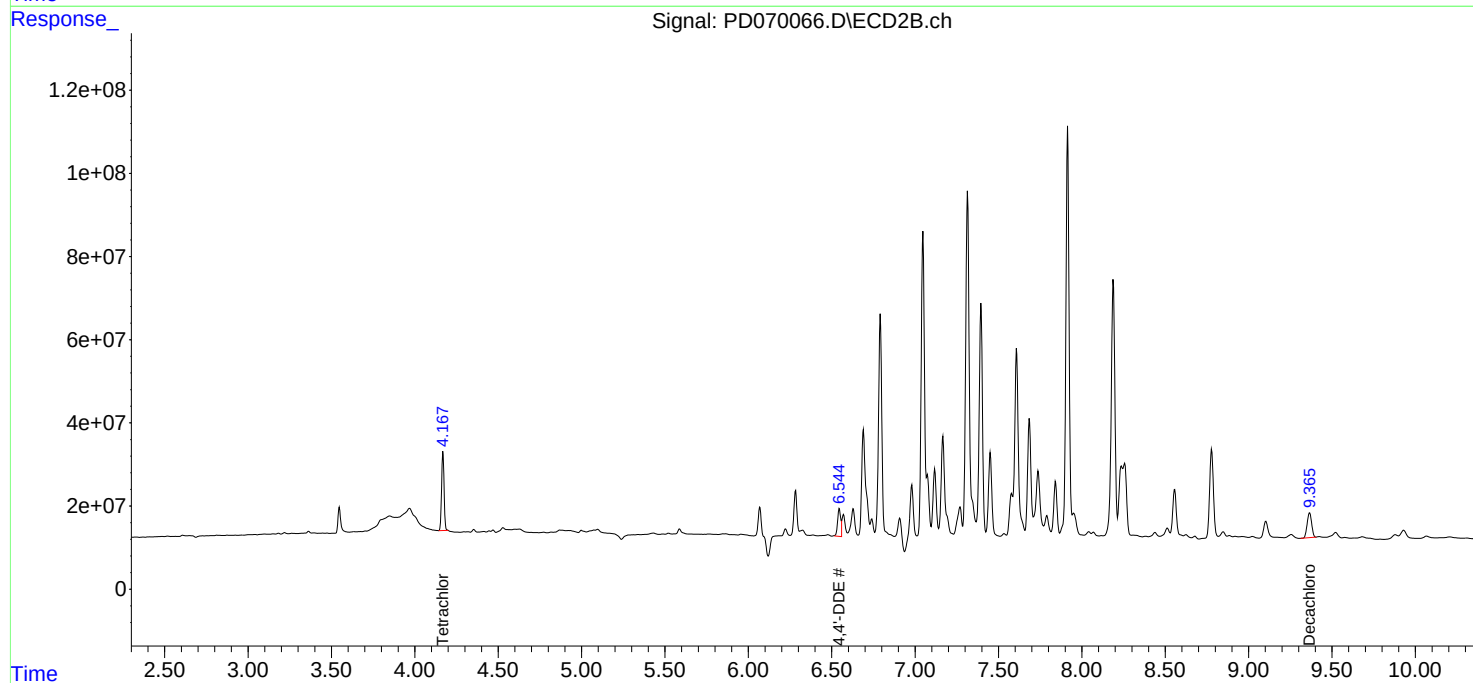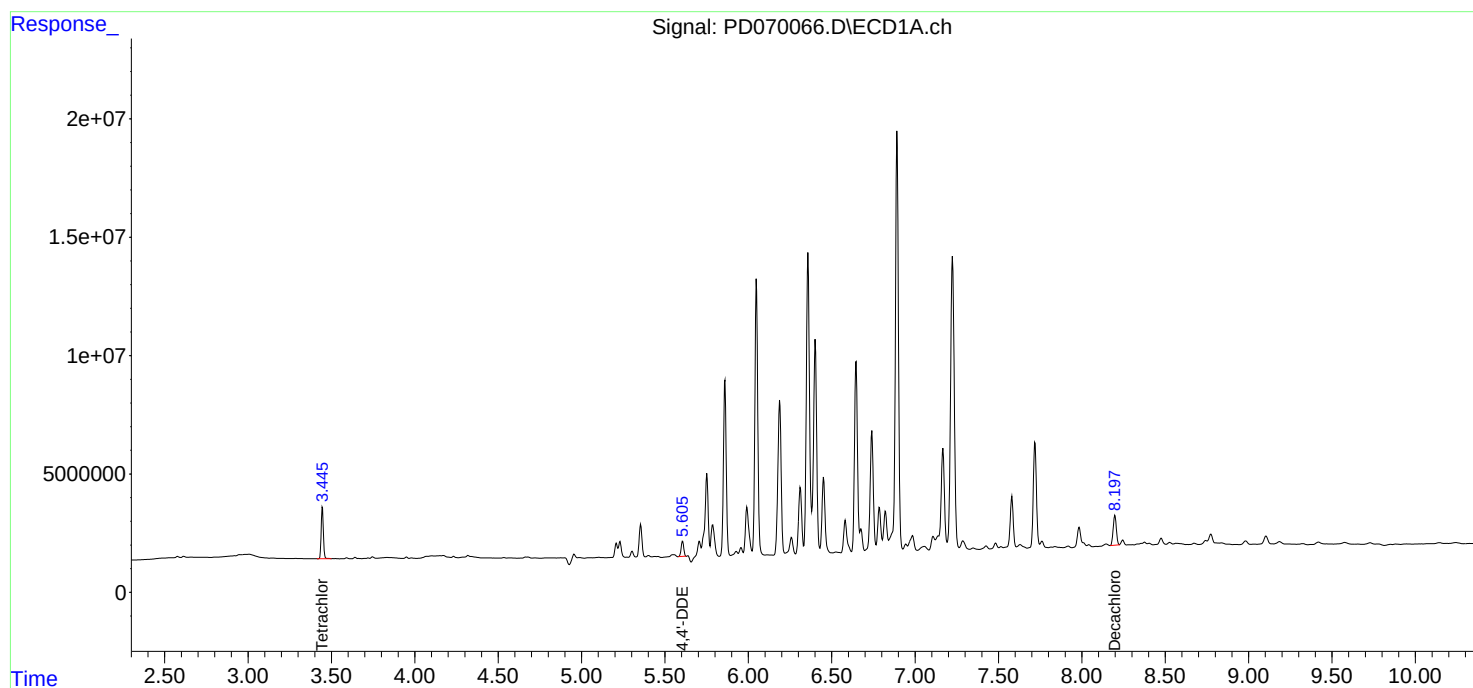

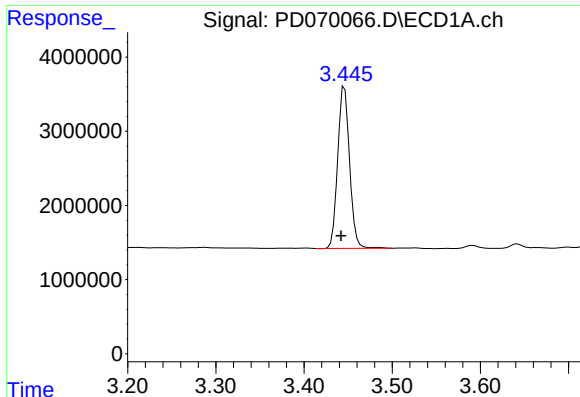


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.004 min
Response: 20427189
Conc: 19.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
P027-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/06/2022
Supervised By :Ankita Jodhani 06/07/2022

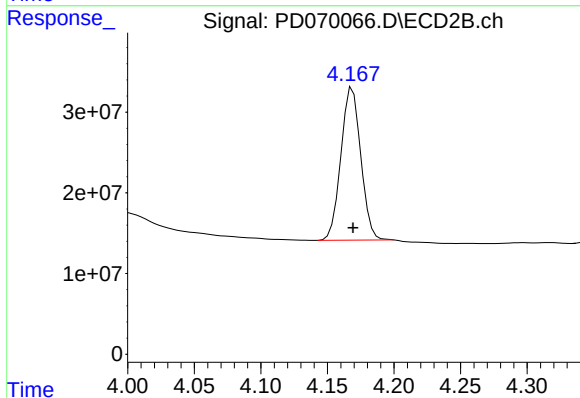


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 196554062
Conc: 22.31 ng/ml

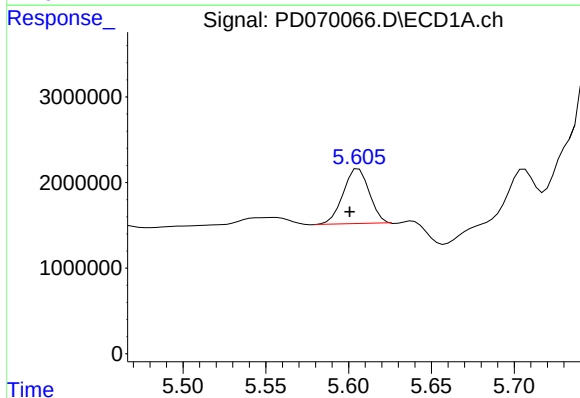


#12 4,4'-DDE

R.T.: 5.605 min
Delta R.T.: 0.004 min
Response: 7005502
Conc: 5.53 ng/ml m

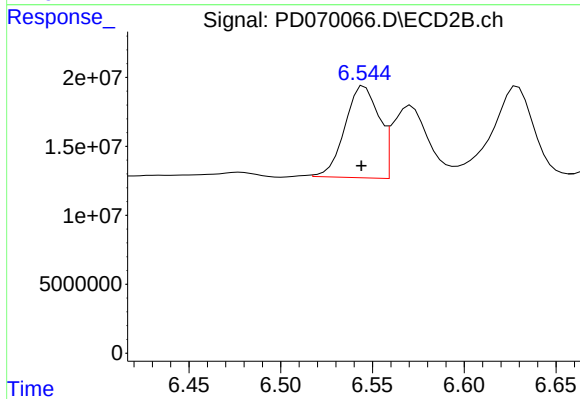

#12 4,4'-DDE

R.T.: 6.544 min
Delta R.T.: 0.000 min
Response: 84367571
Conc: 9.32 ng/ml m

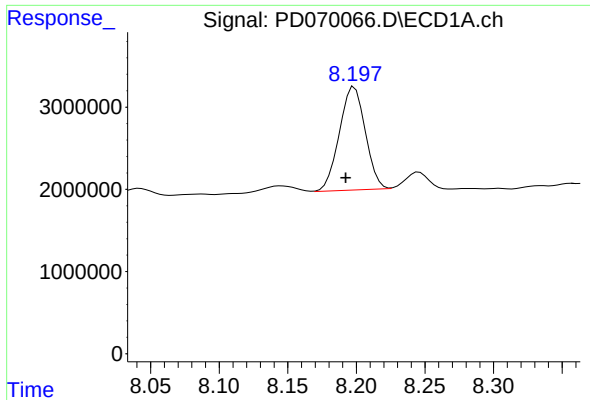


#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: 0.005 min
Response: 16528458
Conc: 15.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
P027-SS001-2430-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/06/2022
Supervised By :Ankita Jodhani 06/07/2022

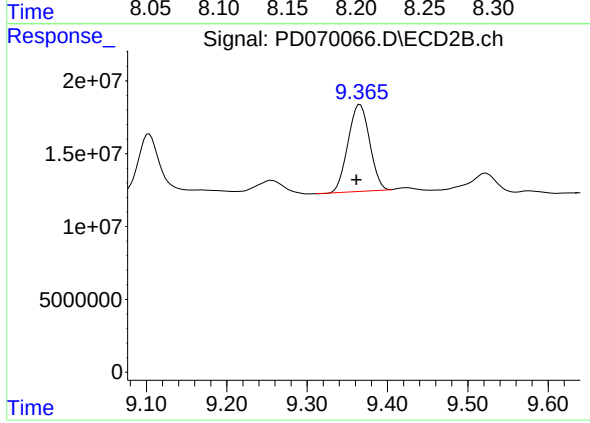

#28 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: 0.005 min
Response: 111124927
Conc: 20.55 ng/ml