

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
 Data File : PD070088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 20:42
 Operator : AR\AJ
 Sample : N2952-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P037-SS001-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/06/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:07:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	4.169	13073661	127.3E6	12.285	14.445
28) SA Decachlor...	8.194	9.364	14865887	86413758	13.629	15.979
Target Compounds						
12) B 4,4'-DDE	5.599	6.547	1169881	9748253	0.923m	1.077

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060522\
Data File : PD070088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 20:42
Operator : AR\AJ
Sample : N2952-07
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P037-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/06/2022
Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:07:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

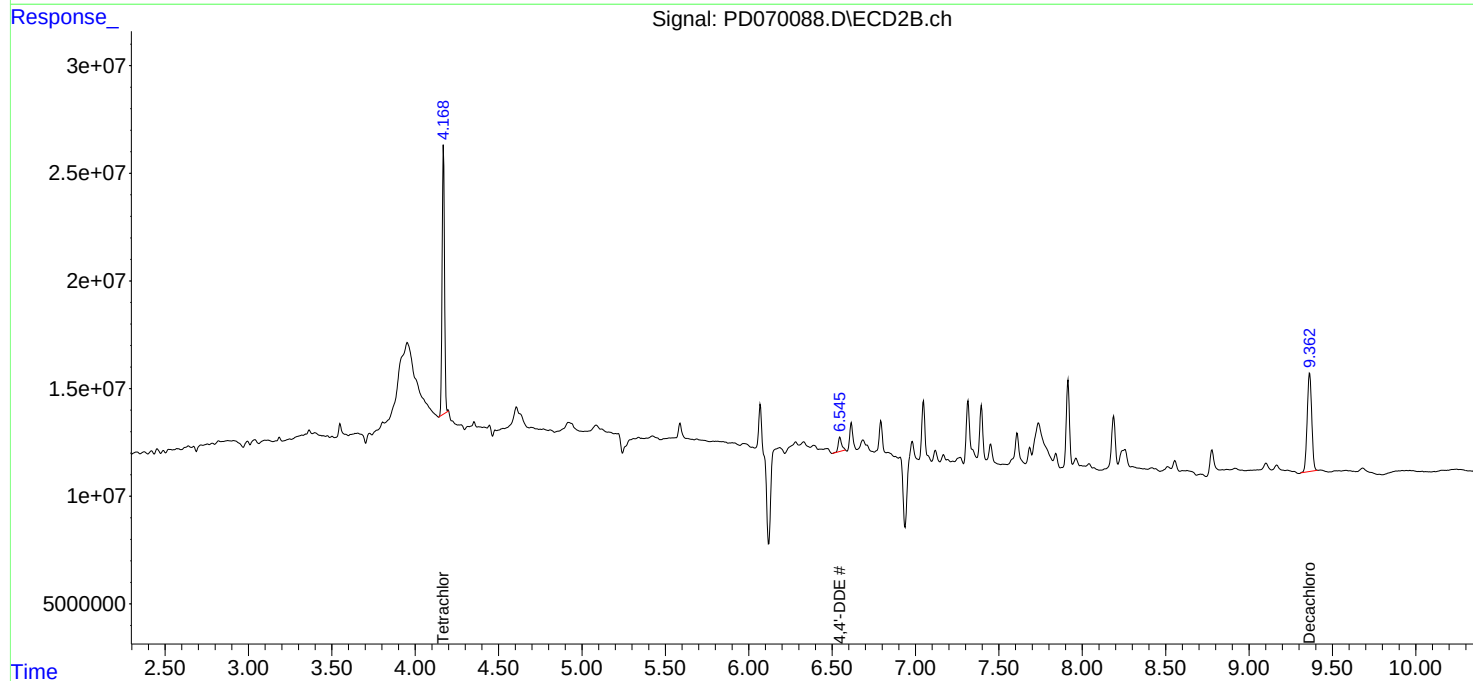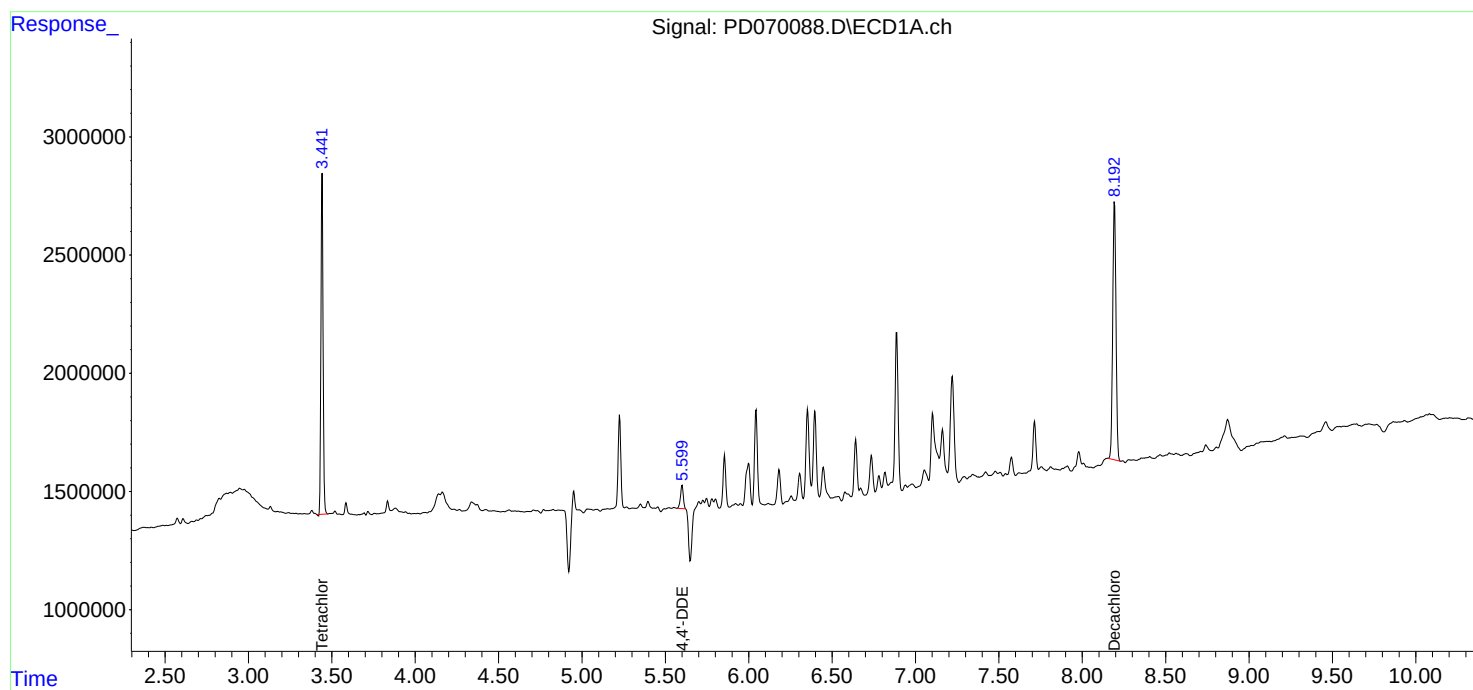

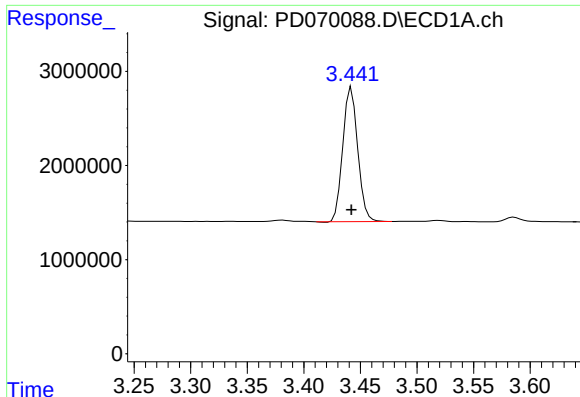


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 13073661
Conc: 12.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
P037-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/06/2022
Supervised By :Ankita Jodhani 06/07/2022

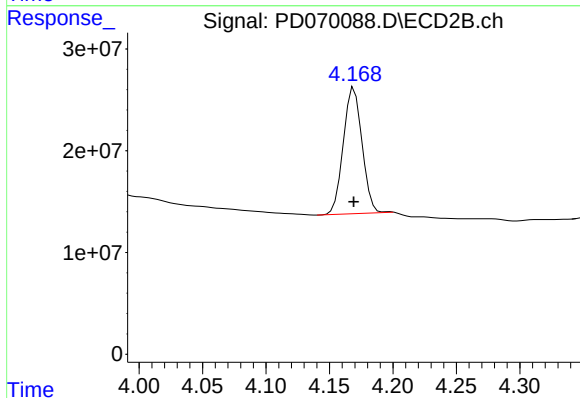


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 127288256
Conc: 14.45 ng/ml

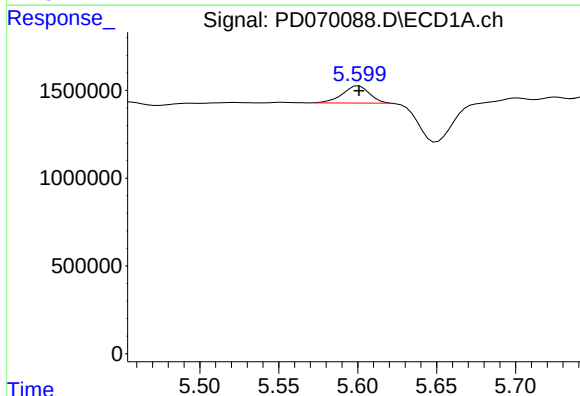


#12 4,4'-DDE

R.T.: 5.599 min
Delta R.T.: -0.001 min
Response: 1169881
Conc: 0.92 ng/ml m

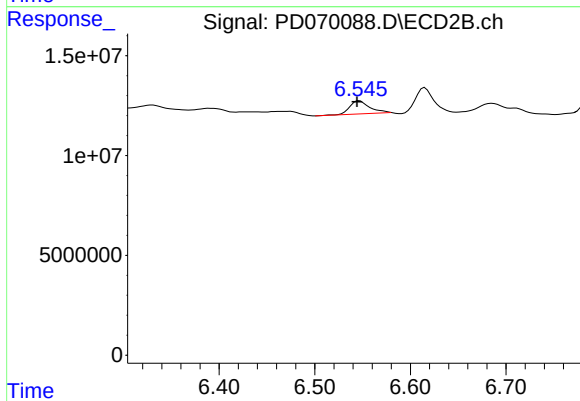

#12 4,4'-DDE

R.T.: 6.547 min
Delta R.T.: 0.003 min
Response: 9748253
Conc: 1.08 ng/ml

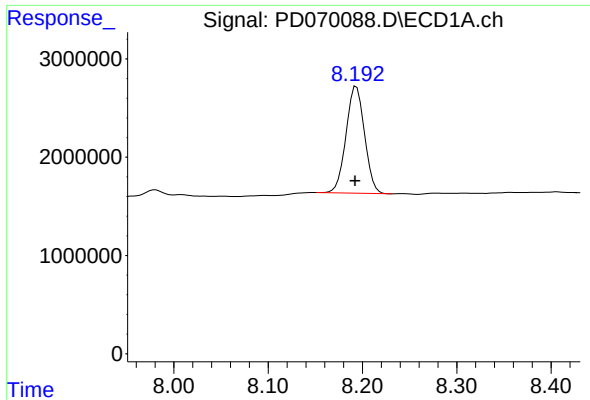


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.001 min
Response: 14865887
Conc: 13.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
P037-SS001-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/06/2022
Supervised By :Ankita Jodhani 06/07/2022

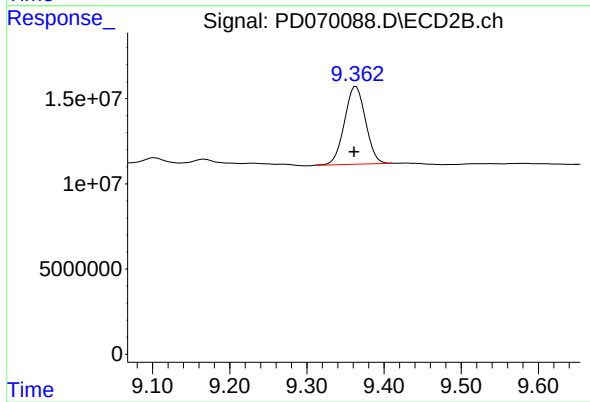

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.002 min
Response: 86413758
Conc: 15.98 ng/ml