

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060524\
 Data File : PD083394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 20:42
 Operator : AR\AJ
 Sample : P2577-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH639MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2024
 Supervised By :Ankita Jodhani 06/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 21:30:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	16695032	69144222	11.637m	14.598m#
2)	SA Decachlor...	9.111	7.898	32339905	77210155	15.826m	15.481
Target Compounds							
2)	A alpha-BHC	4.020	3.272	128.5E6	392.6E6	51.106	54.187
3)	MA gamma-BHC...	4.352	3.601	131.2E6	364.2E6	53.950m	53.660
4)	MA Heptachlor	4.944	3.939	127.6E6	350.8E6	50.549m	52.060
5)	MB Aldrin	5.289	4.218	122.3E6	327.9E6	50.504	50.636
6)	B beta-BHC	4.551	3.897	48349338	145.0E6	45.107	49.275
7)	B delta-BHC	4.800	4.126	130.1E6	370.7E6	49.210	52.612
8)	B Heptachlo...	5.717	4.719	110.6E6	306.5E6	50.362	51.461
9)	A Endosulfan I	6.103	5.089	101.9E6	220.7E6	47.966	40.489
10)	B trans-Chl...	5.972	4.968	112.6E6	324.4E6	51.894m	55.468
11)	B cis-Chlor...	6.053	5.032	115.2E6	322.2E6	51.912	54.053
12)	B 4,4'-DDE	6.224	5.221	192.7E6	641.9E6	86.748	112.357 #
13)	MA Dieldrin	6.380	5.350	233.2E6	708.6E6	103.144	116.828m
14)	MA Endrin	6.610	5.627	180.6E6	575.7E6	97.032	107.365
15)	B Endosulfa...	6.830	5.919	197.3E6	533.6E6	101.427	106.510m
16)	A 4,4'-DDD	6.743	5.774	162.3E6	466.3E6	101.040	100.661
17)	MA 4,4'-DDT	7.059	6.024	188.2E6	541.6E6	115.222	115.979
18)	B Endrin al...	6.960	6.100	129.3E6	358.6E6	89.600	93.530
19)	B Endosulfa...	7.196	6.322	164.0E6	495.2E6	89.762	101.793
20)	A Methoxychlor	7.536	6.598	400.4E6	1107.5E6	435.529	453.057m
21)	B Endrin ke...	7.683	6.827	174.8E6	489.8E6	91.043	91.810

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060524\
Data File : PD083394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 20:42
Operator : AR\AJ
Sample : P2577-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 21:30:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

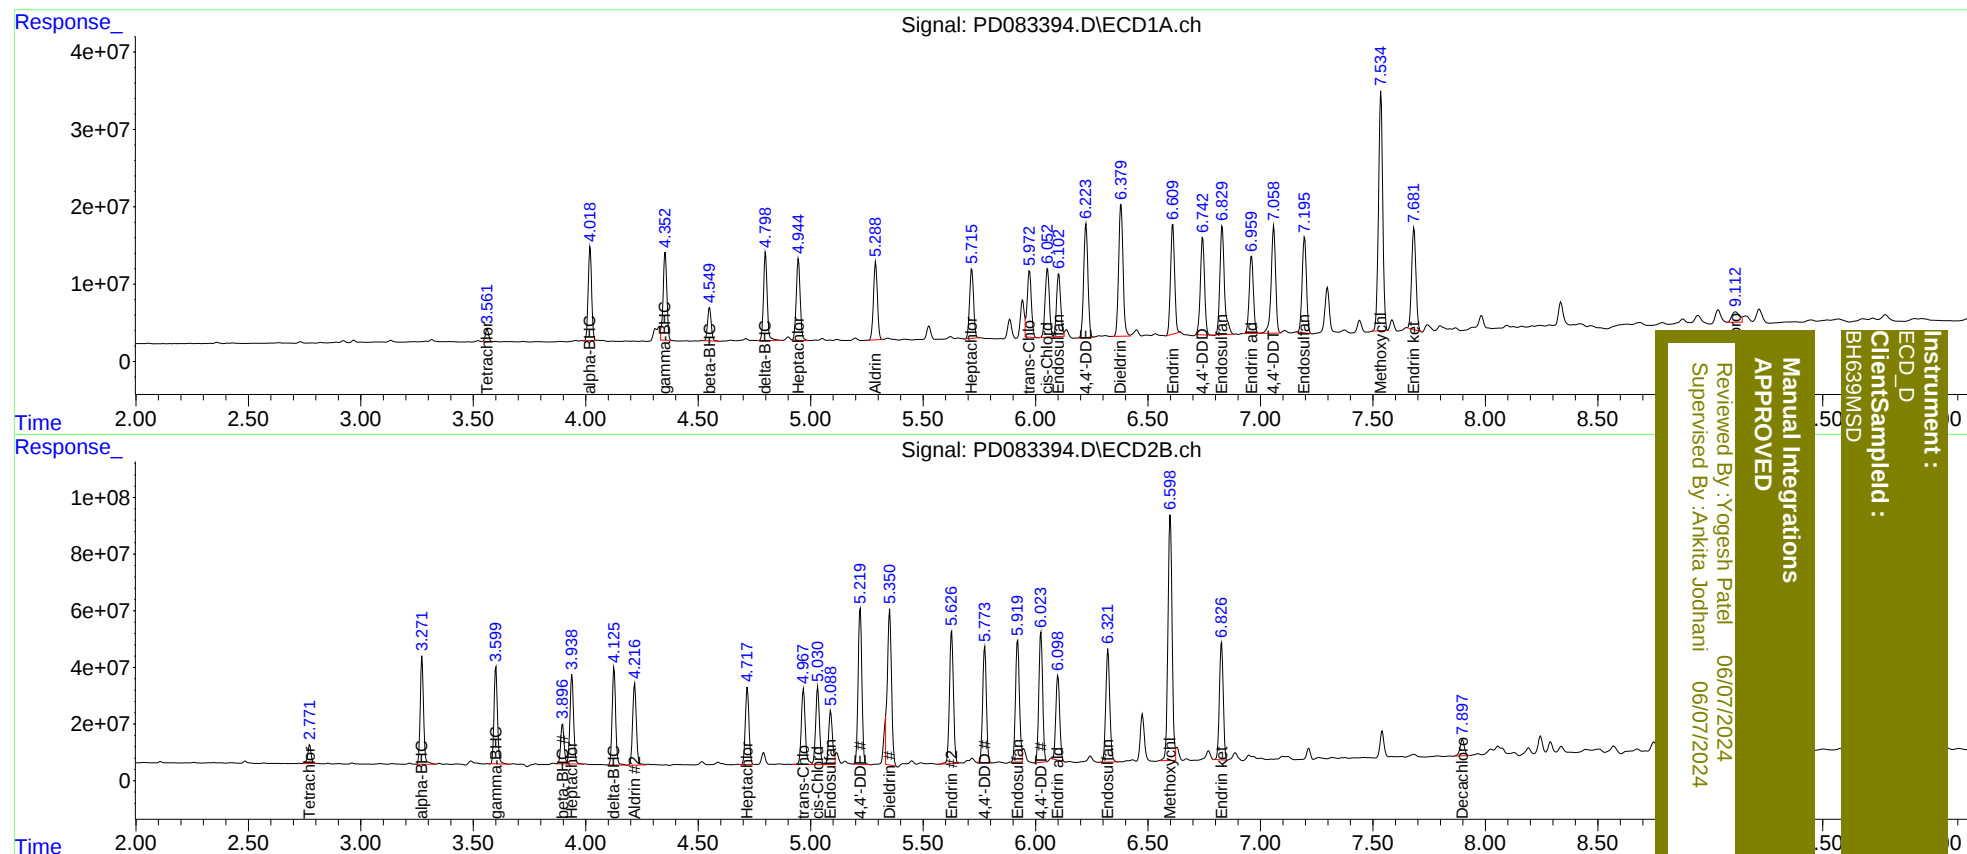

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 06/07/2024
Supervised By : Ankita Jodhani 06/07/2024

Instrument :
ECD_D
Client Sampled :
BH639MSD