

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060524\
 Data File : PD083393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2024 20:15
 Operator : AR\AJ
 Sample : P2577-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH639MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2024
 Supervised By :Ankita Jodhani 06/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 21:29:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.773	16766089	70700777	11.687m	14.927 #
27)	SA Decachlor...	9.111	7.899	29651352	78296877	14.510m	15.699
Target Compounds							
2)	A alpha-BHC	4.020	3.272	129.1E6	389.7E6	51.359	53.775
3)	MA gamma-BHC...	4.352	3.599	126.9E6	362.1E6	52.179m	53.351m
4)	MA Heptachlor	4.945	3.939	125.7E6	349.8E6	49.796m	51.903
5)	MB Aldrin	5.290	4.218	120.5E6	325.5E6	49.743	50.276
6)	B beta-BHC	4.551	3.897	47687620	145.0E6	44.490	49.269
7)	B delta-BHC	4.800	4.126	129.1E6	369.0E6	48.836	52.368
8)	B Heptachlo...	5.717	4.719	109.7E6	304.8E6	49.946	51.178
9)	A Endosulfan I	6.104	5.090	97995904	219.0E6	46.129	40.180
10)	B trans-Chl...	5.972	4.969	110.6E6	323.7E6	50.962m	55.345
11)	B cis-Chlor...	6.053	5.032	113.1E6	321.3E6	50.984	53.904
12)	B 4,4'-DDE	6.225	5.220	191.2E6	640.7E6	86.076	112.146 #
13)	MA Dieldrin	6.380	5.351	232.7E6	722.2E6	102.923	119.071m
14)	MA Endrin	6.610	5.627	181.9E6	575.9E6	97.733	107.413
15)	B Endosulfa...	6.830	5.919	199.5E6	540.1E6	102.557	107.822m
16)	A 4,4'-DDD	6.743	5.774	165.1E6	465.6E6	102.760	100.493
17)	MA 4,4'-DDT	7.058	6.025	191.3E6	541.5E6	117.135	115.948
18)	B Endrin al...	6.961	6.101	130.2E6	359.0E6	90.205	93.640
19)	B Endosulfa...	7.196	6.322	167.0E6	494.4E6	91.416	101.629
20)	A Methoxychlor	7.536	6.600	409.3E6	1153.4E6	445.226	471.828
21)	B Endrin ke...	7.682	6.828	177.9E6	491.0E6	92.642	92.036

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060524\
Data File : PD083393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2024 20:15
Operator : AR\AJ
Sample : P2577-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 21:29:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

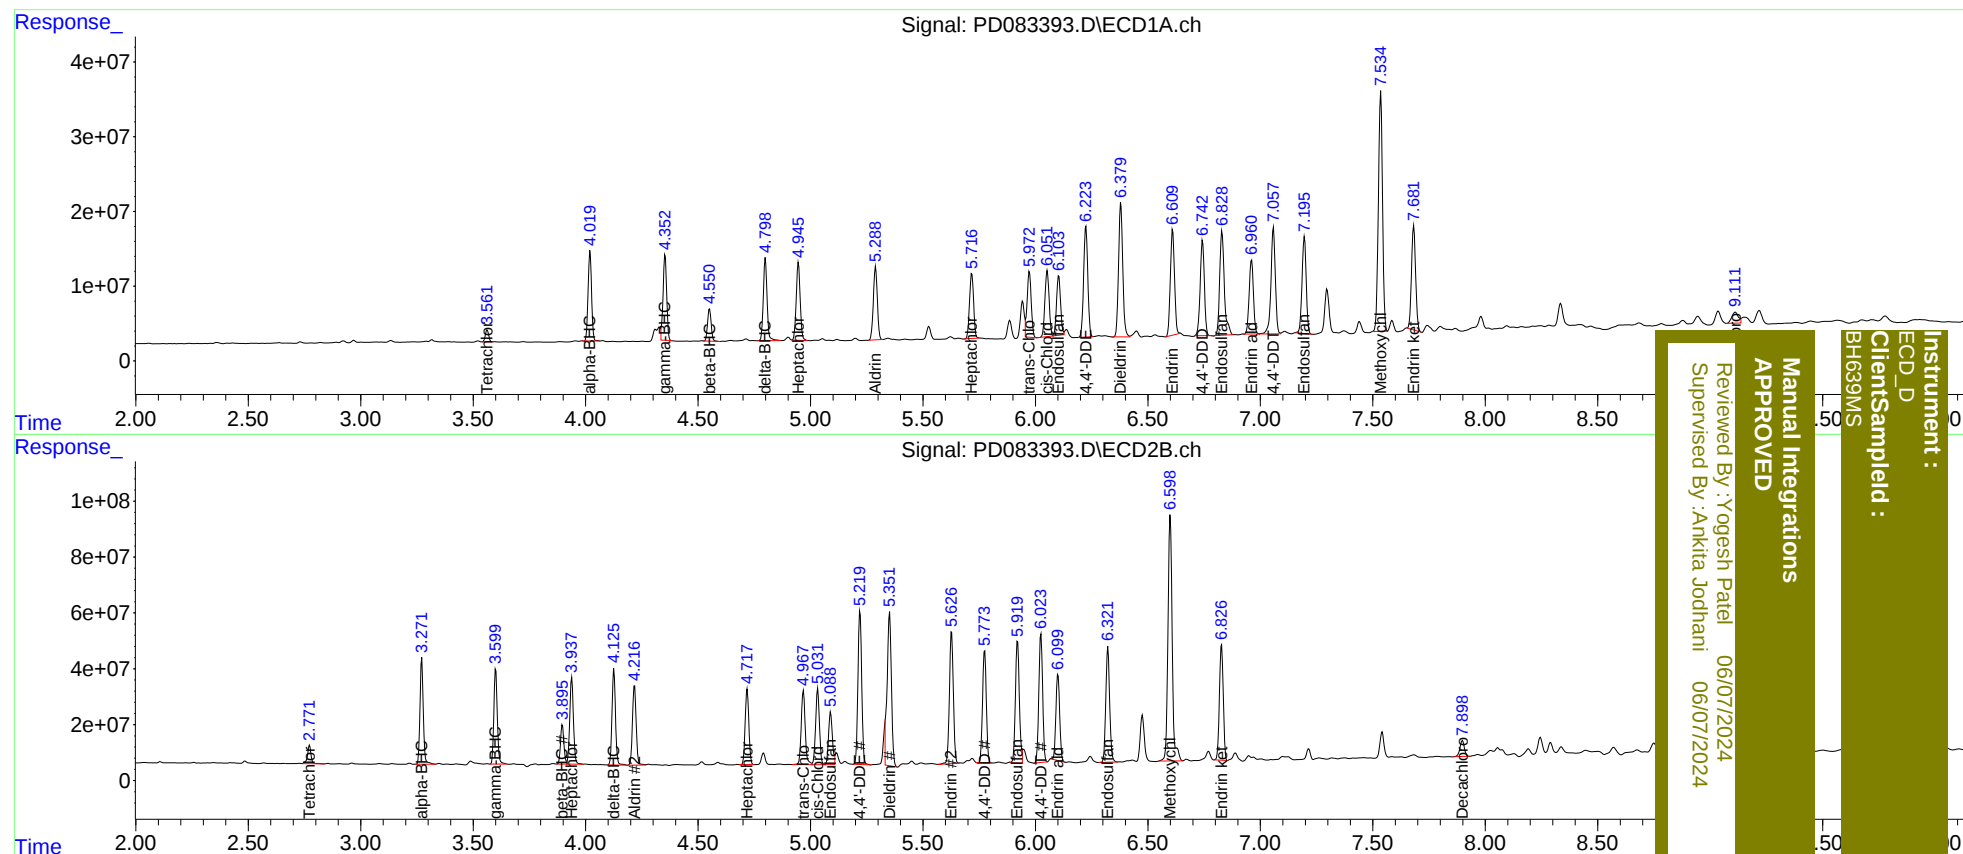

Instrument :
ECD_D
ClientSampled :
BH639MS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 06/07/2024
Supervised By : Ankita Jodhani 06/07/2024