

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 12:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:27:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 06:00:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.168	20778903	192.1E6	19.140	19.675
28)	SA Decachlor...	8.191	9.359	23929436	125.2E6	21.517	20.357
Target Compounds							
6)	B beta-BHC	4.407	0.000	2046006	0	2.844	N.D. #
23)	Chlordane-1	4.336f	0.000	2028575	0	47.388	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 12:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:27:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 06:00:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

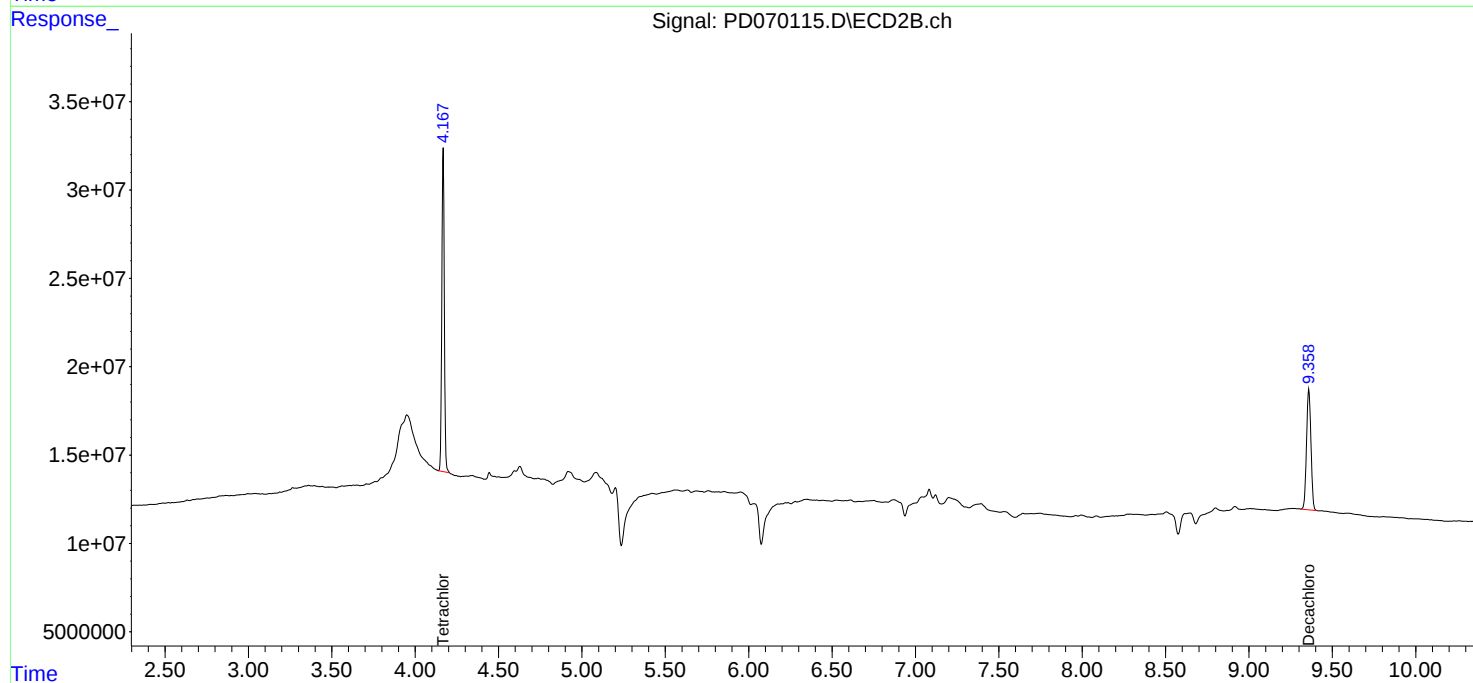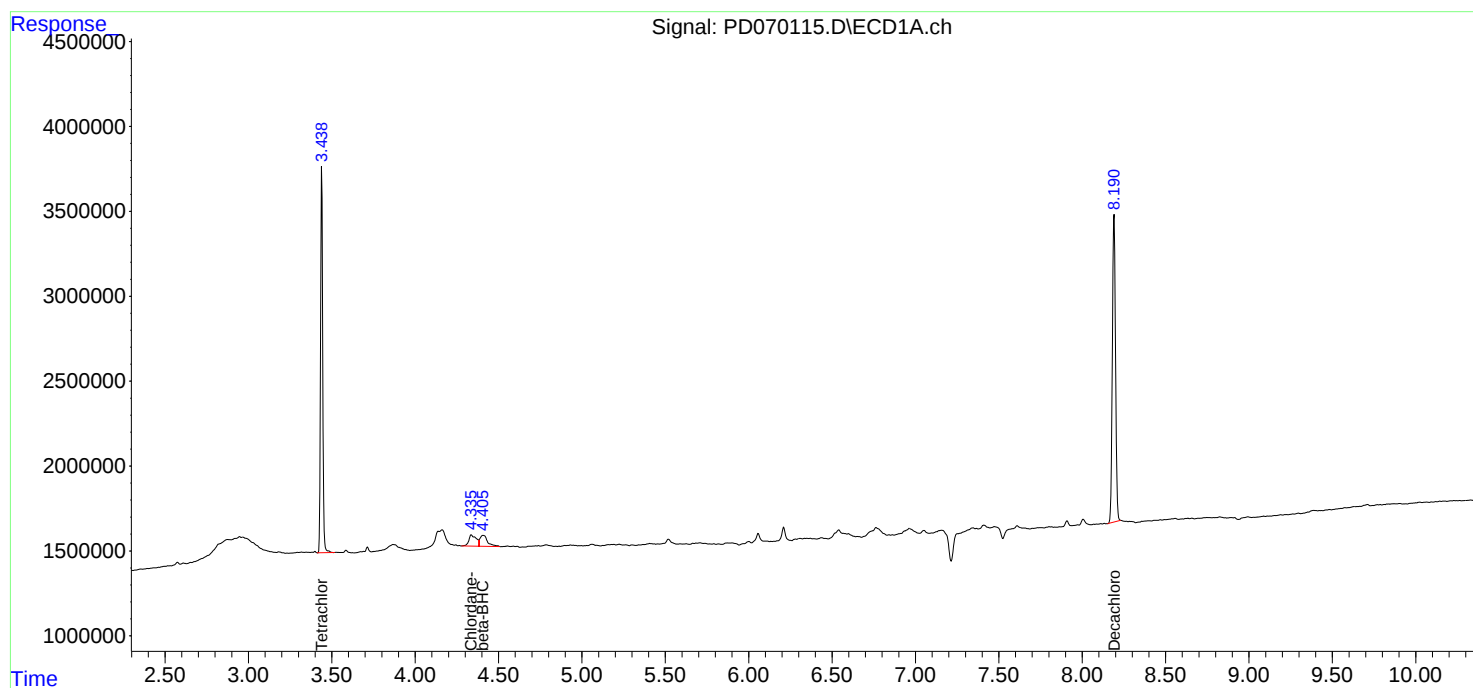


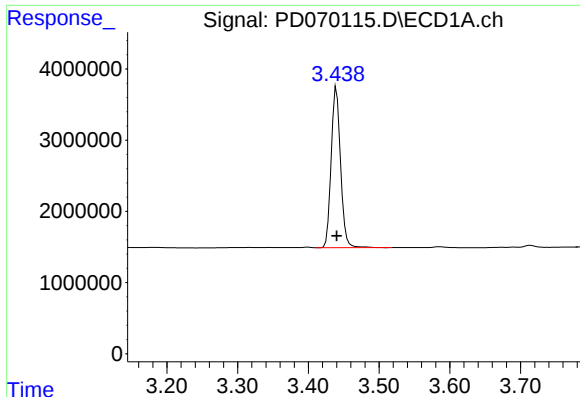

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 20778903
Conc: 19.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

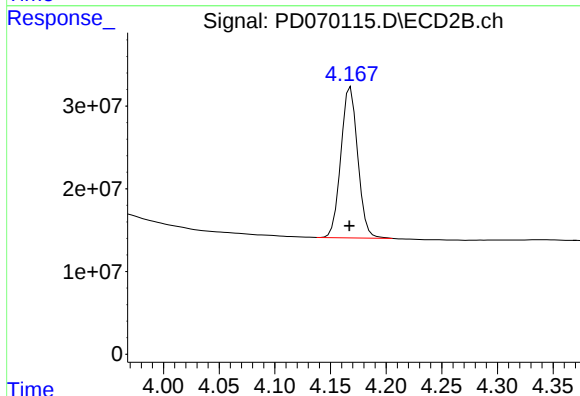


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.001 min
Response: 192055714
Conc: 19.68 ng/ml

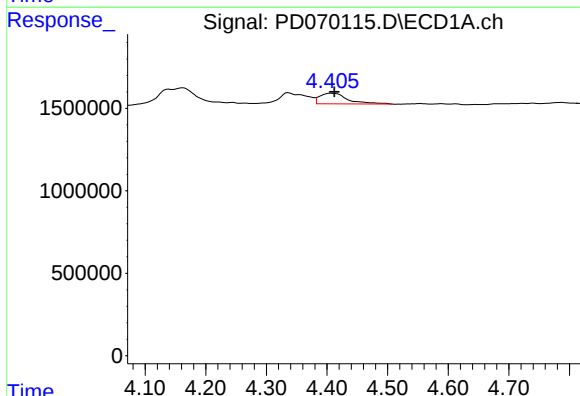


#6 beta-BHC

R.T.: 4.407 min
Delta R.T.: -0.006 min
Response: 2046006
Conc: 2.84 ng/ml

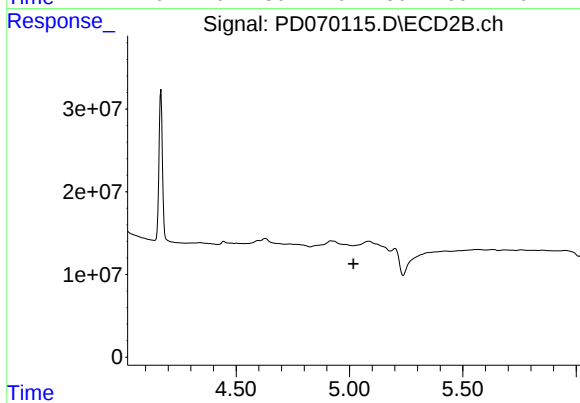

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

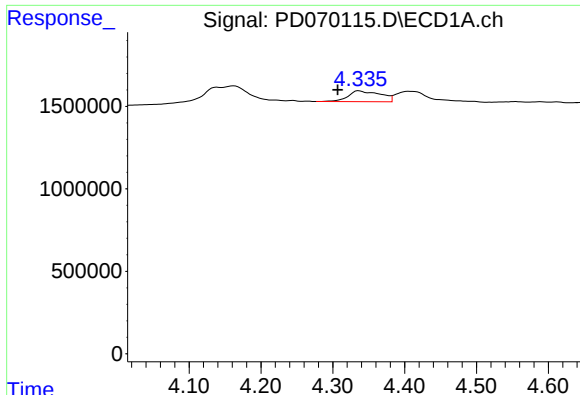

#23 Chlordane-1


R.T.: 4.336 min
Delta R.T.: 0.029 min
Response: 2028575
Conc: 47.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

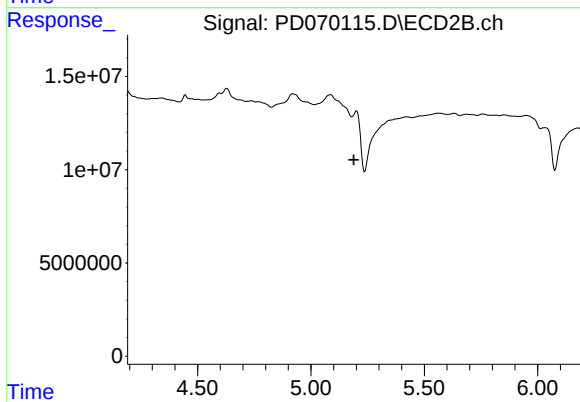


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.189 min
Response: 0
Conc: N.D.

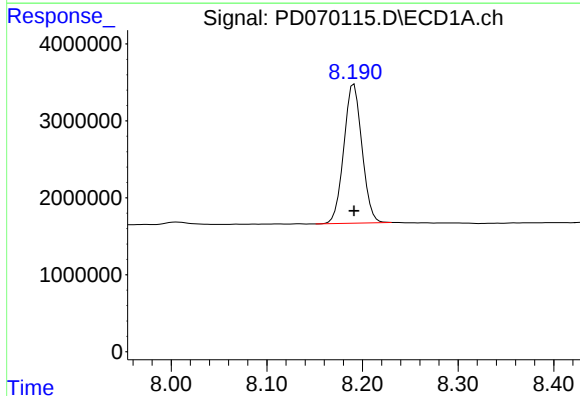

#28 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 23929436
Conc: 21.52 ng/ml

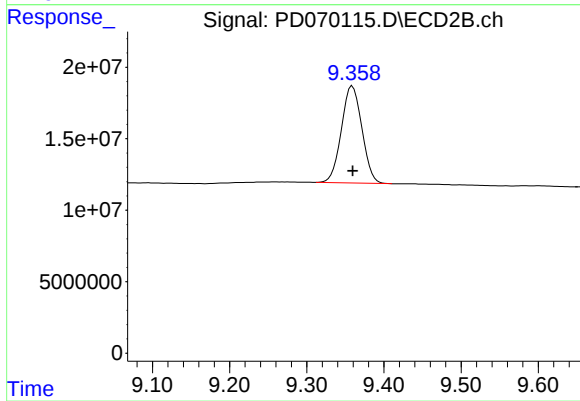

#28 Decachlorobiphenyl

R.T.: 9.359 min
Delta R.T.: 0.000 min
Response: 125204077
Conc: 20.36 ng/ml