

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 22:26
 Operator : AR\AJ
 Sample : PB145307BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:31:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 06:00:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	20682406	190.5E6	19.051	19.516
28)	SA Decachlor...	8.190	9.360	20958811	118.7E6	18.846	19.297
Target Compounds							
2)	A alpha-BHC	3.870	0.000	2135620	0	1.306	N.D. #
9)	A Endosulfan I	0.000	6.450	0	33751275	N.D.	3.187 #
10)	B gamma-Chl...	0.000	6.326	0	160.4E6	N.D.	13.954 #
25)	Chlordane-3	0.000	6.326	0	160.4E6	N.D.	101.233 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 22:26
Operator : AR\AJ
Sample : PB145307BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:31:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 06:00:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

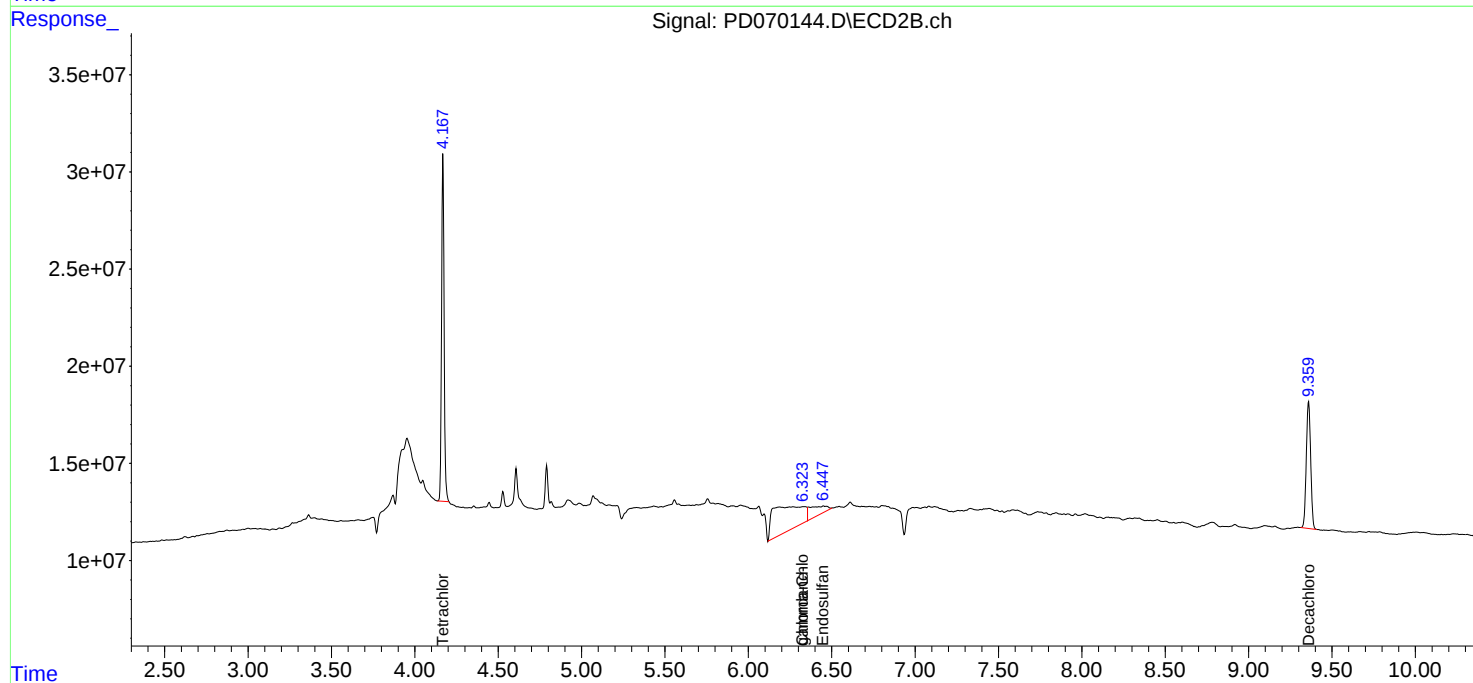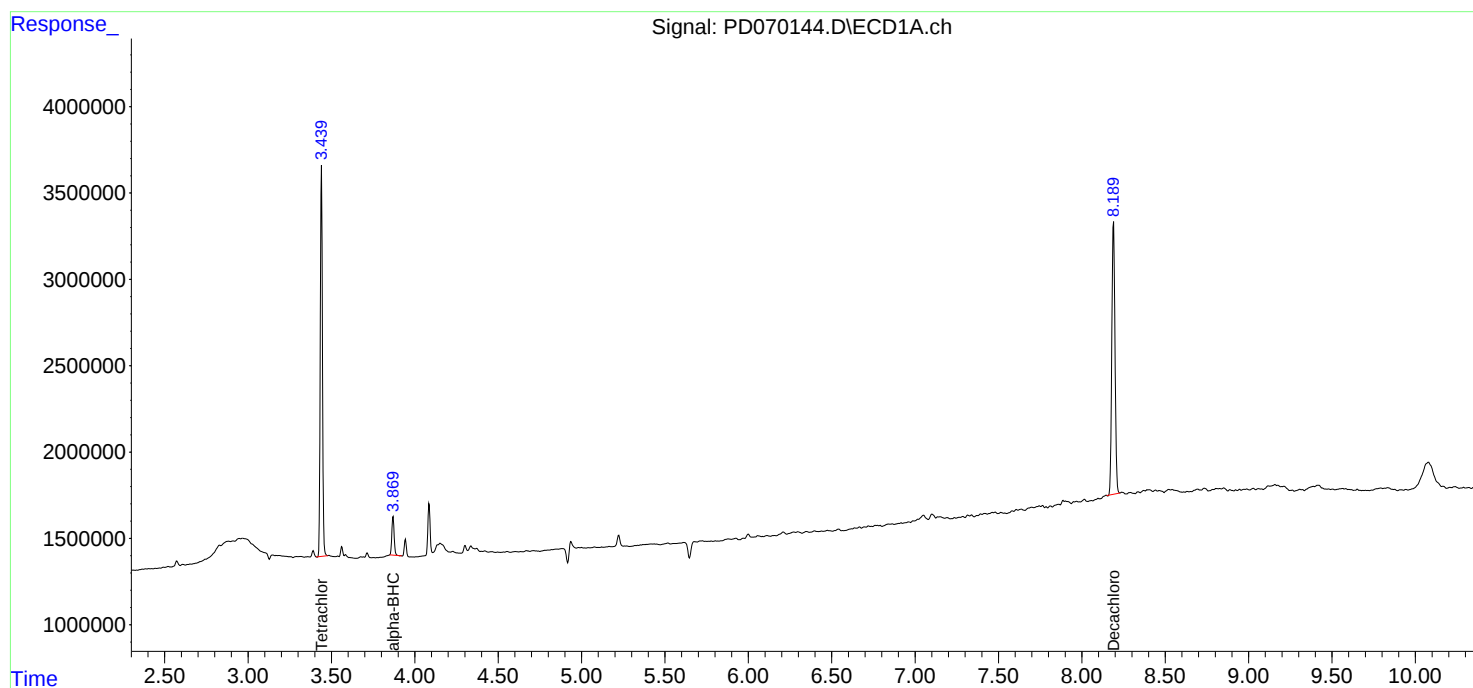


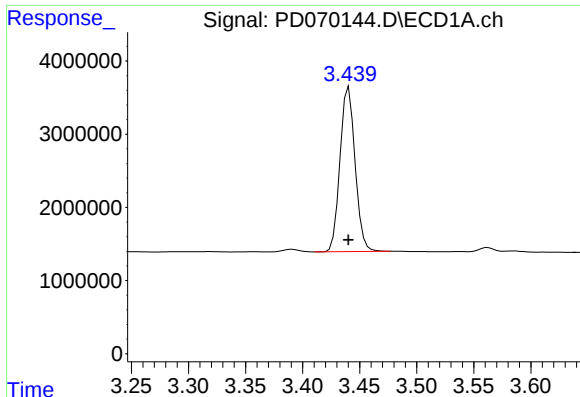

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 20682406
Conc: 19.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

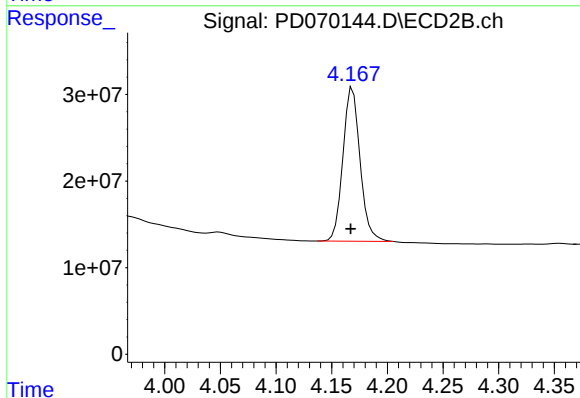


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 190507458
Conc: 19.52 ng/ml

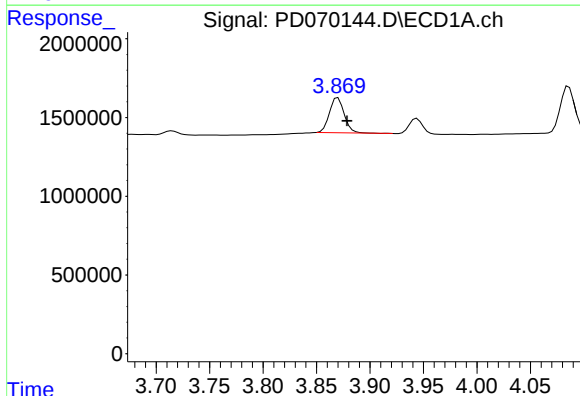


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: -0.009 min
Response: 2135620
Conc: 1.31 ng/ml

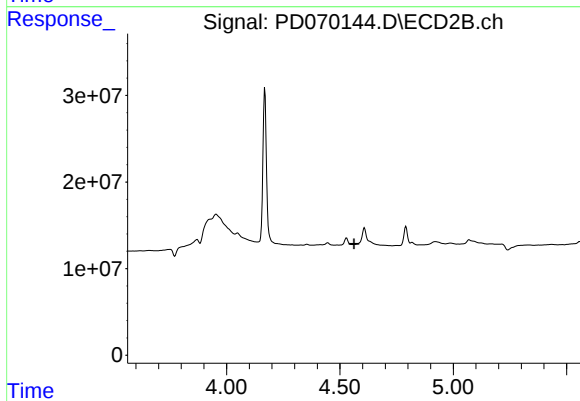

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

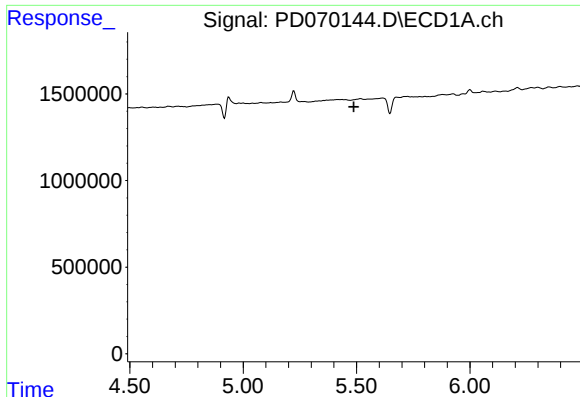

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

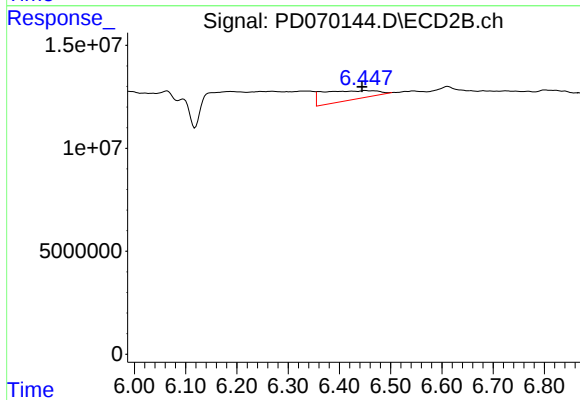


#9 Endosulfan I

R.T.: 6.450 min
Delta R.T.: 0.006 min
Response: 33751275
Conc: 3.19 ng/ml

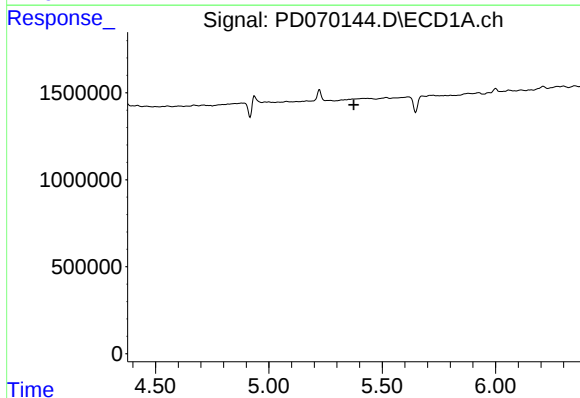


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

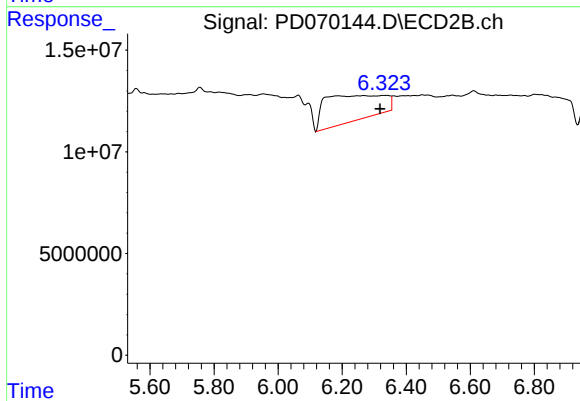

#10 gamma-Chlordane


R.T.: 6.326 min
Delta R.T.: 0.008 min
Response: 160380428
Conc: 13.95 ng/ml

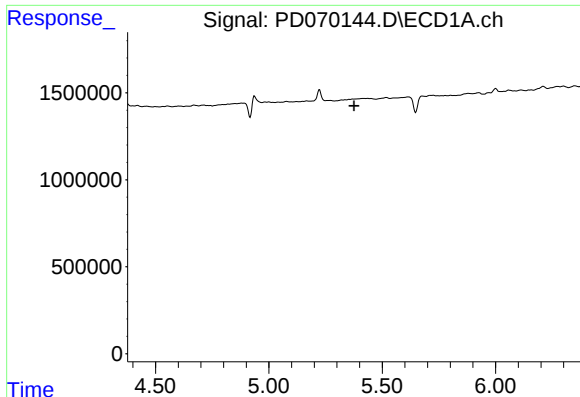

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

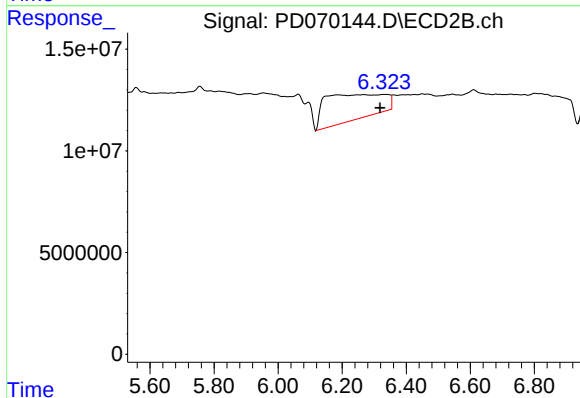


#25 Chlordane-3

R.T.: 6.326 min
Delta R.T.: 0.008 min
Response: 160380428
Conc: 101.23 ng/ml

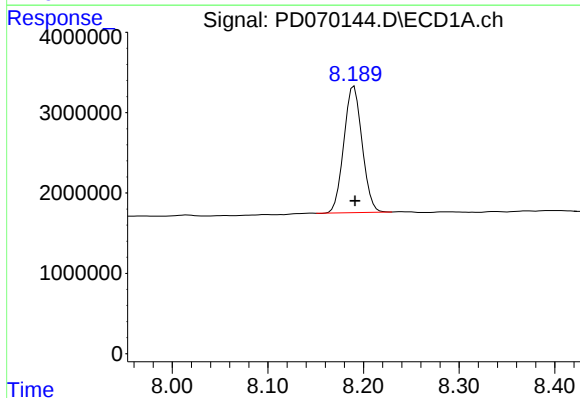

#28 Decachlorobiphenyl

R.T.: 8.190 min
Delta R.T.: -0.001 min
Response: 20958811
Conc: 18.85 ng/ml

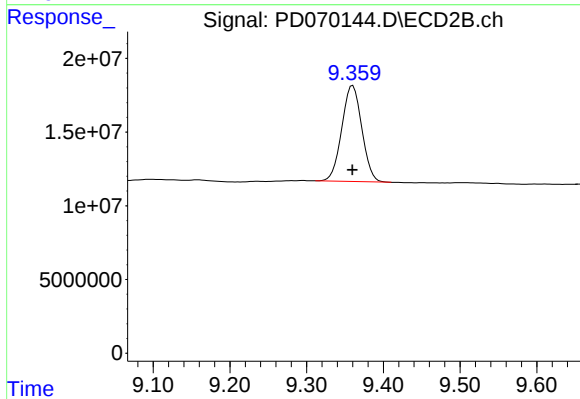

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 118685034
Conc: 19.30 ng/ml