

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 00:05
 Operator : AR\AJ
 Sample : N3205-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:33:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 06:00:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.169	18509449	167.0E6	17.049	17.109
28)	SA Decachlor...	8.191	9.360	13584308	80071644	12.215	13.019
Target Compounds							
3)	MA gamma-BHC...	4.167	0.000	1039904	0	0.675	N.D. #
9)	A Endosulfan I	5.515f	0.000	1410979	0	1.078	N.D. #
10)	B gamma-Chl...	0.000	6.322	0	8869949	N.D.	0.772 #
12)	B 4,4'-DDE	5.599	6.543	1039224	16527274	0.831	1.576 #
13)	MA Dieldrin	5.736	0.000	1612752	0	1.197	N.D. #
16)	A 4,4'-DDD	0.000	7.041	0	22527265	N.D.	2.678 #
17)	MA 4,4'-DDT	6.354	0.000	1232714	0	1.162	N.D. #
23)	Chlordane-1	4.334f	0.000	1149116	0	26.844	N.D. #
25)	Chlordane-3	0.000	6.322	0	8869949	N.D.	5.599 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 00:05
Operator : AR\AJ
Sample : N3205-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:33:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 06:00:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

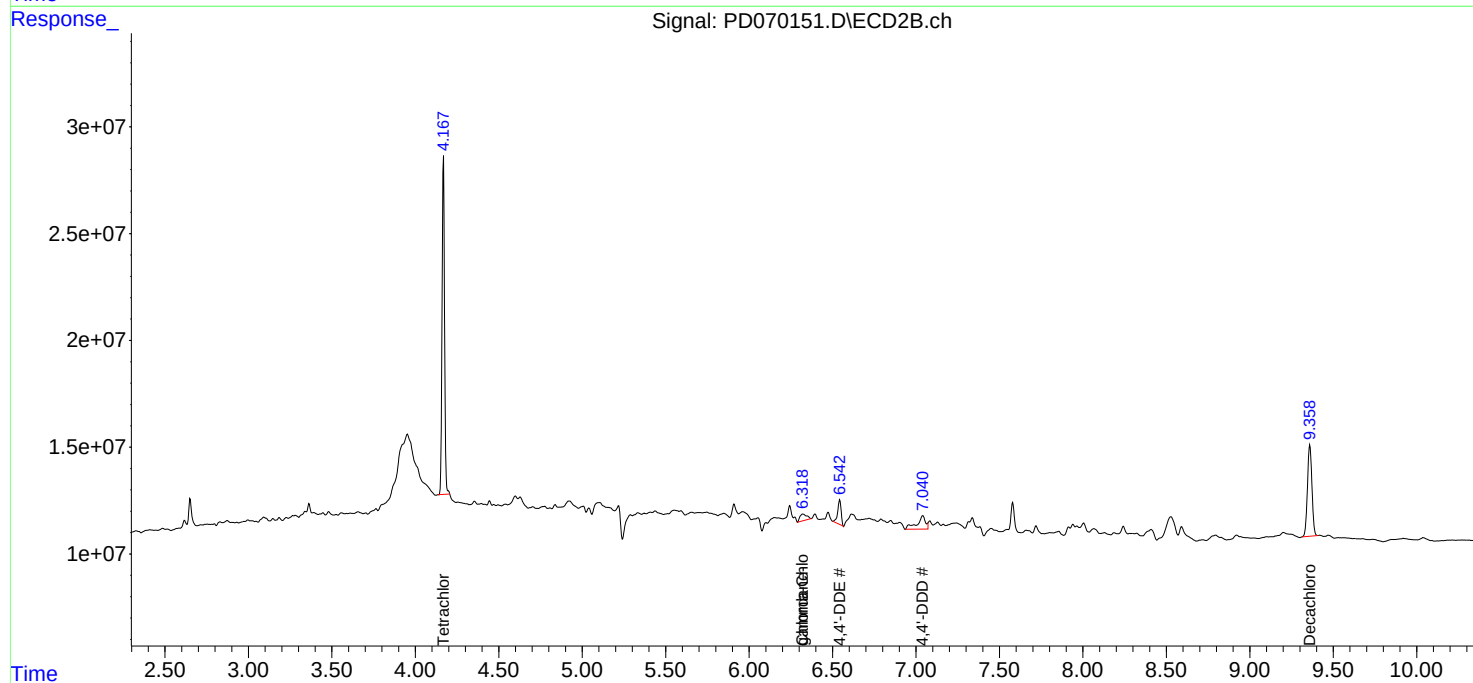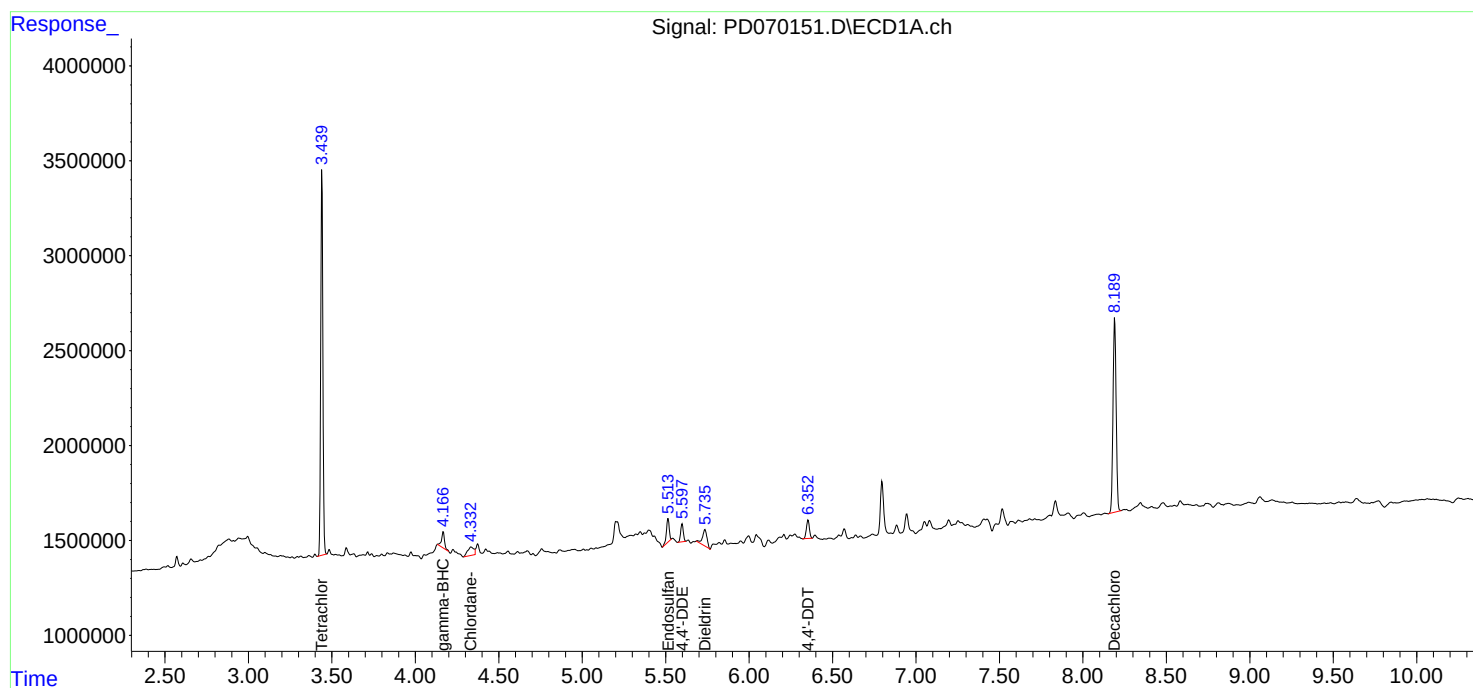


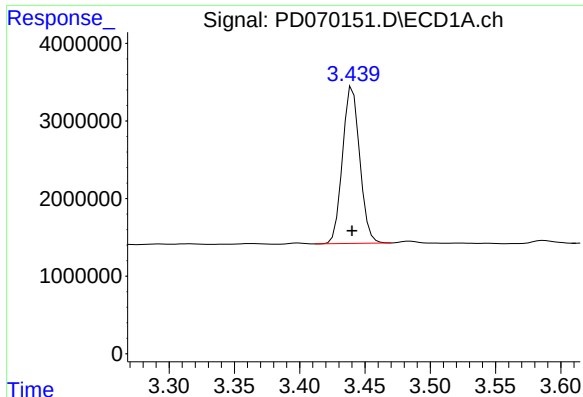

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 18509449
Conc: 17.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

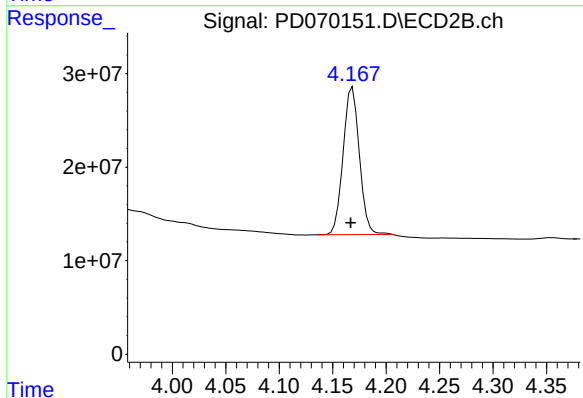


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 167010963
Conc: 17.11 ng/ml

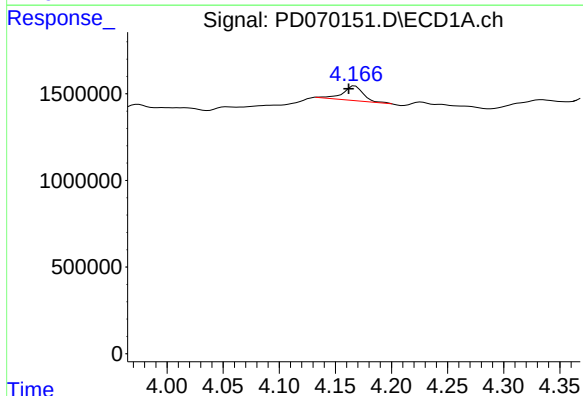


#3 gamma-BHC (Lindane)

R.T.: 4.167 min
Delta R.T.: 0.006 min
Response: 1039904
Conc: 0.68 ng/ml

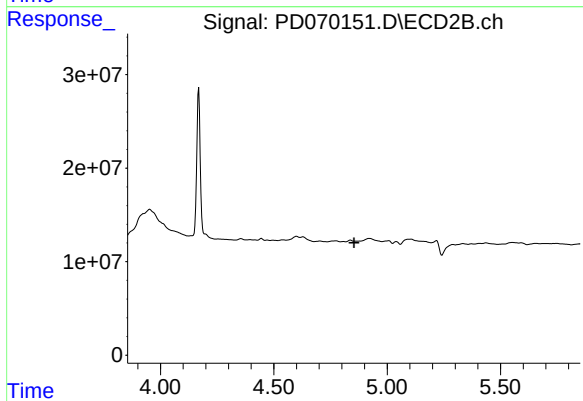

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.854 min
Response: 0
Conc: N.D.

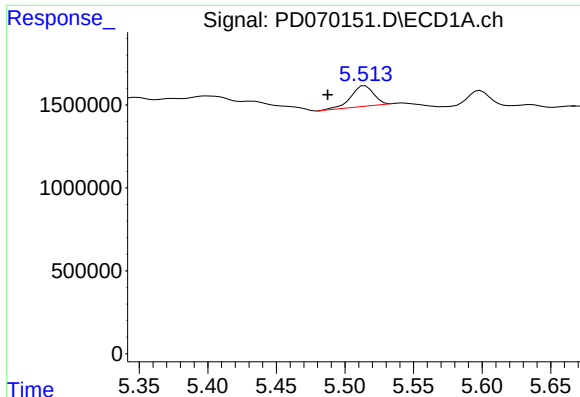

#9 Endosulfan I


R.T.: 5.515 min
Delta R.T.: 0.027 min
Response: 1410979
Conc: 1.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

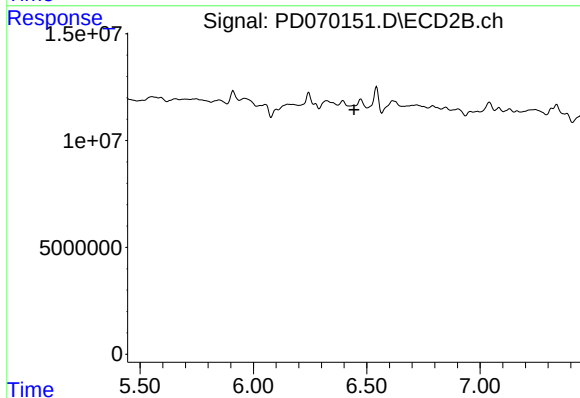


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.444 min
Response: 0
Conc: N.D.

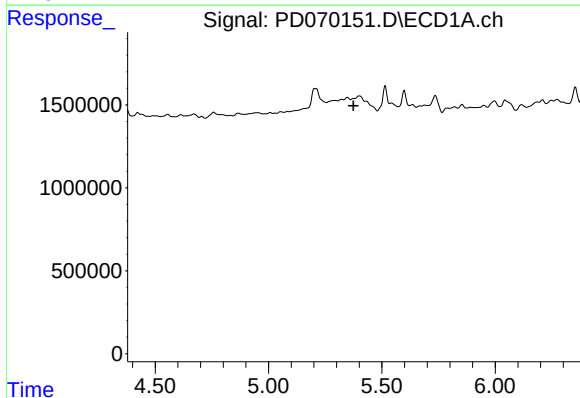


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.375 min
Response: 0
Conc: N.D.

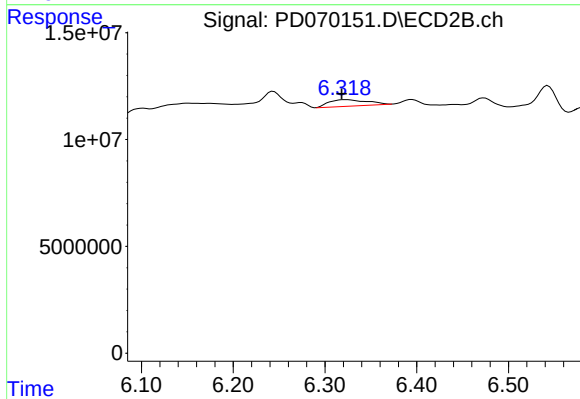

#10 gamma-Chlordane


R.T.: 6.322 min
Delta R.T.: 0.004 min
Response: 8869949
Conc: 0.77 ng/ml

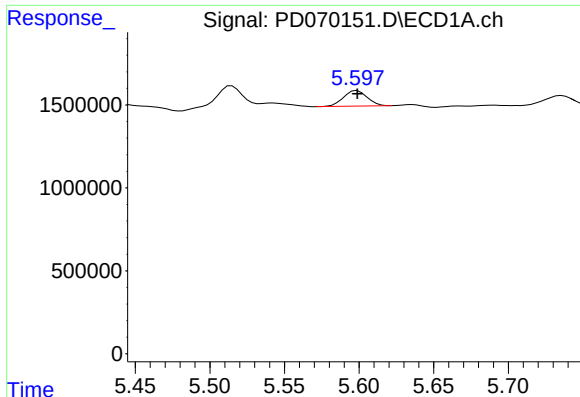

#12 4,4'-DDE


R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 1039224
Conc: 0.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

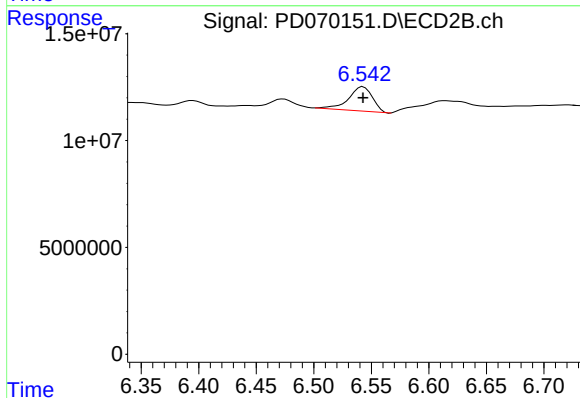


#12 4,4'-DDE

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 16527274
Conc: 1.58 ng/ml

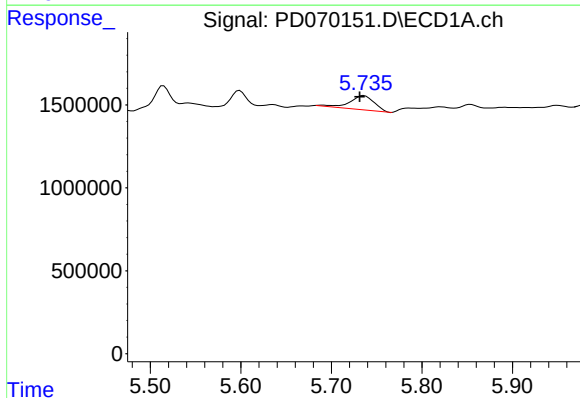


#13 Dieldrin

R.T.: 5.736 min
Delta R.T.: 0.004 min
Response: 1612752
Conc: 1.20 ng/ml

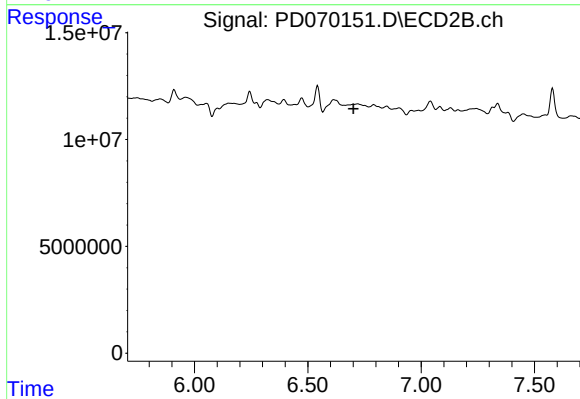

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.702 min
Response: 0
Conc: N.D.

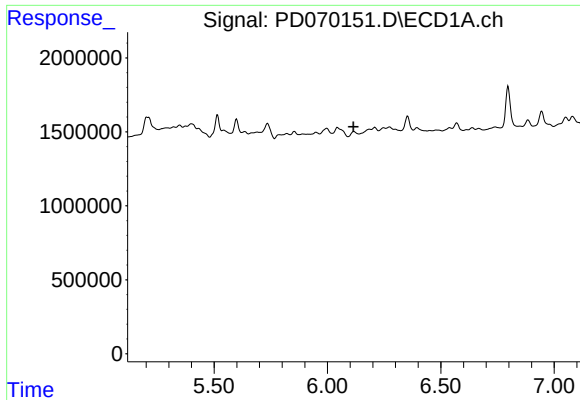

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

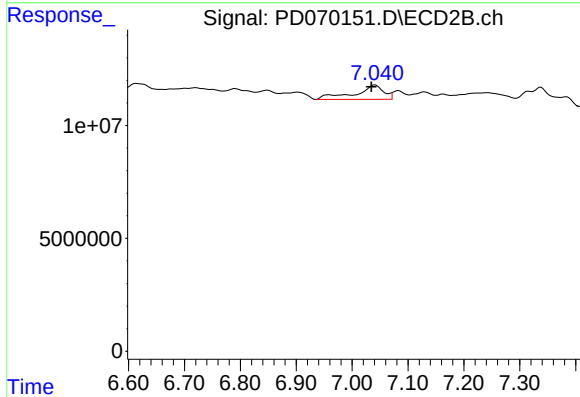


#16 4,4'-DDD

R.T.: 7.041 min
Delta R.T.: 0.006 min
Response: 22527265
Conc: 2.68 ng/ml

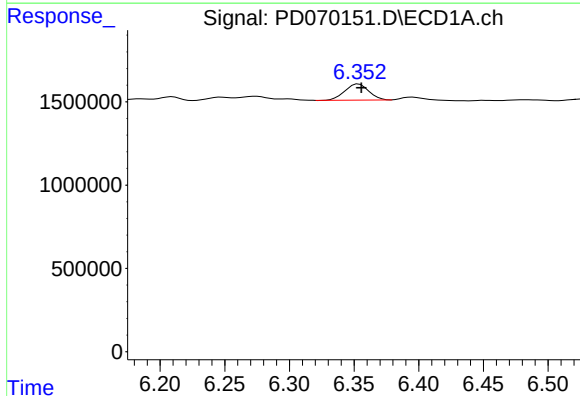


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.002 min
Response: 1232714
Conc: 1.16 ng/ml

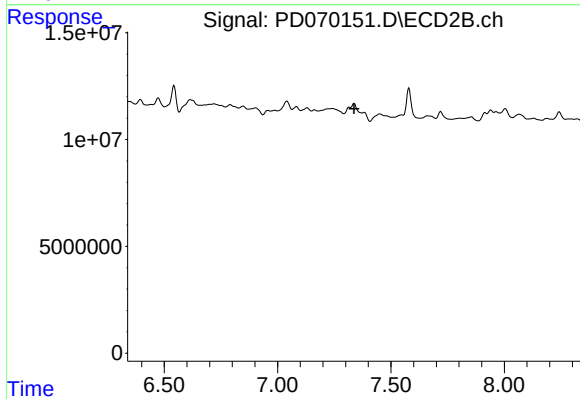

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

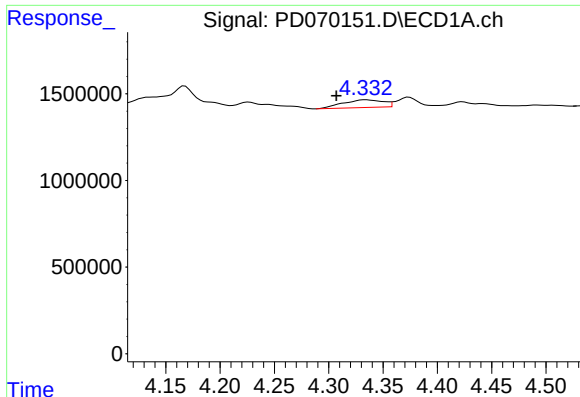

#23 Chlordane-1


R.T.: 4.334 min
Delta R.T.: 0.027 min
Response: 1149116
Conc: 26.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

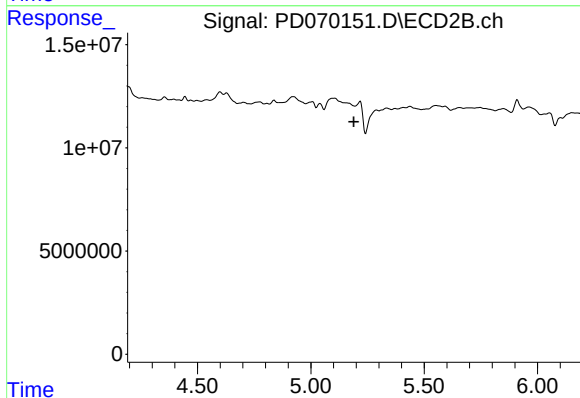


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.189 min
Response: 0
Conc: N.D.

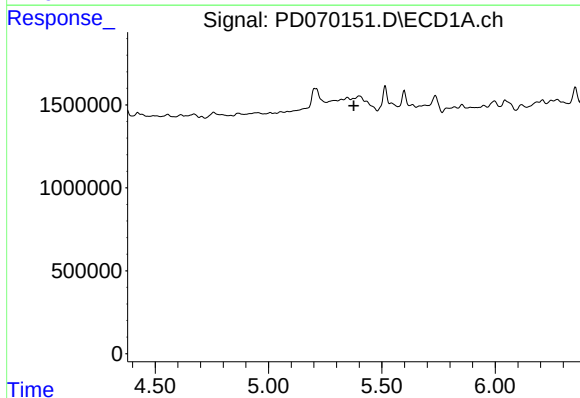


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.376 min
Response: 0
Conc: N.D.

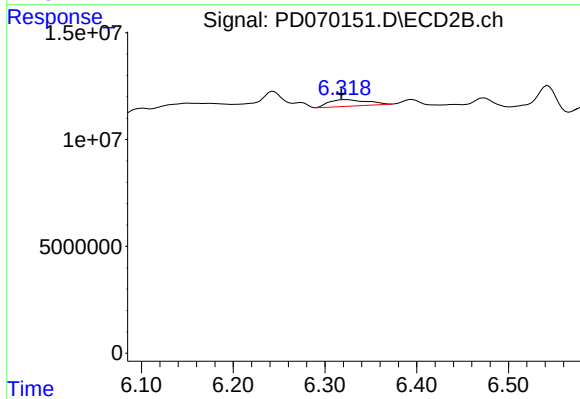

#25 Chlordane-3


R.T.: 6.322 min
Delta R.T.: 0.004 min
Response: 8869949
Conc: 5.60 ng/ml

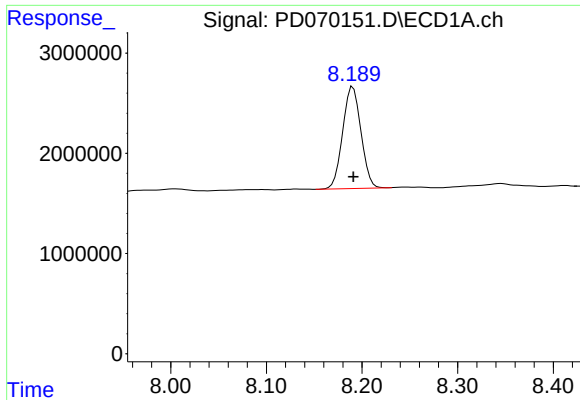

#28 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 13584308
Conc: 12.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

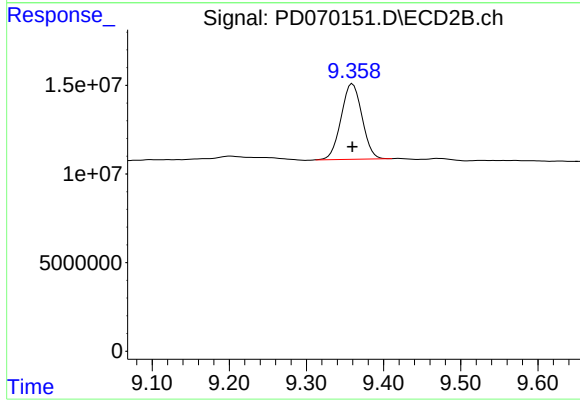

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 80071644
Conc: 13.02 ng/ml