

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 14:41
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 05:45:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 05:45:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.168	125.1E6	896.0E6	99.295	96.257
28)	SA Decachlor...	8.191	9.360	104.0E6	568.7E6	97.189	100.638
Target Compounds							
23)	Chlordane-1	4.307	5.189	38226435	369.2E6	979.263	954.817
24)	Chlordane-2	4.809	5.663	43374318	401.9E6	965.232	938.521
25)	Chlordane-3	5.376	6.318	129.8E6	1384.6E6	1009.157	971.640
26)	Chlordane-4	5.433	6.395	107.5E6	1608.9E6	996.789	971.372
27)	Chlordane-5	6.271	7.206	42871211	282.0E6	976.258	955.498



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 14:41
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 05:45:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 05:45:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

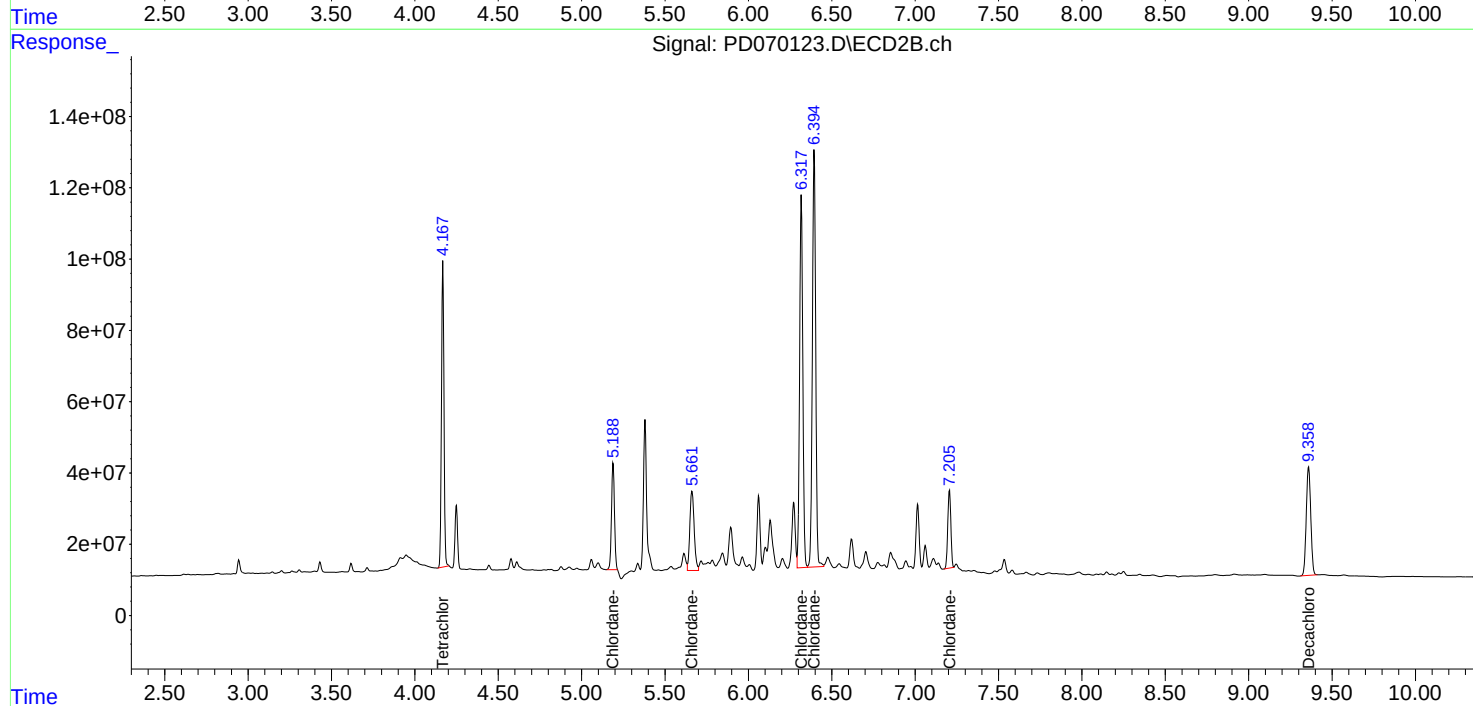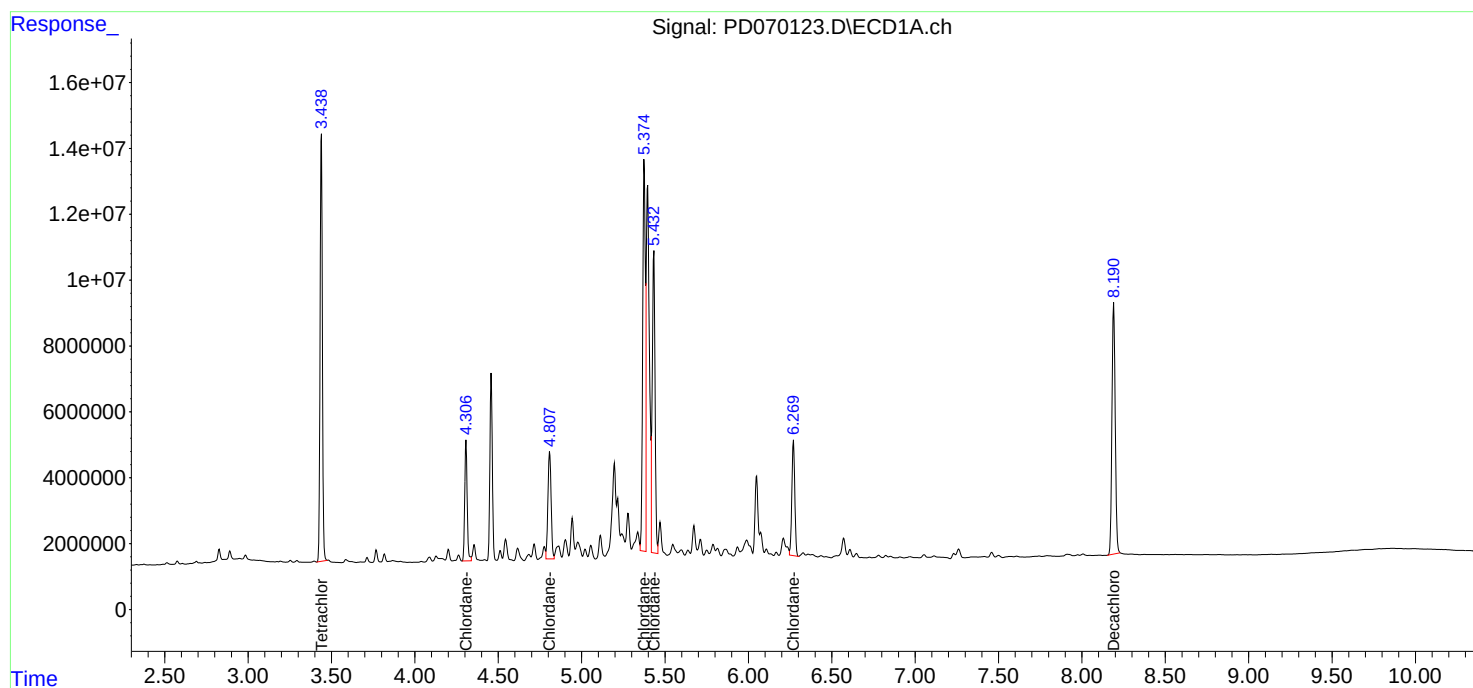


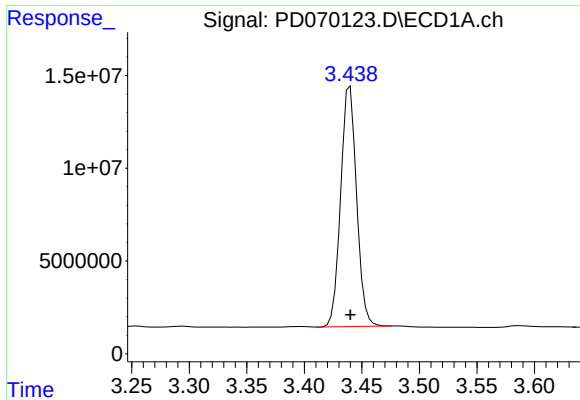

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 125053863
Conc: 99.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

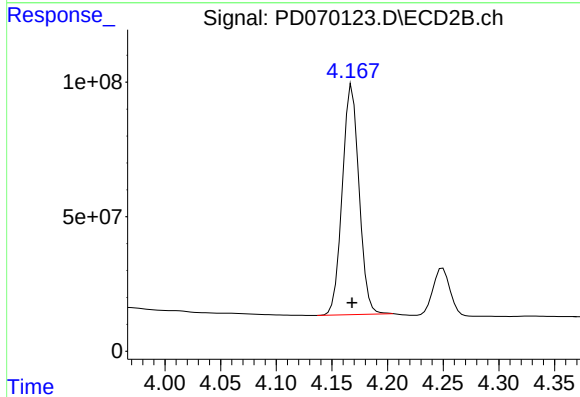


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 895987422
Conc: 96.26 ng/ml

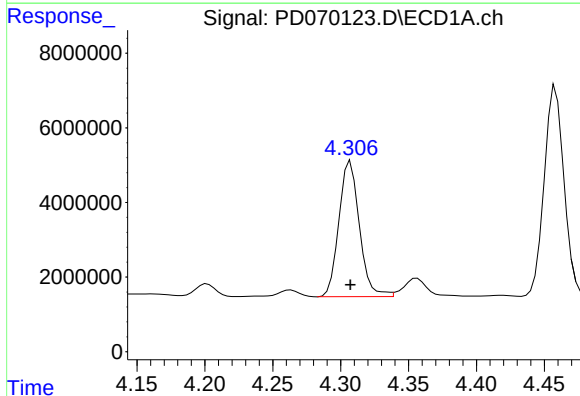


#23 Chlordane-1

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 38226435
Conc: 979.26 ng/ml

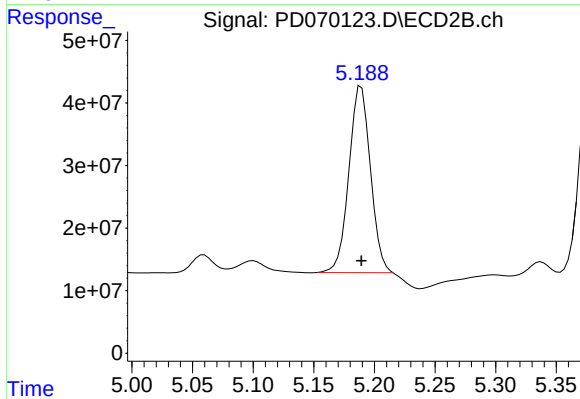

#23 Chlordane-1


R.T.: 5.189 min
Delta R.T.: 0.000 min
Response: 369178041
Conc: 954.82 ng/ml

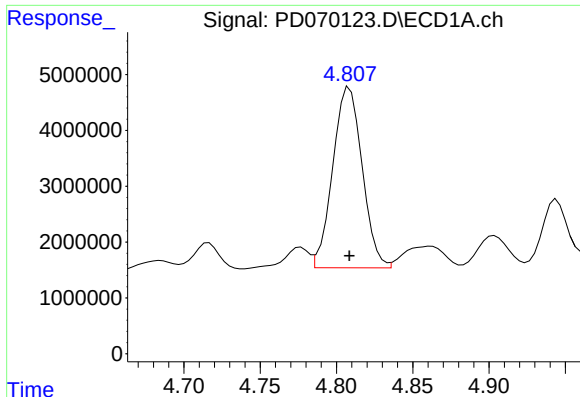

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 43374318
Conc: 965.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

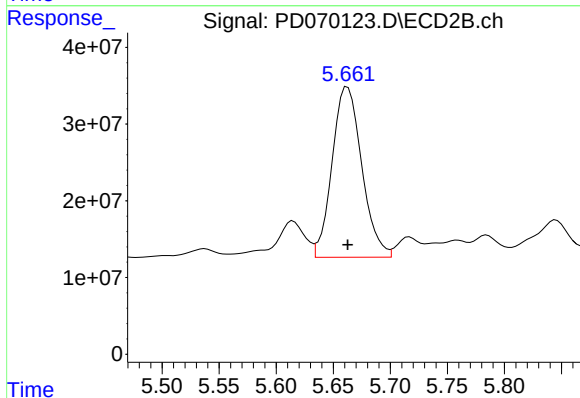


#24 Chlordane-2

R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 401949627
Conc: 938.52 ng/ml

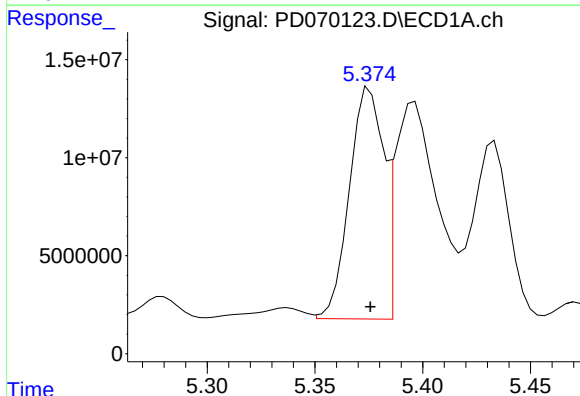


#25 Chlordane-3

R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 129778927
Conc: 1009.16 ng/ml

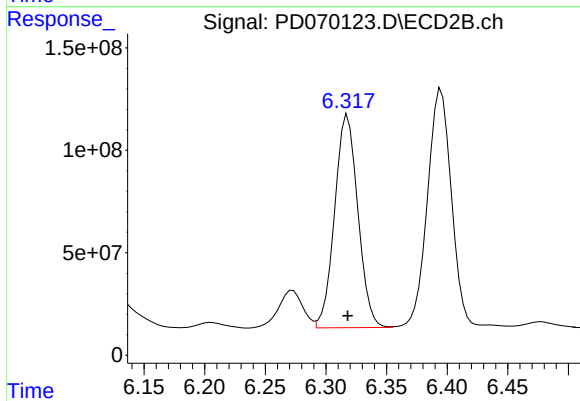

#25 Chlordane-3


R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 1384615988
Conc: 971.64 ng/ml

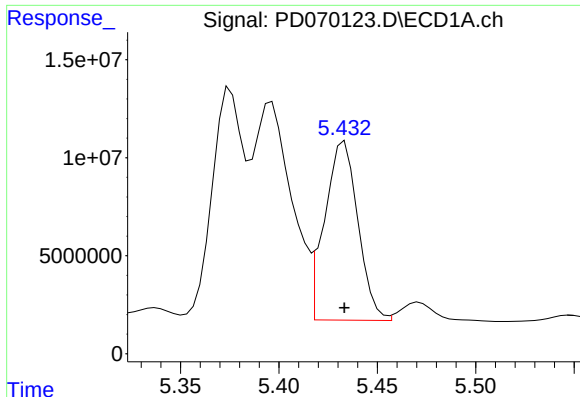

#26 Chlordane-4


R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 107521901
Conc: 996.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

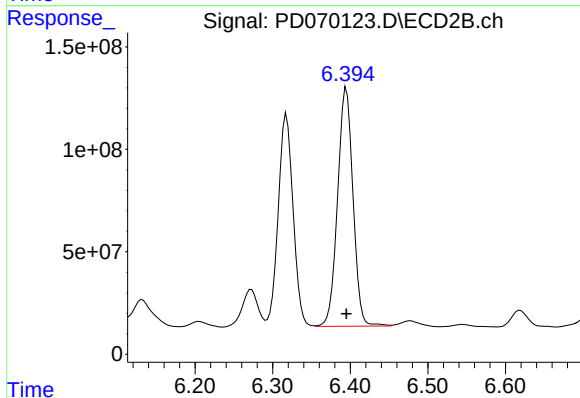


#26 Chlordane-4

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 1608899223
Conc: 971.37 ng/ml

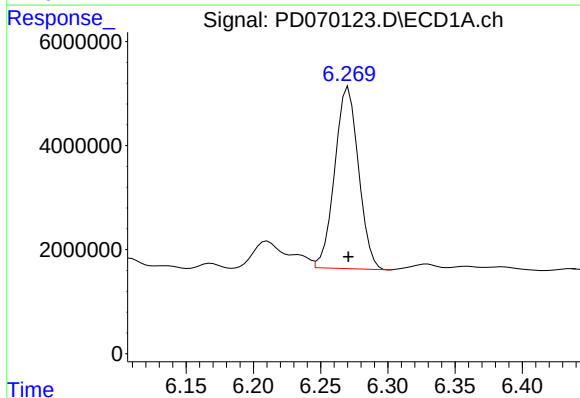


#27 Chlordane-5

R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 42871211
Conc: 976.26 ng/ml

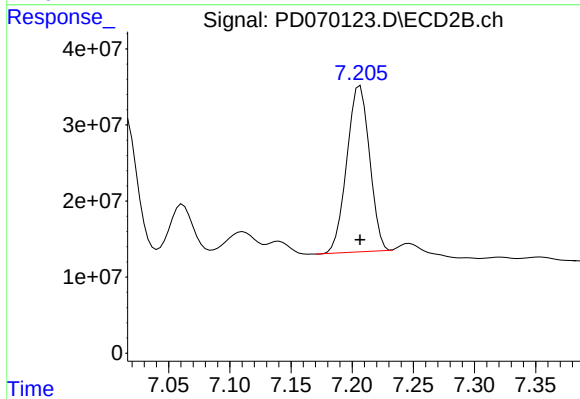

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 281988180
Conc: 955.50 ng/ml

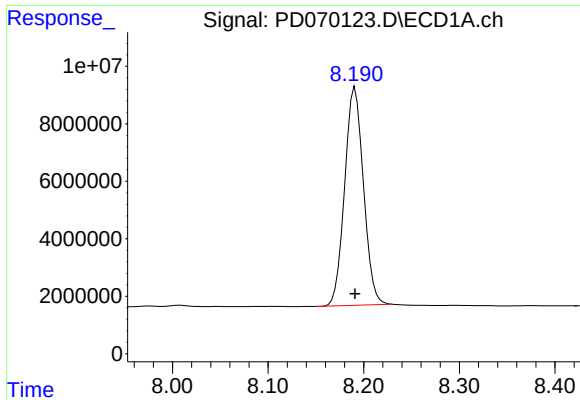

#28 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 104046520
Conc: 97.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

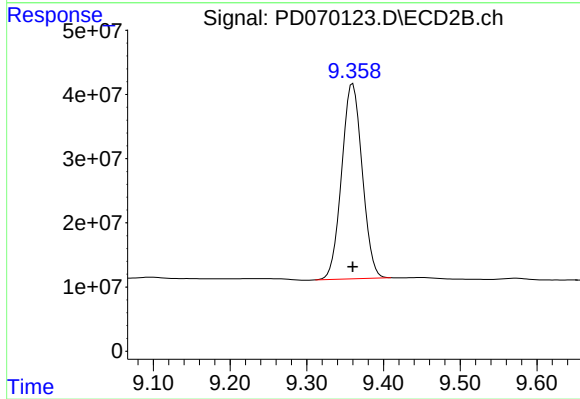

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 568684058
Conc: 100.64 ng/ml