

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 14:55
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 05:47:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 05:47:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.168	98809390	726.6E6	77.269	77.010
28)	SA Decachlor...	8.191	9.360	82469956	453.0E6	76.344	78.363
Target Compounds							
23)	Chlordane-1	4.307	5.189	30233695	298.4E6	766.164	764.401
24)	Chlordane-2	4.808	5.662	35007796	329.2E6	769.118	762.298
25)	Chlordane-3	5.375	6.318	98449697	1107.8E6	760.290	768.030
26)	Chlordane-4	5.433	6.395	82988170	1281.7E6	762.788	765.712
27)	Chlordane-5	6.271	7.207	34439078	229.5E6	772.486	768.283



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 14:55
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 05:47:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 05:47:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

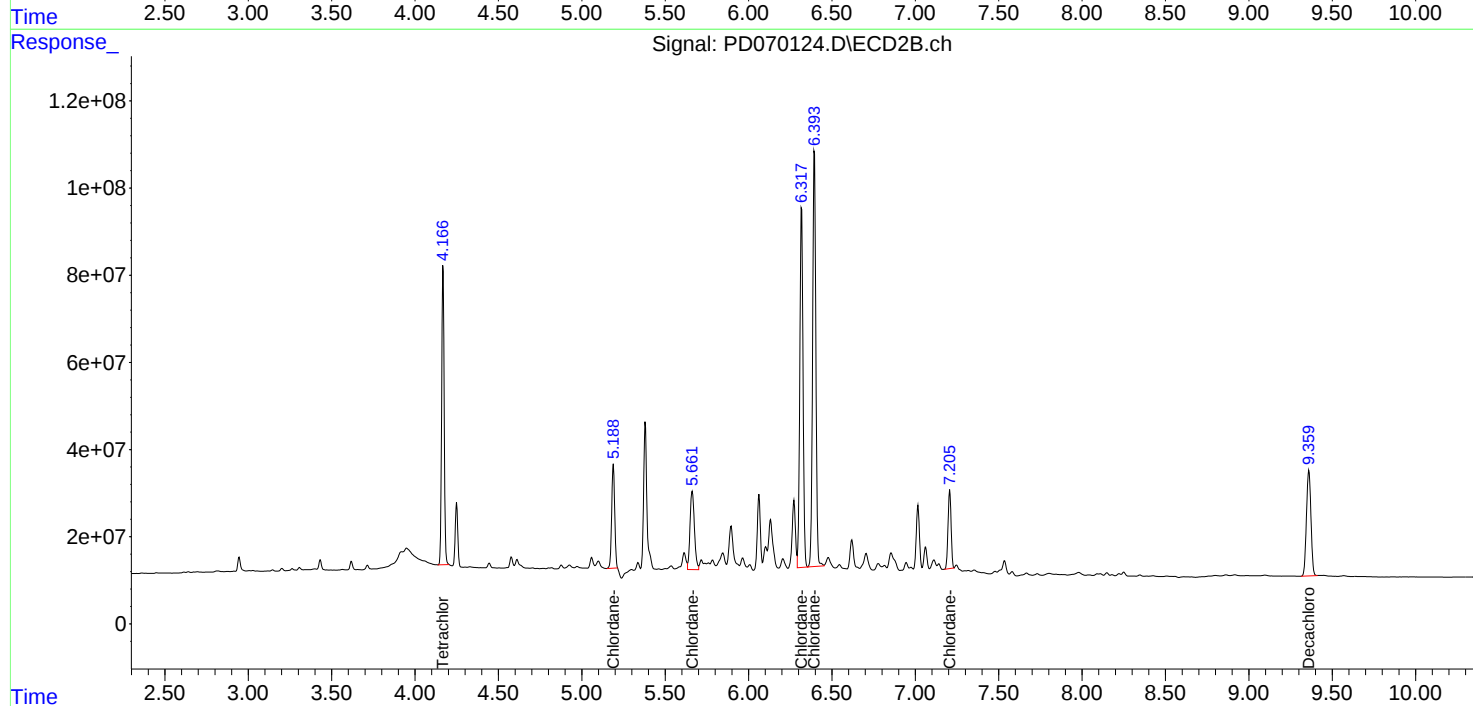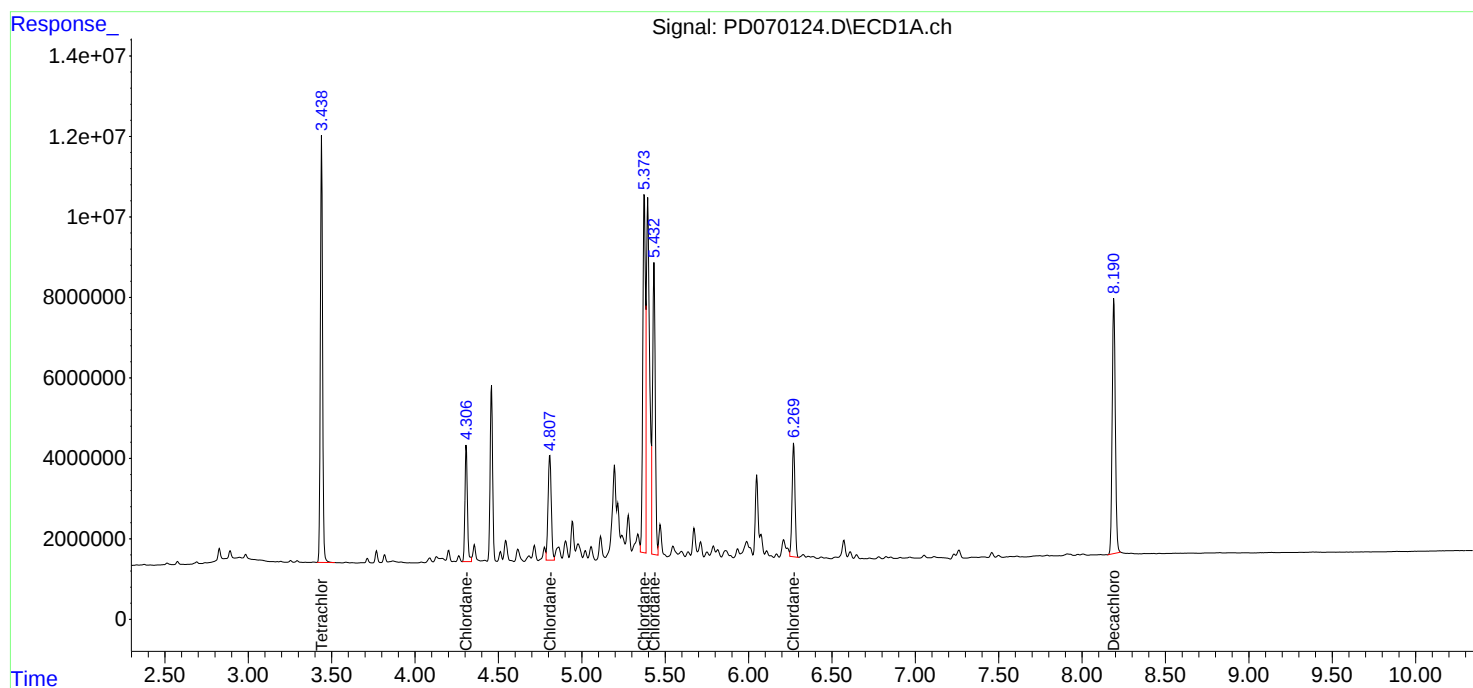


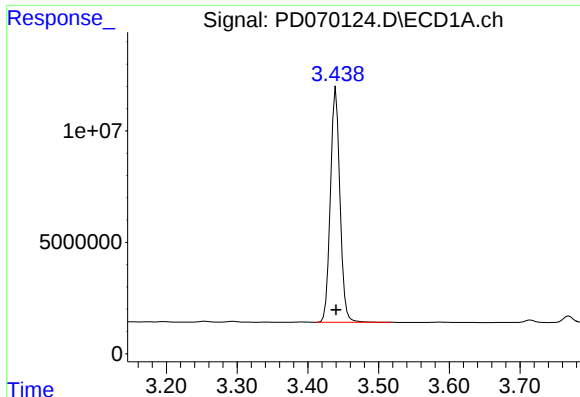

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 98809390
Conc: 77.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

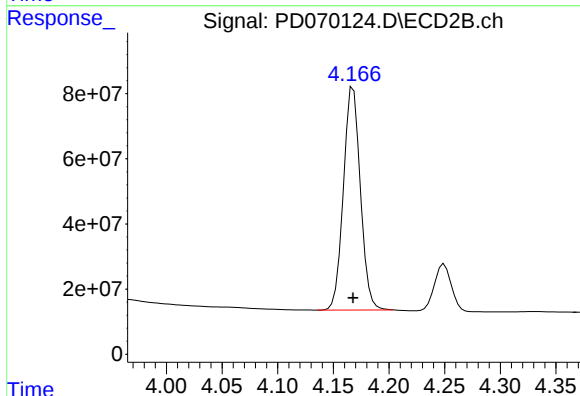


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 726568831
Conc: 77.01 ng/ml

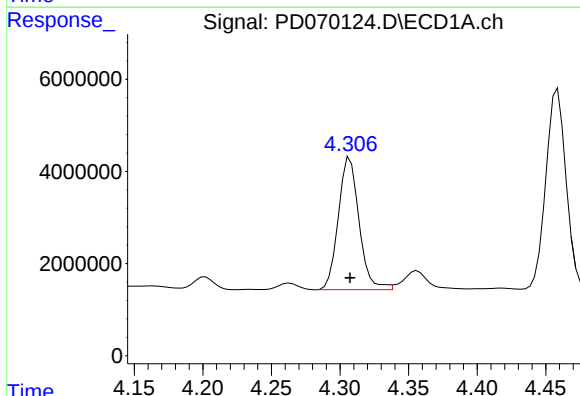


#23 Chlordane-1

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 30233695
Conc: 766.16 ng/ml

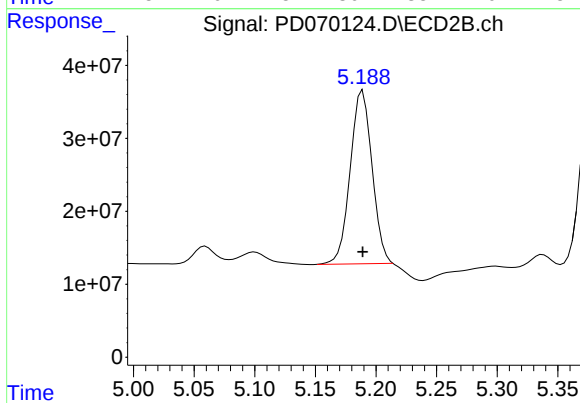

#23 Chlordane-1


R.T.: 5.189 min
Delta R.T.: 0.000 min
Response: 298419083
Conc: 764.40 ng/ml

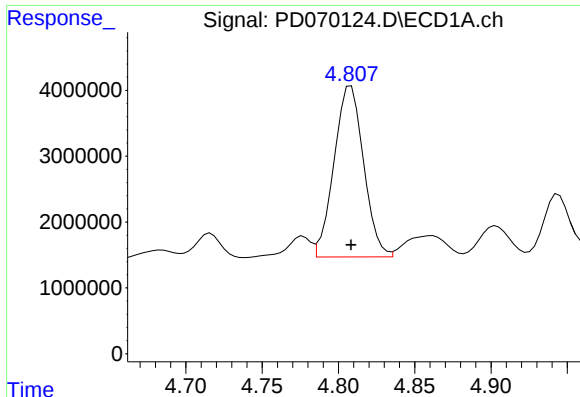

#24 Chlordane-2


R.T.: 4.808 min
Delta R.T.: 0.000 min
Response: 35007796
Conc: 769.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

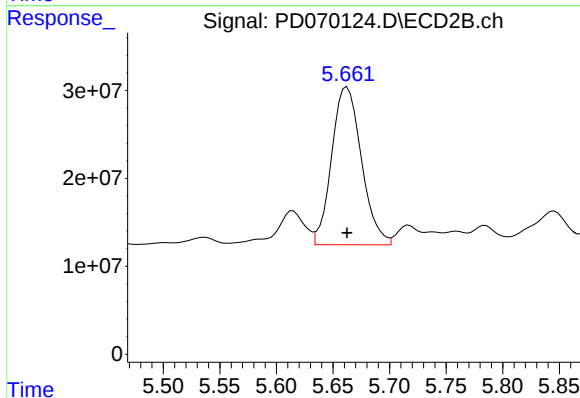


#24 Chlordane-2

R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 329175855
Conc: 762.30 ng/ml

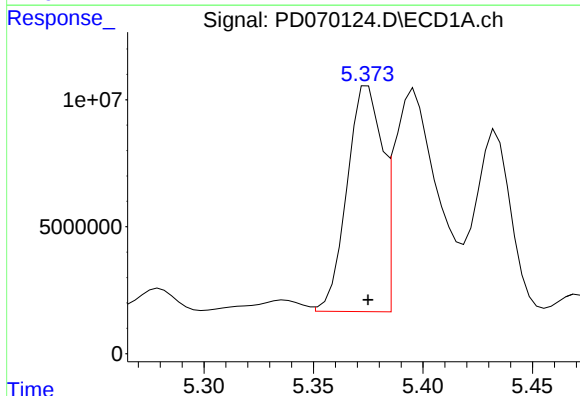


#25 Chlordane-3

R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 98449697
Conc: 760.29 ng/ml

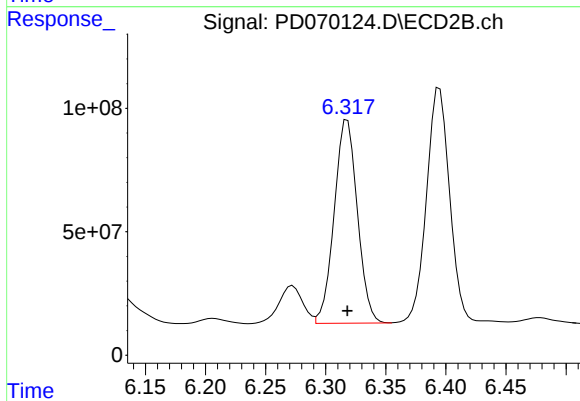

#25 Chlordane-3


R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 1107782520
Conc: 768.03 ng/ml

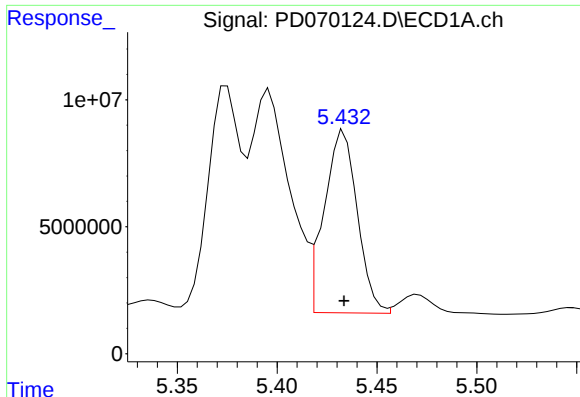

#26 Chlordane-4


R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 82988170
Conc: 762.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

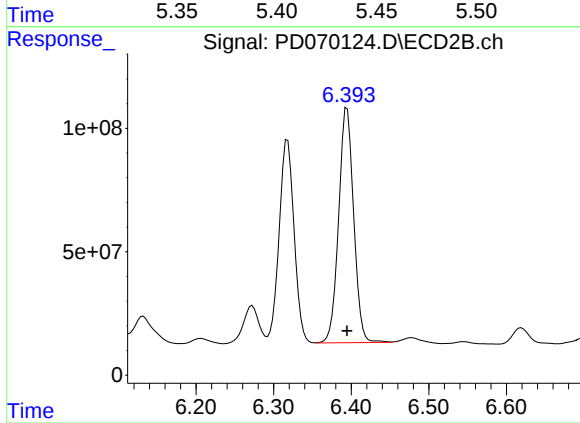


#26 Chlordane-4

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 1281687258
Conc: 765.71 ng/ml

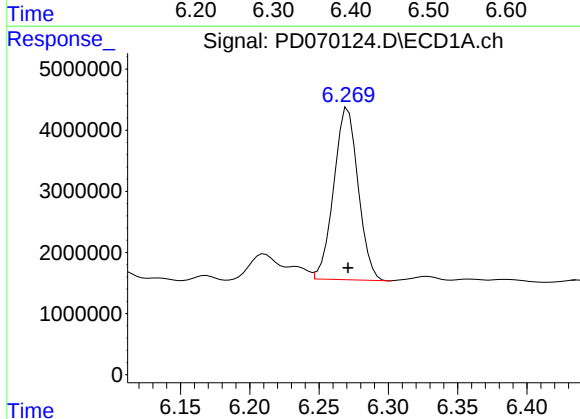


#27 Chlordane-5

R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 34439078
Conc: 772.49 ng/ml

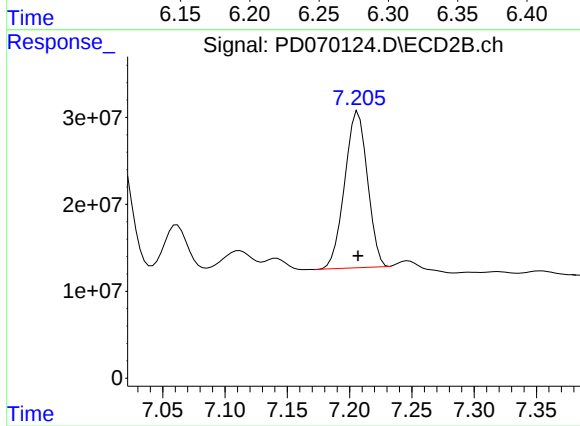

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 229534552
Conc: 768.28 ng/ml

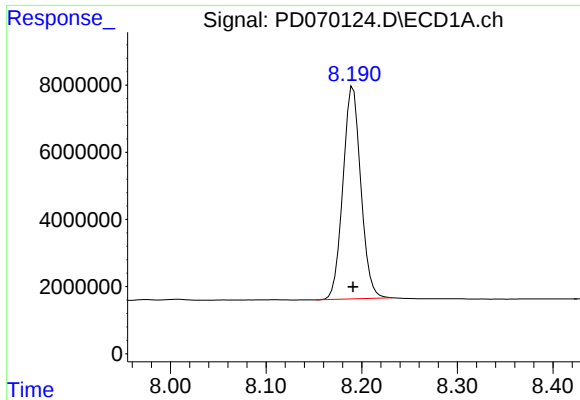

#28 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 82469956
Conc: 76.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

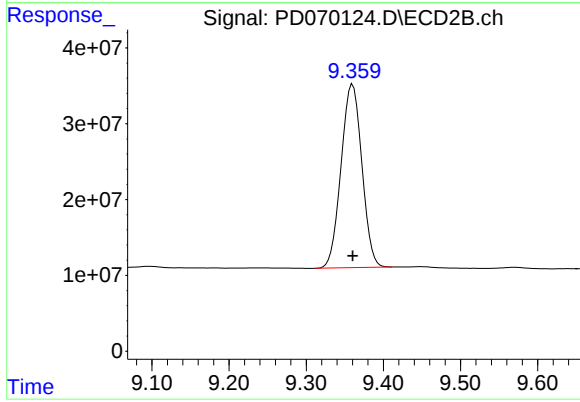

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 452972259
Conc: 78.36 ng/ml